

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
 Data File : PD056987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2020 13:17
 Operator : AJ\MA
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD011820CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 06:21:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	45626744	82780333	55.248	50.588
28)	SA Decachlor...	7.956	8.995	48212500	81936777	49.746	49.160
Target Compounds							
23)	Chlordane-1	4.125	4.947	13758238	32160310	497.510	497.701
24)	Chlordane-2	4.615	5.412	18481712	35921251	527.191	523.666
25)	Chlordane-3	5.170	6.056	48455625	142.7E6	494.825	505.723
26)	Chlordane-4	5.226	6.129	43132351	169.4E6	495.988	501.550
27)	Chlordane-5	6.049	6.930	17016700	29485450	491.828	528.156



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011820\
Data File : PD056987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2020 13:17
Operator : AJ\MA
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD011820CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 06:21:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

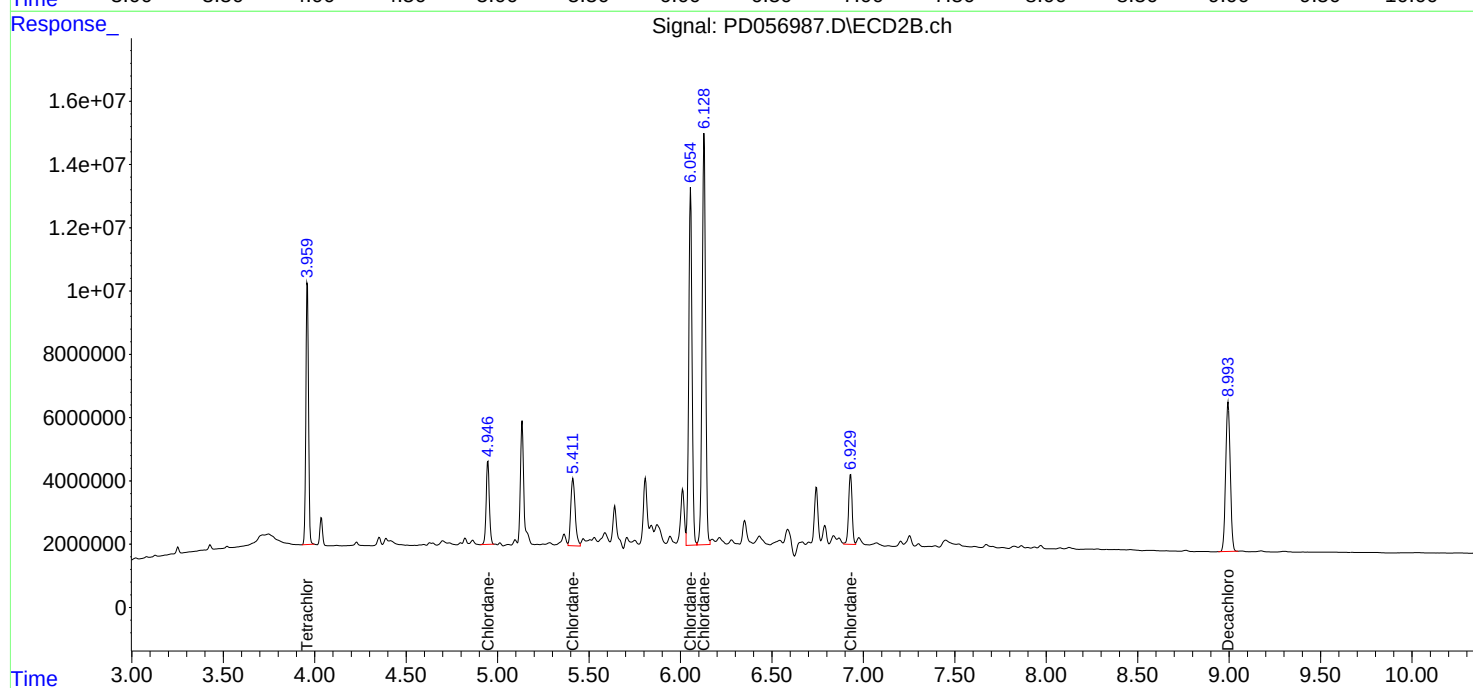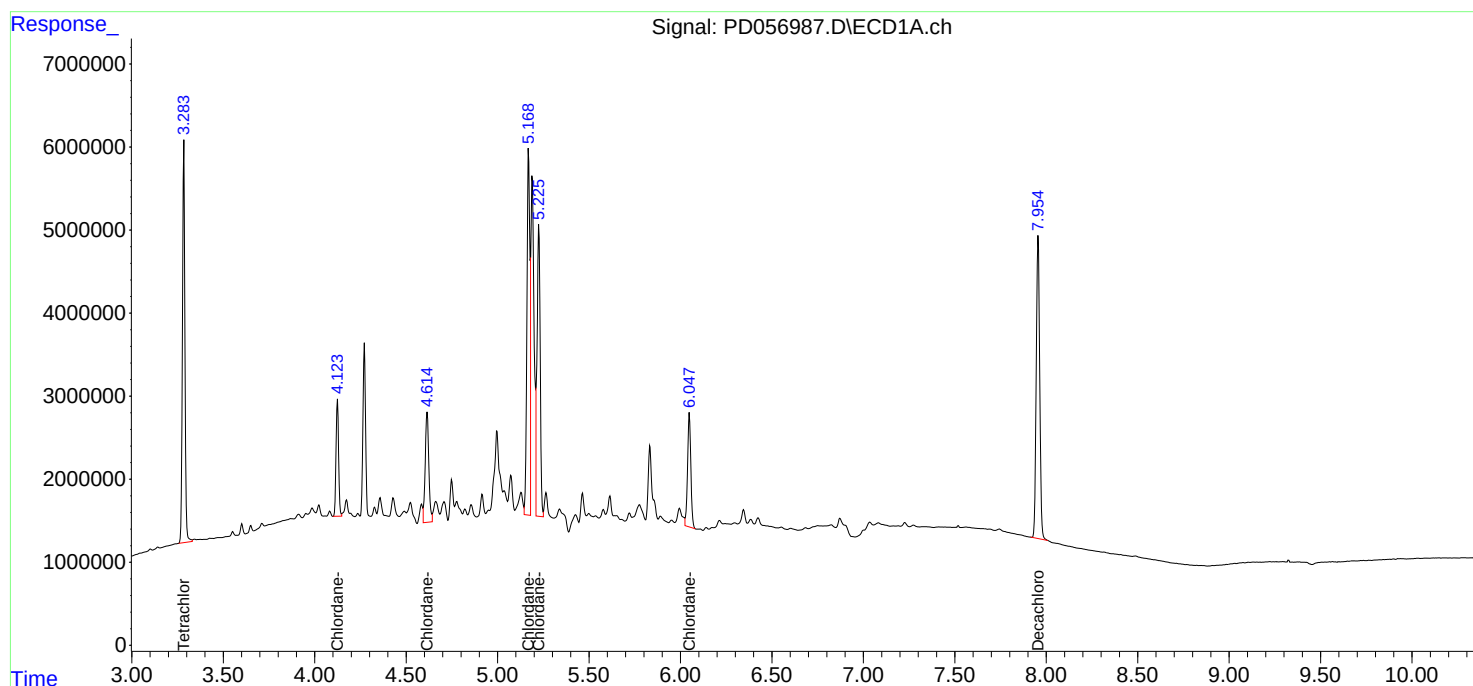


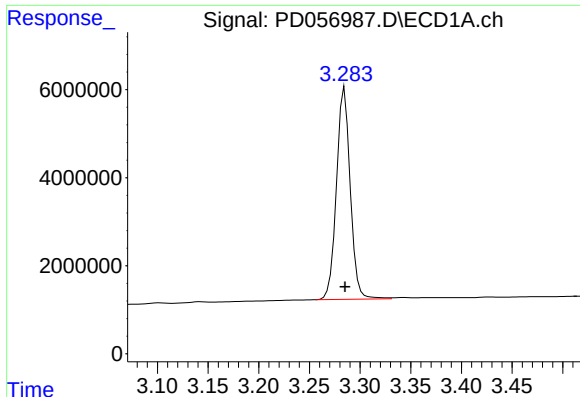

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 45626744
Conc: 55.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD011820CHLOR

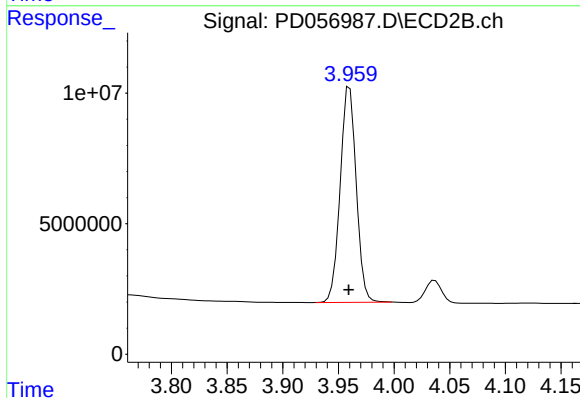


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 82780333
Conc: 50.59 ng/ml

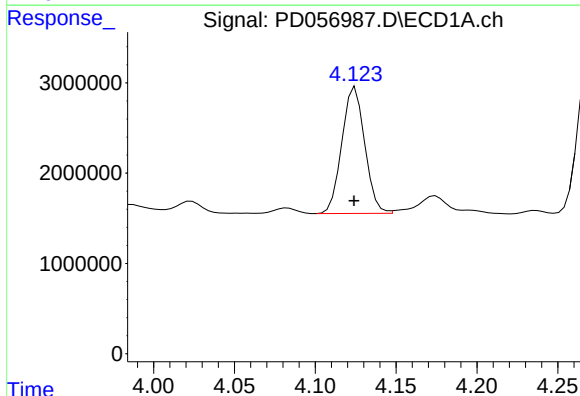


#23 Chlordane-1

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 13758238
Conc: 497.51 ng/ml

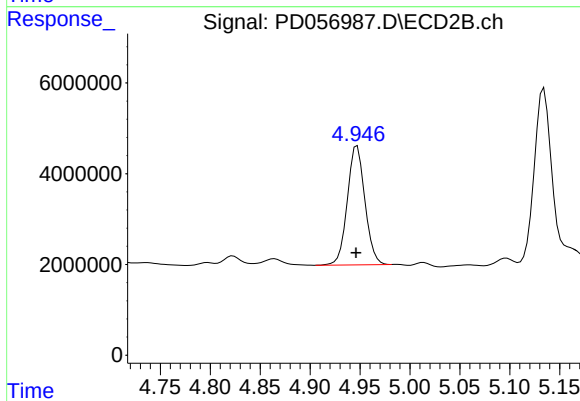

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.001 min
Response: 32160310
Conc: 497.70 ng/ml

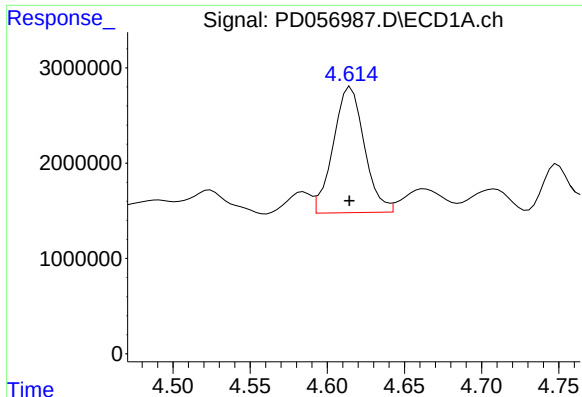

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: 0.000 min
Response: 18481712
Conc: 527.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD011820CHLOR

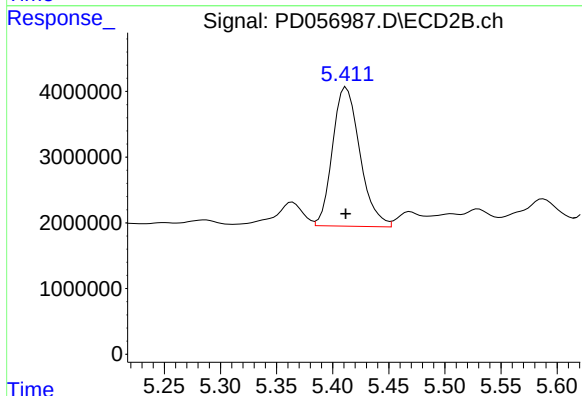


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 35921251
Conc: 523.67 ng/ml

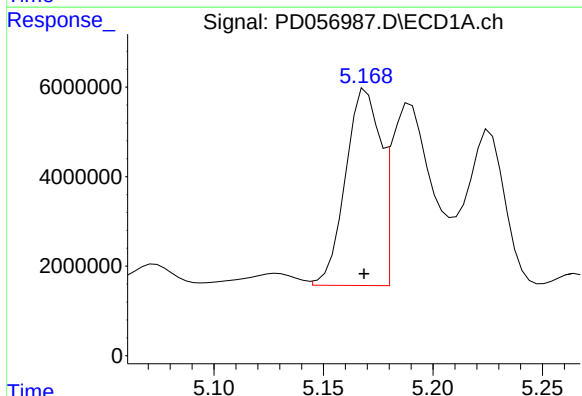


#25 Chlordane-3

R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 48455625
Conc: 494.83 ng/ml

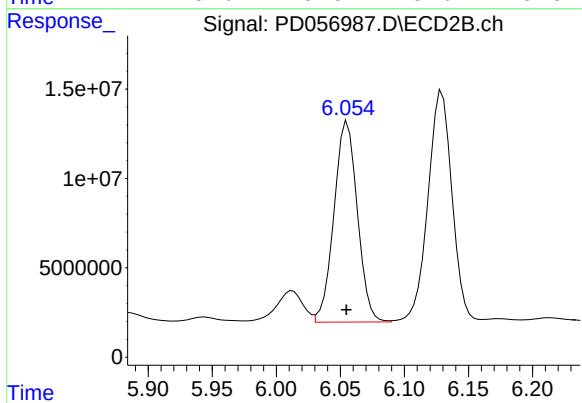

#25 Chlordane-3


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 142690380
Conc: 505.72 ng/ml

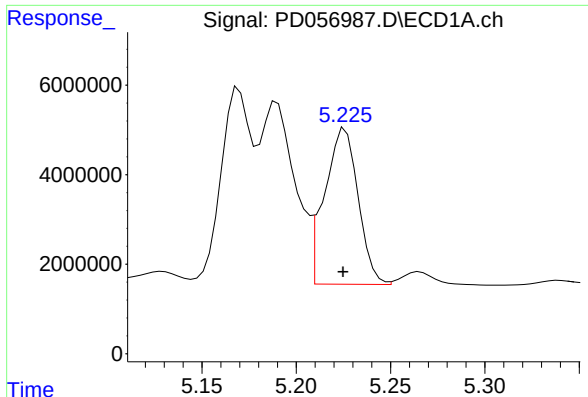

#26 Chlordane-4


R.T.: 5.226 min
Delta R.T.: 0.001 min
Response: 43132351
Conc: 495.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD011820CHLOR

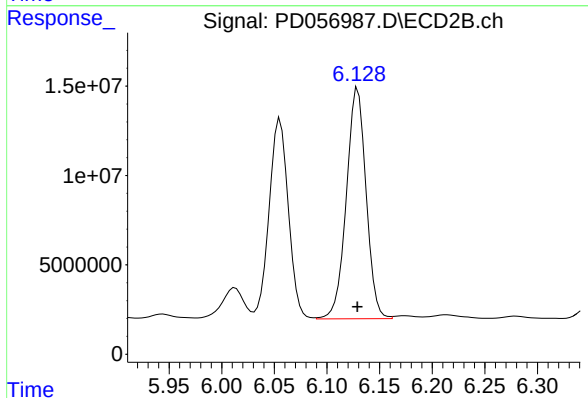


#26 Chlordane-4

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 169363942
Conc: 501.55 ng/ml

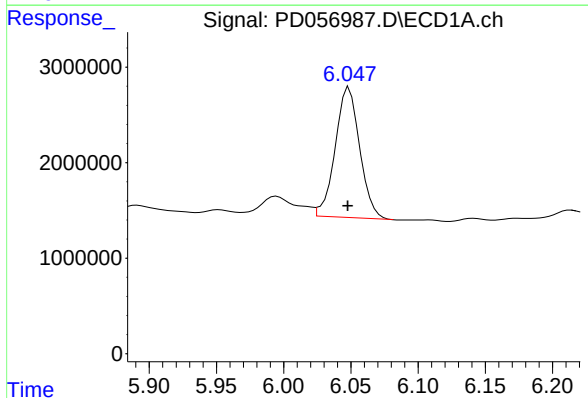


#27 Chlordane-5

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 17016700
Conc: 491.83 ng/ml

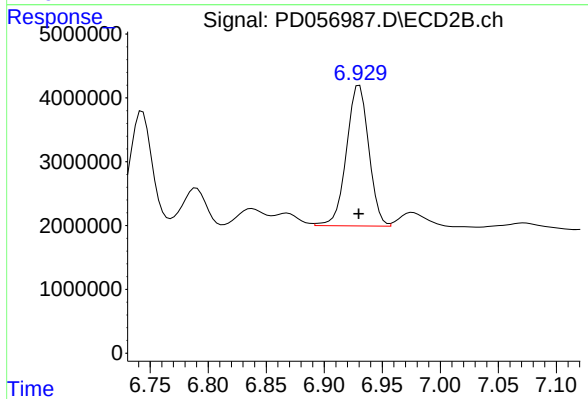

#27 Chlordane-5

R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 29485450
Conc: 528.16 ng/ml

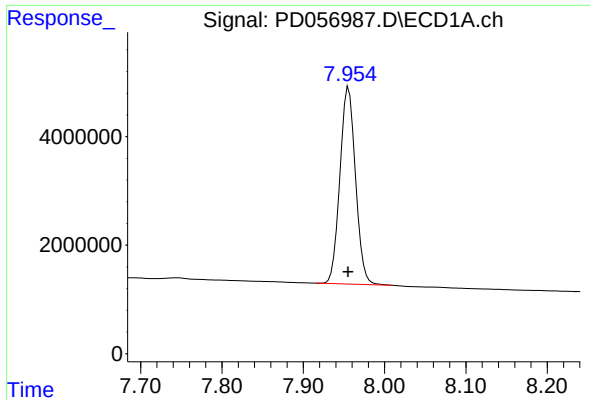

#28 Decachlorobiphenyl


R.T.: 7.956 min

Delta R.T.: 0.000 min

Response: 48212500

Conc: 49.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD011820CHLOR

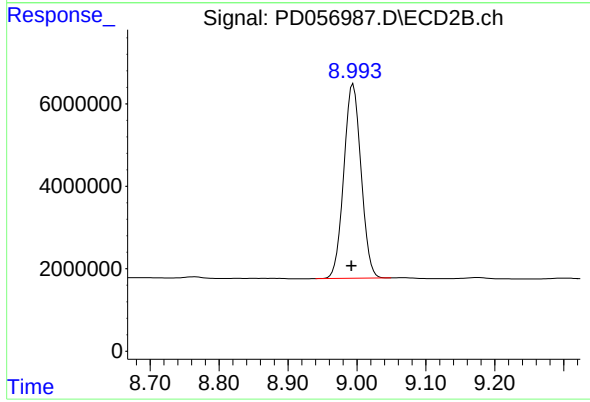

#28 Decachlorobiphenyl

R.T.: 8.995 min

Delta R.T.: 0.002 min

Response: 81936777

Conc: 49.16 ng/ml