

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011822\
 Data File : PD067698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2022 09:17
 Operator : AR\AJ
 Sample : PIBLK200
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 02:12:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.431	3.960	39226391	154.0E6	17.314	19.006
2) SA Decachlor...	8.154	9.014	34567894	181.2E6	36.093	35.859
Target Compounds						
6) B beta-BHC	0.000	4.831	0	593581	N.D.	0.128
7) B delta-BHC	0.000	5.055	0	984319	N.D.	0.105


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011822\
Data File : PD067698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2022 09:17
Operator : AR\AJ
Sample : PIBLK200
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 02:12:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

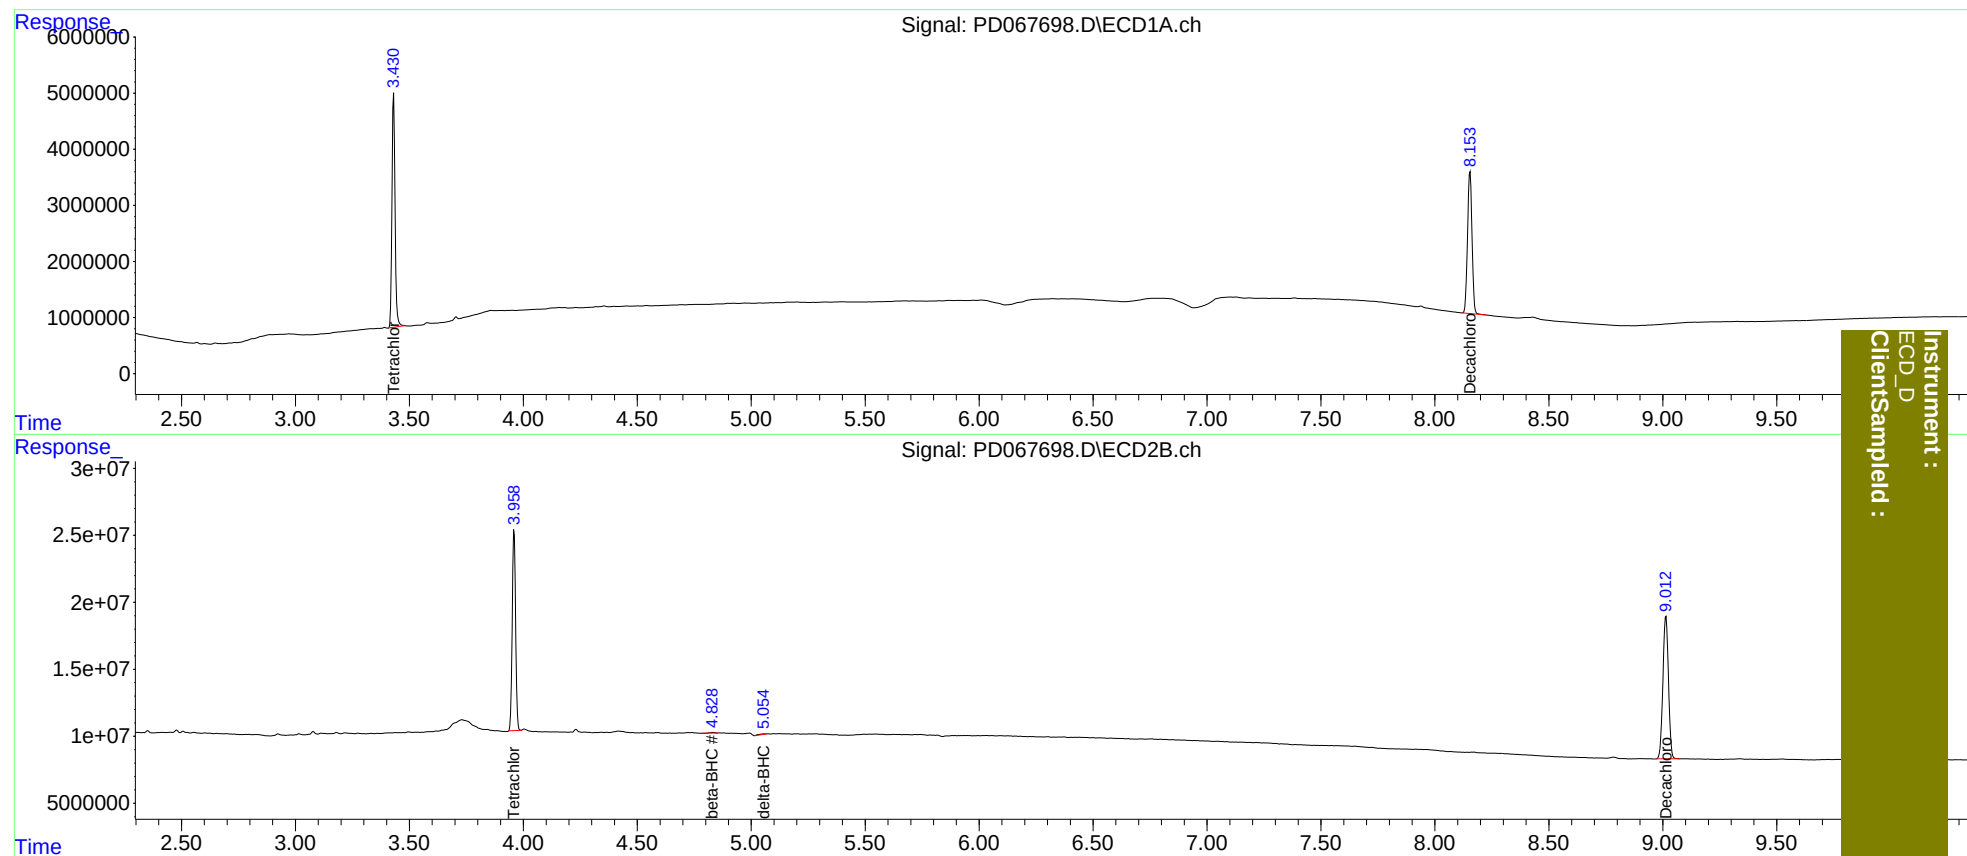


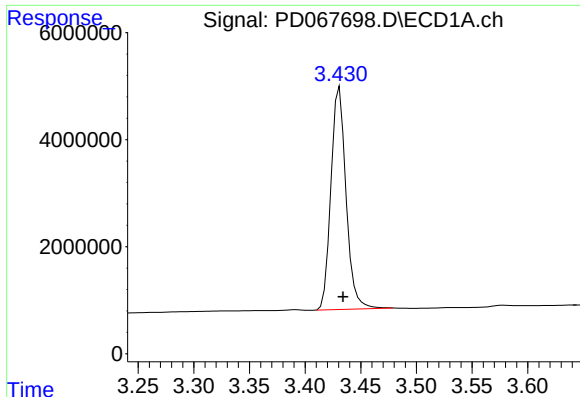

#1 Tetrachloro-m-xylene


R.T.: 3.431 min
Delta R.T.: -0.003 min
Response: 39226391
Conc: 17.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

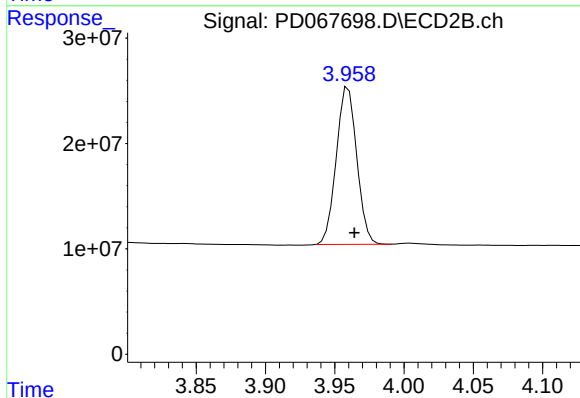


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.004 min
Response: 154038885
Conc: 19.01 ng/ml

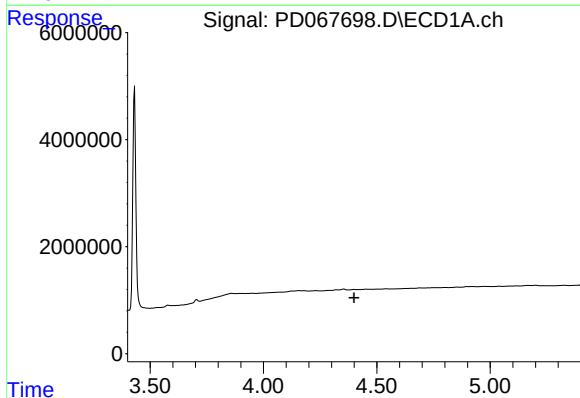


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.400 min
Response: 0
Conc: N.D.

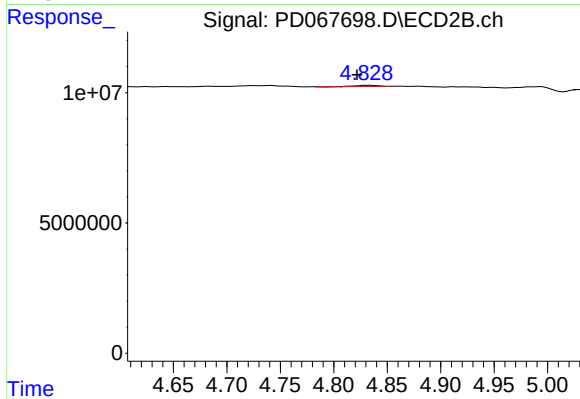

#6 beta-BHC


R.T.: 4.831 min
Delta R.T.: 0.009 min
Response: 593581
Conc: 0.13 ng/ml

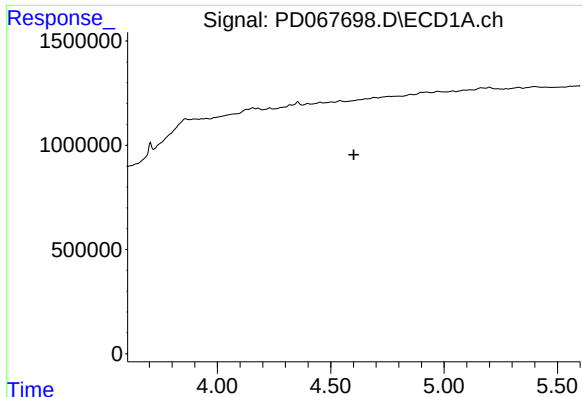

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.602 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

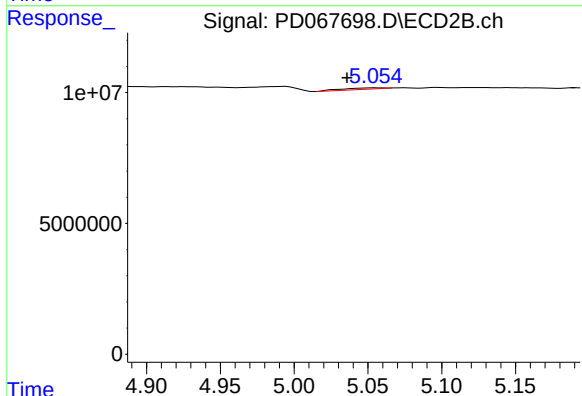


#7 delta-BHC

R.T.: 5.055 min
Delta R.T.: 0.019 min
Response: 984319
Conc: 0.10 ng/ml

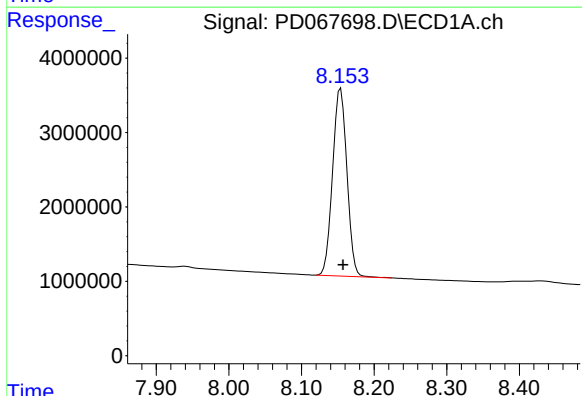

#27 Decachlorobiphenyl

R.T.: 8.154 min
Delta R.T.: -0.003 min
Response: 34567894
Conc: 36.09 ng/ml

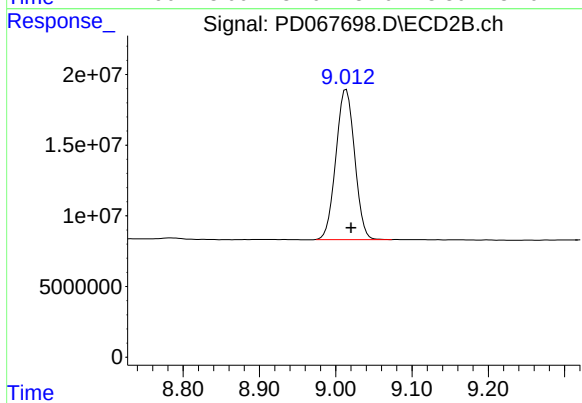

#27 Decachlorobiphenyl

R.T.: 9.014 min
Delta R.T.: -0.006 min
Response: 181198317
Conc: 35.86 ng/ml