

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011922\
 Data File : PD067721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2022 14:48
 Operator : AR\AJ
 Sample : PIBLK203
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 01:08:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.430	3.960	38081254	142.6E6	16.808	17.590
27)	SA Decachlor...	8.150	9.013	31056919	159.5E6	32.427	31.566
Target Compounds							
7)	B delta-BHC	0.000	5.042	0	2218417	N.D.	0.237
8)	B Heptachlo...	5.196f	0.000	3419542	0	1.230	N.D. #
13)	MA Dieldrin	0.000	6.483	0	1415855	N.D.	0.188
14)	MA Endrin	0.000	6.716f	0	1362324	N.D.	0.244
15)	B Endosulfa...	6.289f	0.000	16263322	0	7.518	N.D. #
17)	MA 4,4'-DDT	6.330	7.141f	6168520	-6760936	2.995	N.D. #
18)	B Endrin al...	0.000	6.955f	0	1504482	N.D.	0.318
19)	B Endosulfa...	0.000	7.289f	0	2846407	N.D.	0.488
20)	A Methoxychlor	0.000	7.567	0	4113896	N.D.	1.492
24)	Toxaphene-3	6.289	7.141	16263322	-6760936	428.130	N.D. #
26)	Toxaphene-5	0.000	7.567	0	4113896	N.D.	53.950


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011922\
Data File : PD067721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2022 14:48
Operator : AR\AJ
Sample : PIBLK203
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 01:08:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

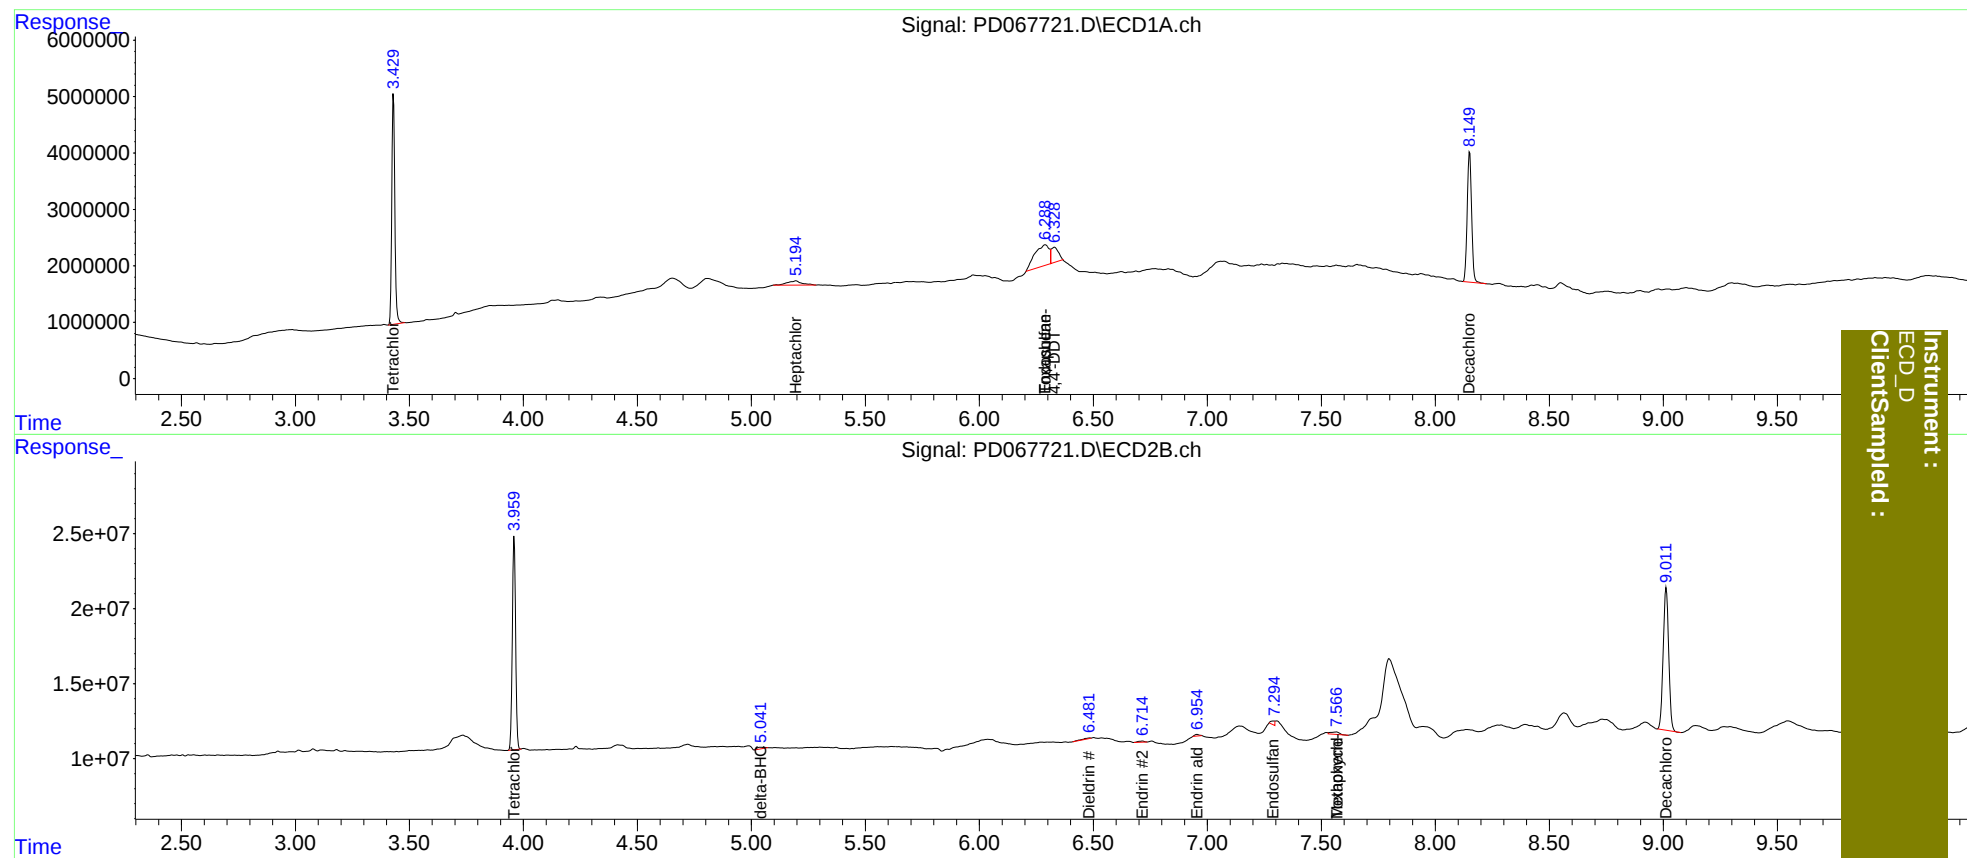


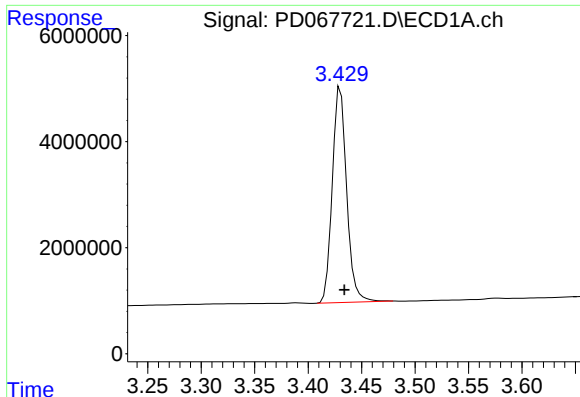

#1 Tetrachloro-m-xylene


R.T.: 3.430 min
Delta R.T.: -0.004 min
Response: 38081254
Conc: 16.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

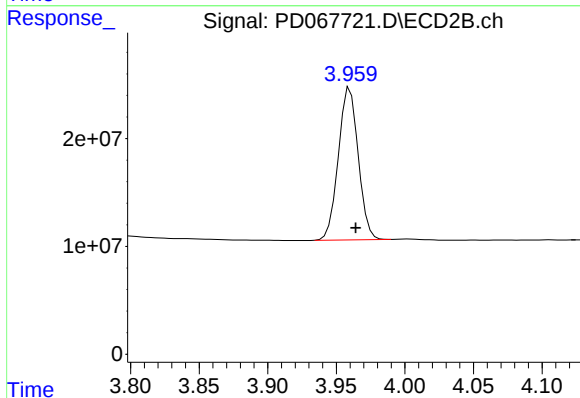


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.004 min
Response: 142563088
Conc: 17.59 ng/ml

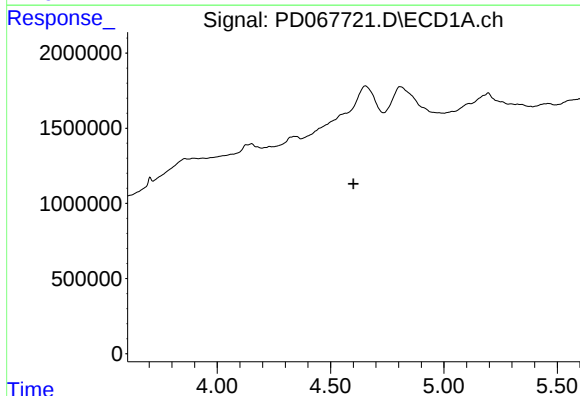


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.602 min
Response: 0
Conc: N.D.

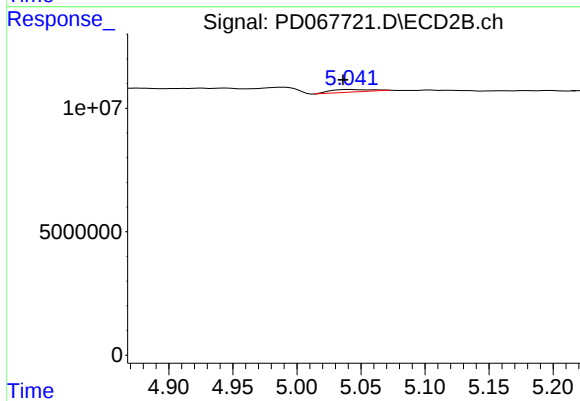

#7 delta-BHC


R.T.: 5.042 min
Delta R.T.: 0.006 min
Response: 2218417
Conc: 0.24 ng/ml

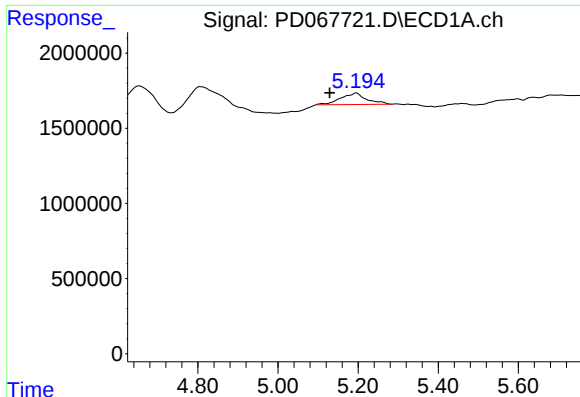

#8 Heptachlor epoxide


R.T.: 5.196 min
Delta R.T.: 0.066 min
Response: 3419542
Conc: 1.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

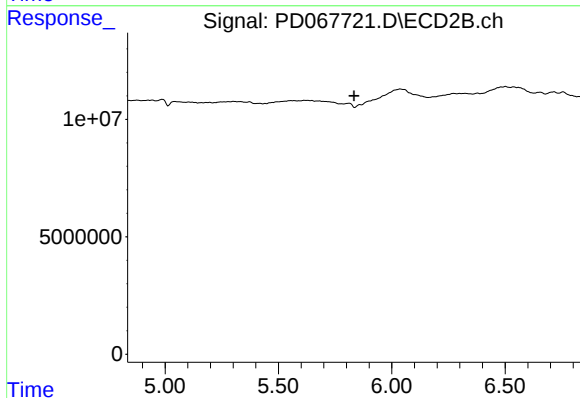


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.833 min
Response: 0
Conc: N.D.

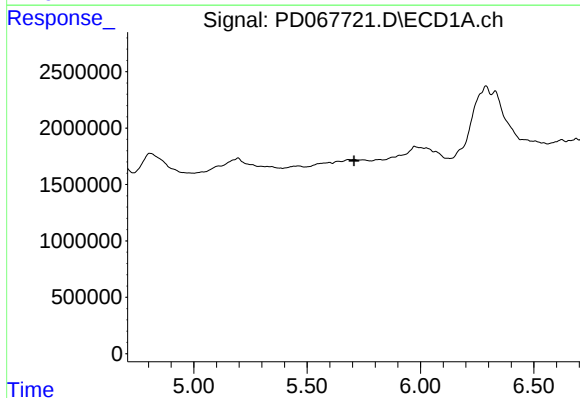


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.708 min
Response: 0
Conc: N.D.

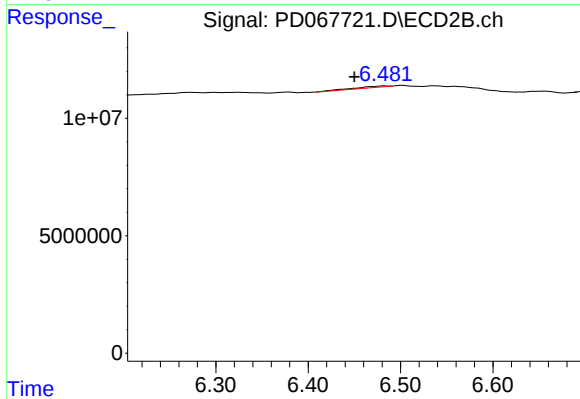

#13 Dieldrin


R.T.: 6.483 min
Delta R.T.: 0.033 min
Response: 1415855
Conc: 0.19 ng/ml

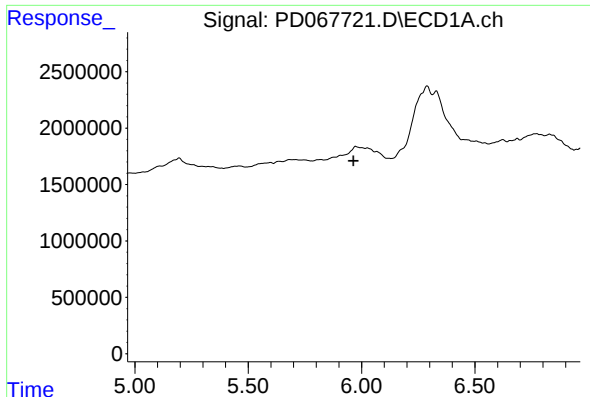

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

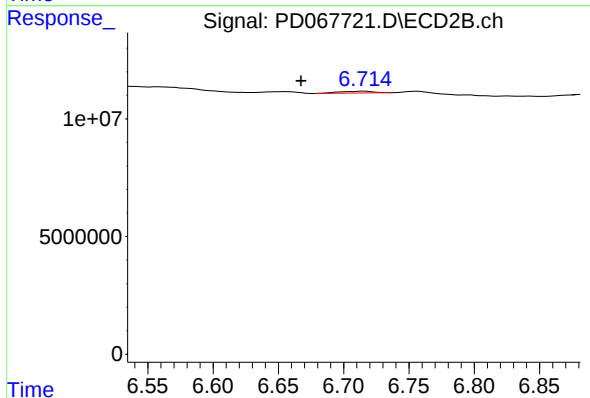


#14 Endrin

R.T.: 6.716 min
Delta R.T.: 0.049 min
Response: 1362324
Conc: 0.24 ng/ml

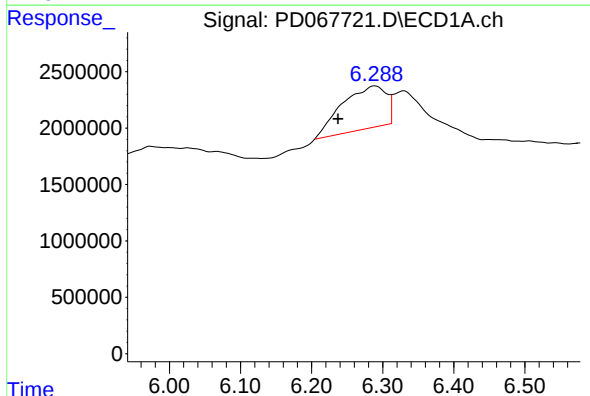


#15 Endosulfan II

R.T.: 6.289 min
Delta R.T.: 0.052 min
Response: 16263322
Conc: 7.52 ng/ml

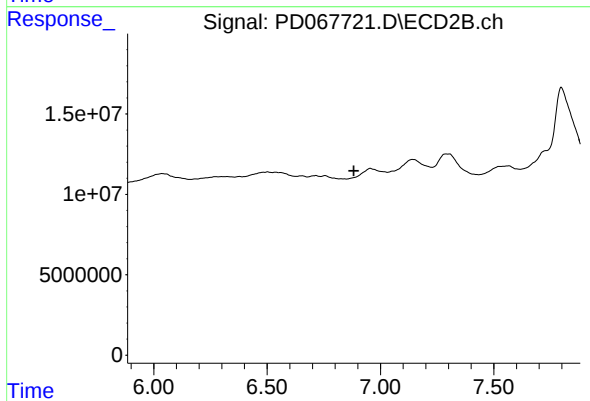

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.883 min
Response: 0
Conc: N.D.

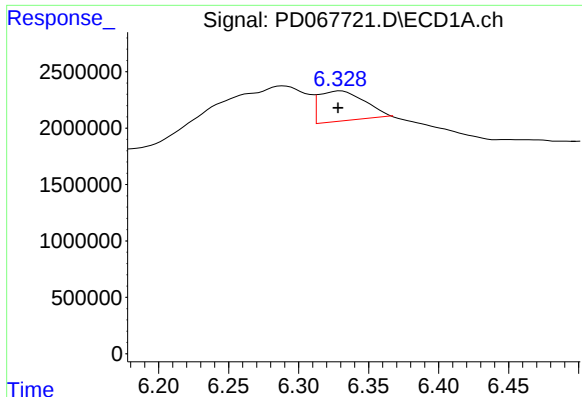

#17 4,4'-DDT


R.T.: 6.330 min
Delta R.T.: 0.002 min
Response: 6168520
Conc: 3.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

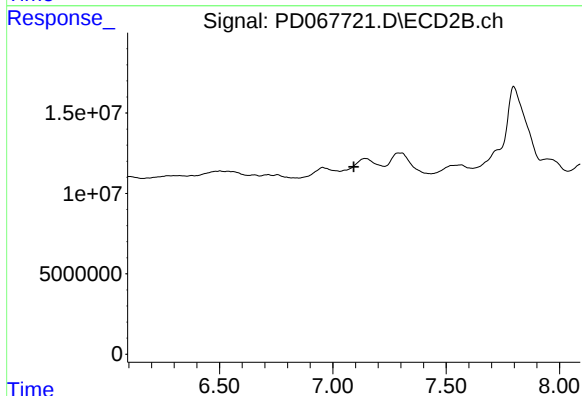


#17 4,4'-DDT

R.T.: 7.141 min
Delta R.T.: 0.048 min
Response: -6760936
Conc: N.D.

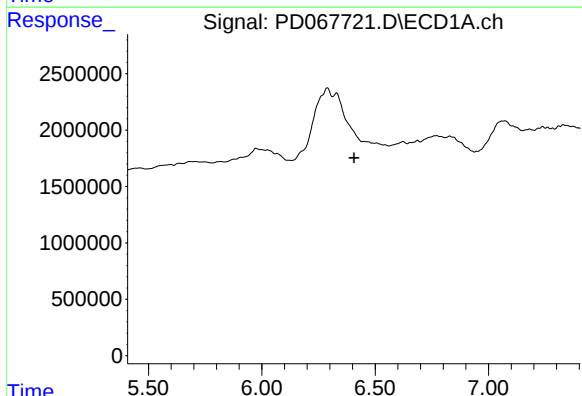


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.407 min
Response: 0
Conc: N.D.

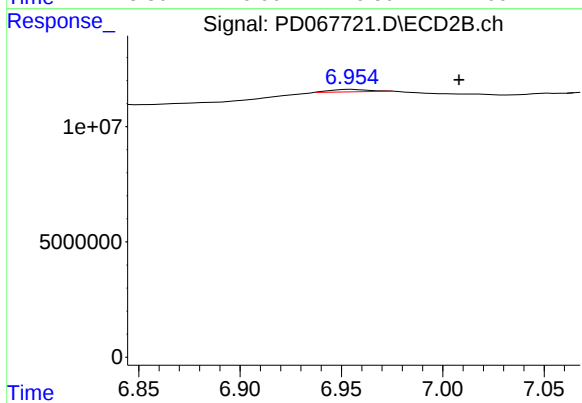

#18 Endrin aldehyde


R.T.: 6.955 min
Delta R.T.: -0.053 min
Response: 1504482
Conc: 0.32 ng/ml

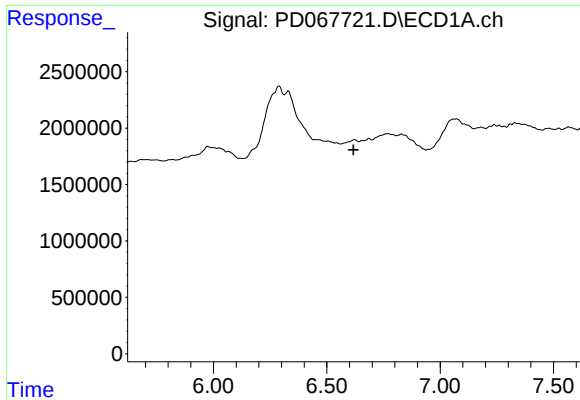

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.618 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

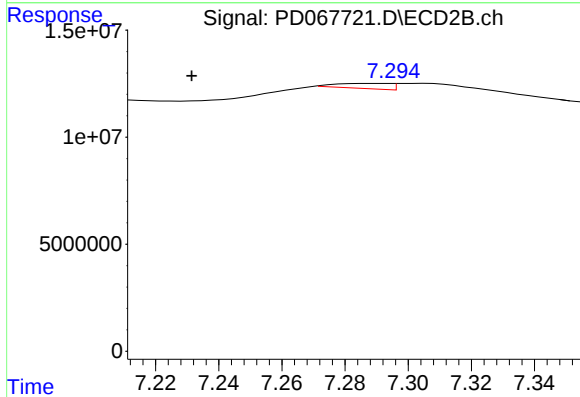


#19 Endosulfan Sulfate

R.T.: 7.289 min
Delta R.T.: 0.057 min
Response: 2846407
Conc: 0.49 ng/ml

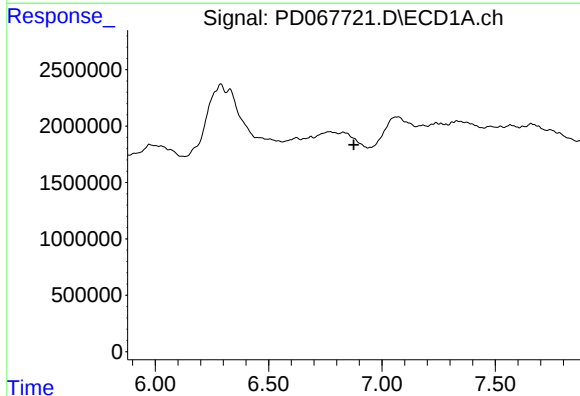


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.876 min
Response: 0
Conc: N.D.

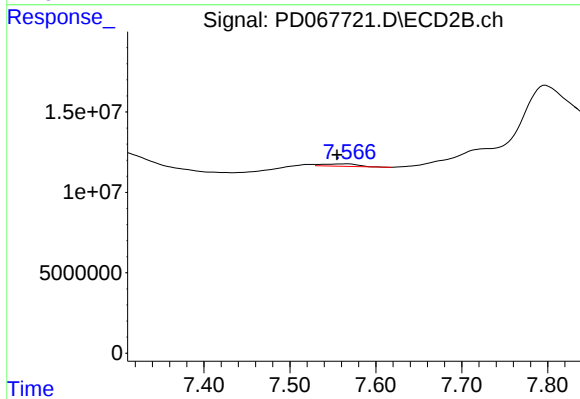

#20 Methoxychlor


R.T.: 7.567 min
Delta R.T.: 0.012 min
Response: 4113896
Conc: 1.49 ng/ml

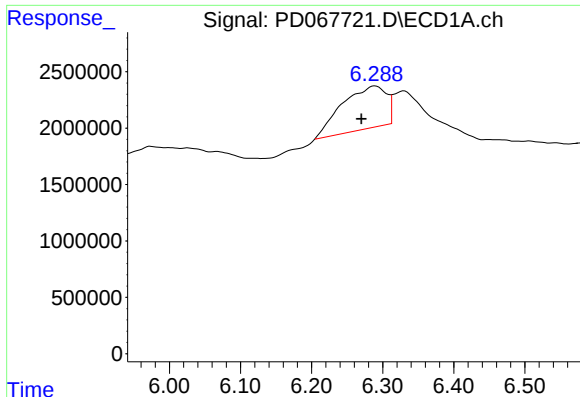

#24 Toxaphene-3


R.T.: 6.289 min
Delta R.T.: 0.019 min
Response: 16263322
Conc: 428.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

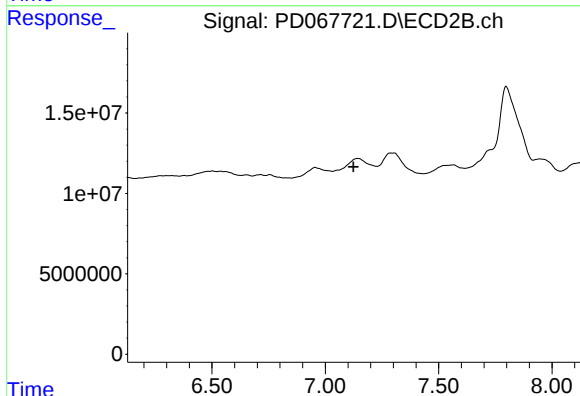


#24 Toxaphene-3

R.T.: 7.141 min
Delta R.T.: 0.016 min
Response: -6760936
Conc: N.D.

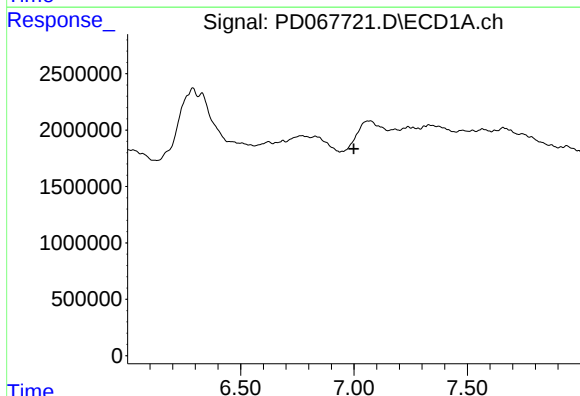


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.000 min
Response: 0
Conc: N.D.

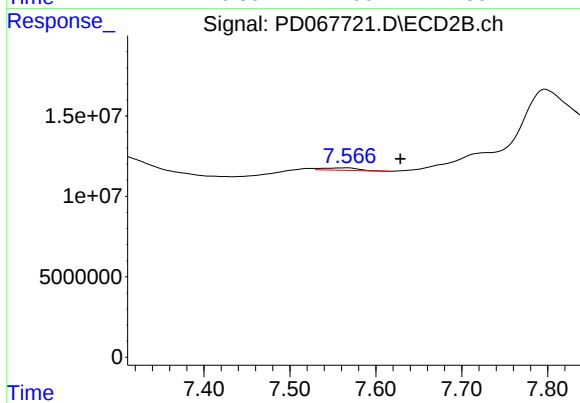

#26 Toxaphene-5


R.T.: 7.567 min
Delta R.T.: -0.061 min
Response: 4113896
Conc: 53.95 ng/ml

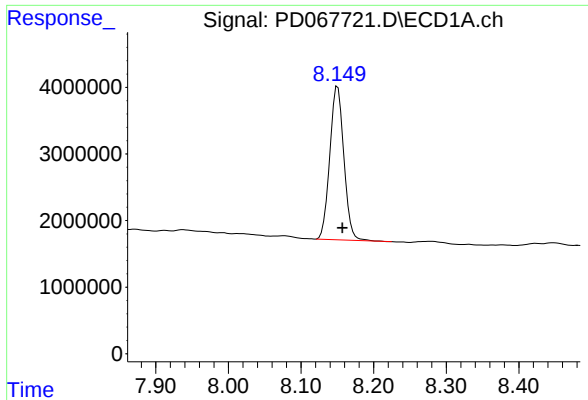

#27 Decachlorobiphenyl

R.T.: 8.150 min
Delta R.T.: -0.007 min
Response: 31056919
Conc: 32.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

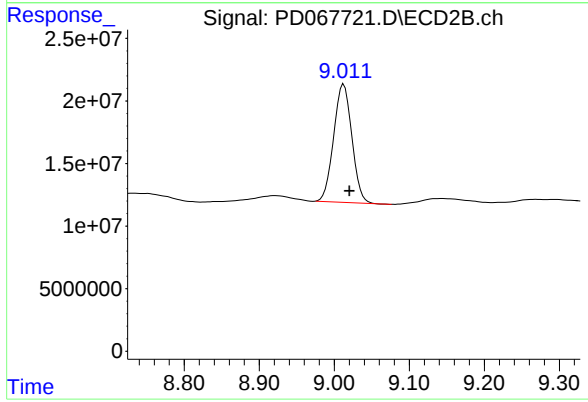

#27 Decachlorobiphenyl

R.T.: 9.013 min
Delta R.T.: -0.008 min
Response: 159504067
Conc: 31.57 ng/ml