

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
 Data File : PD073625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 16:14
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 02:47:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
4) MA	Heptachlor	4.953	0.000	777801	0	0.209	N.D. #
8) B	Heptachlo...	5.701	0.000	2783834	0	0.872	N.D. #
9) A	Endosulfan I	6.092	0.000	1986742	0	0.647	N.D. #
10) B	gamma-Chl...	5.931f	0.000	4413402	0	1.340	N.D. #
14) MA	Endrin	0.000	5.666f	0	297829	N.D.	0.268 #
15) B	Endosulfa...	6.842f	0.000	526789	0	0.199	N.D. #
21) B	Endrin ke...	7.700f	0.000	303148	0	0.100	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
Data File : PD073625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 16:14
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 02:47:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

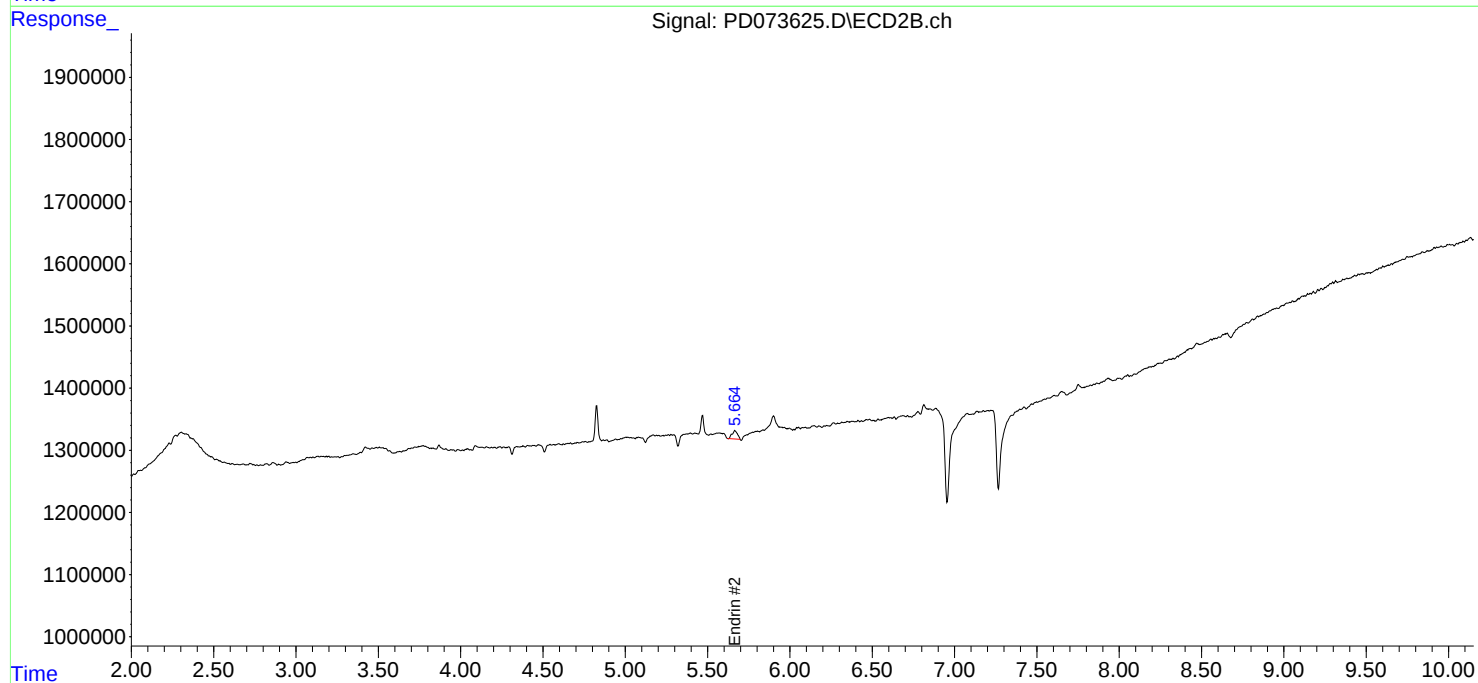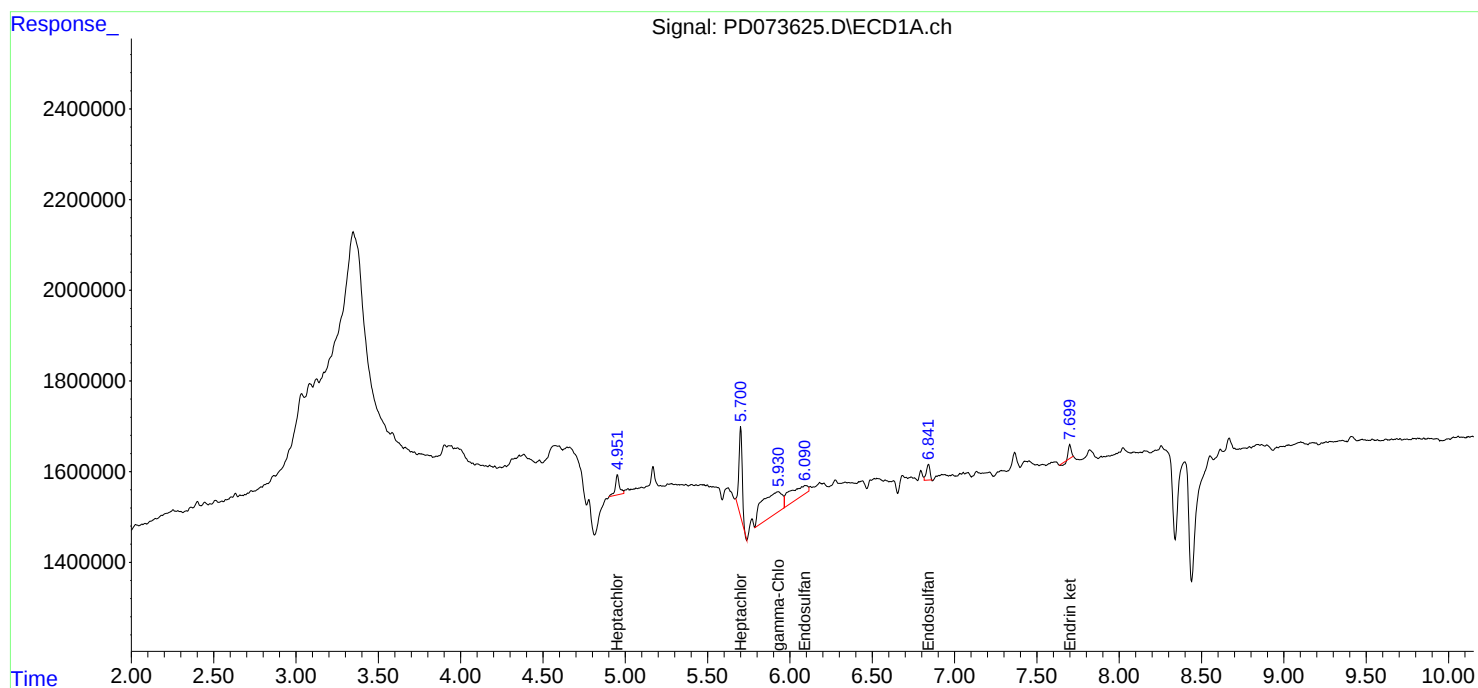


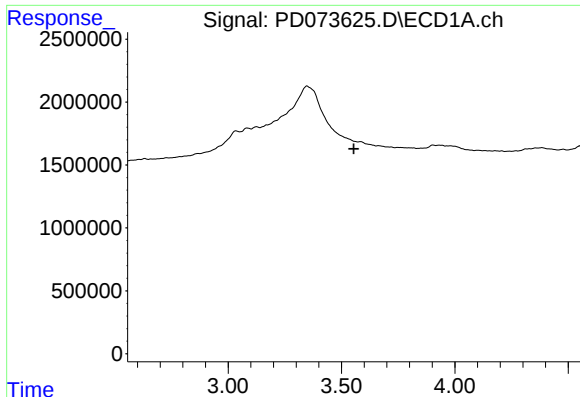

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.555 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

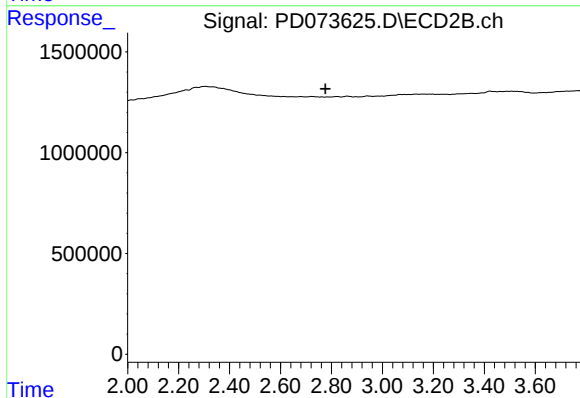


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.777 min
Response: 0
Conc: N.D.

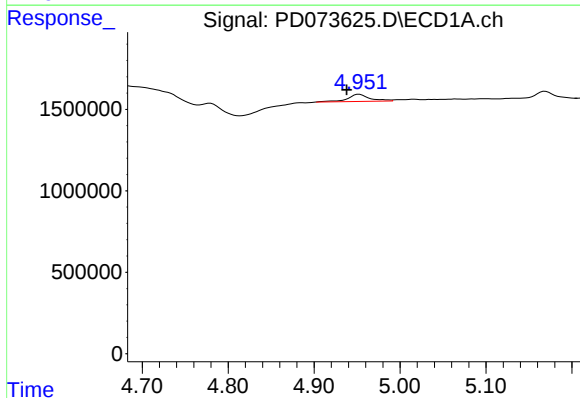


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.015 min
Response: 777801
Conc: 0.21 ng/ml

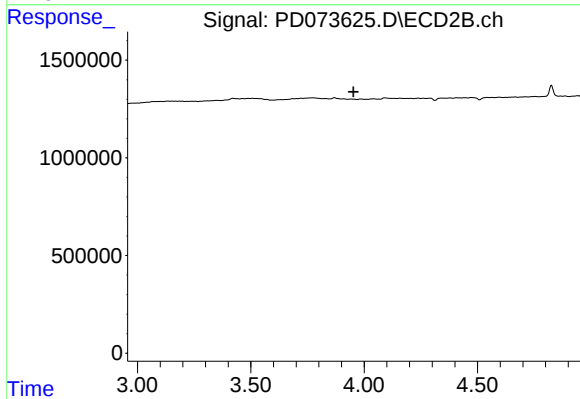

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.953 min
Response: 0
Conc: N.D.

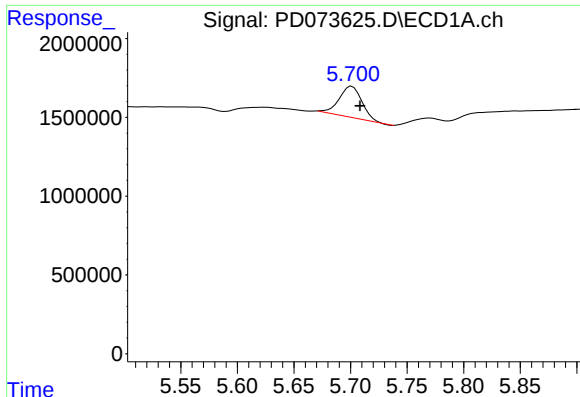

#8 Heptachlor epoxide


R.T.: 5.701 min
Delta R.T.: -0.007 min
Response: 2783834
Conc: 0.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

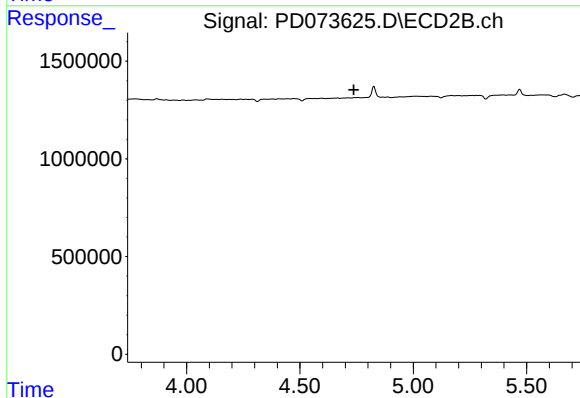


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

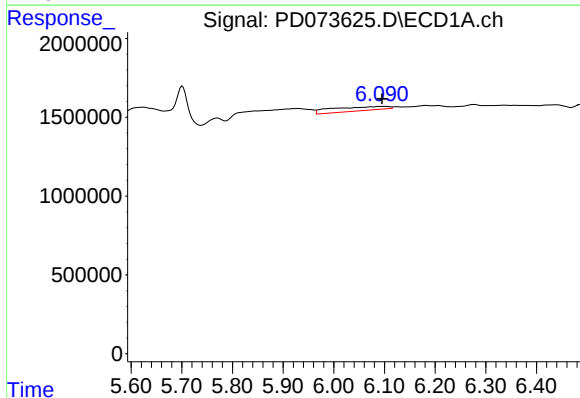


#9 Endosulfan I

R.T.: 6.092 min
Delta R.T.: -0.004 min
Response: 1986742
Conc: 0.65 ng/ml

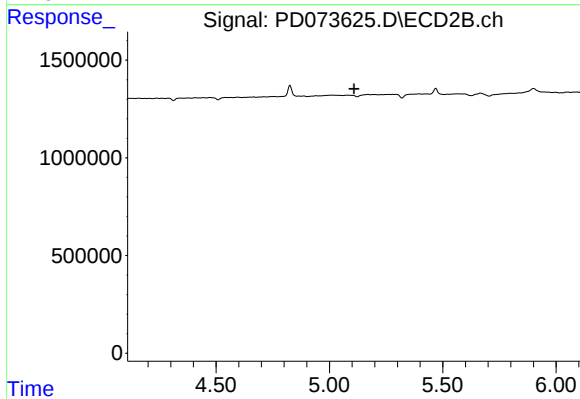

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

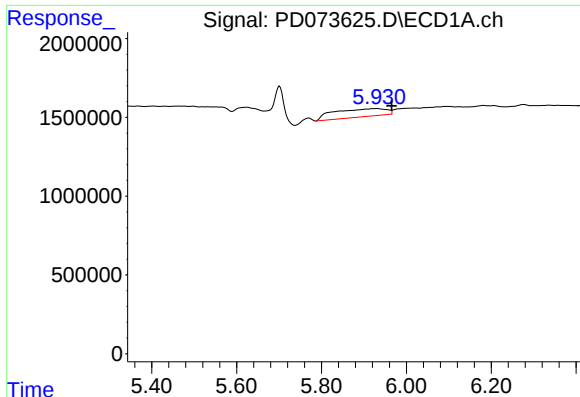

#10 gamma-Chlordane


R.T.: 5.931 min
Delta R.T.: -0.034 min
Response: 4413402
Conc: 1.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

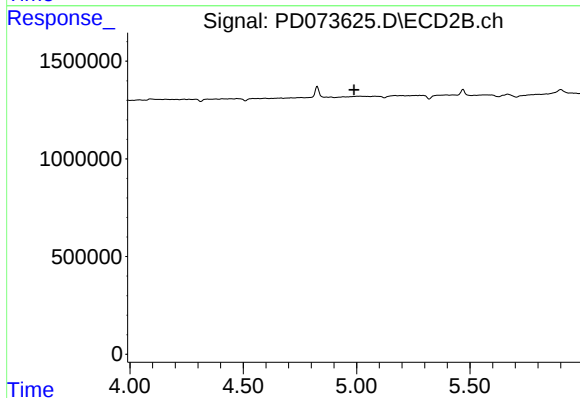


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

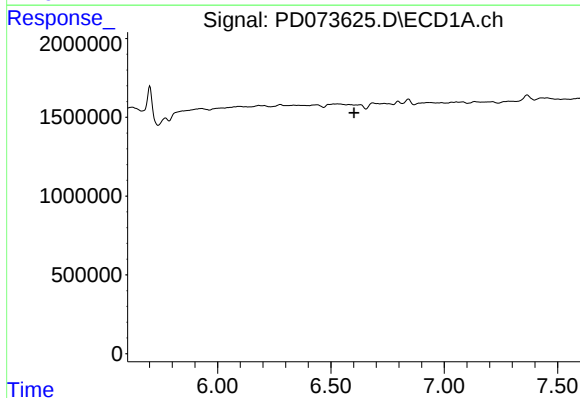


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.602 min
Response: 0
Conc: N.D.

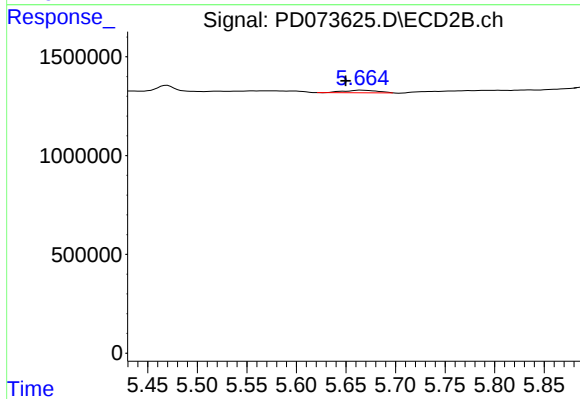

#14 Endrin


R.T.: 5.666 min
Delta R.T.: 0.016 min
Response: 297829
Conc: 0.27 ng/ml

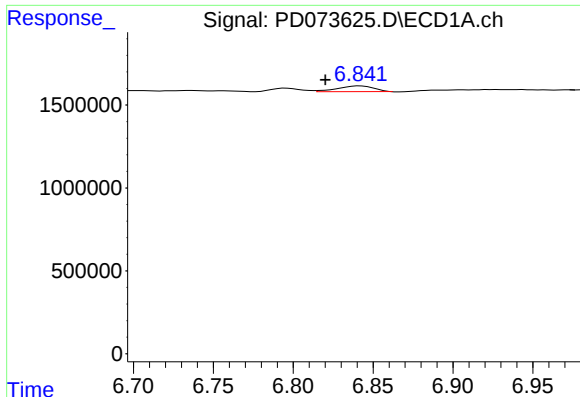

#15 Endosulfan II


R.T.: 6.842 min
Delta R.T.: 0.022 min
Response: 526789
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

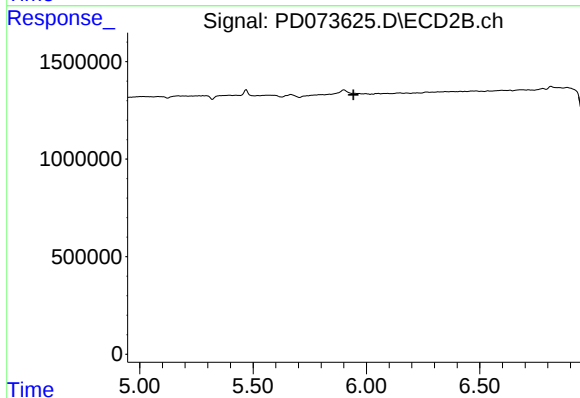


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

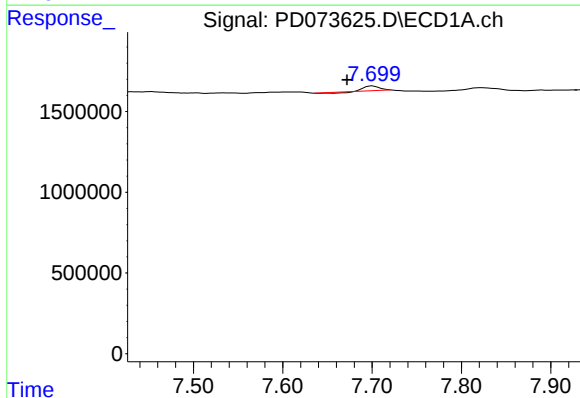


#21 Endrin ketone

R.T.: 7.700 min
Delta R.T.: 0.028 min
Response: 303148
Conc: 0.10 ng/ml

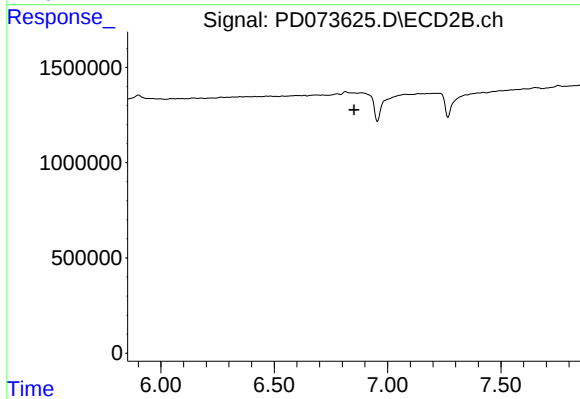

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

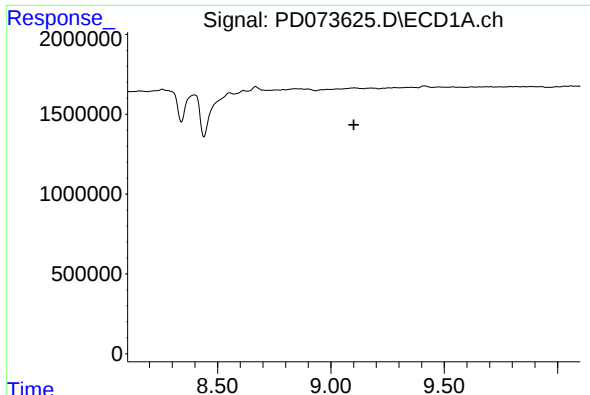

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

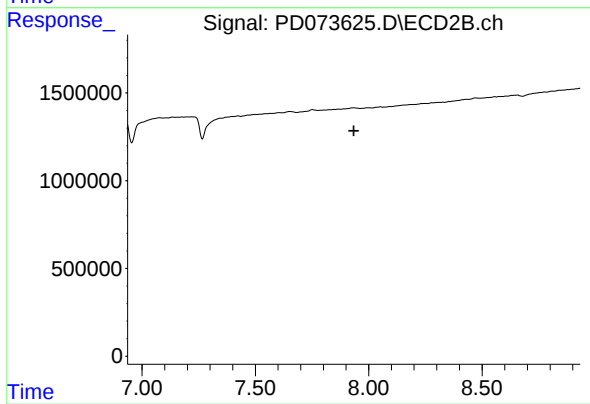

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.934 min
Response: 0
Conc: N.D.