

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
 Data File : PD073626.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 16:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 02:47:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.777	48703691	27754075	20.836	21.801
28)	SA Decachlor...	9.102	7.934	63314698	26157120	22.468	22.482
Target Compounds							
4)	MA Heptachlor	4.924	0.000	276555	0	0.074	N.D. #
5)	MB Aldrin	5.263f	0.000	144326	0	0.040	N.D. #
6)	B beta-BHC	4.563f	0.000	239052	0	0.154	N.D. #
7)	B delta-BHC	4.779	0.000	1857416	0	0.552	N.D. #
8)	B Heptachlo...	5.697	0.000	832362	0	0.261	N.D. #
9)	A Endosulfan I	6.095	0.000	696387	0	0.227	N.D. #
10)	B gamma-Chl...	5.931f	0.000	1479182	0	0.449	N.D. #
11)	B alpha-Chl...	6.058	0.000	582358	0	0.177	N.D. #
15)	B Endosulfa...	6.843f	0.000	724443	0	0.274	N.D. #
21)	B Endrin ke...	7.700f	0.000	542822	0	0.180	N.D. #
24)	Chlordane-2	5.263	0.000	144326	0	1.141	N.D. #
26)	Chlordane-4	6.058	0.000	582358	0	1.017	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
Data File : PD073626.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 16:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 02:47:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

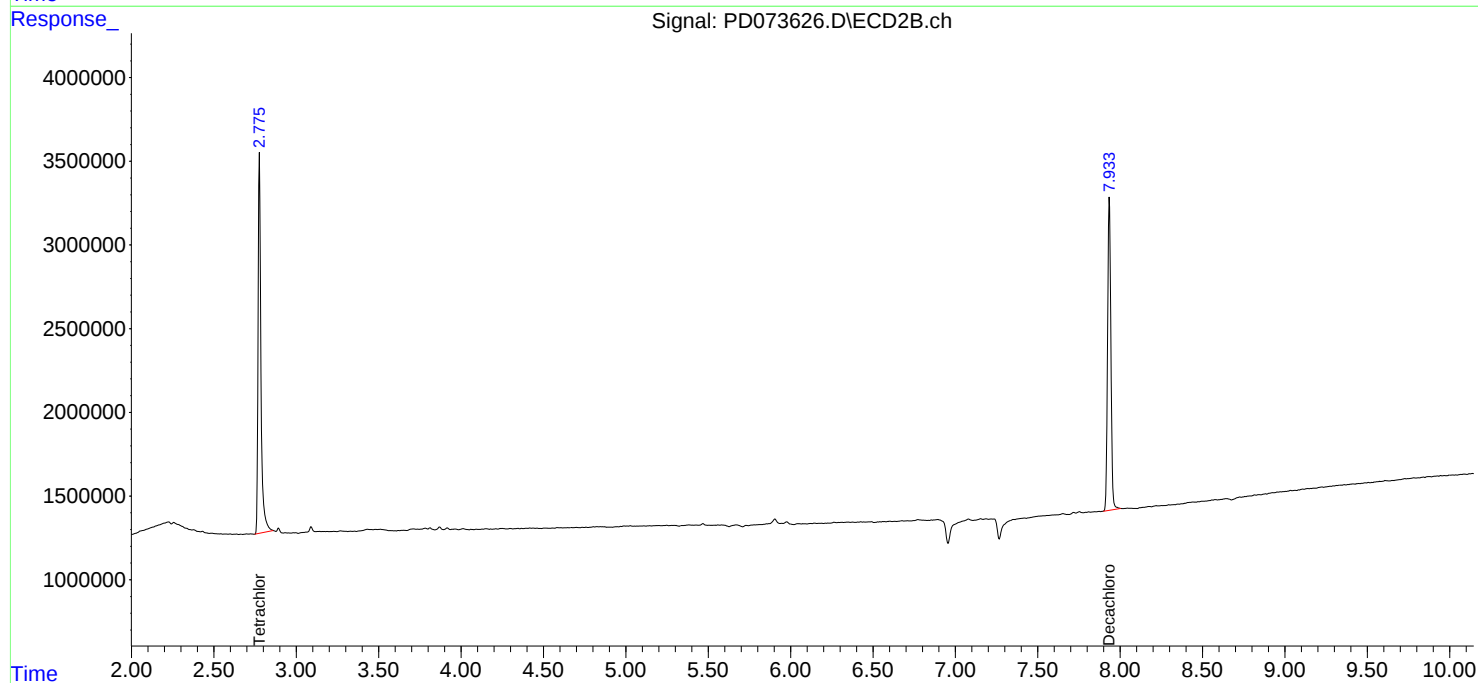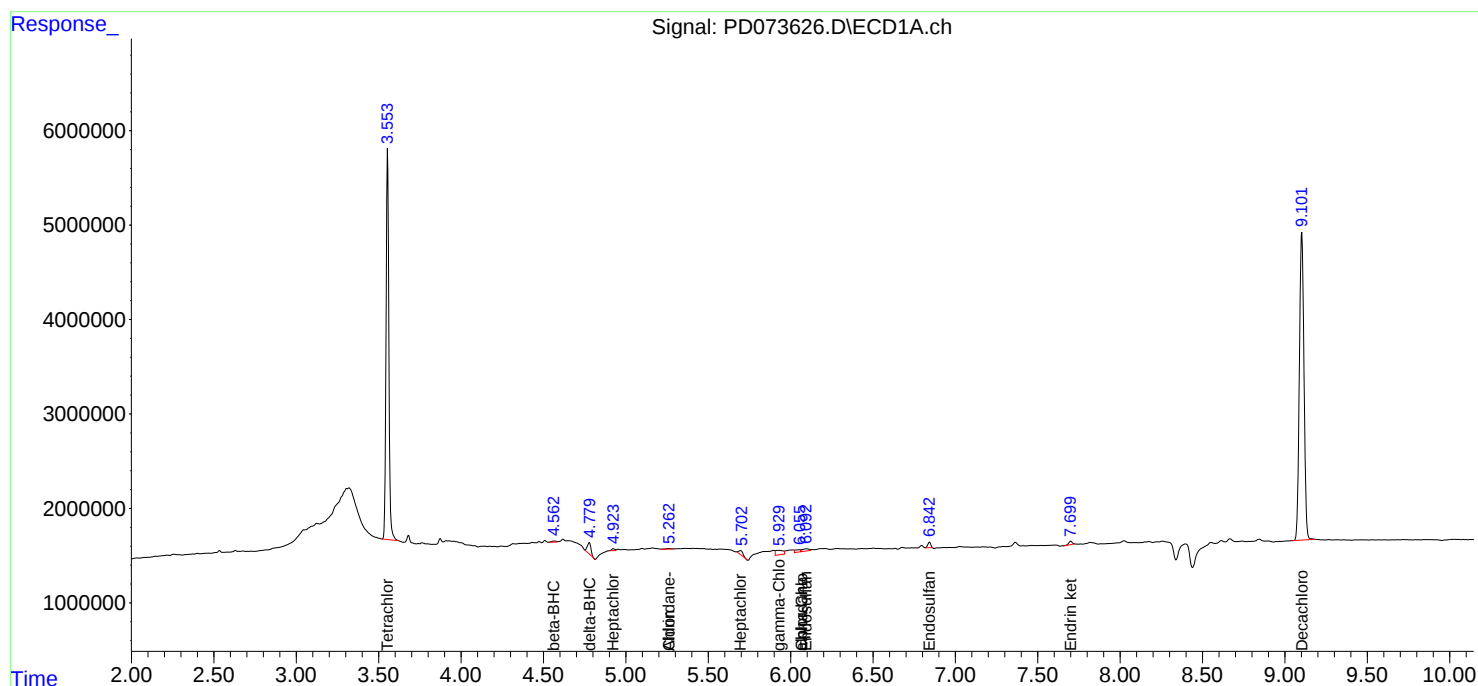


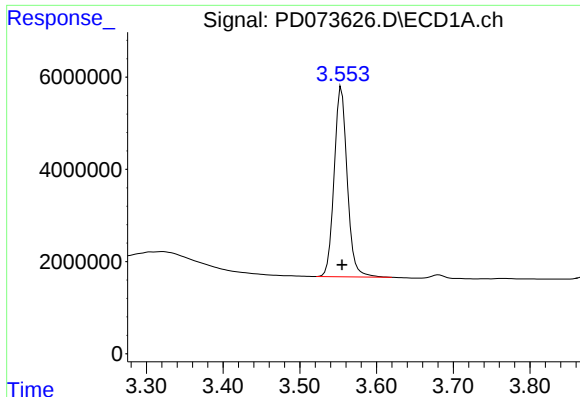

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 48703691
Conc: 20.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

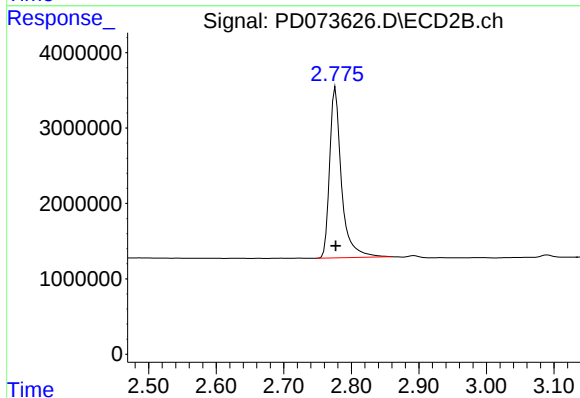


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 27754075
Conc: 21.80 ng/ml

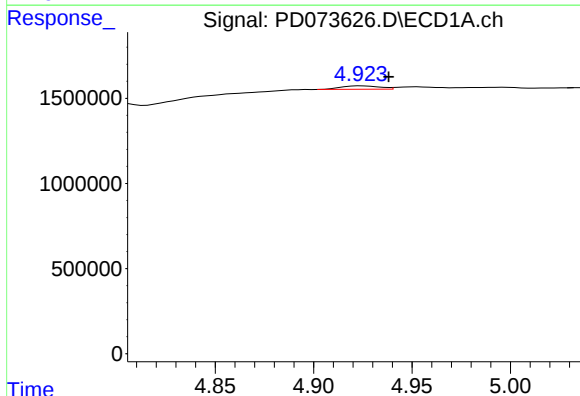


#4 Heptachlor

R.T.: 4.924 min
Delta R.T.: -0.014 min
Response: 276555
Conc: 0.07 ng/ml

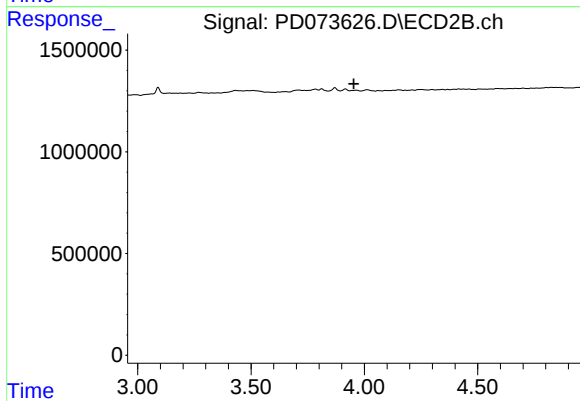

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.953 min
Response: 0
Conc: N.D.

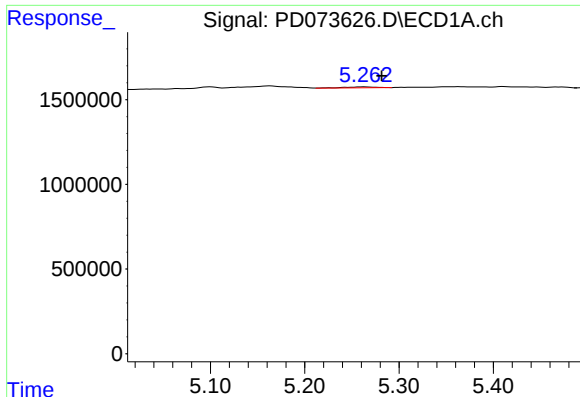

#5 Aldrin


R.T.: 5.263 min
Delta R.T.: -0.018 min
Response: 144326
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

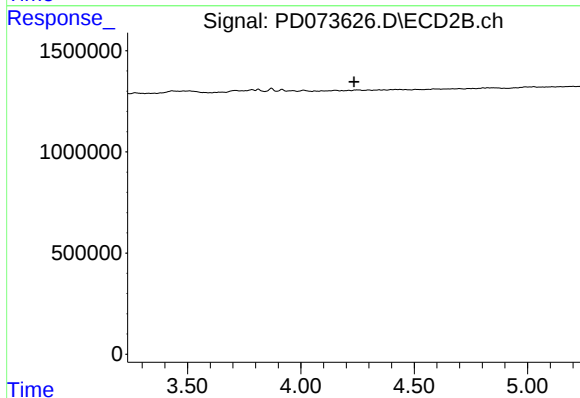


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.235 min
Response: 0
Conc: N.D.

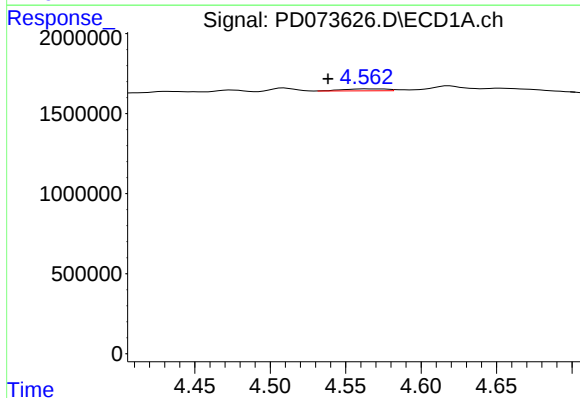


#6 beta-BHC

R.T.: 4.563 min
Delta R.T.: 0.025 min
Response: 239052
Conc: 0.15 ng/ml

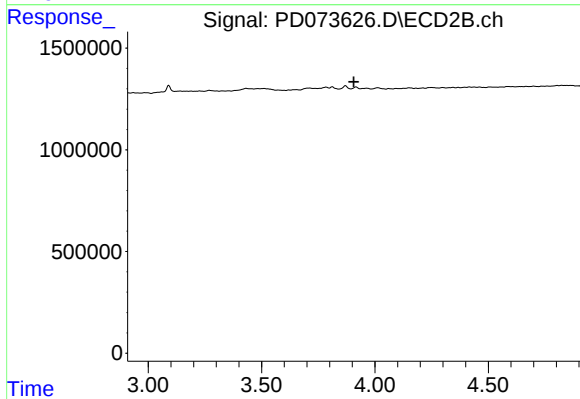

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.906 min
Response: 0
Conc: N.D.

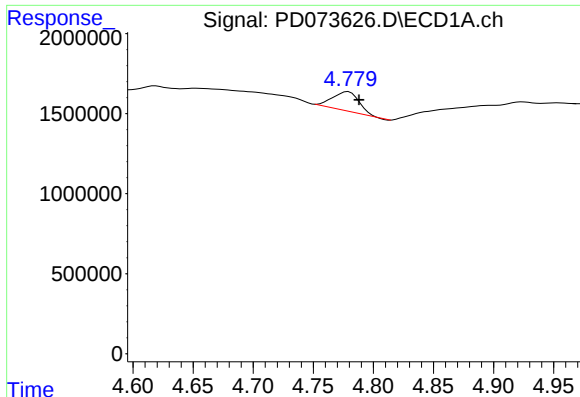

#7 delta-BHC


R.T.: 4.779 min
Delta R.T.: -0.009 min
Response: 1857416
Conc: 0.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

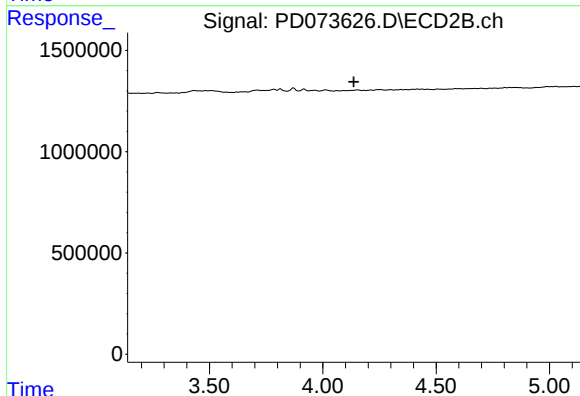


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

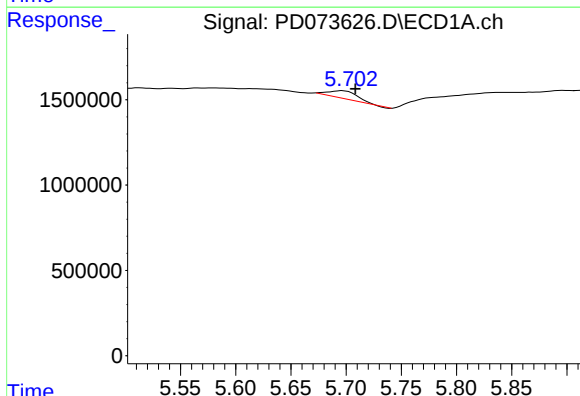


#8 Heptachlor epoxide

R.T.: 5.697 min
Delta R.T.: -0.012 min
Response: 832362
Conc: 0.26 ng/ml

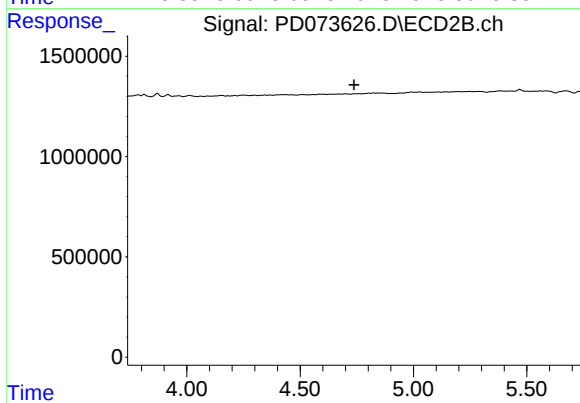

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

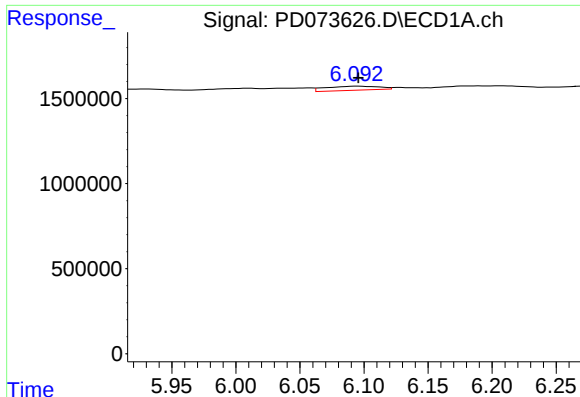

#9 Endosulfan I


R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 696387
Conc: 0.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

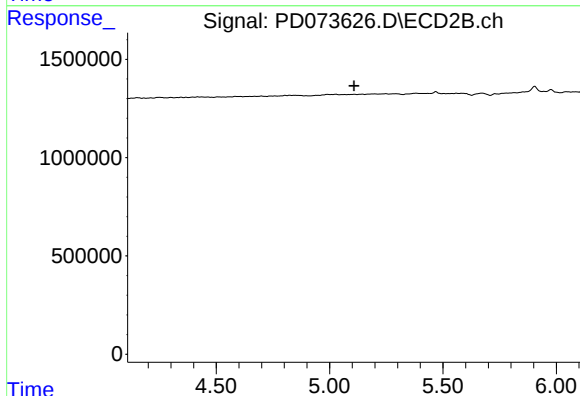


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

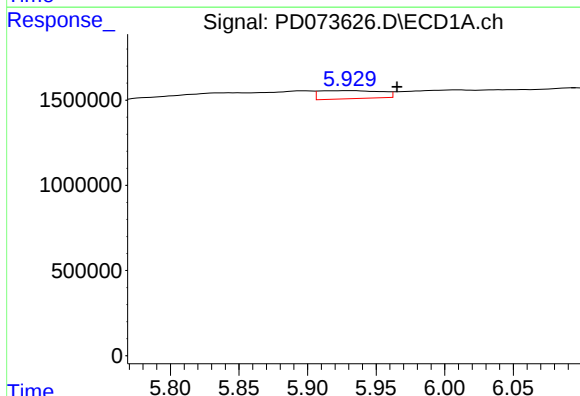


#10 gamma-Chlordane

R.T.: 5.931 min
Delta R.T.: -0.034 min
Response: 1479182
Conc: 0.45 ng/ml

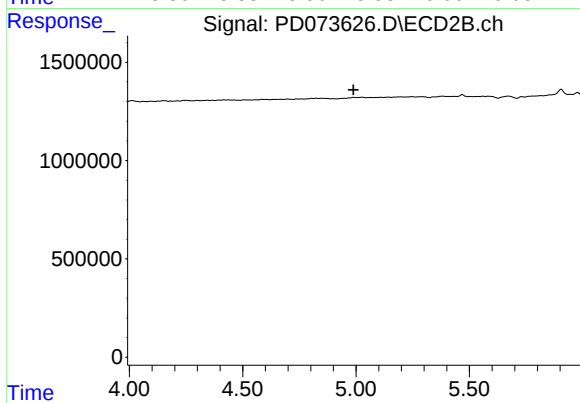

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

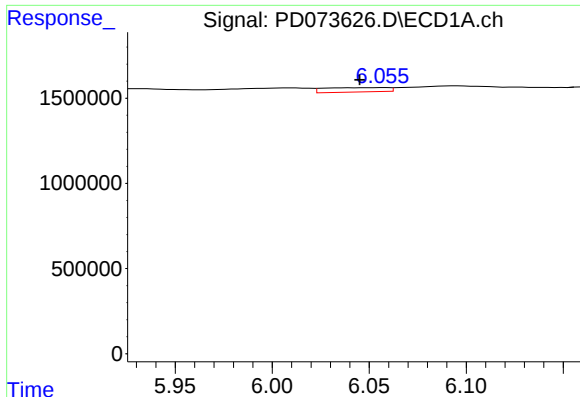

#11 alpha-Chlordane


R.T.: 6.058 min
Delta R.T.: 0.013 min
Response: 582358
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

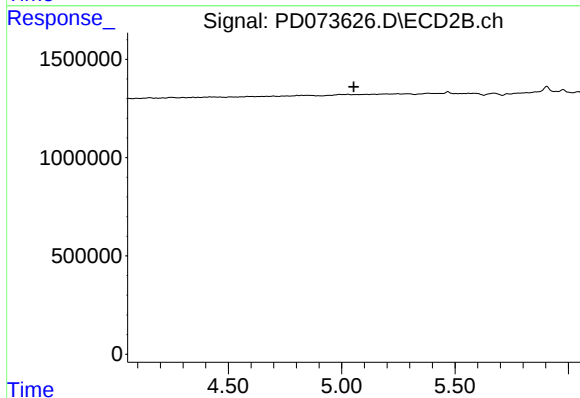


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

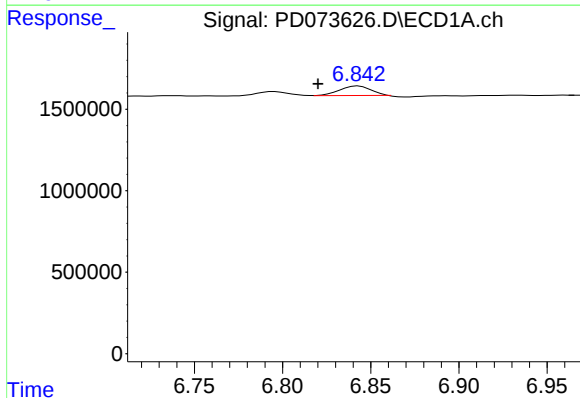


#15 Endosulfan II

R.T.: 6.843 min
Delta R.T.: 0.023 min
Response: 724443
Conc: 0.27 ng/ml

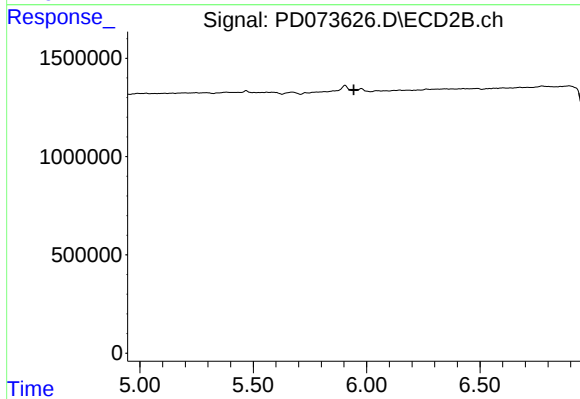

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

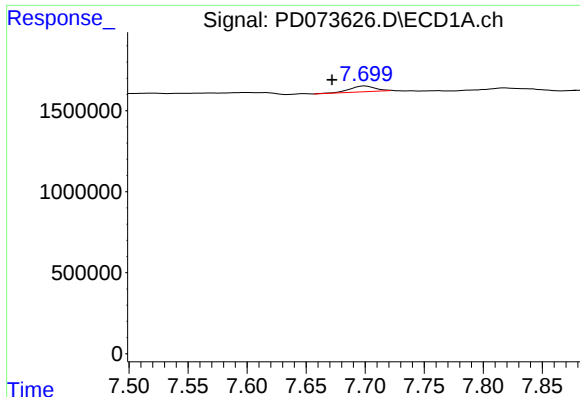

#21 Endrin ketone


R.T.: 7.700 min
Delta R.T.: 0.028 min
Response: 542822
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

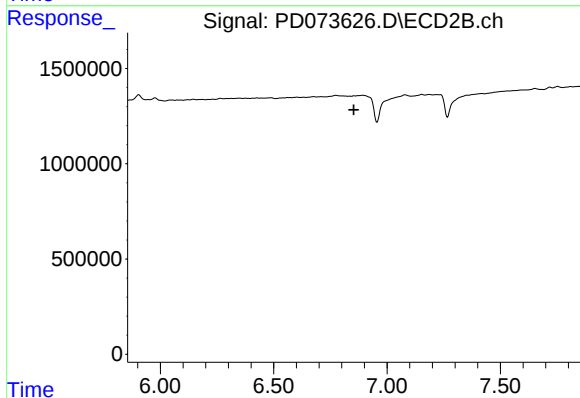


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

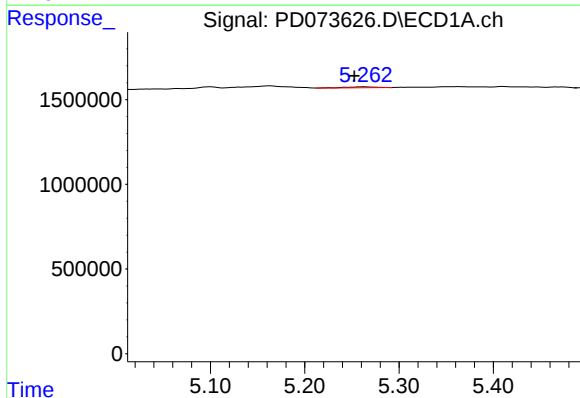


#24 Chlordane-2

R.T.: 5.263 min
Delta R.T.: 0.011 min
Response: 144326
Conc: 1.14 ng/ml

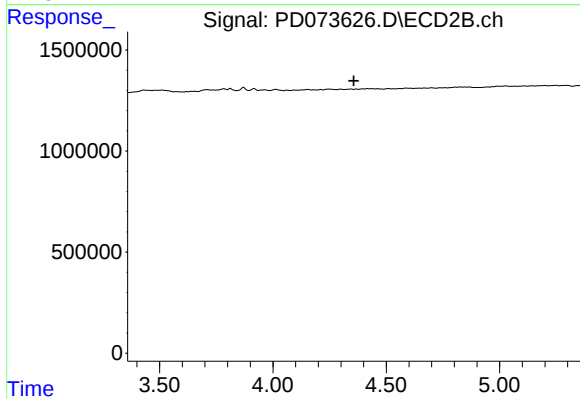

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

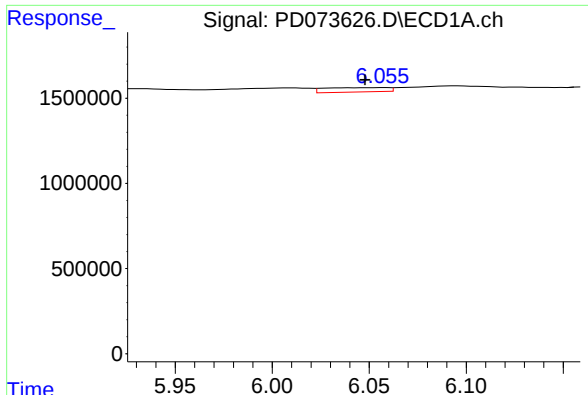

#26 Chlordane-4


R.T.: 6.058 min
Delta R.T.: 0.010 min
Response: 582358
Conc: 1.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

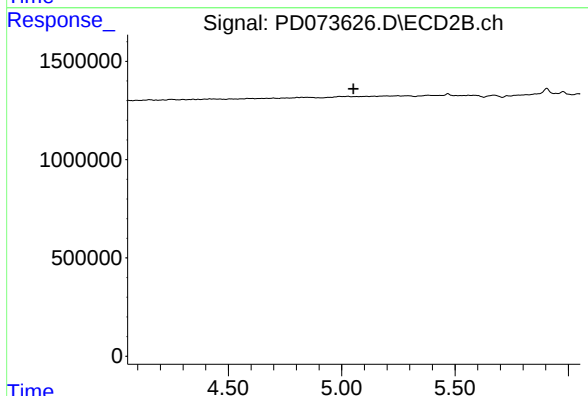


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.053 min
Response: 0
Conc: N.D.

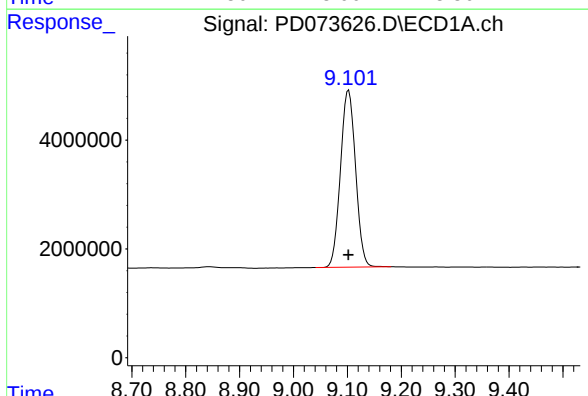

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 63314698
Conc: 22.47 ng/ml

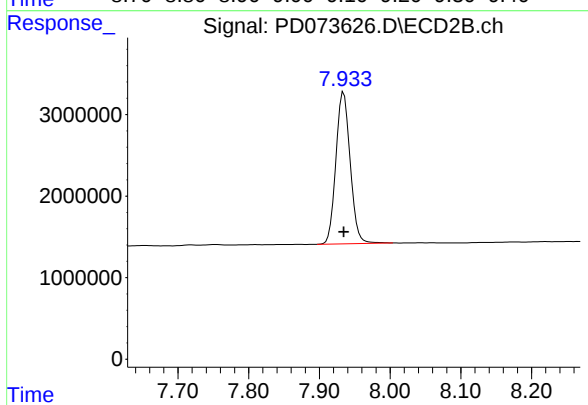

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 26157120
Conc: 22.48 ng/ml