

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
 Data File : PD073636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 18:43
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 00:35:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 00:27:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.776	118.6E6	73941166	50.000	50.000
28)	SA Decachlor...	9.102	7.934	138.3E6	59425539	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.722	3.779	57066401	22862063	500.000	500.000
24)	Chlordane-2	5.252	4.356	62000842	24954851	500.000	500.000
25)	Chlordane-3	5.964	4.988	240.3E6	73156629	500.000	500.000
26)	Chlordane-4	6.047	5.052	292.7E6	69358115	500.000	500.000
27)	Chlordane-5	6.899	5.949	51374028	25501781	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
Data File : PD073636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 18:43
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 00:35:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 00:27:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

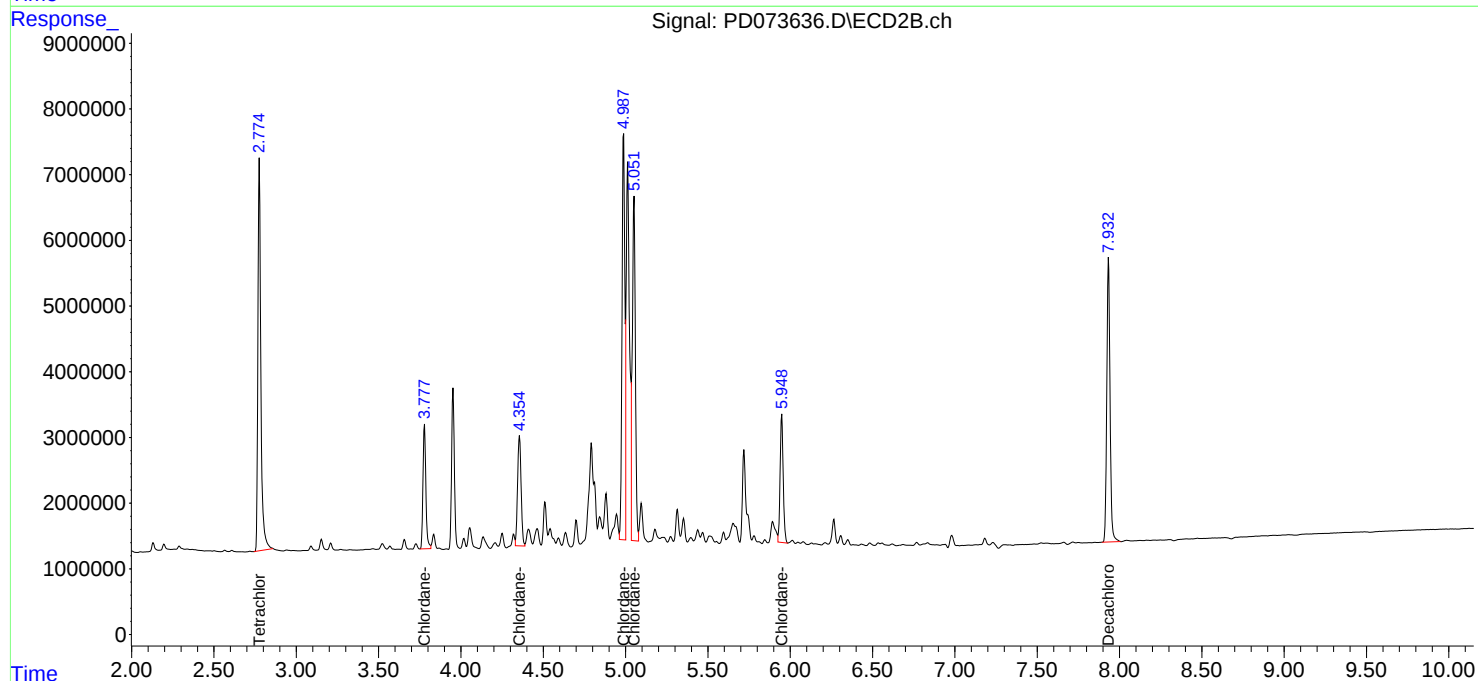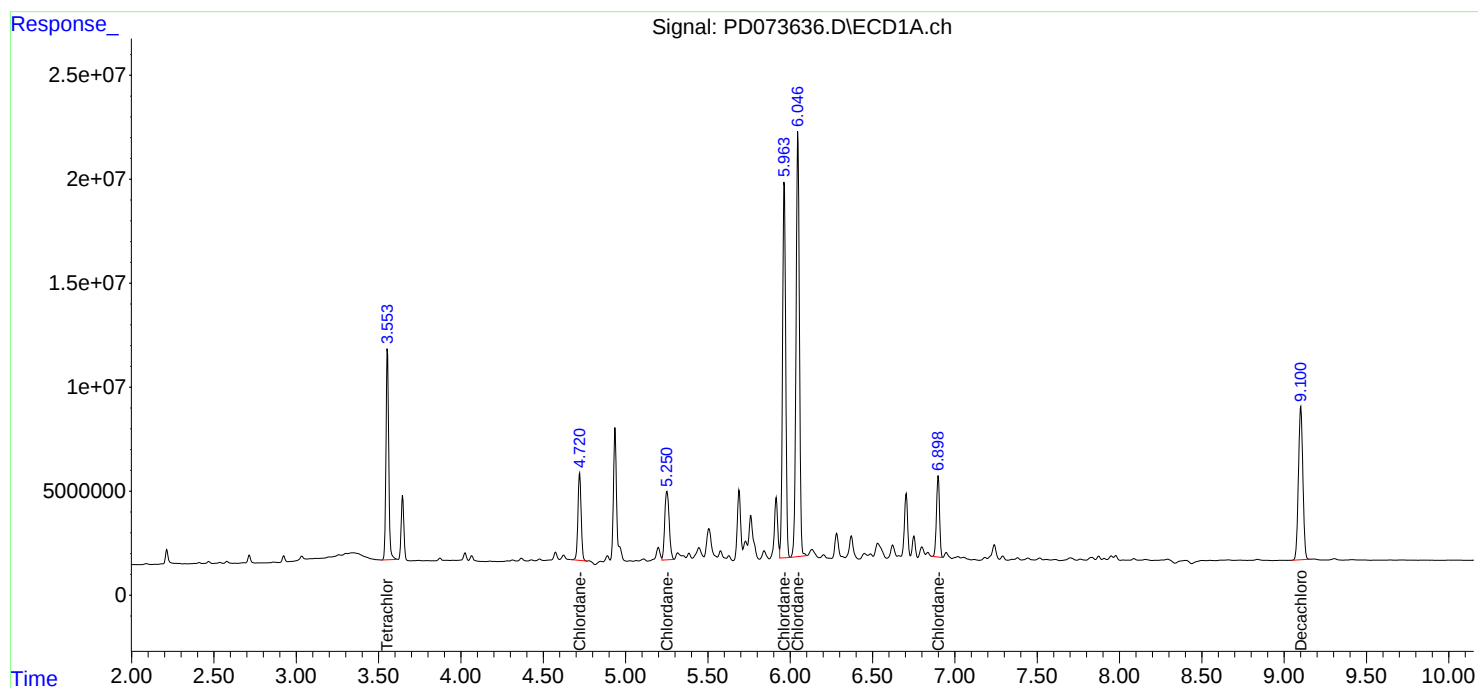


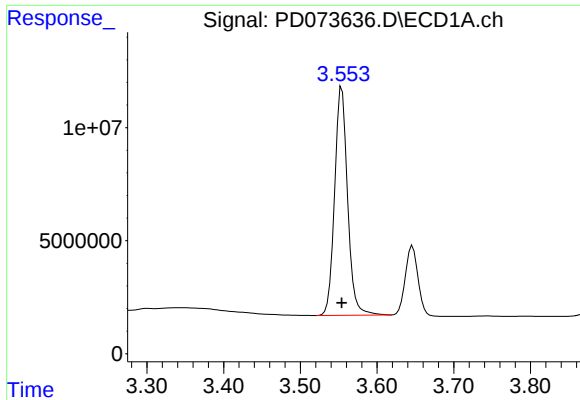

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 118592421
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

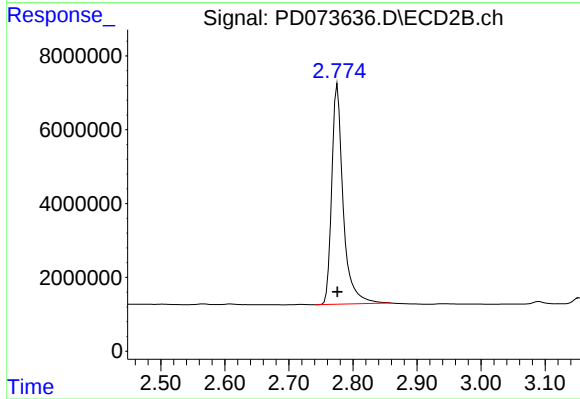


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 73941166
Conc: 50.00 ng/ml

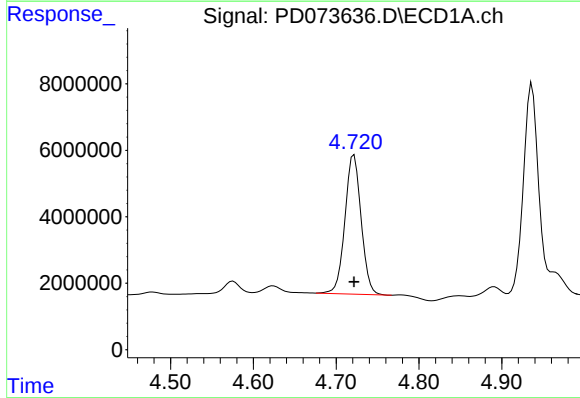


#23 Chlordane-1

R.T.: 4.722 min
Delta R.T.: 0.000 min
Response: 57066401
Conc: 500.00 ng/ml

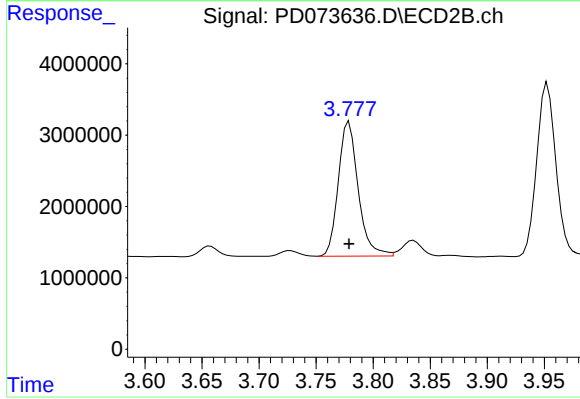

#23 Chlordane-1


R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 22862063
Conc: 500.00 ng/ml

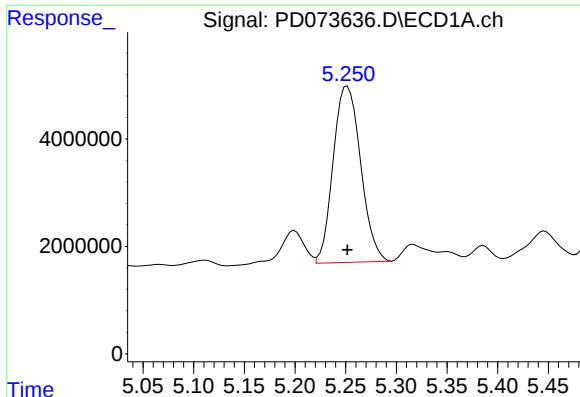

#24 Chlordane-2


R.T.: 5.252 min
Delta R.T.: 0.000 min
Response: 62000842
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

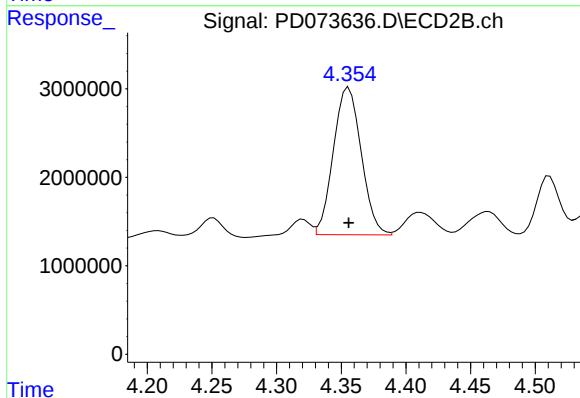


#24 Chlordane-2

R.T.: 4.356 min
Delta R.T.: 0.000 min
Response: 24954851
Conc: 500.00 ng/ml

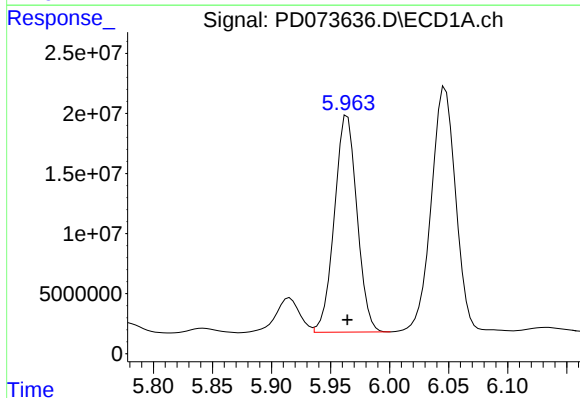


#25 Chlordane-3

R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 240302288
Conc: 500.00 ng/ml

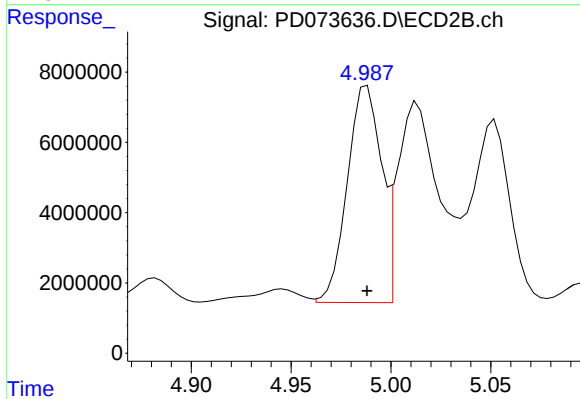

#25 Chlordane-3


R.T.: 4.988 min
Delta R.T.: 0.000 min
Response: 73156629
Conc: 500.00 ng/ml

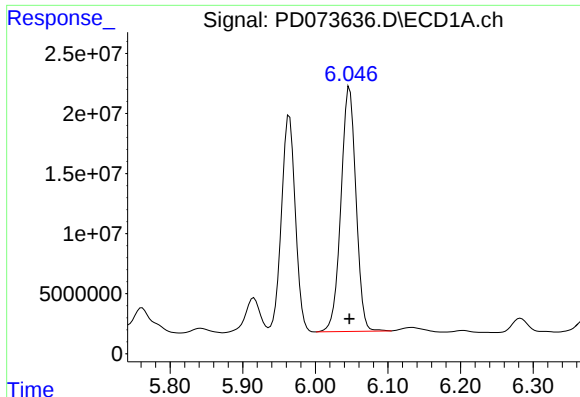

#26 Chlordane-4


R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 292677813
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

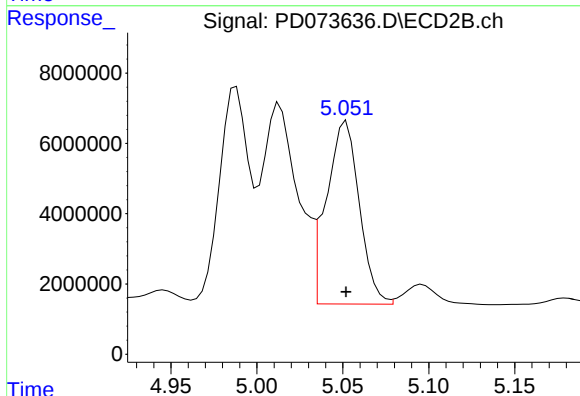


#26 Chlordane-4

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 69358115
Conc: 500.00 ng/ml

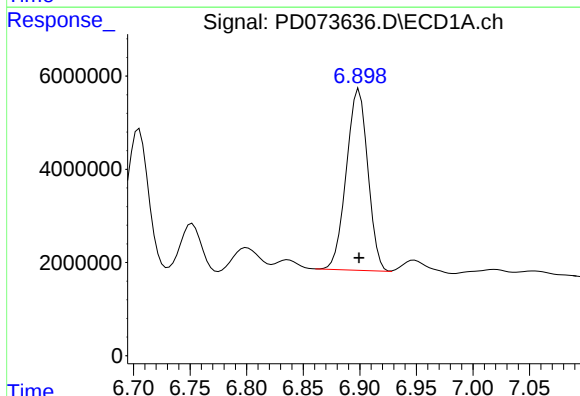


#27 Chlordane-5

R.T.: 6.899 min
Delta R.T.: 0.000 min
Response: 51374028
Conc: 500.00 ng/ml

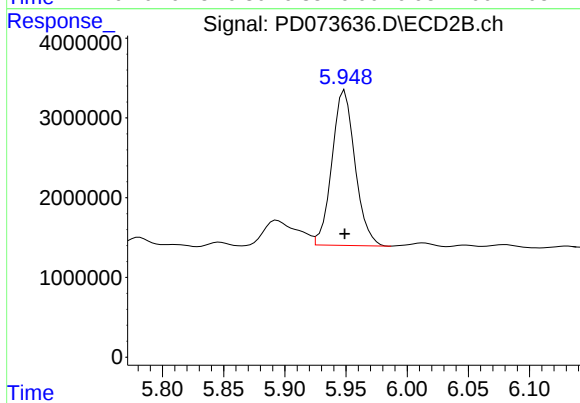

#27 Chlordane-5


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 25501781
Conc: 500.00 ng/ml

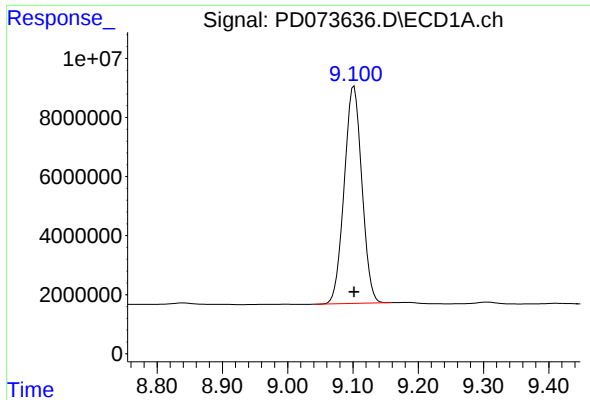

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 138325280
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

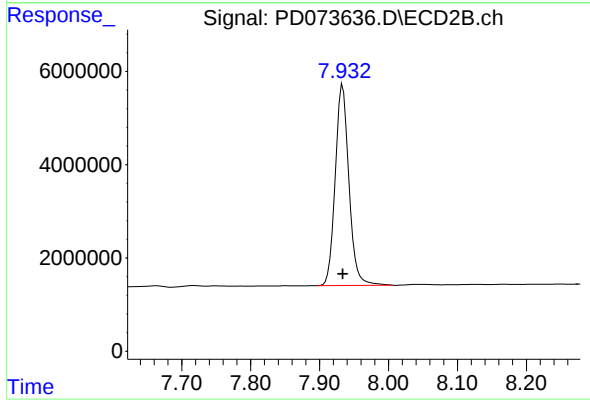

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 59425539
Conc: 50.00 ng/ml