

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
 Data File : PD073637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 18:56
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 00:35:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 00:27:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.776	57430901	36300223	24.214	24.547
28)	SA Decachlor...	9.101	7.934	72709370	30449027	26.282	25.619
Target Compounds							
23)	Chlordane-1	4.722	3.779	30118800	11418277	263.893	249.721
24)	Chlordane-2	5.252	4.356	31887726	13035271	257.156	261.177
25)	Chlordane-3	5.964	4.989	112.7E6	35462812	234.548	242.376
26)	Chlordane-4	6.047	5.052	139.4E6	34615249	238.169	249.540
27)	Chlordane-5	6.899	5.949	25378999	12869535	247.002	252.326



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
Data File : PD073637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 18:56
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 00:35:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 00:27:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

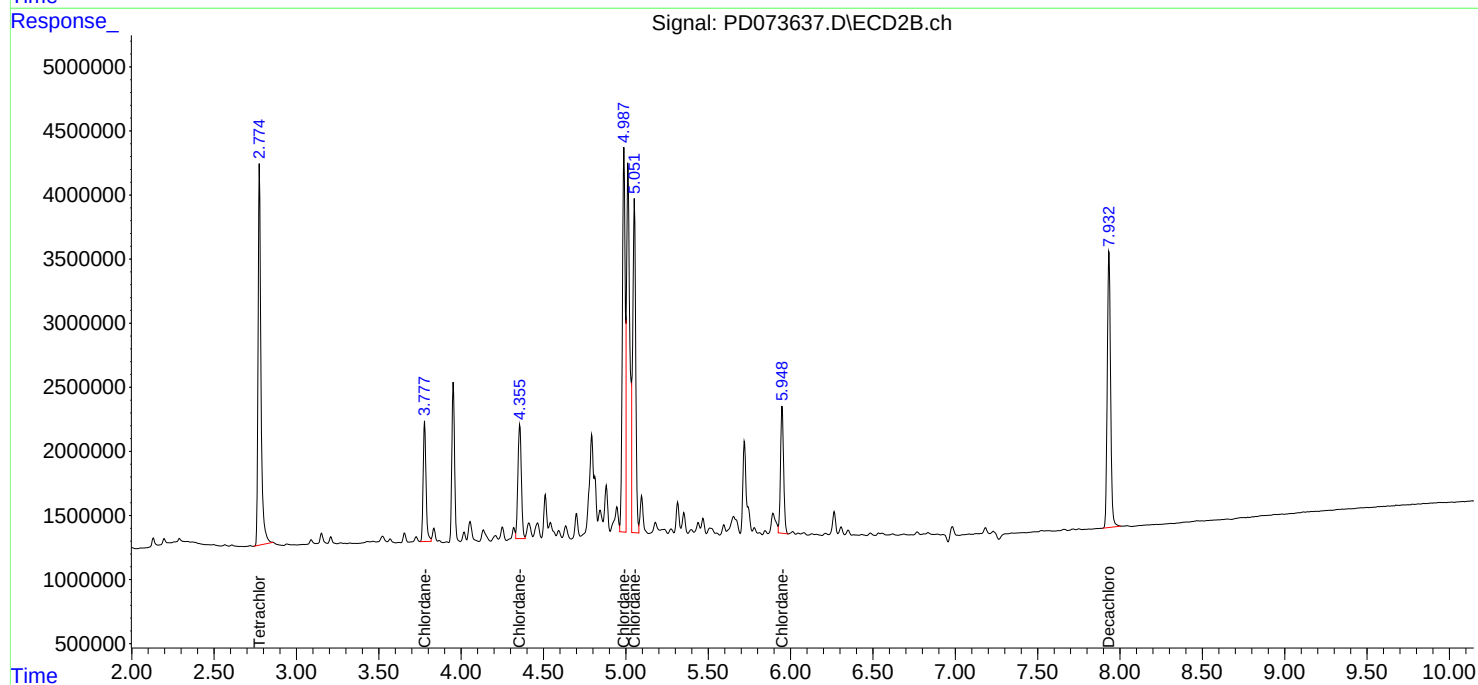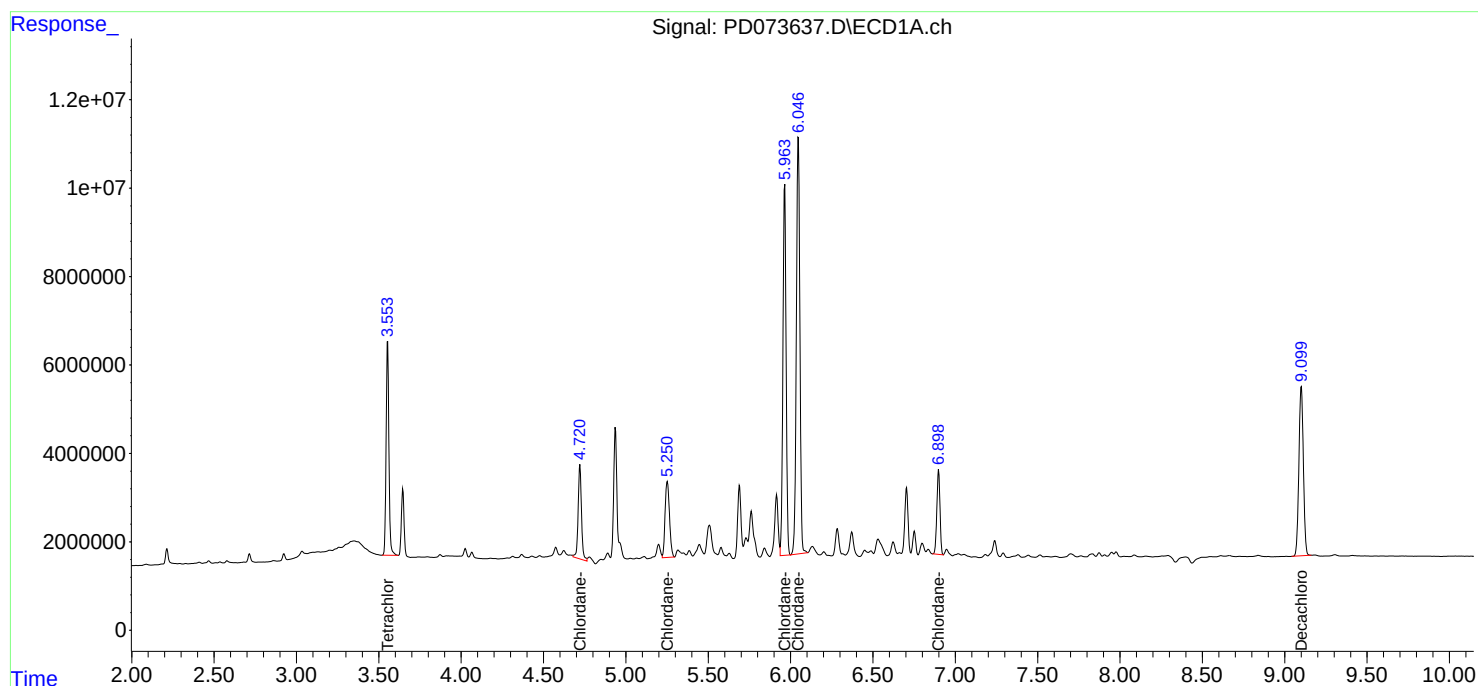


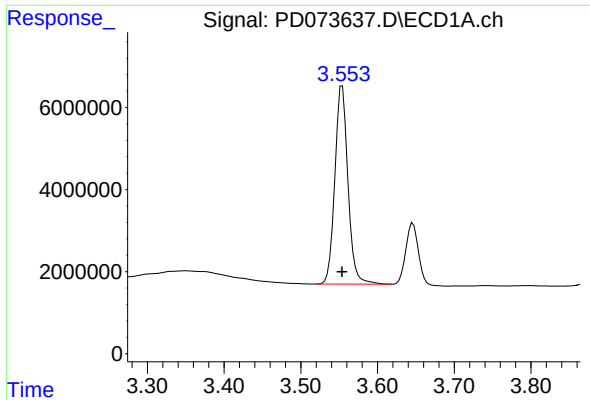

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 57430901
Conc: 24.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

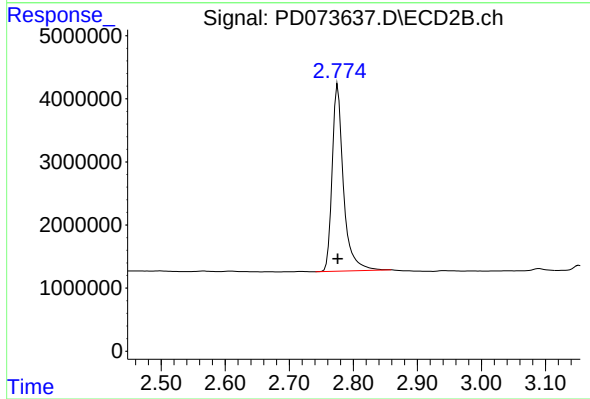


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 36300223
Conc: 24.55 ng/ml

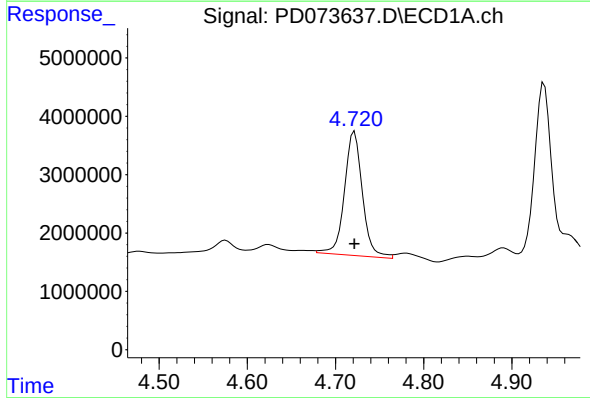


#23 Chlordane-1

R.T.: 4.722 min
Delta R.T.: 0.000 min
Response: 30118800
Conc: 263.89 ng/ml

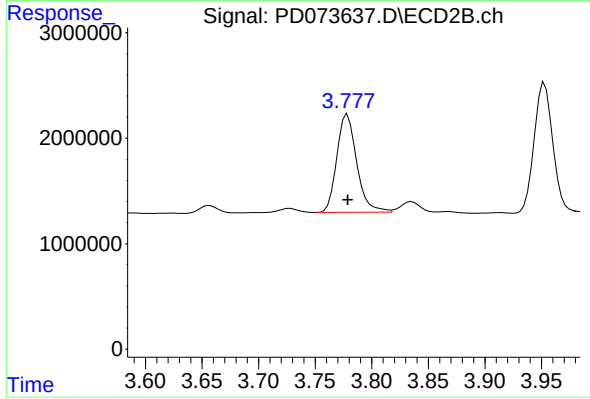

#23 Chlordane-1


R.T.: 3.779 min
Delta R.T.: 0.000 min
Response: 11418277
Conc: 249.72 ng/ml

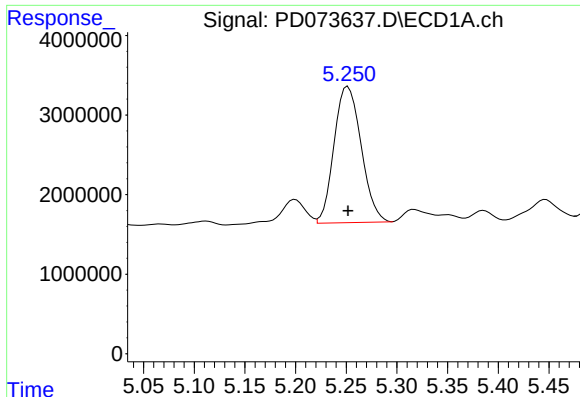

#24 Chlordane-2


R.T.: 5.252 min
Delta R.T.: 0.000 min
Response: 31887726
Conc: 257.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

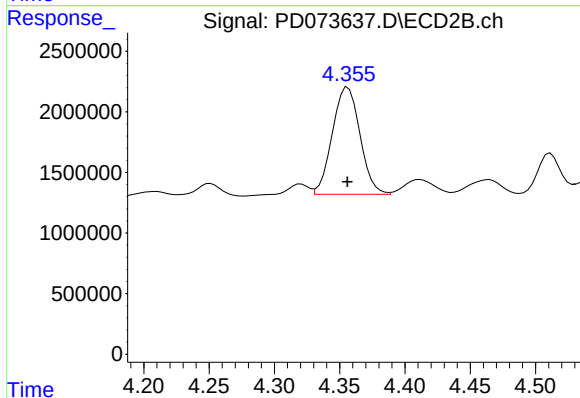


#24 Chlordane-2

R.T.: 4.356 min
Delta R.T.: 0.000 min
Response: 13035271
Conc: 261.18 ng/ml

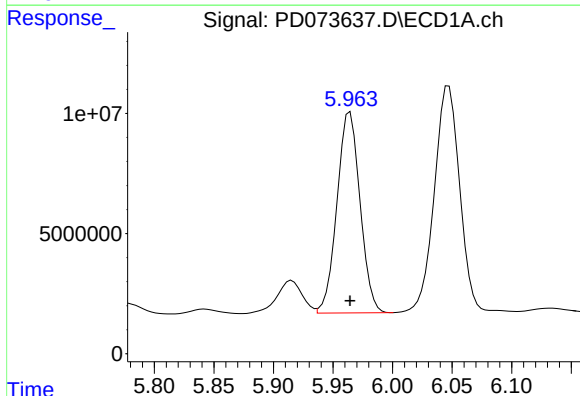


#25 Chlordane-3

R.T.: 5.964 min
Delta R.T.: 0.000 min
Response: 112724647
Conc: 234.55 ng/ml

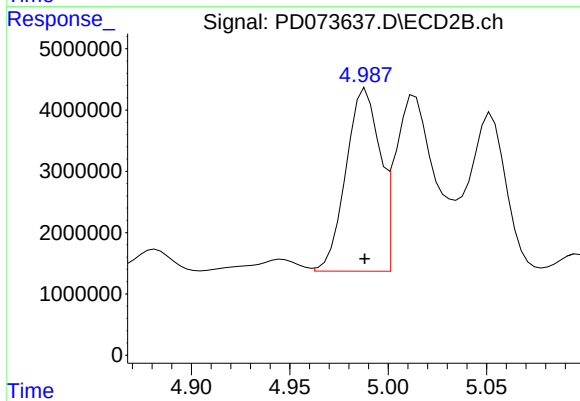

#25 Chlordane-3


R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 35462812
Conc: 242.38 ng/ml

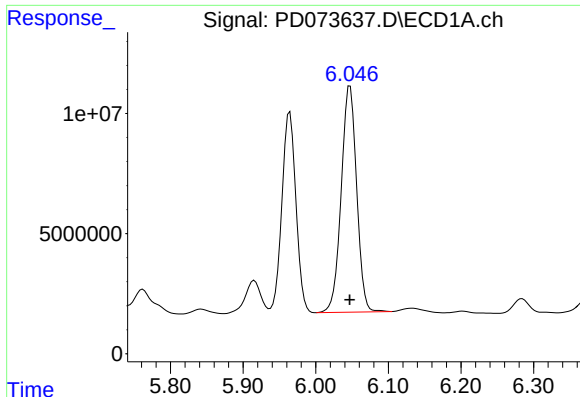

#26 Chlordane-4


R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 139413581
Conc: 238.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

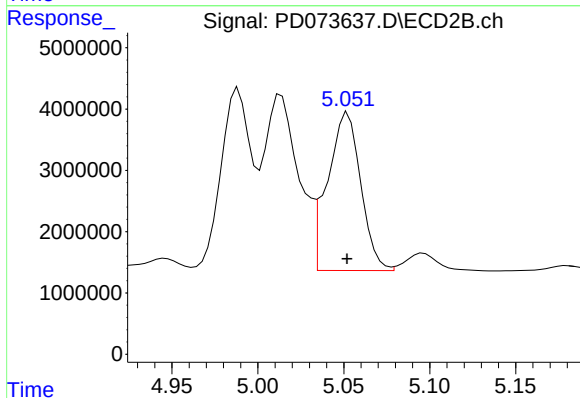


#26 Chlordane-4

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 34615249
Conc: 249.54 ng/ml

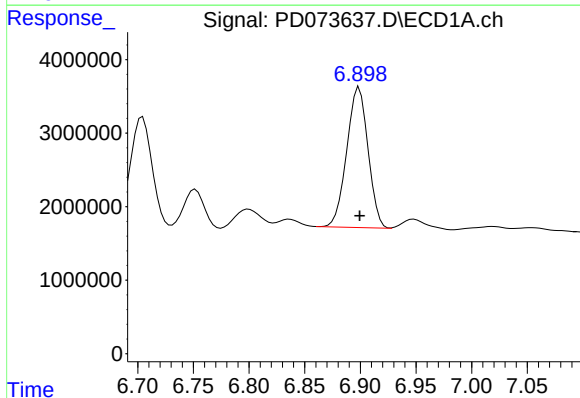


#27 Chlordane-5

R.T.: 6.899 min
Delta R.T.: 0.000 min
Response: 25378999
Conc: 247.00 ng/ml

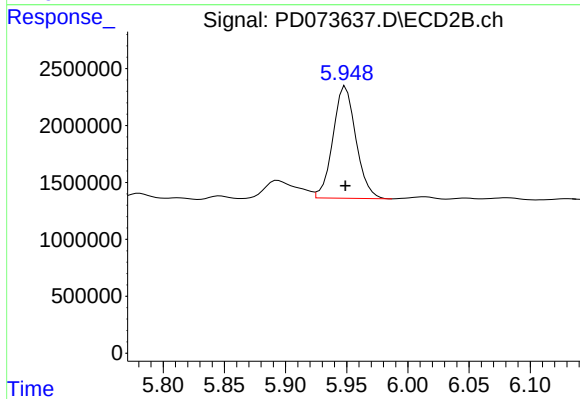

#27 Chlordane-5


R.T.: 5.949 min
Delta R.T.: 0.000 min
Response: 12869535
Conc: 252.33 ng/ml

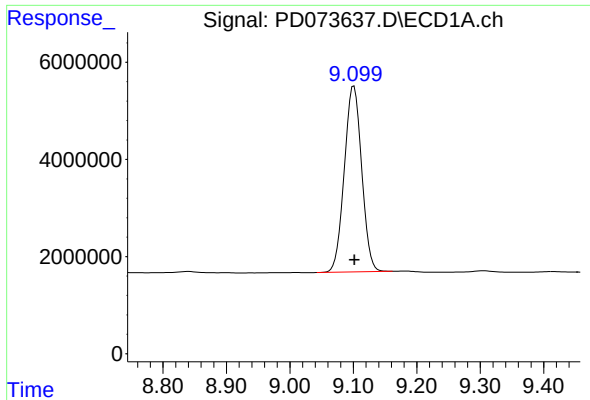

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.000 min
Response: 72709370
Conc: 26.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

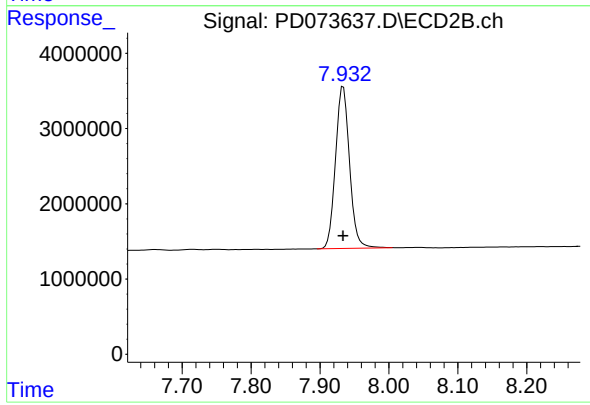

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 30449027
Conc: 25.62 ng/ml