

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
 Data File : PD073628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2023 16:55
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 02:48:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.777	52425125	28862040	22.428	22.671
28)	SA Decachlor...	9.102	7.934	61712485	25488863	21.899	21.908
Target Compounds							
9)	A Endosulfan I	6.095	5.109	33134401	14843859	10.791	11.040
10)	B gamma-Chl...	5.964	4.989	36274909	16639921	11.018	11.243
12)	B 4,4'-DDE	6.216	5.243	62281024	28397898	20.621	21.282
13)	MA Dieldrin	6.371	5.374	68236971	28683987	21.401	21.883
19)	B Endosulfa...	7.185	6.346	52300883	21976859	19.533	19.524
20)	A Methoxychlor	7.524	6.627	147.3E6	48071247	95.061	91.844
21)	B Endrin ke...	7.671	6.853	64430290	27415721	21.307	21.397



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011823\
Data File : PD073628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2023 16:55
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 02:48:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

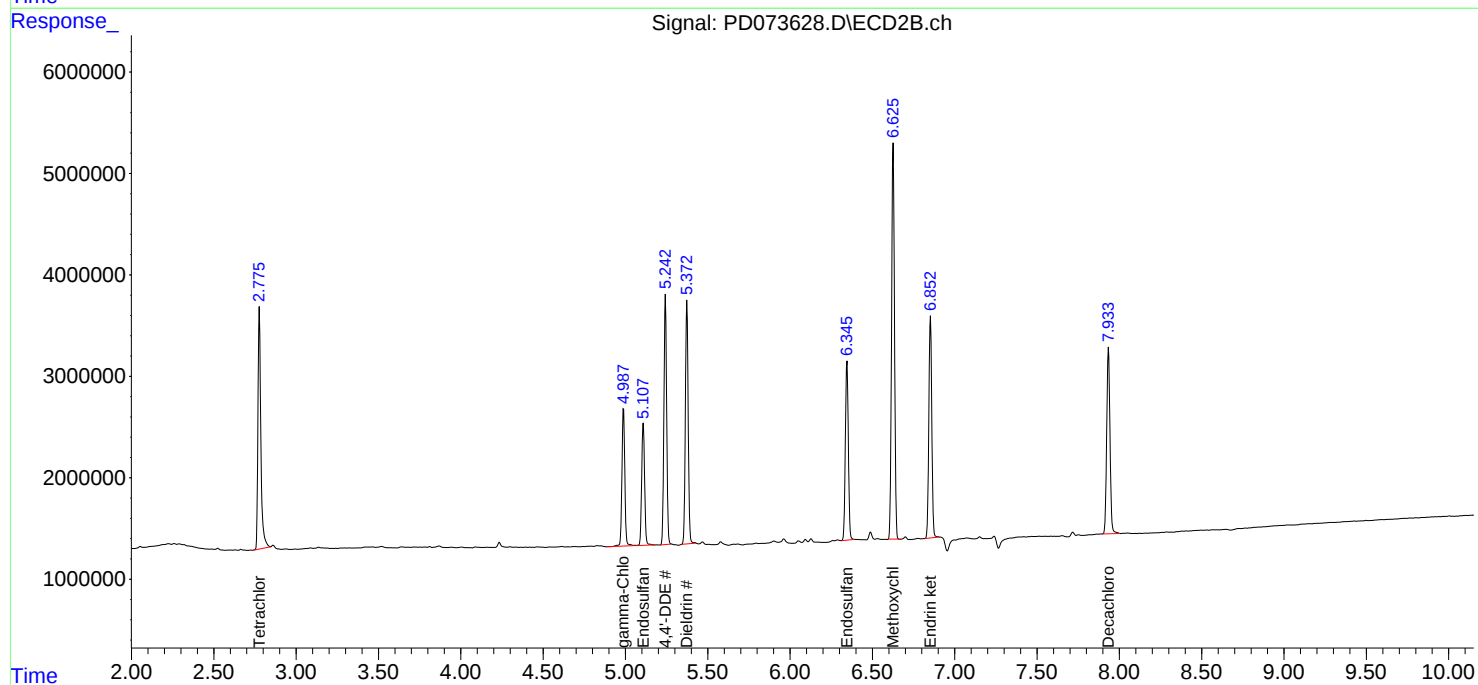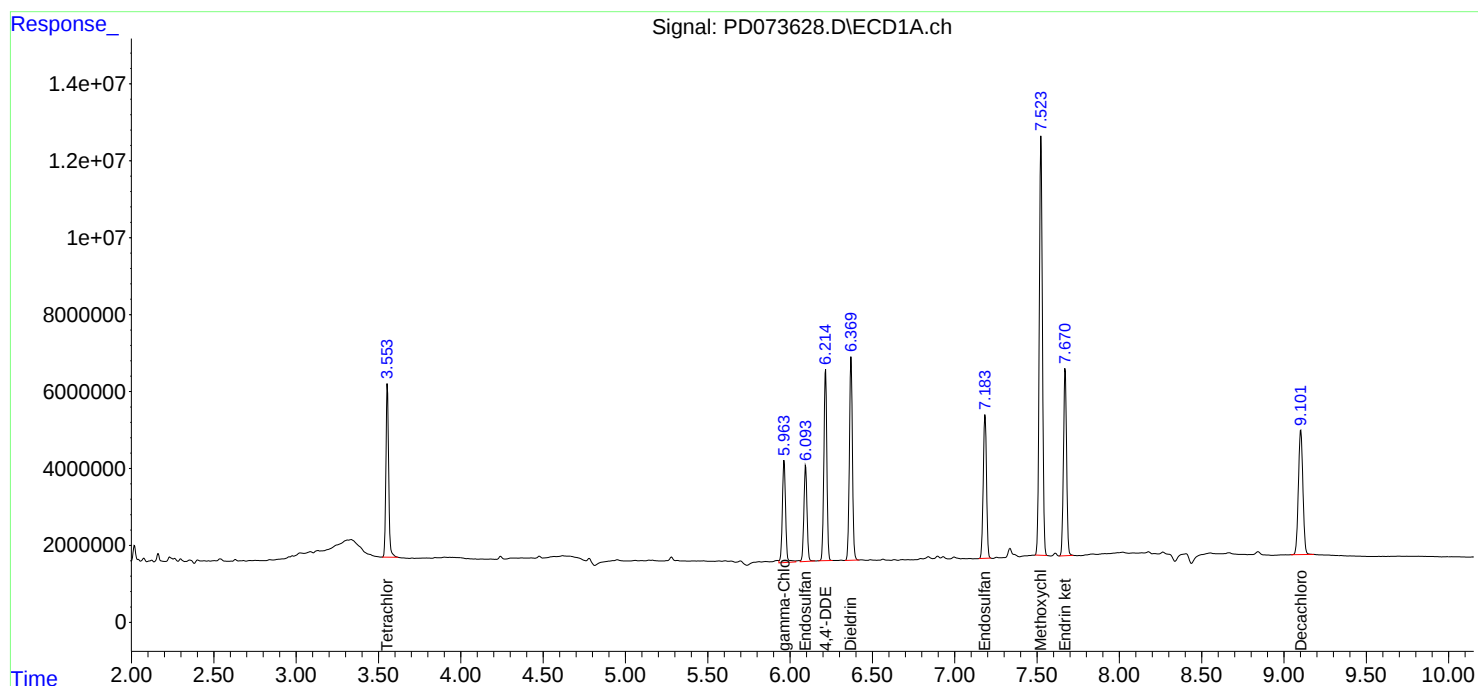


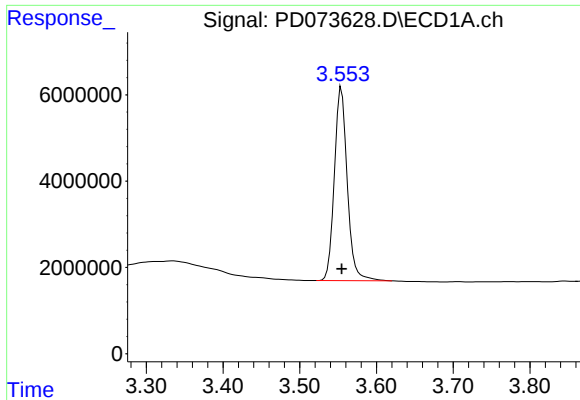

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 52425125
Conc: 22.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

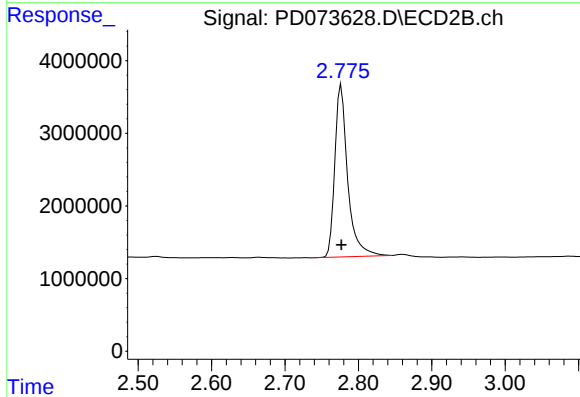


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 28862040
Conc: 22.67 ng/ml

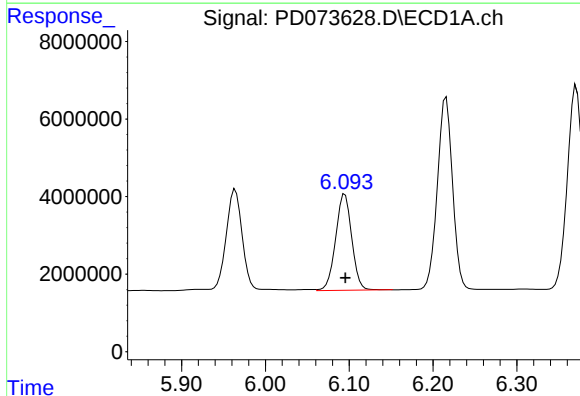


#9 Endosulfan I

R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 33134401
Conc: 10.79 ng/ml

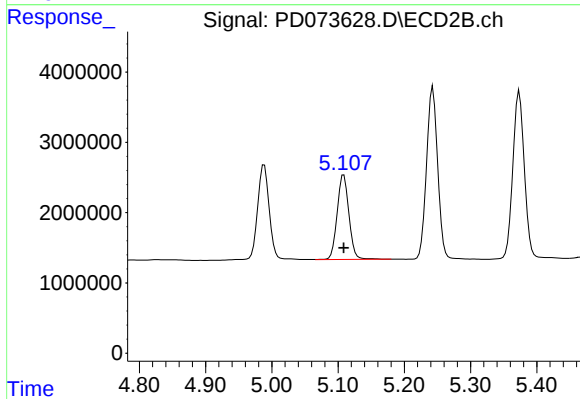

#9 Endosulfan I


R.T.: 5.109 min
Delta R.T.: 0.000 min
Response: 14843859
Conc: 11.04 ng/ml

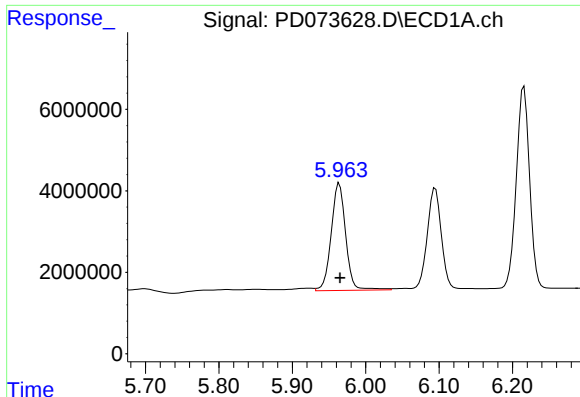

#10 gamma-Chlordane


R.T.: 5.964 min
Delta R.T.: -0.001 min
Response: 36274909
Conc: 11.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

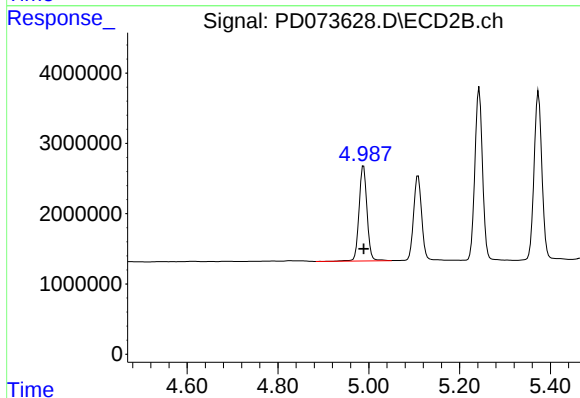


#10 gamma-Chlordane

R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 16639921
Conc: 11.24 ng/ml

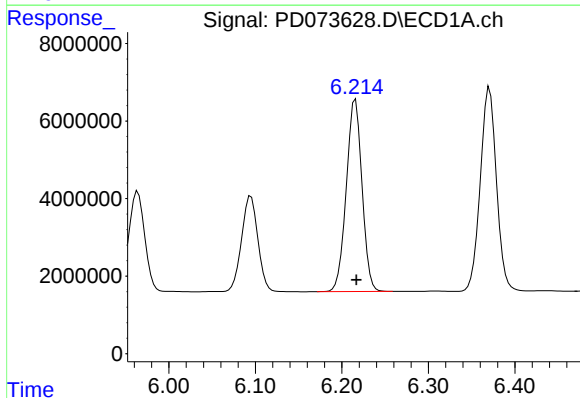


#12 4,4'-DDE

R.T.: 6.216 min
Delta R.T.: -0.001 min
Response: 62281024
Conc: 20.62 ng/ml

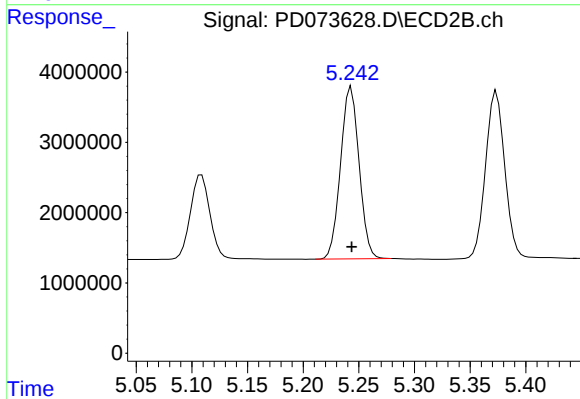

#12 4,4'-DDE


R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 28397898
Conc: 21.28 ng/ml

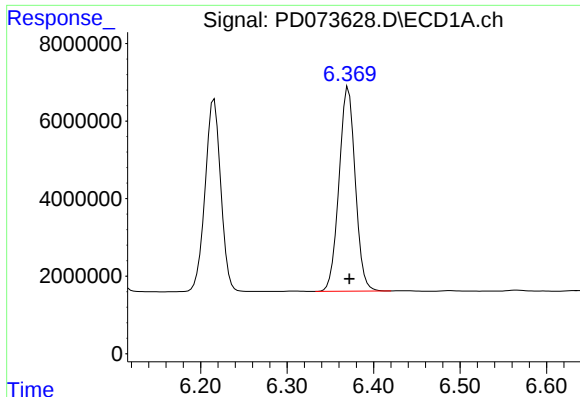

#13 Dieldrin


R.T.: 6.371 min
Delta R.T.: -0.001 min
Response: 68236971
Conc: 21.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

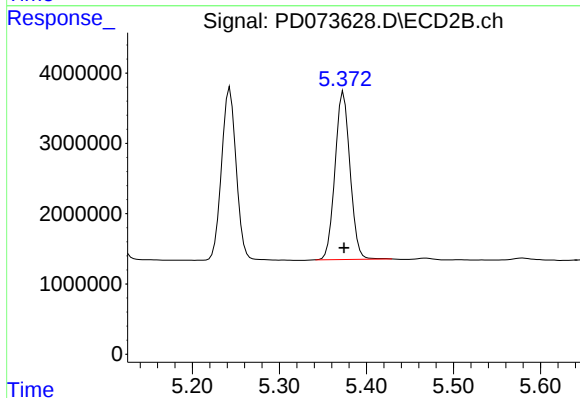


#13 Dieldrin

R.T.: 5.374 min
Delta R.T.: 0.000 min
Response: 28683987
Conc: 21.88 ng/ml

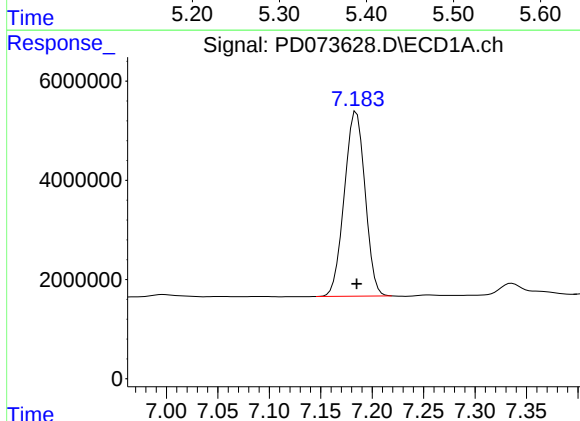


#19 Endosulfan Sulfate

R.T.: 7.185 min
Delta R.T.: 0.000 min
Response: 52300883
Conc: 19.53 ng/ml

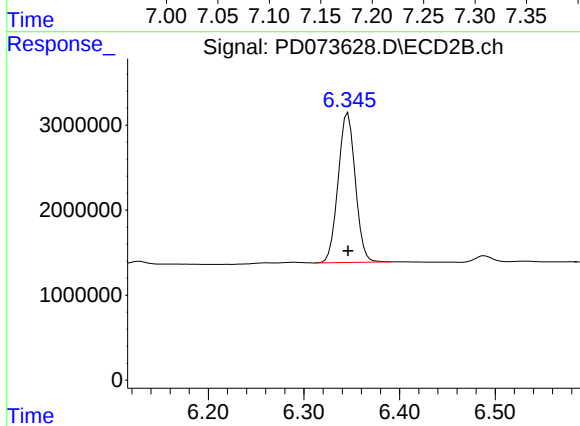

#19 Endosulfan Sulfate


R.T.: 6.346 min
Delta R.T.: 0.000 min
Response: 21976859
Conc: 19.52 ng/ml

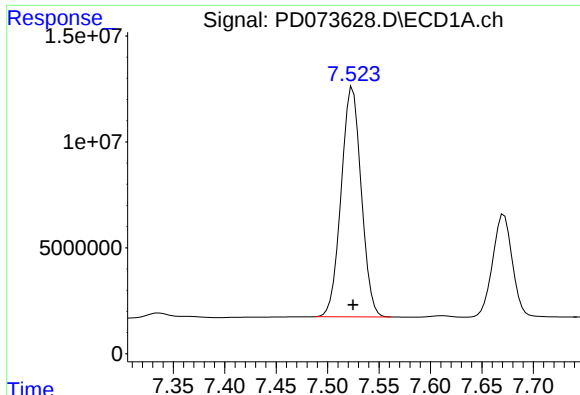

#20 Methoxychlor


R.T.: 7.524 min
Delta R.T.: 0.000 min
Response: 147260499
Conc: 95.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

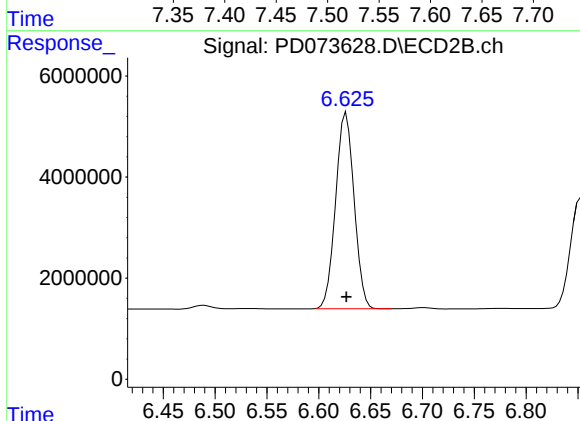


#20 Methoxychlor

R.T.: 6.627 min
Delta R.T.: 0.000 min
Response: 48071247
Conc: 91.84 ng/ml

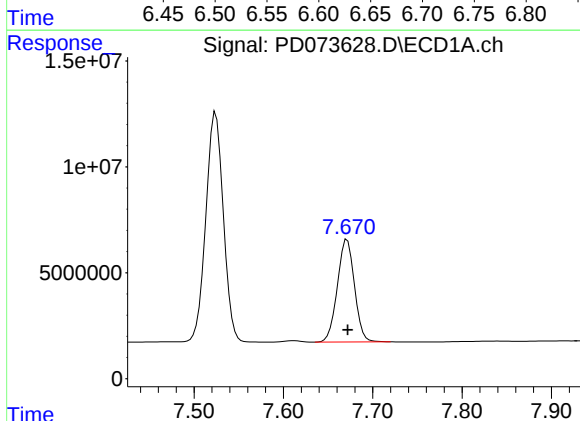


#21 Endrin ketone

R.T.: 7.671 min
Delta R.T.: 0.000 min
Response: 64430290
Conc: 21.31 ng/ml

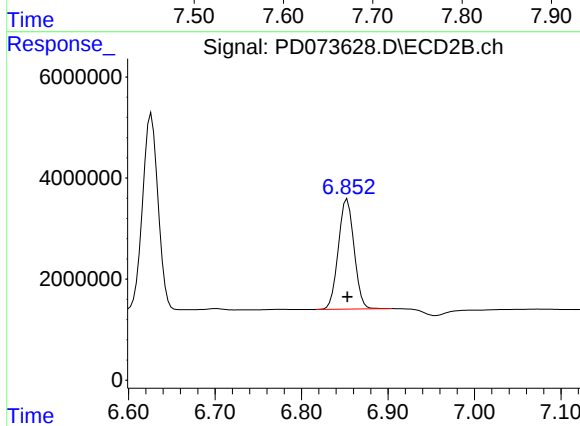

#21 Endrin ketone


R.T.: 6.853 min
Delta R.T.: 0.000 min
Response: 27415721
Conc: 21.40 ng/ml

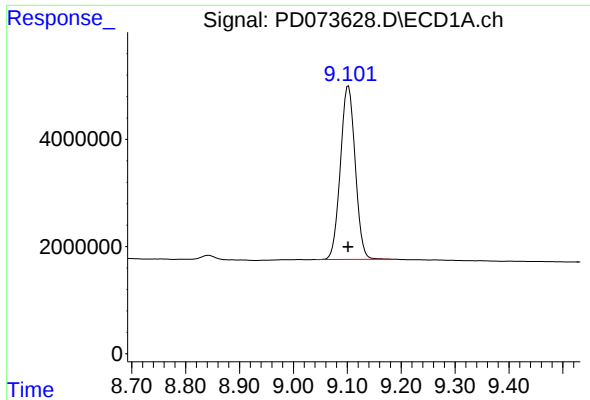

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 61712485
Conc: 21.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

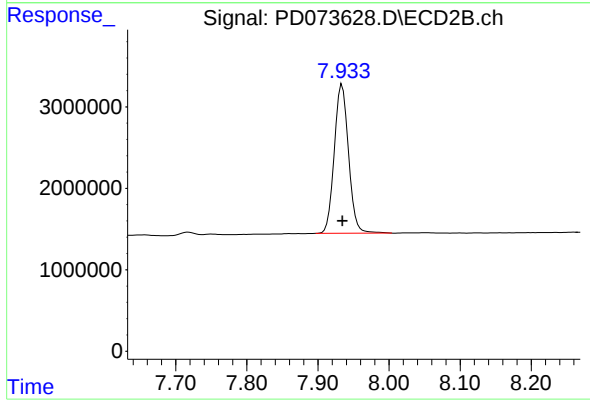

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 25488863
Conc: 21.91 ng/ml