

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011824\
 Data File : PD080813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jan 2024 16:47
 Operator : AR\AJ
 Sample : P1160-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 XA316

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/19/2024
 Supervised By :Ankita Jodhani 01/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 21:57:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 10 14:12:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	29825422	53099616	20.959	20.795
27)	SA Decachlor...	9.112	7.935	43711199	61347356	22.255	22.943
Target Compounds							
2)	A alpha-BHC	4.023	3.298	2138.7E6	2968.5E6	908.142	725.611
3)	MA gamma-BHC...	4.357	3.628	951.4E6	1442.9E6	415.539	378.099
4)	MA Heptachlor	4.949	3.969	1045.3E6	1567.1E6	432.322	424.287
5)	MB Aldrin	5.293	4.249	1137.9E6	1576.0E6	502.685	430.817
6)	B beta-BHC	4.551	3.923	323.7E6	540.7E6	313.915	306.466
7)	B delta-BHC	4.800	4.154	1253.5E6	1910.4E6	525.503	485.435
8)	B Heptachlo...	5.719	4.751	845.1E6	1318.1E6	387.999	383.846
9)	A Endosulfan I	6.105	5.121	1337.2E6	1925.5E6	630.018m	598.600
10)	B trans-Chl...	5.976	5.001	495.5E6	793.3E6	240.204	238.217
11)	B cis-Chlor...	6.053	5.065	2111.4E6	3150.8E6	994.888m	917.375
12)	B 4,4'-DDE	6.226	5.253	1675.6E6	2514.9E6	852.345	798.443
13)	MA Dieldrin	6.382	5.385	2434.7E6	3569.2E6	1090.812	1008.605
14)	MA Endrin	6.612	5.660	1579.4E6	2440.2E6	867.382	822.091
15)	B Endosulfa...	6.830	5.953	1066.1E6	1660.1E6	544.827	559.311
16)	A 4,4'-DDD	6.744	5.807	781.3E6	1208.0E6	467.931	445.954
17)	MA 4,4'-DDT	7.056	6.058	710.5E6	985.7E6	418.925m	366.136
18)	B Endrin al...	6.960	6.132	892.3E6	1338.5E6	619.602	597.709
19)	B Endosulfa...	7.195	6.355	1602.1E6	2280.4E6	894.545	814.908
20)	A Methoxychlor	7.532	6.633	376.1E6	564.5E6	407.183	398.780
21)	B Endrin ke...	7.681	6.861	2063.7E6	2897.4E6	1050.448	920.889

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011824\
Data File : PD080813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jan 2024 16:47
Operator : AR\AJ
Sample : P1160-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 21:57:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

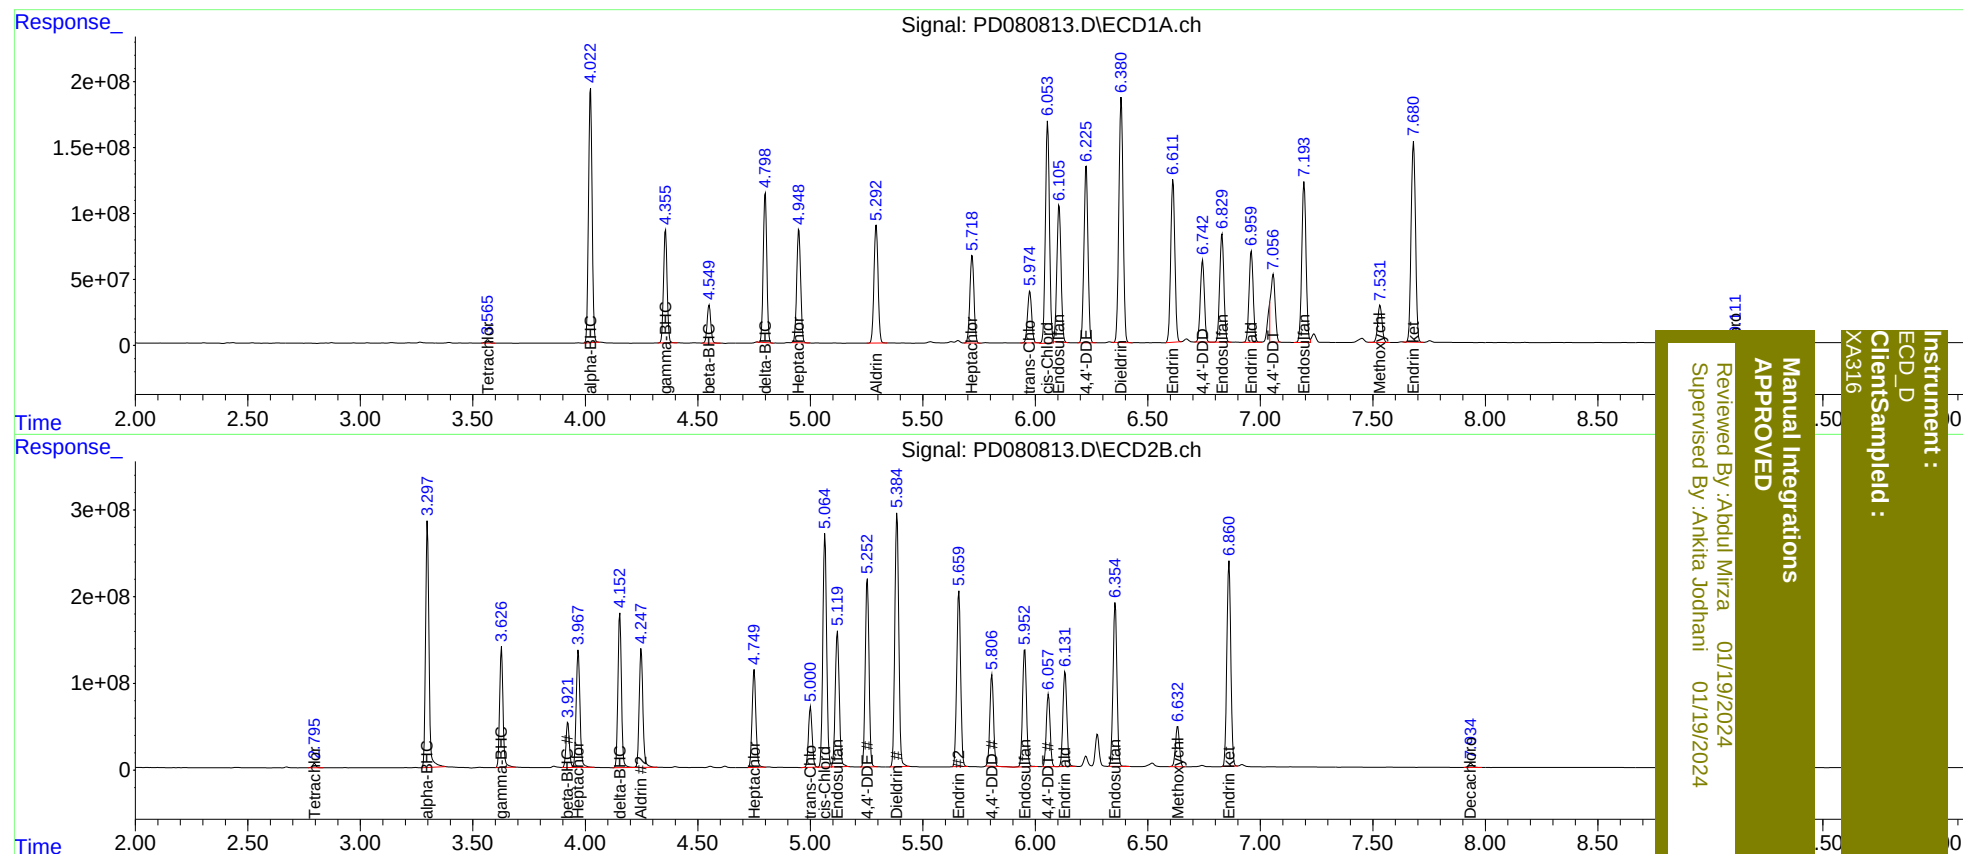

Instrument :
ECD_D
ClientSampled :
XA316

Manual Integrations
APPROVED

Reviewed By: Abul Mirza 01/19/2024
Supervised By: Ankita Jodhani 01/19/2024