

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011922\
 Data File : PD067716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2022 13:39
 Operator : AR\AJ
 Sample : N1129-04MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBLZ8MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/20/2022
 Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 01:06:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	3.981	24182357	108.8E6	10.673	13.429 #
27)	SA Decachlor...	8.152	9.032	22446268	109.4E6	23.436	21.655m
Target Compounds							
2)	A alpha-BHC	3.867	4.373	130.0E6	399.0E6	39.236	38.076m
3)	MA gamma-BHC...	4.148	4.659	125.7E6	394.0E6	39.745	39.937
4)	MA Heptachlor	4.441	5.157	128.0E6	353.7E6	41.303	39.551m
5)	MB Aldrin	4.686	5.462	124.0E6	338.3E6	39.658	40.340
6)	B beta-BHC	4.397	4.838	51010563	169.6E6	37.957	36.677
7)	B delta-BHC	4.598	5.052	63118313	194.5E6	21.340	20.742
8)	B Heptachlo...	5.126	5.849	129.7E6	287.9E6	46.639	34.320m#
9)	A Endosulfan I	5.462	6.207	87035077	256.6E6	32.883	35.720
10)	B trans-Chl...	5.350	6.083	150.6E6	720.9E6	53.332m	96.399m#
11)	B cis-Chlor...	5.408	6.155	237.7E6	1452.9E6	86.718	197.156m#
12)	B 4,4'-DDE	5.571	6.315	310.2E6	762.8E6	123.499	112.971m
13)	MA Dieldrin	5.704	6.465	243.5E6	556.5E6	86.393	74.014m
14)	MA Endrin	5.960	6.683	201.6E6	495.9E6	90.479	88.893m
15)	B Endosulfa...	6.234	6.899	194.2E6	462.2E6	89.766	73.171
16)	A 4,4'-DDD	6.084	6.811	172.5E6	521.2E6	86.598m	88.684
17)	MA 4,4'-DDT	6.324	7.108	194.2E6	528.2E6	94.308	90.913
18)	B Endrin al...	6.403	7.023	133.3E6	404.4E6	85.563	85.579m
19)	B Endosulfa...	6.614	7.247	130.8E6	376.9E6	72.003	64.608
20)	A Methoxychlor	6.871	7.571	362.8E6	1052.5E6	411.373	381.721
21)	B Endrin ke...	7.106	7.720	146.6E6	486.5E6	77.058	73.462

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011922\
Data File : PD067716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2022 13:39
Operator : AR\AJ
Sample : N1129-04MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 01:06:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

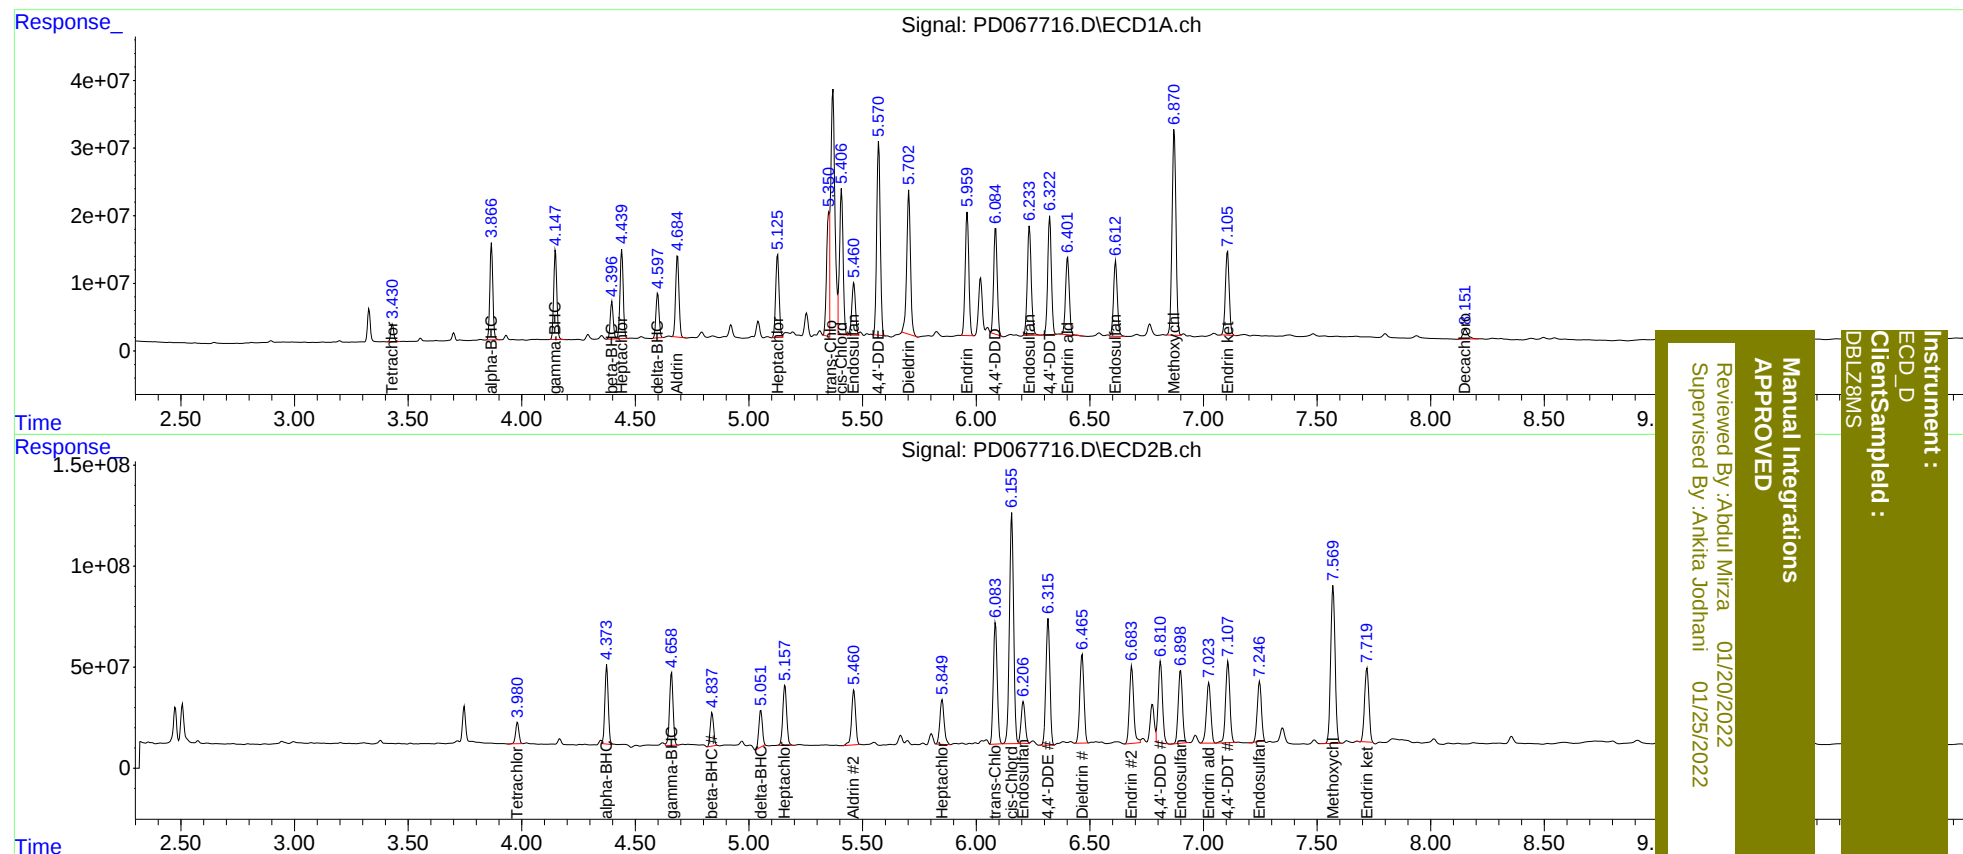

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/20/2022
Supervised By: Ankita Jodhani 01/25/2022

Instrument :
ECD_D
Client Sampled :
DBLZ8MS