

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011922\
 Data File : PD067711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2022 11:32
 Operator : AR\AJ
 Sample : PB142086BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS086

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/20/2022
 Supervised By :Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 01:04:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	3.960	36283591	145.4E6	16.015	17.944
27)	SA Decachlor...	8.152	9.012	32587280	174.2E6	34.025	34.480
Target Compounds							
2)	A alpha-BHC	3.867	4.353	11646524	45548012	3.514	4.346
3)	MA gamma-BHC...	4.148	4.638	11940002	44329305	3.774	4.493
4)	MA Heptachlor	4.440	5.138	11997010	42843113	3.870	4.791
5)	MB Aldrin	4.685	5.440	12707038	39693288	4.064	4.733
6)	B beta-BHC	4.397	4.817	6058359	22932034	4.508	4.959
7)	B delta-BHC	4.598	5.031	8975154	36417702	3.035	3.884 #
8)	B Heptachlo...	5.126	5.829	12046360	35274790	4.333	4.205
9)	A Endosulfan I	5.462	6.186	11140566	33874420	4.209	4.715
10)	B trans-Chl...	5.350	6.064	12105912	34557104	4.288	4.621
11)	B cis-Chlor...	5.408	6.135	12192550	35043353	4.448	4.755
12)	B 4,4'-DDE	5.572	6.296	21769303	66755981	8.667	9.887
13)	MA Dieldrin	5.704	6.444	23361315	69197071	8.288	9.202
14)	MA Endrin	5.961	6.663	16355631	47041239	7.341	8.433
15)	B Endosulfa...	6.235	6.878	19523048	64167793	9.025	10.158
16)	A 4,4'-DDD	6.085	6.790	18673052	61290498	9.373m	10.428
17)	MA 4,4'-DDT	6.324	7.087	13480931	43172435	6.546	7.431
18)	B Endrin al...	6.403	7.003	17528625	53799773	11.254	11.384
19)	B Endosulfa...	6.614	7.225	14509346	48586843	7.986	8.328
20)	A Methoxychlor	6.873	7.550	35505027	117.1E6	40.256	42.466
21)	B Endrin ke...	7.106	7.698	20154125	68865328	10.592	10.400

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011922\
Data File : PD067711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2022 11:32
Operator : AR\AJ
Sample : PB142086BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 01:04:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

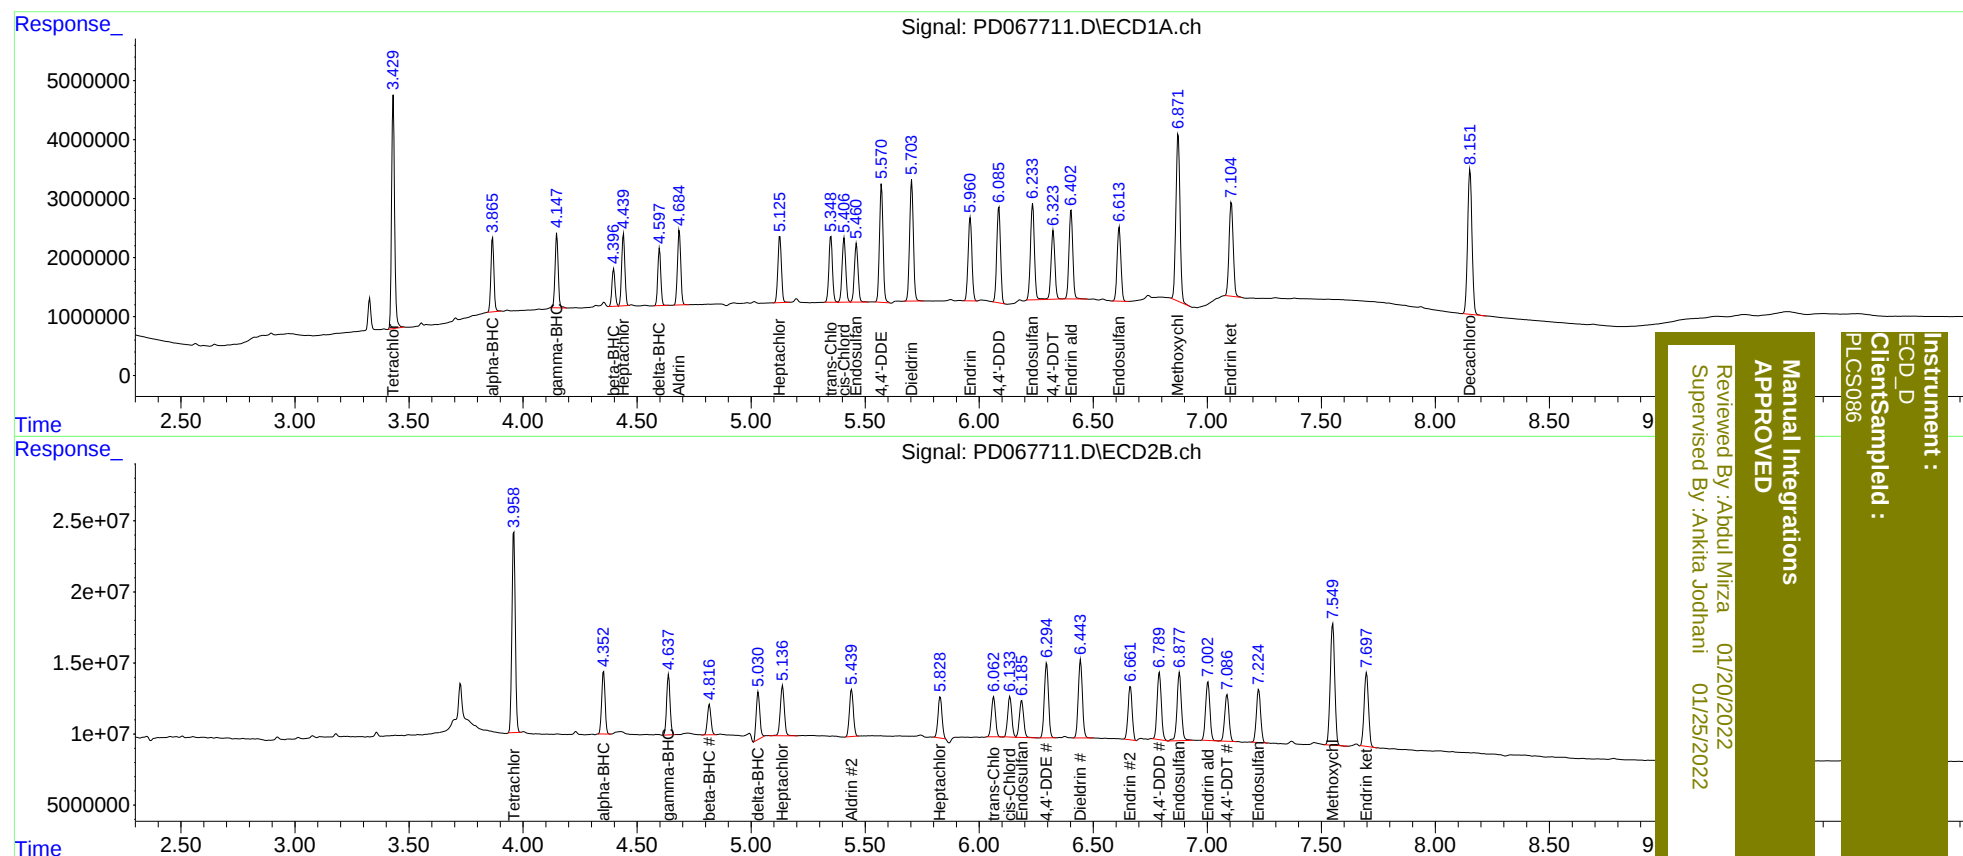

Instrument :
ECD_D
ClientSampled :
PLCS086

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 01/20/2022
Supervised By: Ankita Jodhani 01/25/2022