

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011922\
 Data File : PD067713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2022 12:57
 Operator : AR\AJ
 Sample : N1129-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBLZ6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/20/2022
 Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 01:05:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	3.960	29700427	117.4E6	13.109	14.484
2)	SA Decachlor...	8.152	9.012	23054072	152.1E6	24.071	30.093m#
Target Compounds							
10)	B trans-Chl...	5.350	6.063	8293707	135.5E6	2.938	18.113m#
12)	B 4,4'-DDE	5.571	6.294	73198447	195.7E6	29.143	28.978m
16)	A 4,4'-DDD	6.091	6.790	3302596	24097559	1.658m	4.100m#
17)	MA 4,4'-DDT	6.324	7.088	45377473	154.0E6	22.036	26.499

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011922\
Data File : PD067713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2022 12:57
Operator : AR\AJ
Sample : N1129-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 01:05:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

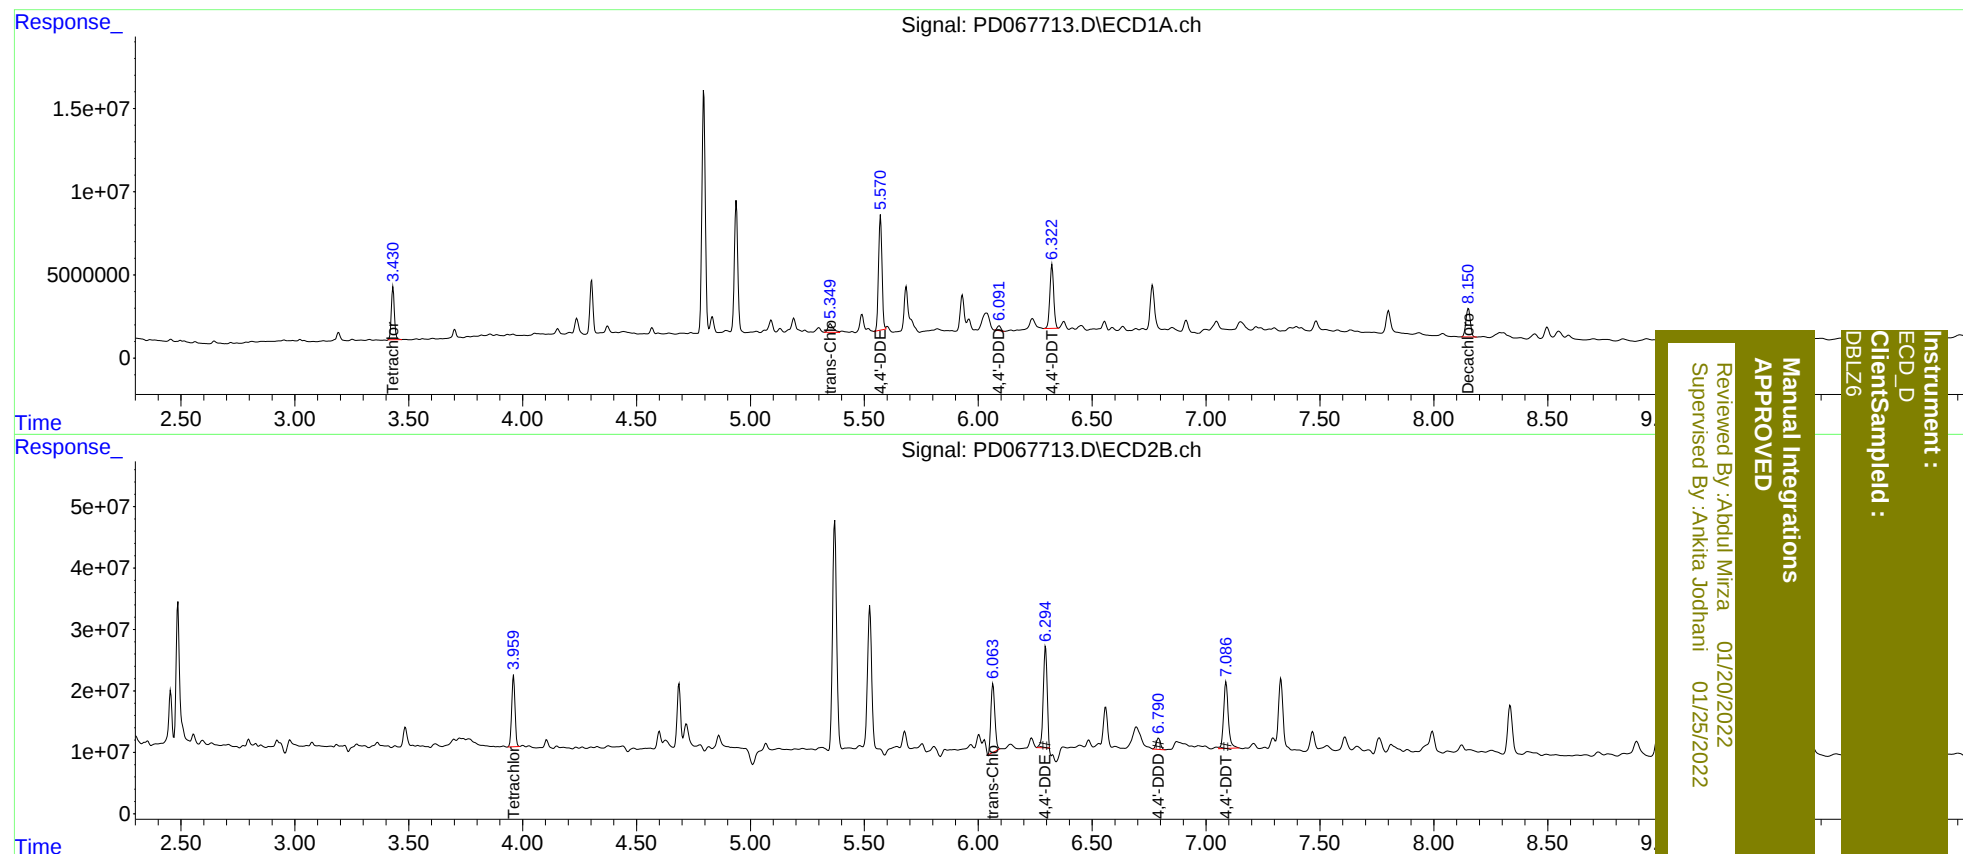

Reviewed By: Abdul Mirza 01/20/2022
Supervised By: Ankita Jodhani 01/25/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client/Sampled :
DBLZ6