

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011923\
 Data File : PD073651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2023 08:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 20:34:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.776	50198104	29105175	21.475	22.862
28)	SA Decachlor...	9.103	7.934	63937147	27127656	22.688	23.316
Target Compounds							
4)	MA Heptachlor	4.925	0.000	194460	0	0.052	N.D. #
6)	B beta-BHC	4.566f	3.916	307288	42727	0.198	0.064 #
7)	B delta-BHC	4.781	0.000	2813478	0	0.836	N.D. #
8)	B Heptachlo...	5.702	0.000	930866	0	0.292	N.D. #
9)	A Endosulfan I	6.096	0.000	226226	0	0.074	N.D. #
10)	B gamma-Chl...	5.957	0.000	152735	0	0.046	N.D. #
11)	B alpha-Chl...	6.041	0.000	267140	0	0.081	N.D. #
15)	B Endosulfa...	6.845f	0.000	500159	0	0.189	N.D. #
21)	B Endrin ke...	7.701f	0.000	523281	0	0.173	N.D. #
25)	Chlordane-3	5.957	0.000	152735	0	0.326	N.D. #
26)	Chlordane-4	6.041	0.000	267140	0	0.467	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011923\
Data File : PD073651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2023 08:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 20:34:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

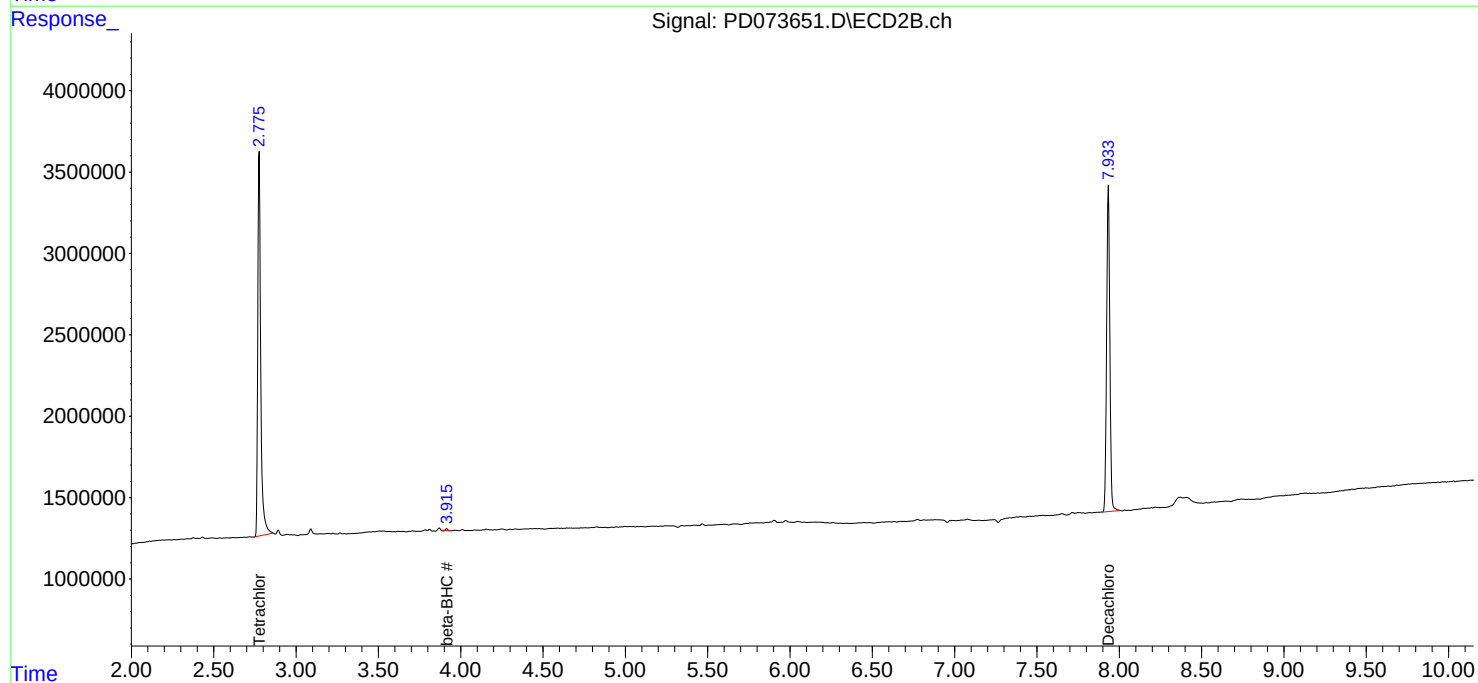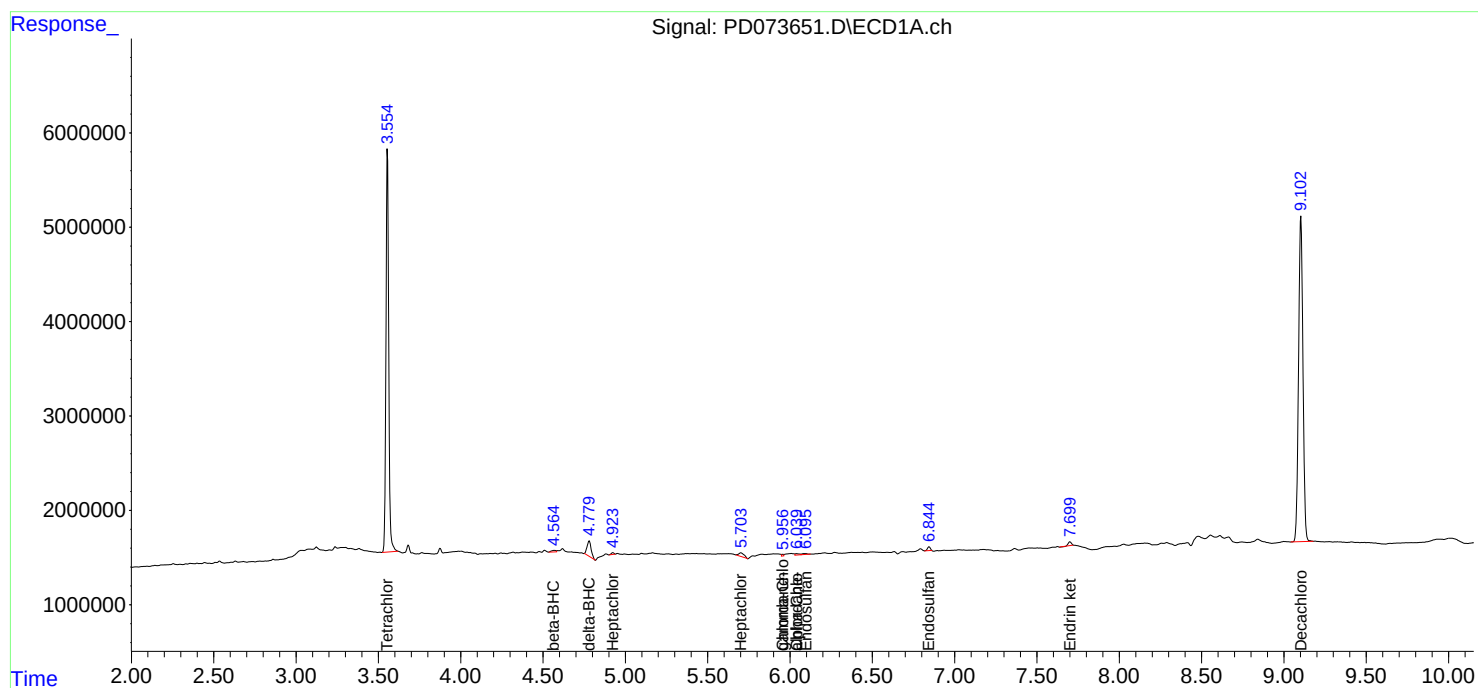


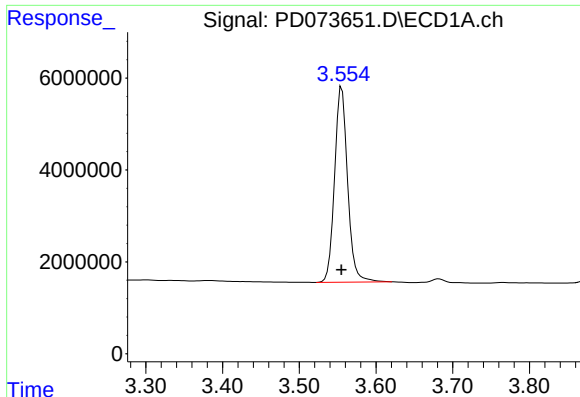

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 50198104
Conc: 21.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

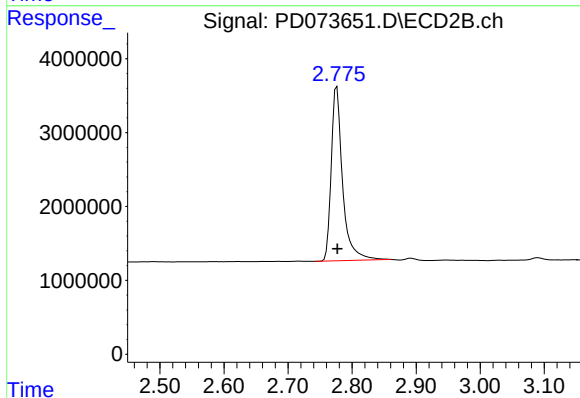


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 29105175
Conc: 22.86 ng/ml

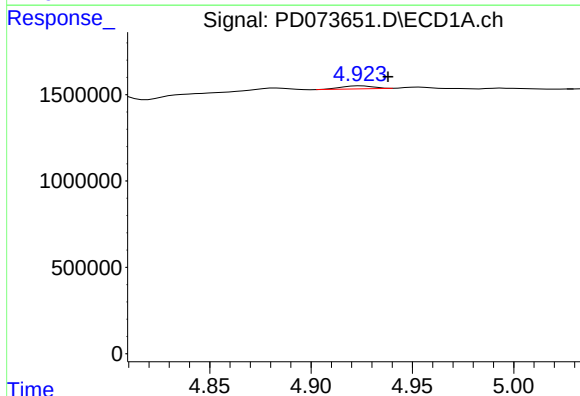


#4 Heptachlor

R.T.: 4.925 min
Delta R.T.: -0.013 min
Response: 194460
Conc: 0.05 ng/ml

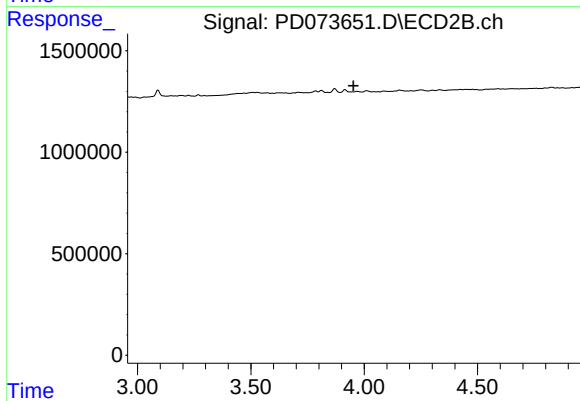

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.953 min
Response: 0
Conc: N.D.

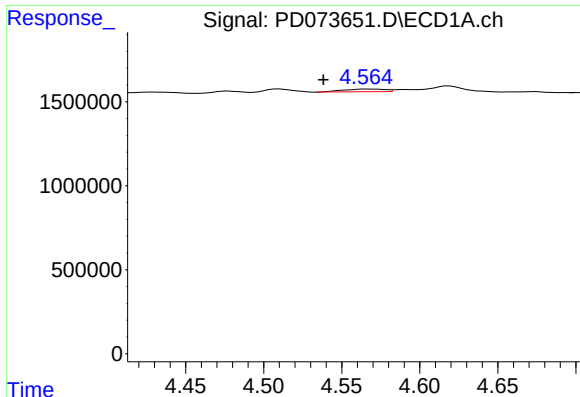

#6 beta-BHC


R.T.: 4.566 min
Delta R.T.: 0.028 min
Response: 307288
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

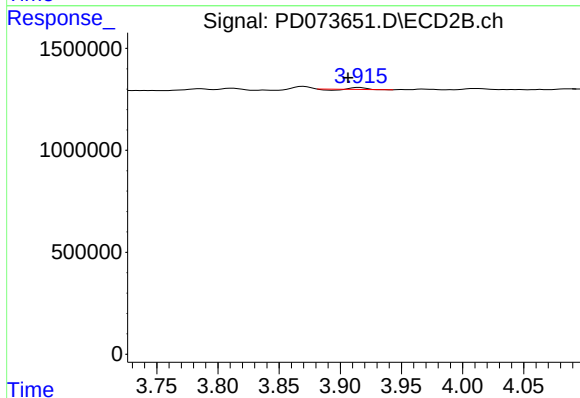


#6 beta-BHC

R.T.: 3.916 min
Delta R.T.: 0.010 min
Response: 42727
Conc: 0.06 ng/ml

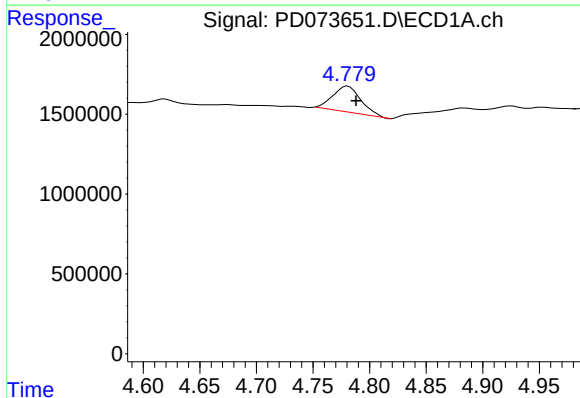


#7 delta-BHC

R.T.: 4.781 min
Delta R.T.: -0.007 min
Response: 2813478
Conc: 0.84 ng/ml

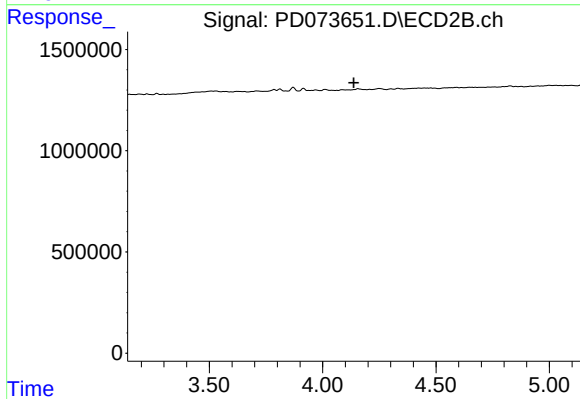

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

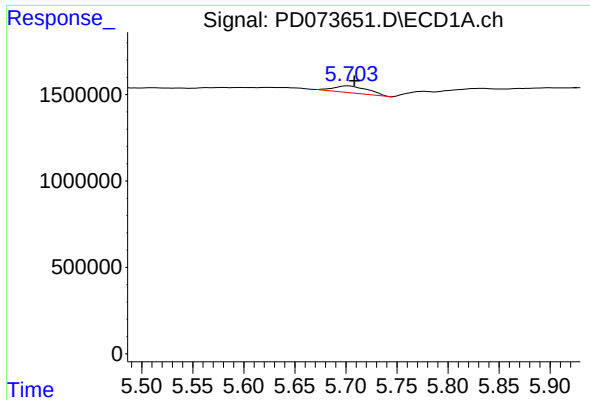

#8 Heptachlor epoxide


R.T.: 5.702 min
Delta R.T.: -0.006 min
Response: 930866
Conc: 0.29 ng/ml

Instrument :
ECD_D
ClientSampleId :

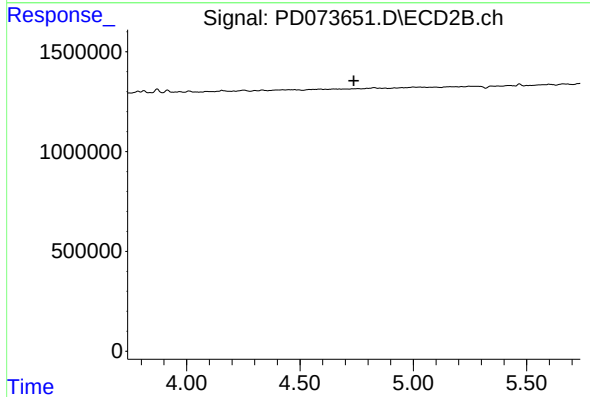


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

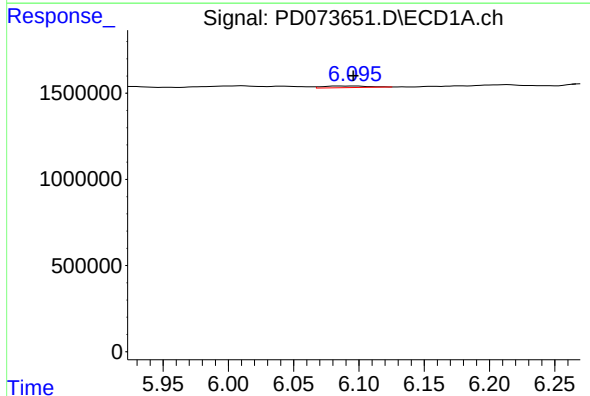


#9 Endosulfan I

R.T.: 6.096 min
Delta R.T.: 0.000 min
Response: 226226
Conc: 0.07 ng/ml

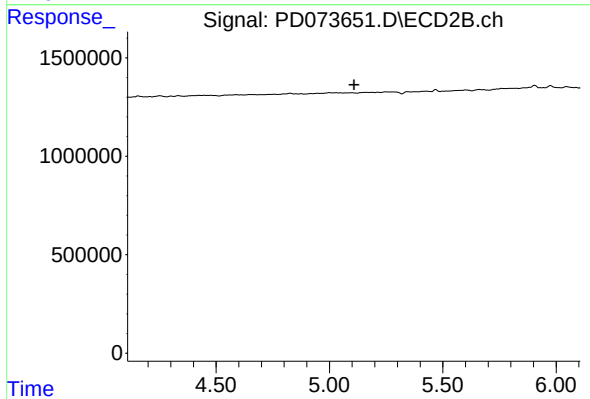

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

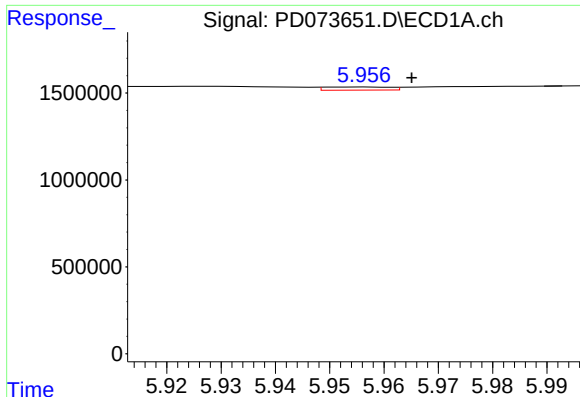

#10 gamma-Chlordane


R.T.: 5.957 min
Delta R.T.: -0.008 min
Response: 152735
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

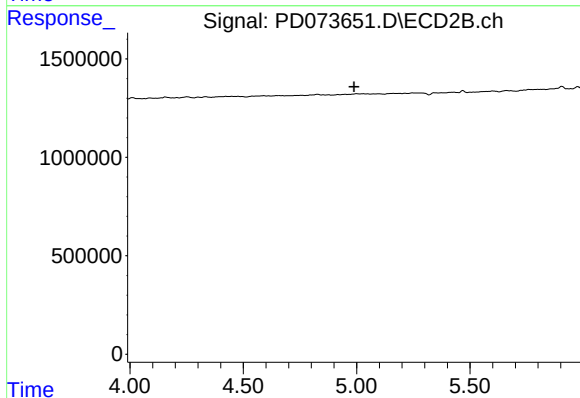


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

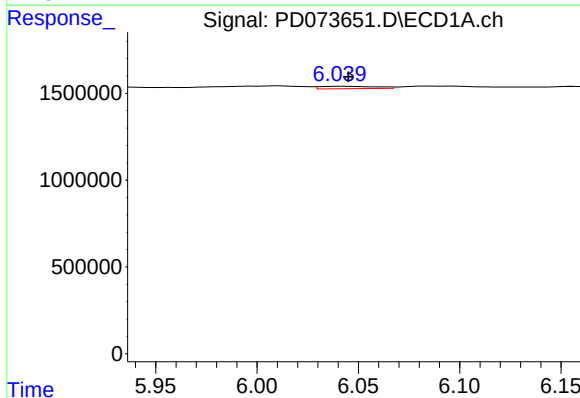


#11 alpha-Chlordane

R.T.: 6.041 min
Delta R.T.: -0.004 min
Response: 267140
Conc: 0.08 ng/ml

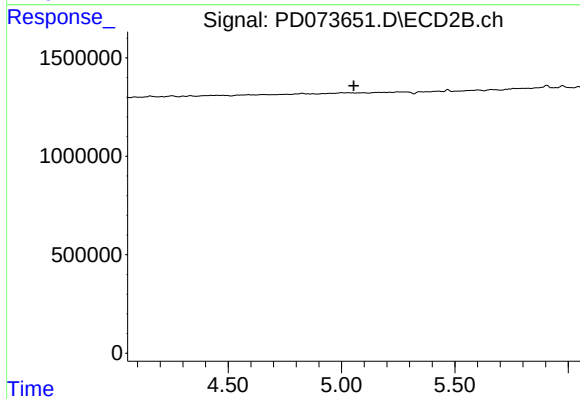

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

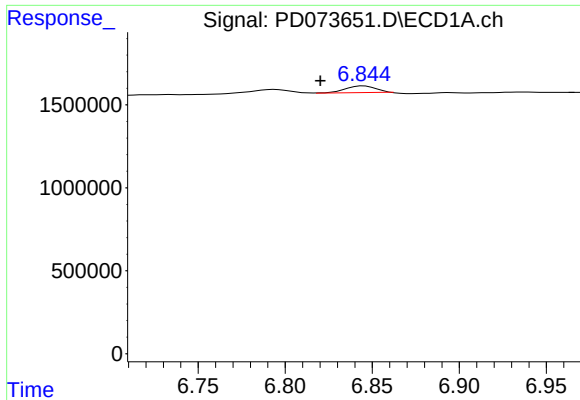

#15 Endosulfan II


R.T.: 6.845 min
Delta R.T.: 0.025 min
Response: 500159
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

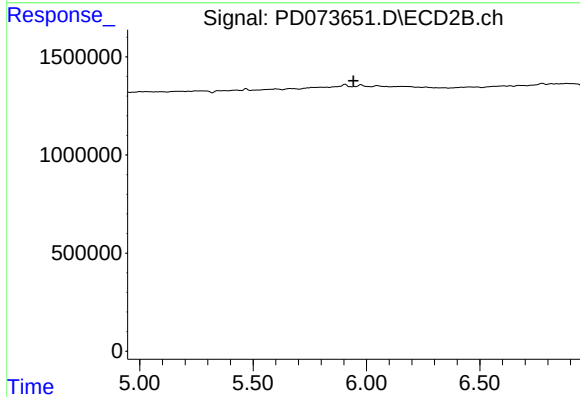


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

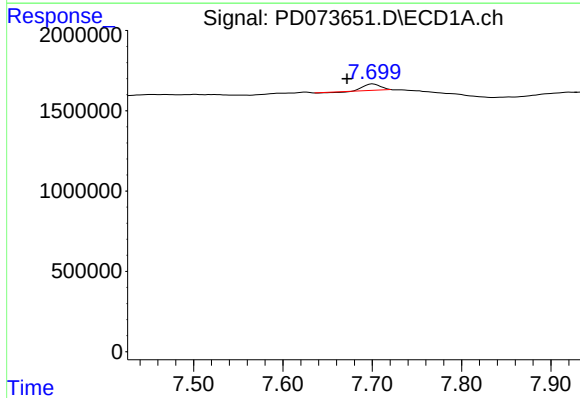


#21 Endrin ketone

R.T.: 7.701 min
Delta R.T.: 0.029 min
Response: 523281
Conc: 0.17 ng/ml

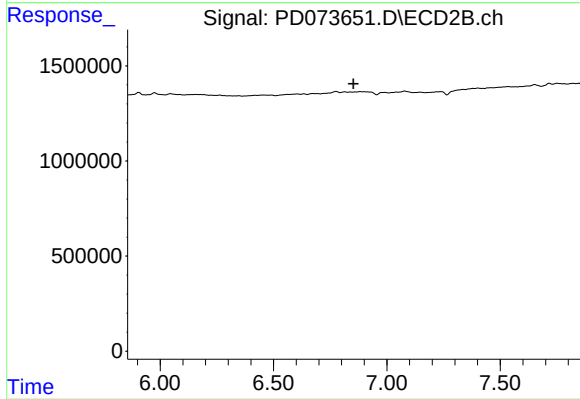

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

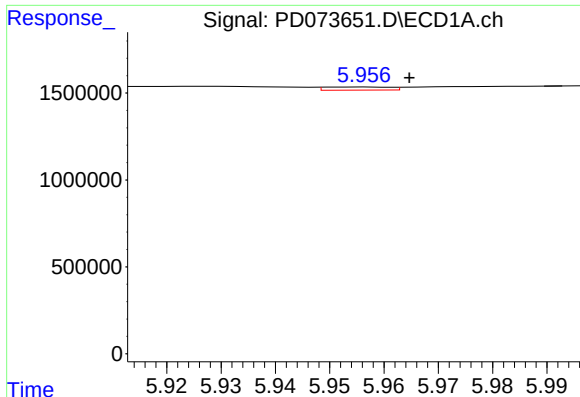

#25 Chlordane-3


R.T.: 5.957 min
Delta R.T.: -0.008 min
Response: 152735
Conc: 0.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

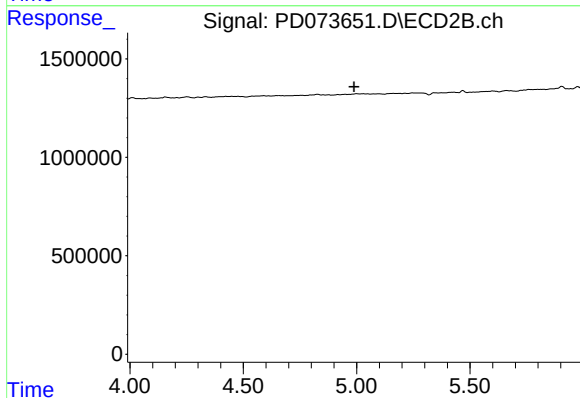


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

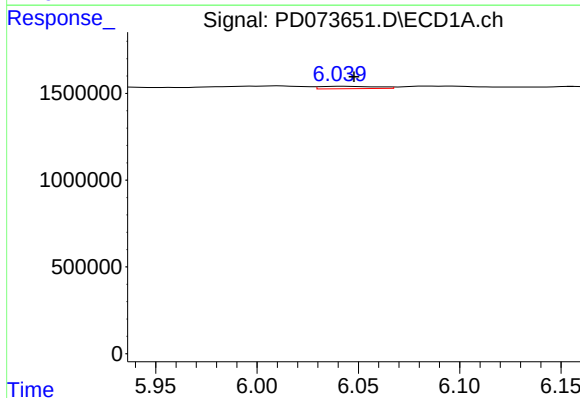


#26 Chlordane-4

R.T.: 6.041 min
Delta R.T.: -0.006 min
Response: 267140
Conc: 0.47 ng/ml

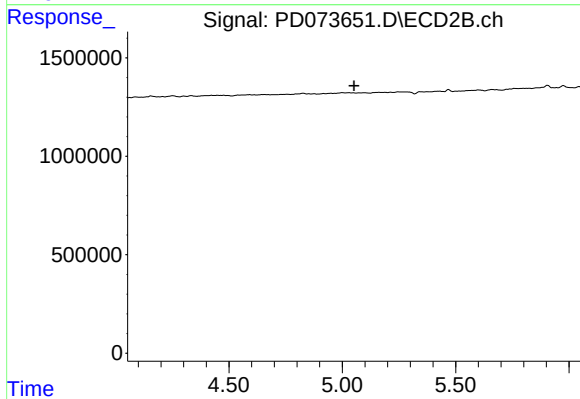

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.053 min
Response: 0
Conc: N.D.

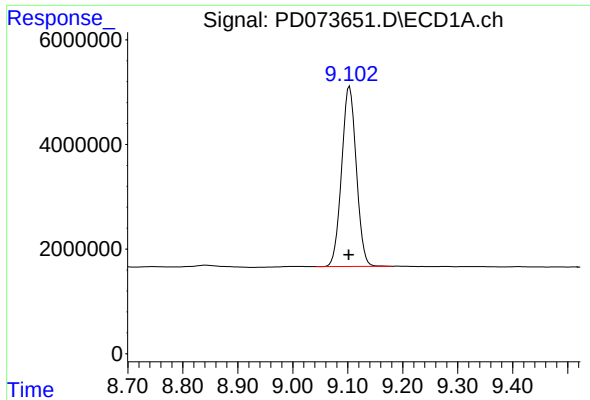

#28 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: 0.002 min
Response: 63937147
Conc: 22.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

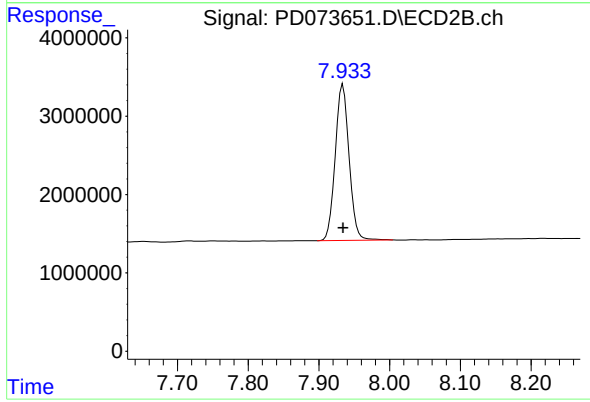

#28 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 27127656
Conc: 23.32 ng/ml