

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011923\
 Data File : PD073654.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2023 12:45
 Operator : AR\AJ
 Sample : PB150334BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 20:36:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.775	40211876	22575353	17.203	17.733
28)	SA Decachlor...	9.113	7.936	55111301	21761471	19.557	18.704
Target Compounds							
4)	MA Heptachlor	4.960f	0.000	1133251	0	0.305	N.D. #
7)	B delta-BHC	4.791	0.000	2458695	0	0.731	N.D. #
8)	B Heptachlo...	5.708	0.000	459681	0	0.144	N.D. #
10)	B gamma-Chl...	5.959	0.000	348951	0	0.106	N.D. #
11)	B alpha-Chl...	6.017f	0.000	77945	0	0.024	N.D. #
25)	Chlordane-3	5.959	0.000	348951	0	0.745	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011923\
Data File : PD073654.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2023 12:45
Operator : AR\AJ
Sample : PB150334BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 20:36:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

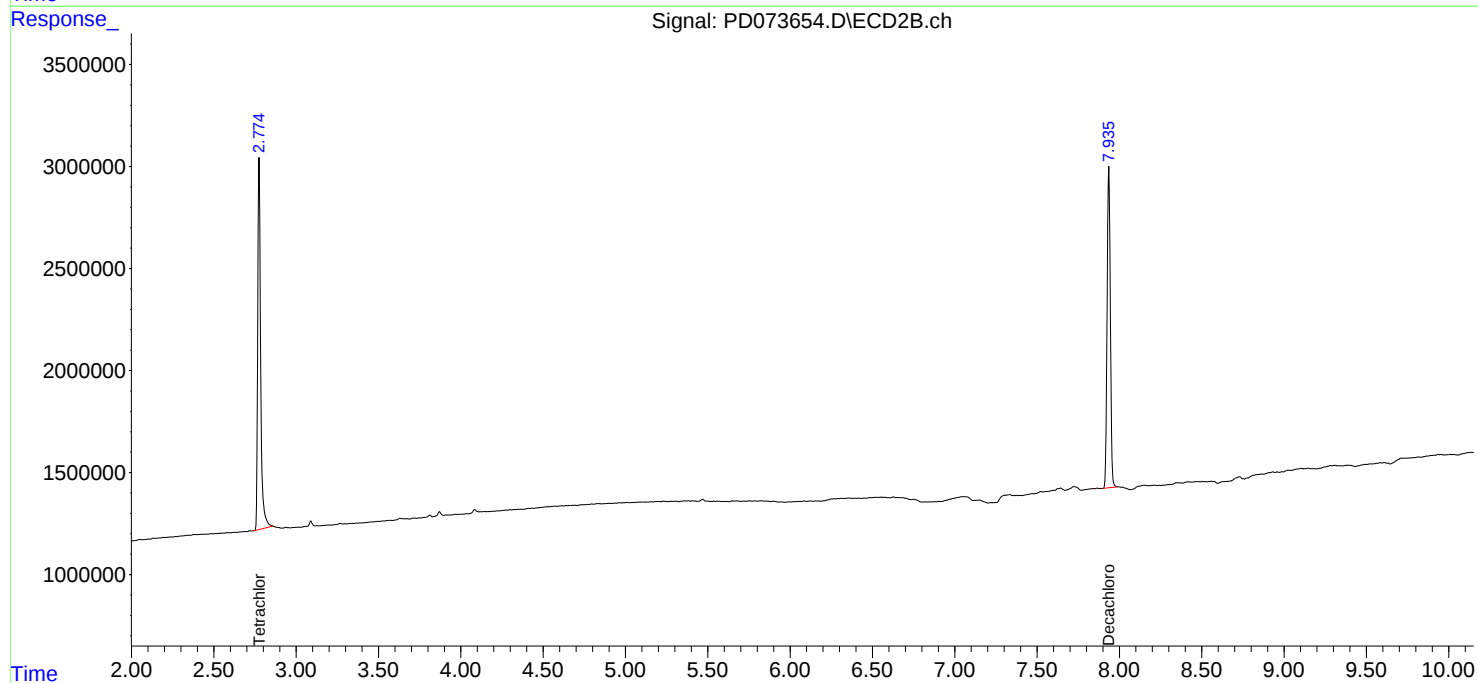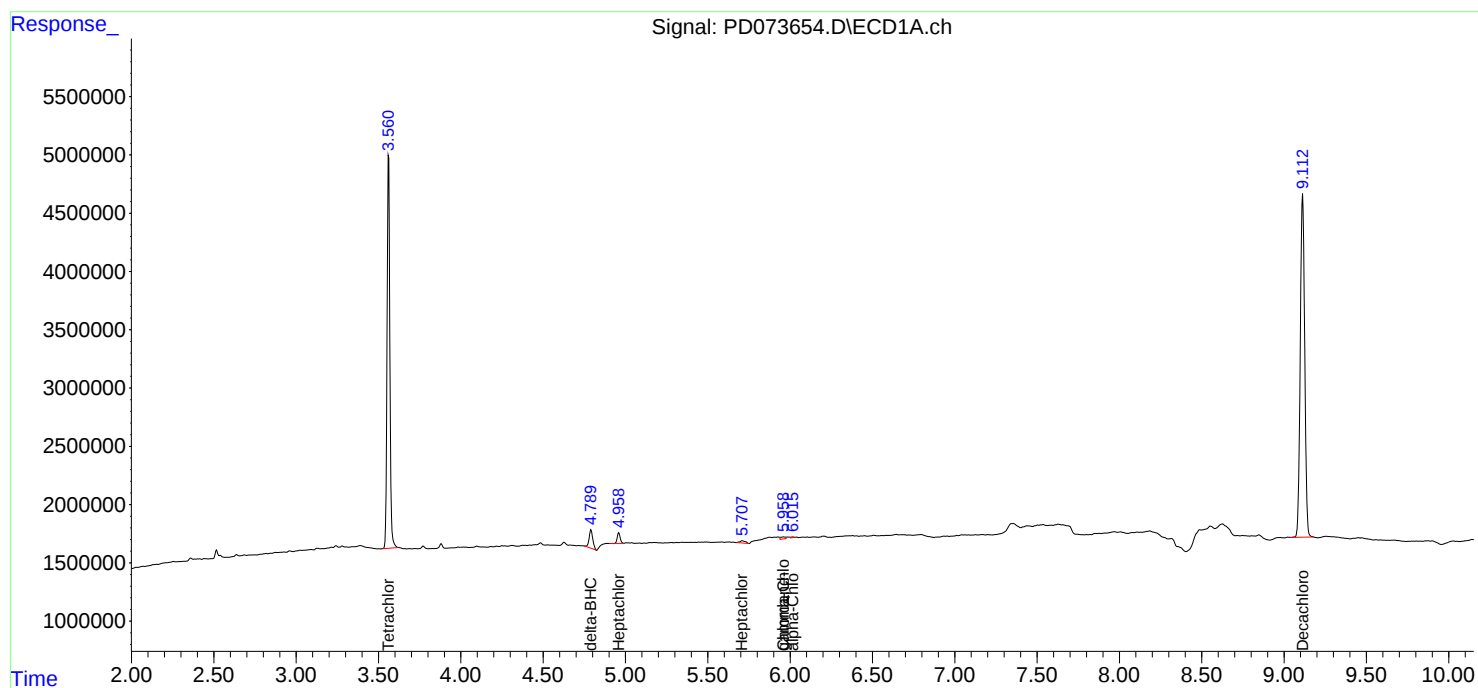


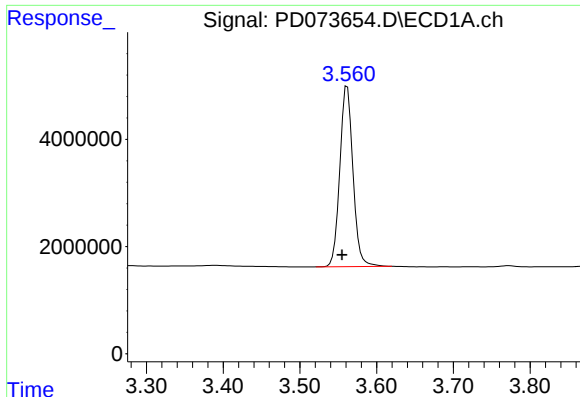

#1 Tetrachloro-m-xylene


R.T.: 3.562 min
Delta R.T.: 0.007 min
Response: 40211876
Conc: 17.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

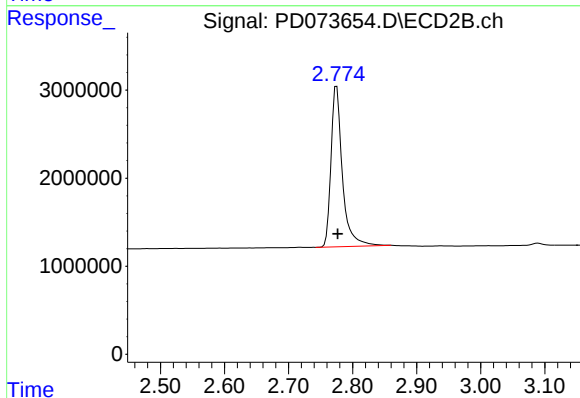


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: -0.002 min
Response: 22575353
Conc: 17.73 ng/ml

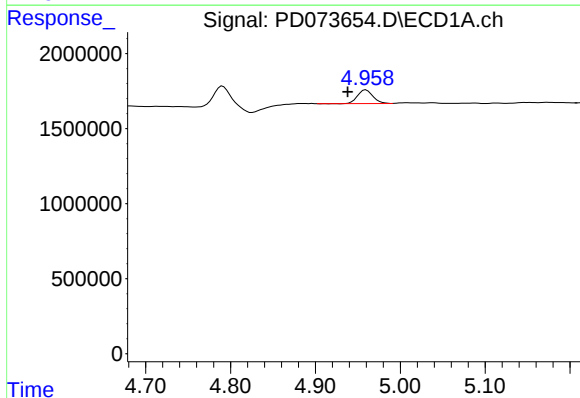


#4 Heptachlor

R.T.: 4.960 min
Delta R.T.: 0.022 min
Response: 1133251
Conc: 0.31 ng/ml

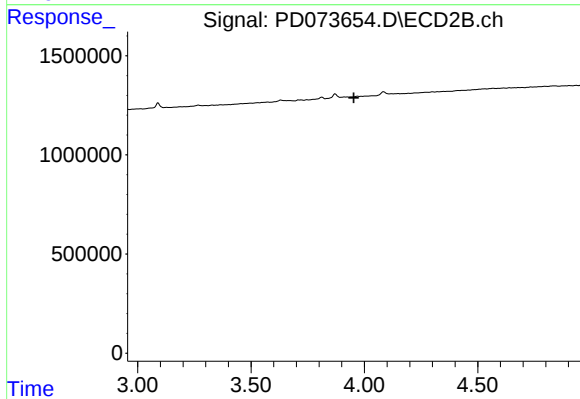

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.953 min
Response: 0
Conc: N.D.

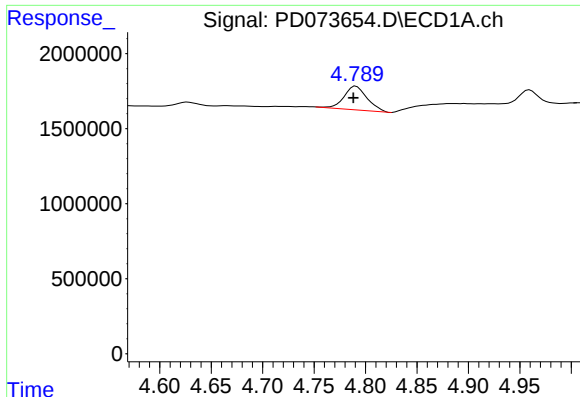

#7 delta-BHC


R.T.: 4.791 min
Delta R.T.: 0.003 min
Response: 2458695
Conc: 0.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

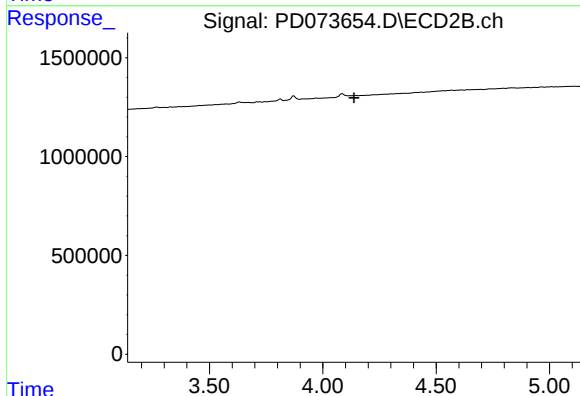


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

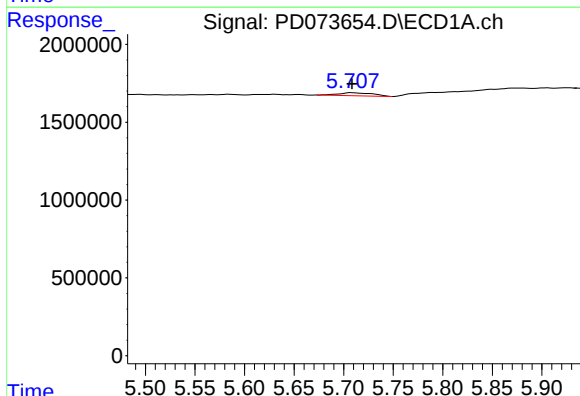


#8 Heptachlor epoxide

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 459681
Conc: 0.14 ng/ml

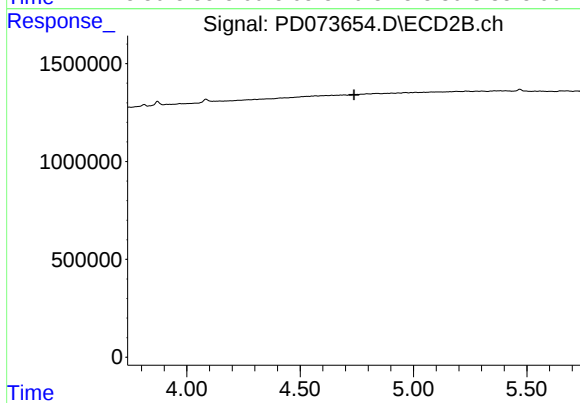

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

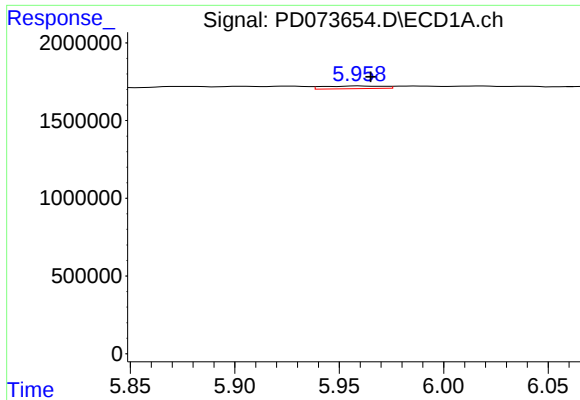

#10 gamma-Chlordane


R.T.: 5.959 min
Delta R.T.: -0.006 min
Response: 348951
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

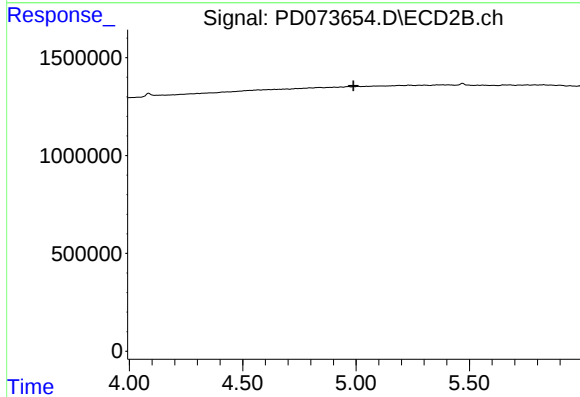


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

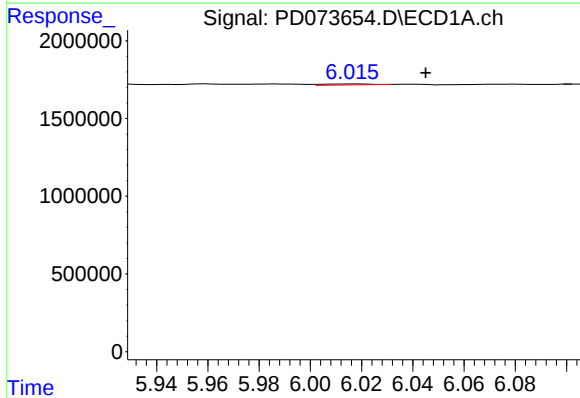


#11 alpha-Chlordane

R.T.: 6.017 min
Delta R.T.: -0.028 min
Response: 77945
Conc: 0.02 ng/ml

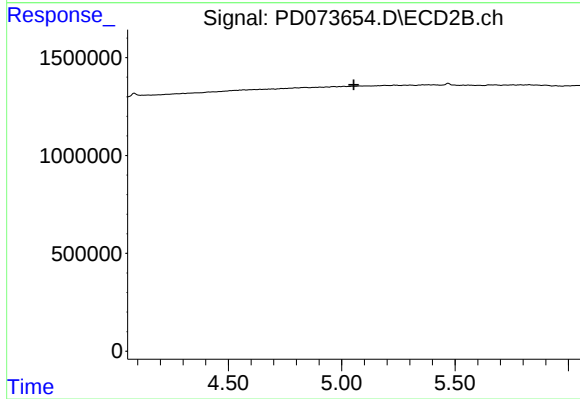

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

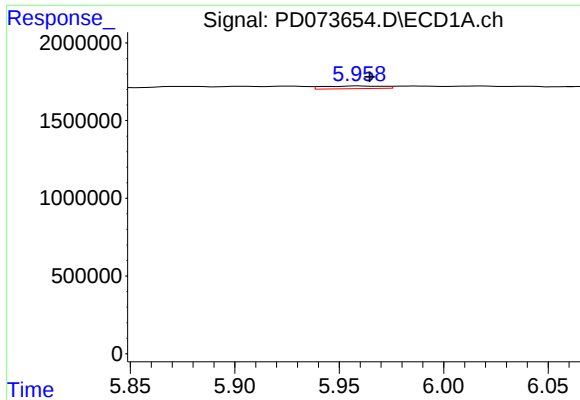

#25 Chlordane-3


R.T.: 5.959 min
Delta R.T.: -0.005 min
Response: 348951
Conc: 0.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

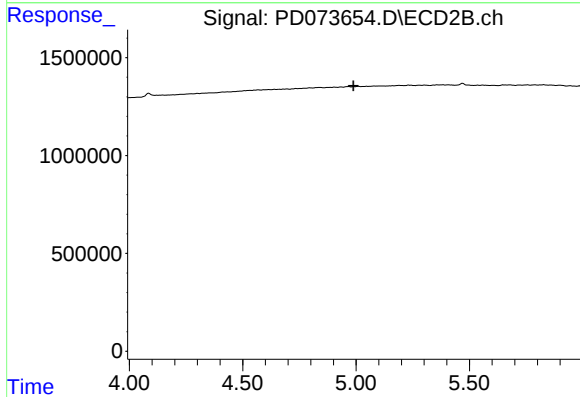


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

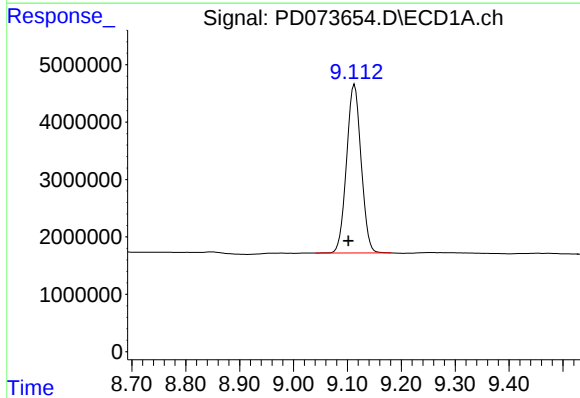

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.011 min
Response: 55111301
Conc: 19.56 ng/ml

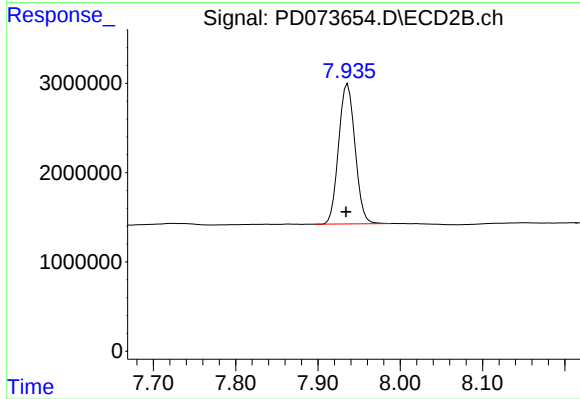

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.002 min
Response: 21761471
Conc: 18.70 ng/ml