

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011923\
 Data File : PD073662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2023 14:33
 Operator : AR\AJ
 Sample : 01214-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 20:46:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.777	41219666	22958007	17.634	18.034
28)	SA Decachlor...	9.101	7.933	41918588	17177744	14.875	14.764
Target Compounds							
4)	MA Heptachlor	4.951	0.000	1297044	0	0.349	N.D. #
6)	B beta-BHC	4.552	0.000	838036	0	0.540	N.D. #
7)	B delta-BHC	4.780	0.000	2149001	0	0.639	N.D. #
10)	B gamma-Chl...	5.992f	0.000	293794	0	0.089	N.D. #
15)	B Endosulfa...	6.796f	0.000	204045	0	0.077	N.D. #
18)	B Endrin al...	6.931f	0.000	177481	0	0.082	N.D. #
21)	B Endrin ke...	7.697f	0.000	912139	0	0.302	N.D. #
25)	Chlordane-3	5.938f	0.000	545523	0	1.165	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011923\
Data File : PD073662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2023 14:33
Operator : AR\AJ
Sample : 01214-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 20:46:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

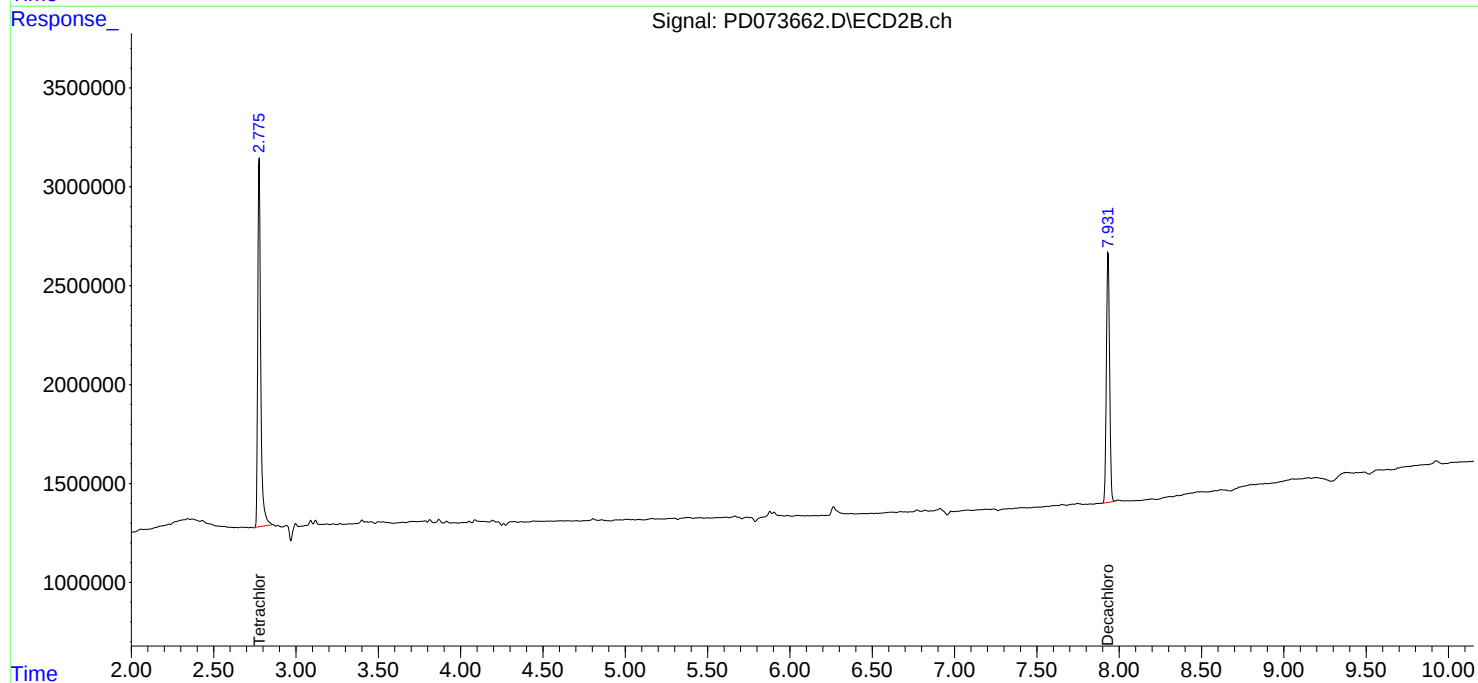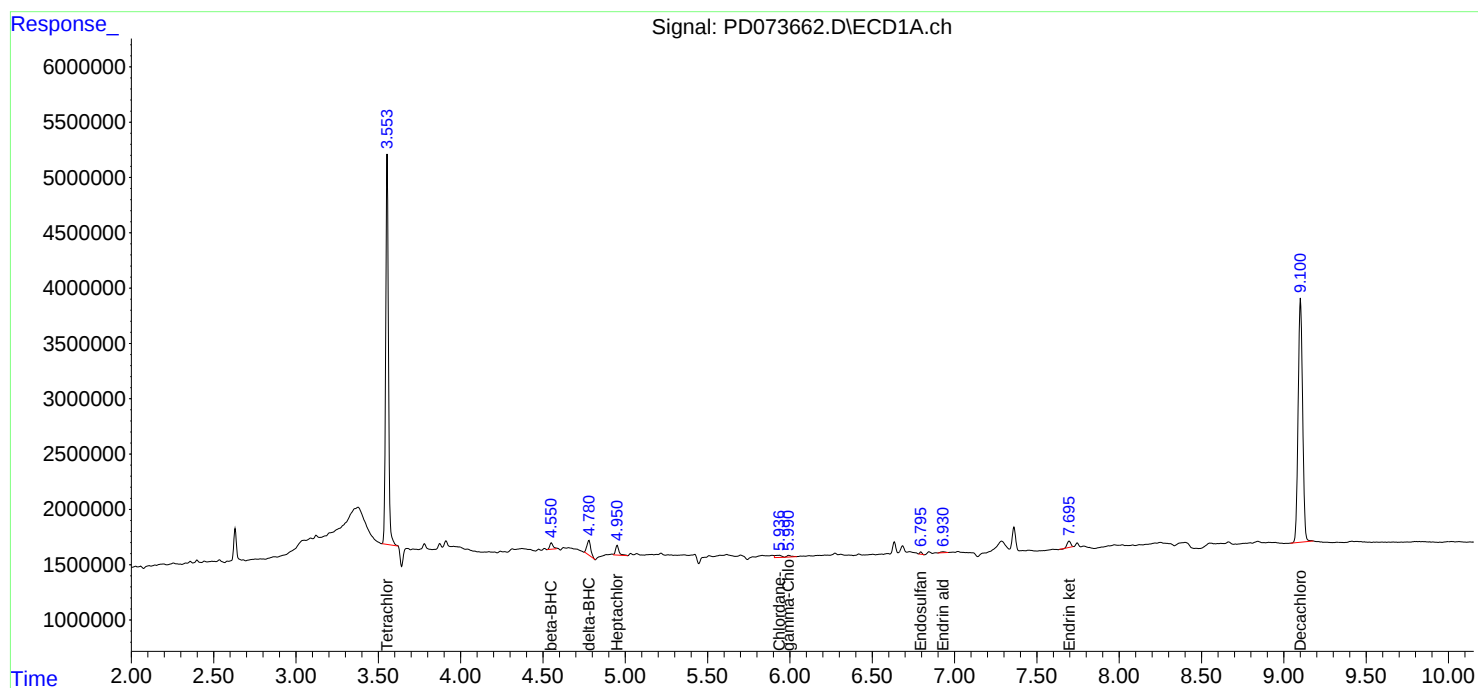


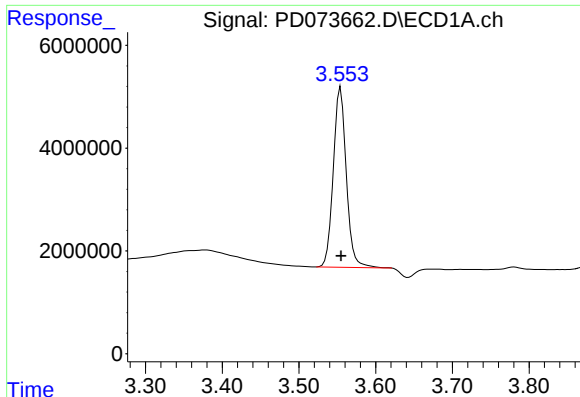

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 41219666
Conc: 17.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

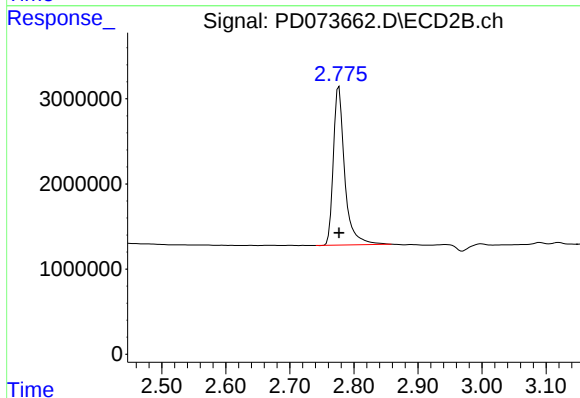


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 22958007
Conc: 18.03 ng/ml

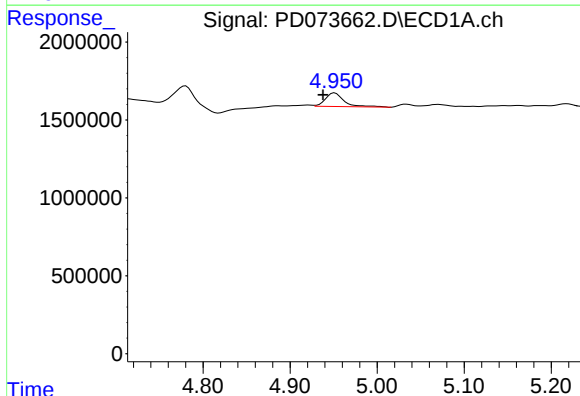


#4 Heptachlor

R.T.: 4.951 min
Delta R.T.: 0.013 min
Response: 1297044
Conc: 0.35 ng/ml

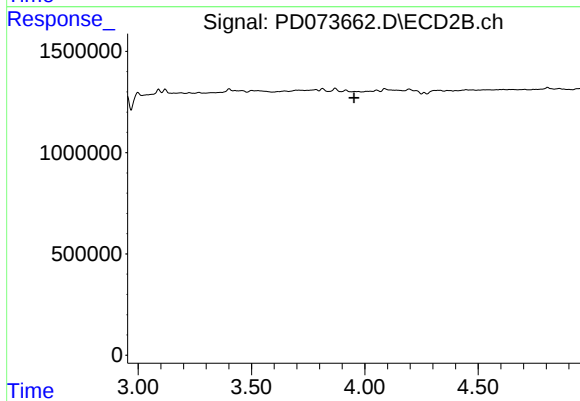

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.953 min
Response: 0
Conc: N.D.

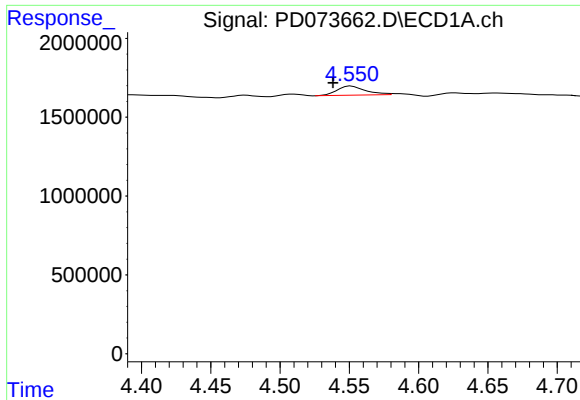

#6 beta-BHC


R.T.: 4.552 min
Delta R.T.: 0.013 min
Response: 838036
Conc: 0.54 ng/ml

Instrument :
ECD_D
ClientSampleId :

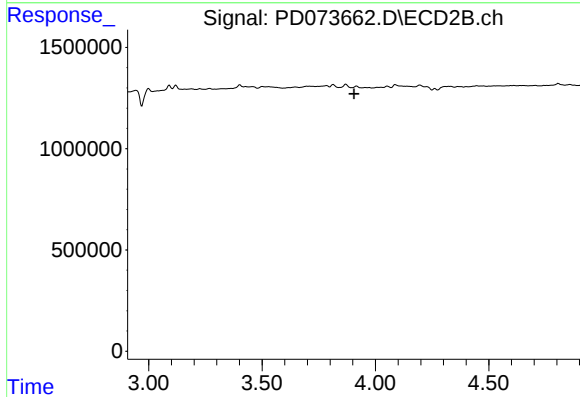


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.906 min
Response: 0
Conc: N.D.

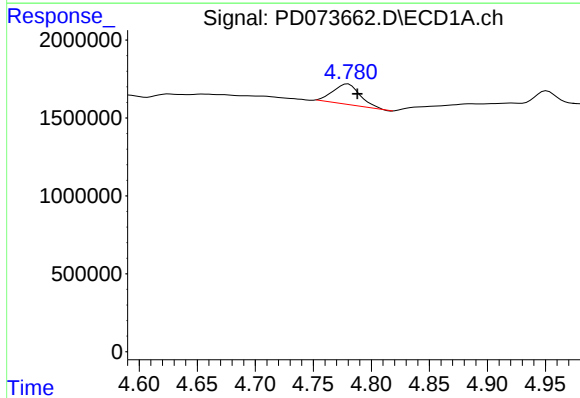


#7 delta-BHC

R.T.: 4.780 min
Delta R.T.: -0.008 min
Response: 2149001
Conc: 0.64 ng/ml

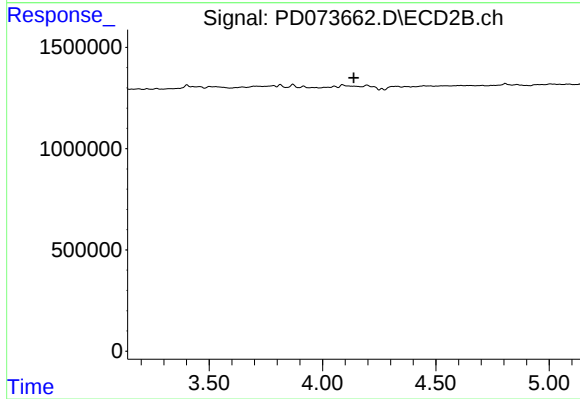

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

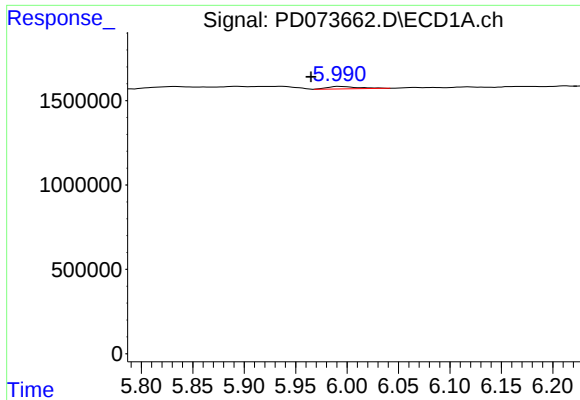

#10 gamma-Chlordane


R.T.: 5.992 min
Delta R.T.: 0.027 min
Response: 293794
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

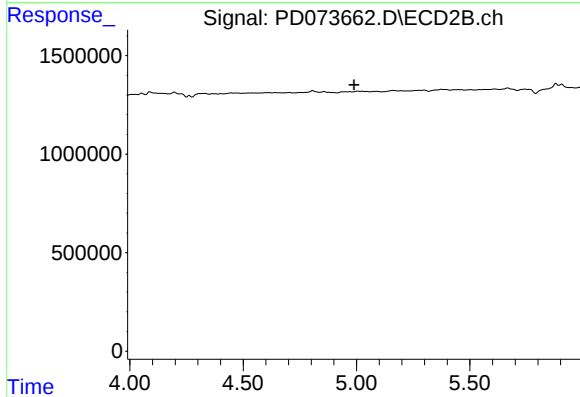


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

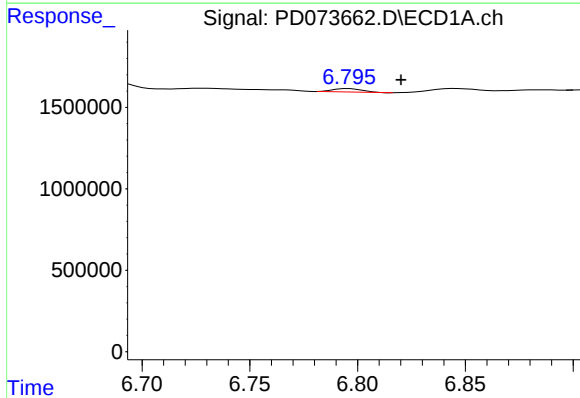


#15 Endosulfan II

R.T.: 6.796 min
Delta R.T.: -0.024 min
Response: 204045
Conc: 0.08 ng/ml

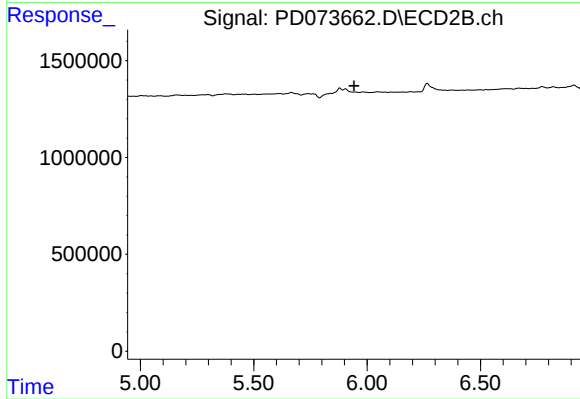

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

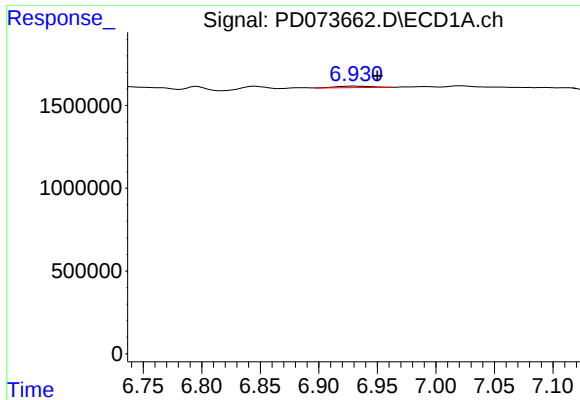

#18 Endrin aldehyde


R.T.: 6.931 min
Delta R.T.: -0.019 min
Response: 177481
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

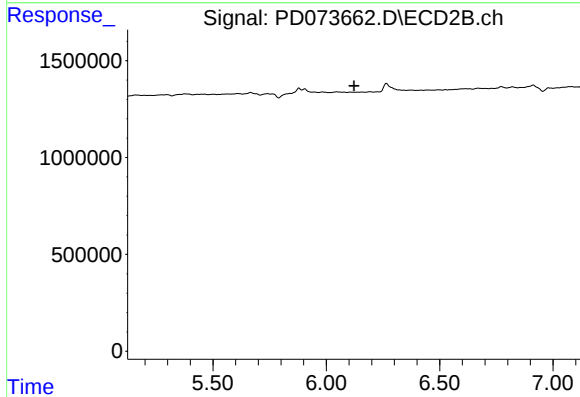


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

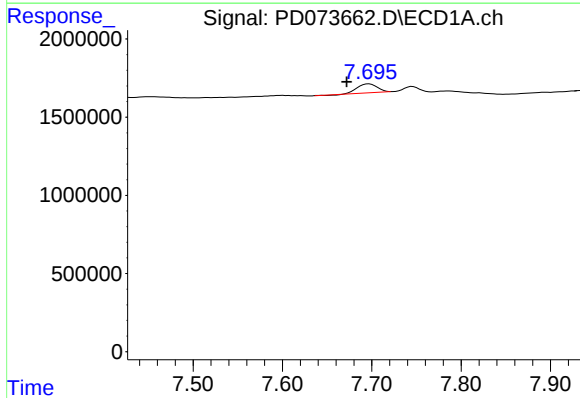


#21 Endrin ketone

R.T.: 7.697 min
Delta R.T.: 0.025 min
Response: 912139
Conc: 0.30 ng/ml

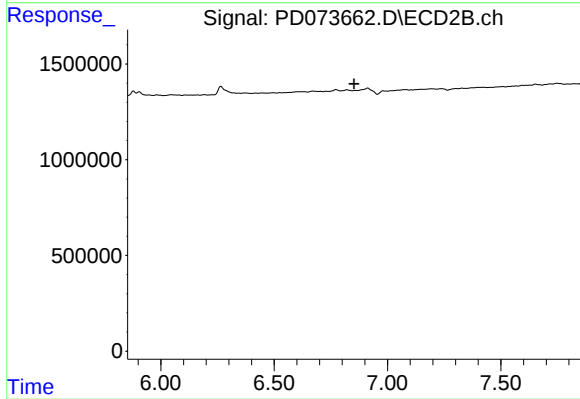

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

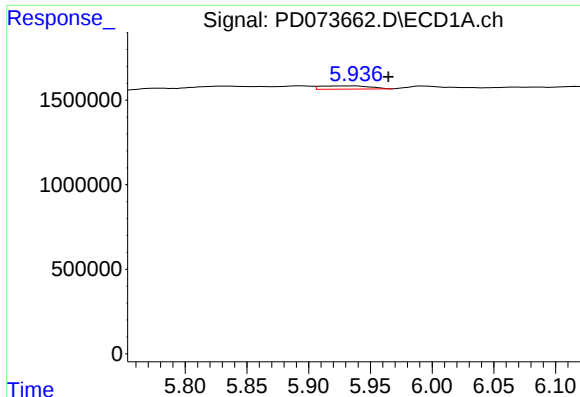

#25 Chlordane-3


R.T.: 5.938 min
Delta R.T.: -0.027 min
Response: 545523
Conc: 1.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

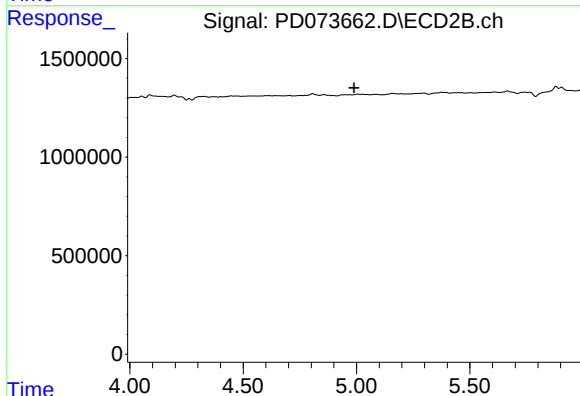


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

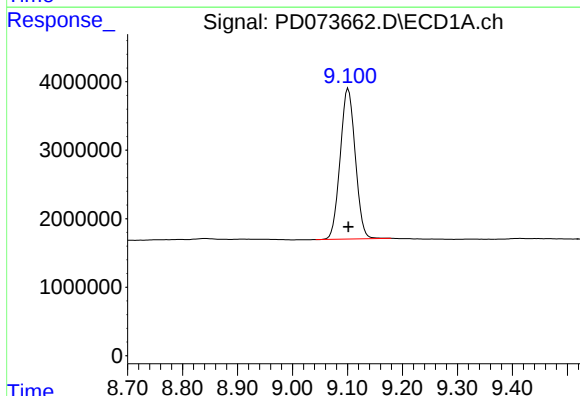

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.000 min
Response: 41918588
Conc: 14.88 ng/ml

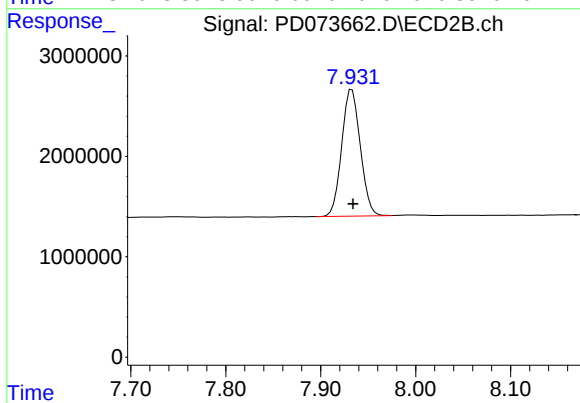

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: -0.001 min
Response: 17177744
Conc: 14.76 ng/ml