

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011923\
 Data File : PD073662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jan 2023 14:33
 Operator : AR\AJ
 Sample : 01214-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TJRC-011823-B3-30-40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 20:46:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.777	41219666	22958007	17.634	18.034
28)	SA Decachlor...	9.101	7.933	41918588	17177744	14.875	14.764

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD011923\
Data File : PD073662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jan 2023 14:33
Operator : AR\AJ
Sample : 01214-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TJRC-011823-B3-30-40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 20:46:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

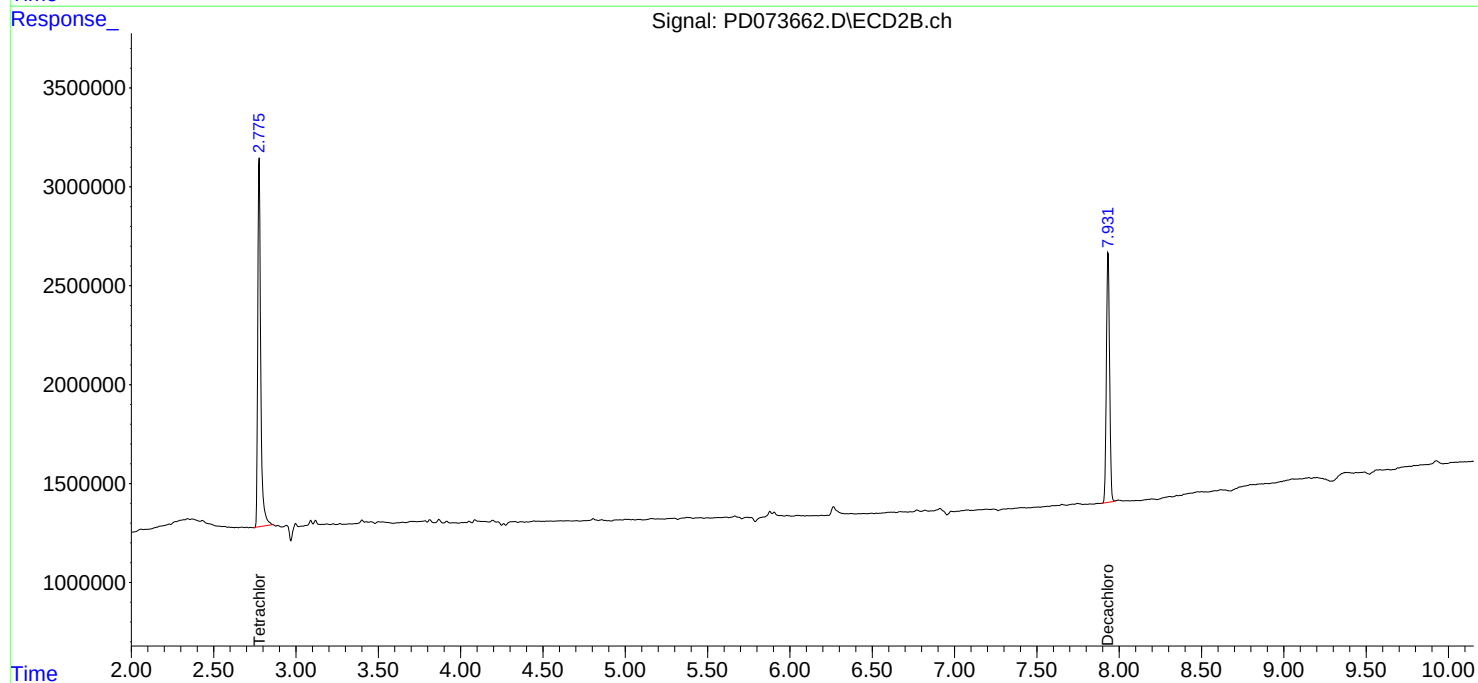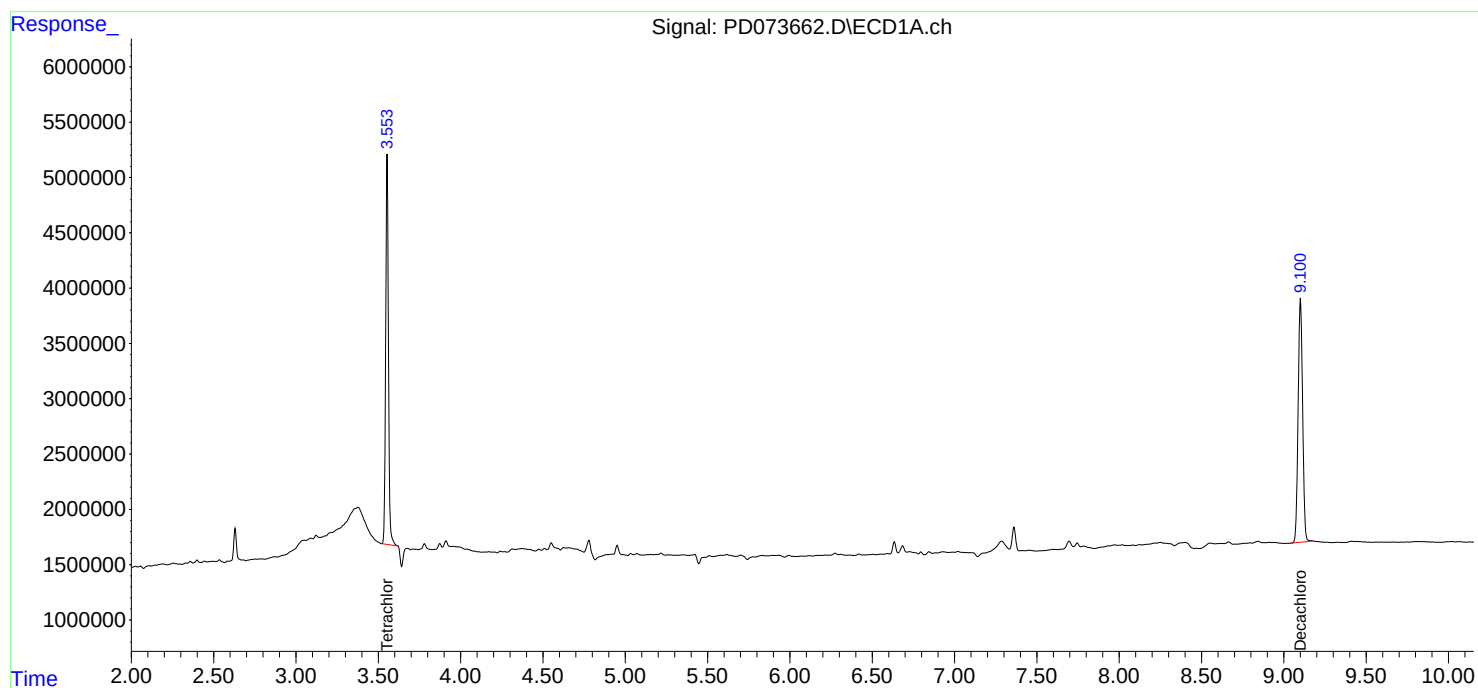


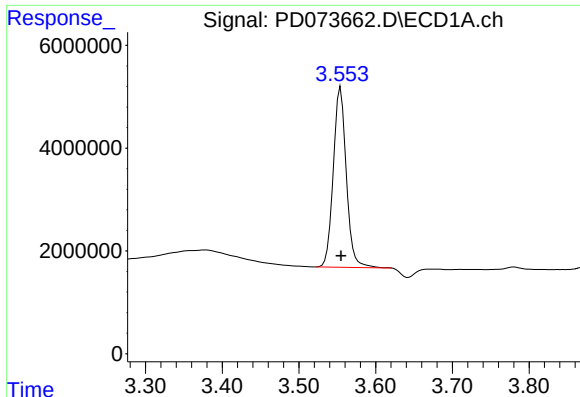

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 41219666
Conc: 17.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
TJRC-011823-B3-30-40

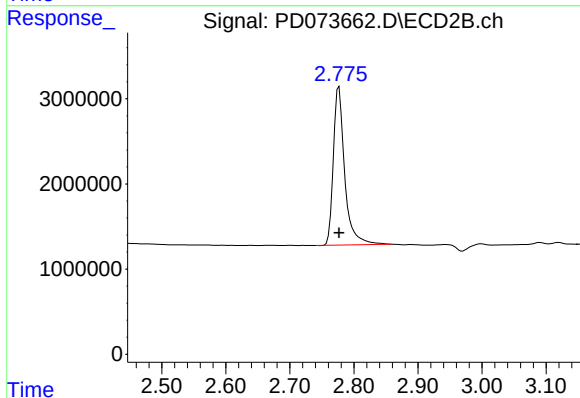


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 22958007
Conc: 18.03 ng/ml

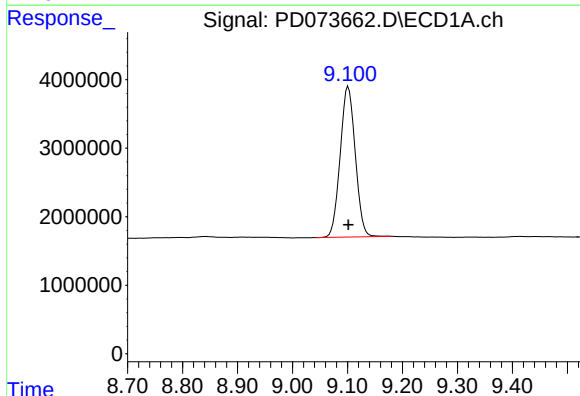

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: 0.000 min
Response: 41918588
Conc: 14.88 ng/ml

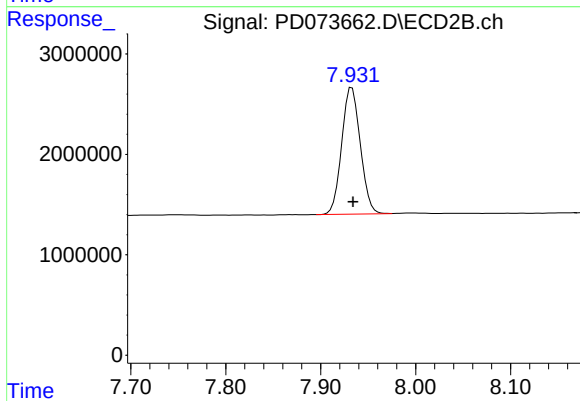

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: -0.001 min
Response: 17177744
Conc: 14.76 ng/ml