

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012020\
 Data File : PD057009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 13:34
 Operator : AJ\MA
 Sample : L1161-07
 Misc : TOX LOD 50 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 05:34:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 06:13:56 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.285	3.960	19664352	38918250	23.940	23.926
7) SA Decachlor...	7.956	8.995	23738927	40598429	24.368	24.491
Target Compounds						
2) Toxaphene-1	5.696	6.523	430095	952027	42.707	59.241 #
3) Toxaphene-2	6.068	6.822	825663	809610	53.749	39.830 #
4) Toxaphene-3	6.317	7.104	548846	2284119	36.377	51.687 #
5) Toxaphene-4	6.455	7.191	253717	1192992	38.141	44.100
6) Toxaphene-5	6.737	7.602	445639	1351131	67.084	49.674 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012020\
Data File : PD057009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 13:34
Operator : AJ\MA
Sample : L1161-07
Misc : TOX LOD 50 PPB
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 05:34:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 06:13:56 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

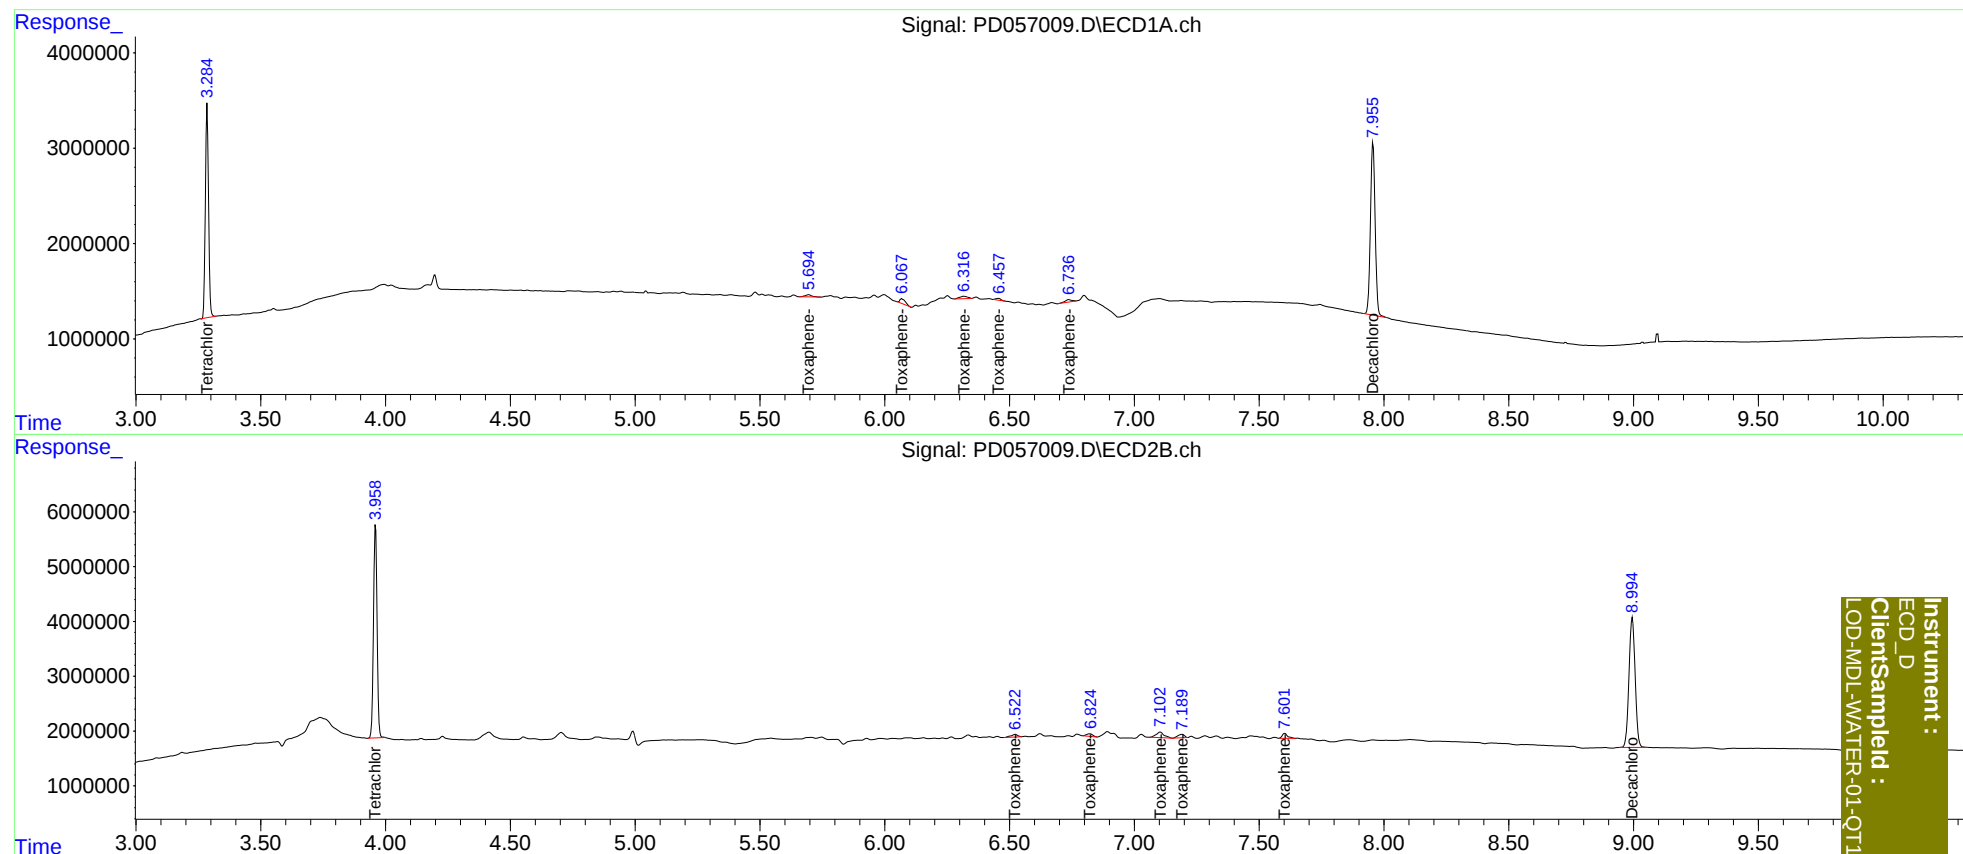

Instrument :
ECD_D
ClientSample :
LOD-MDL-WATER-01-QT1-2020