

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012020\
 Data File : PD057003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 12:10
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:10:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	44054255	79833602	53.344	48.787
28)	SA Decachlor...	7.956	8.995	46240997	76942887	47.711	46.163
Target Compounds							
23)	Chlordane-1	4.125	4.947	13643659	31490332	493.367	487.333
24)	Chlordane-2	4.615	5.412	16204346	33094955	462.229	482.464
25)	Chlordane-3	5.169	6.055	47707808	137.5E6	487.188	487.210
26)	Chlordane-4	5.225	6.130	41384308	164.2E6	475.887	486.242
27)	Chlordane-5	6.048	6.930	16475924	28737944	476.198	514.766



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012020\
Data File : PD057003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 12:10
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:10:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

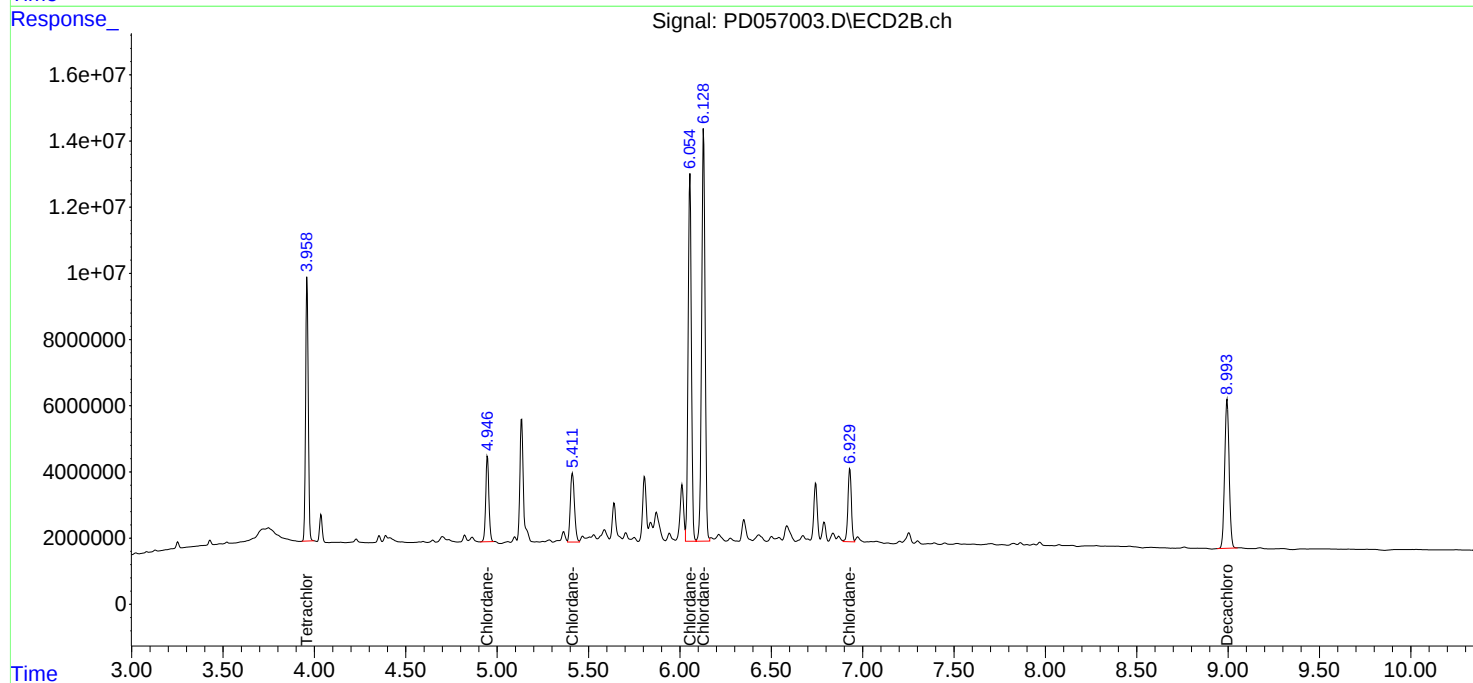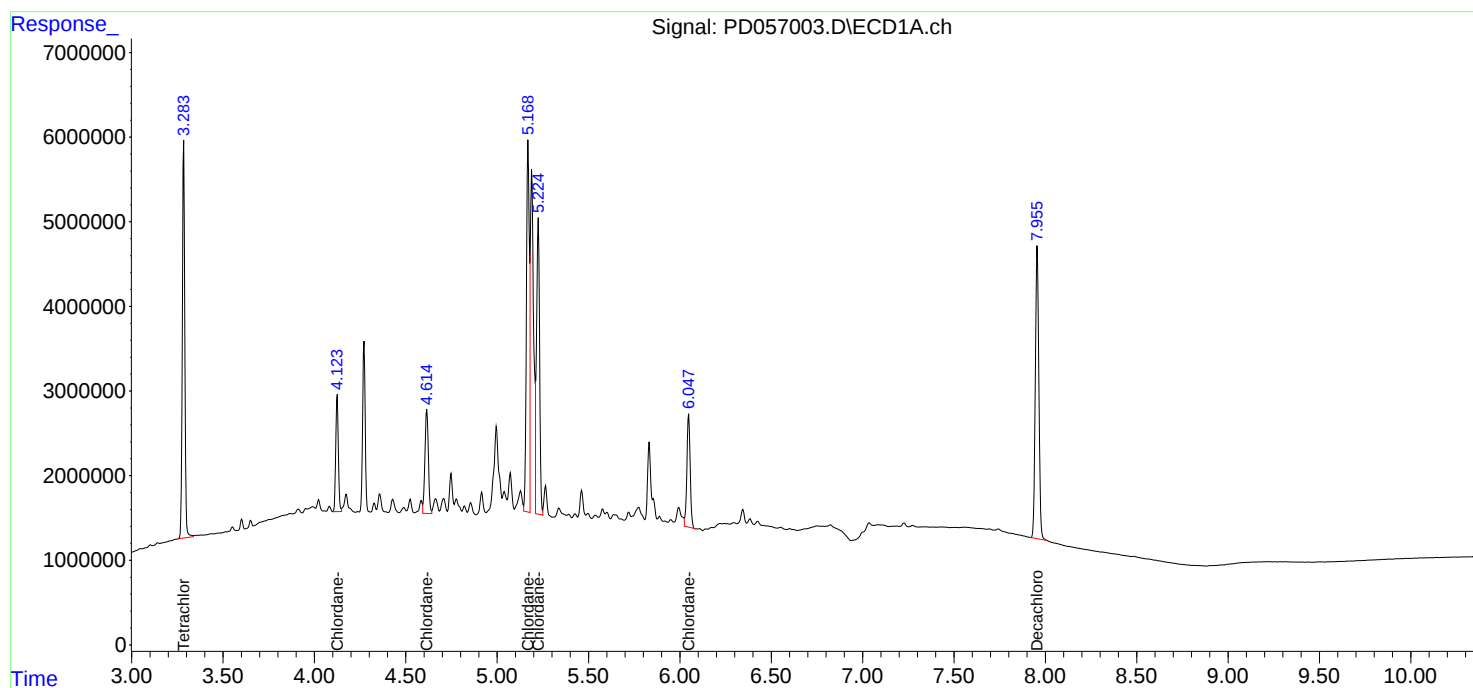


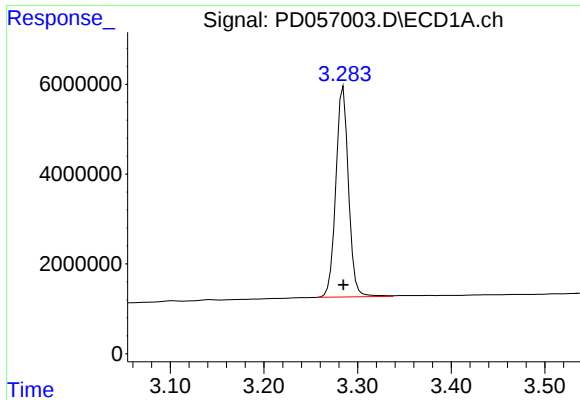

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 44054255
Conc: 53.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

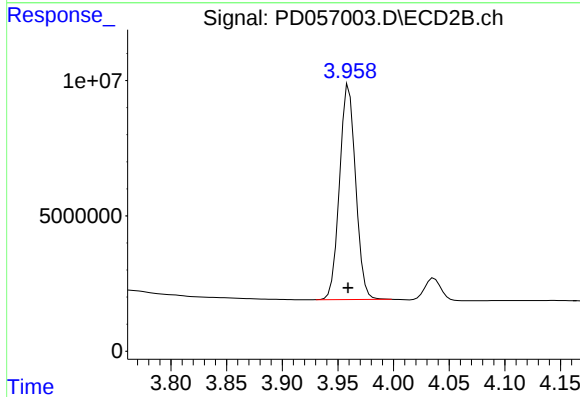


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 79833602
Conc: 48.79 ng/ml

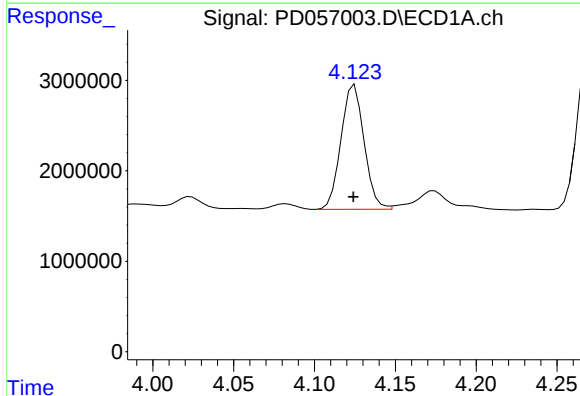


#23 Chlordane-1

R.T.: 4.125 min
Delta R.T.: 0.000 min
Response: 13643659
Conc: 493.37 ng/ml

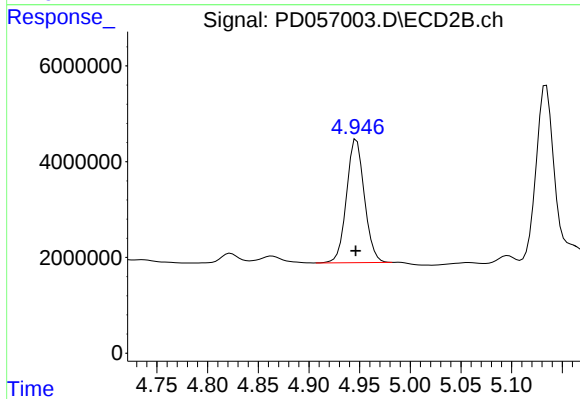

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 31490332
Conc: 487.33 ng/ml

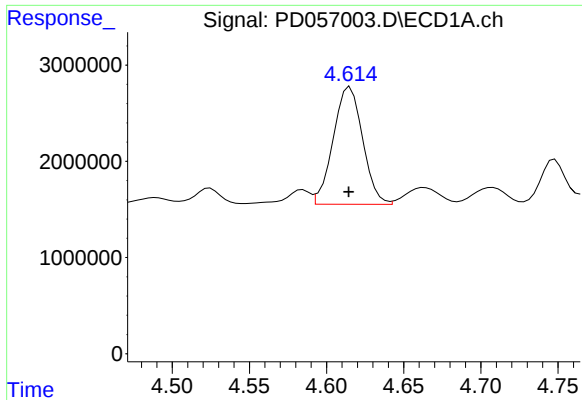

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: 0.000 min
Response: 16204346
Conc: 462.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

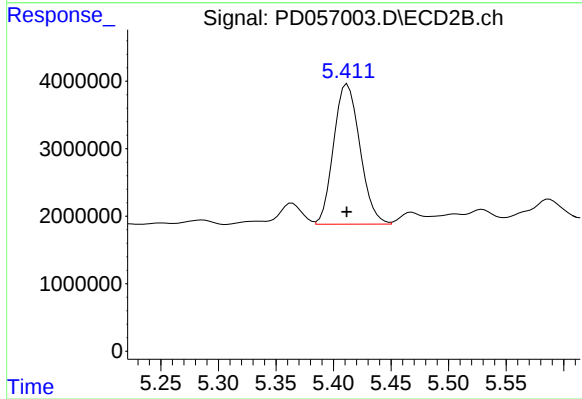


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 33094955
Conc: 482.46 ng/ml

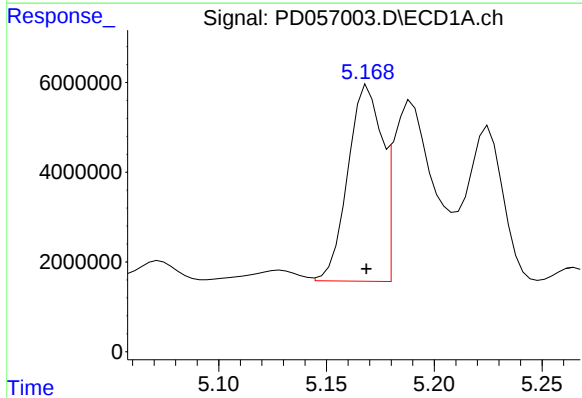


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 47707808
Conc: 487.19 ng/ml

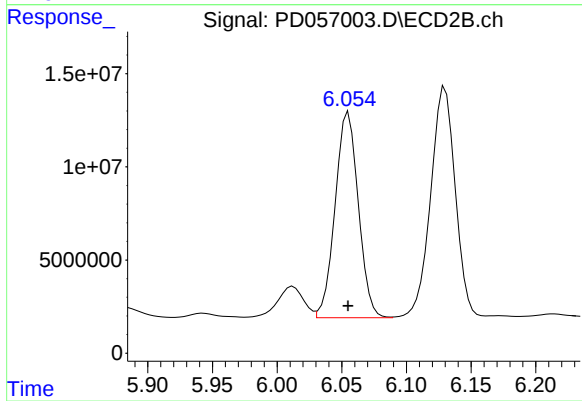

#25 Chlordane-3


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 137467005
Conc: 487.21 ng/ml

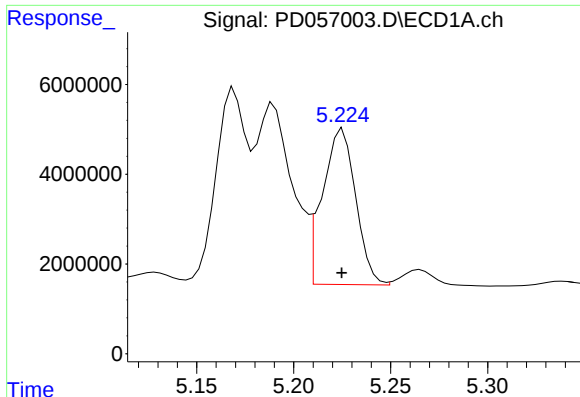

#26 Chlordane-4


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 41384308
Conc: 475.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

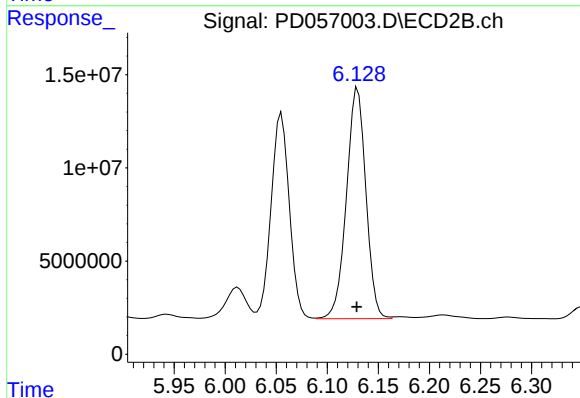


#26 Chlordane-4

R.T.: 6.130 min
Delta R.T.: 0.001 min
Response: 164194621
Conc: 486.24 ng/ml

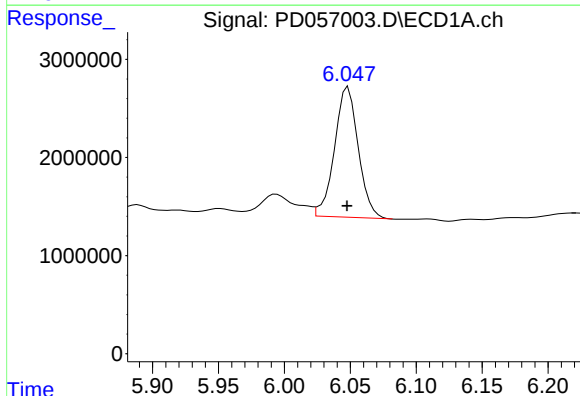


#27 Chlordane-5

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 16475924
Conc: 476.20 ng/ml

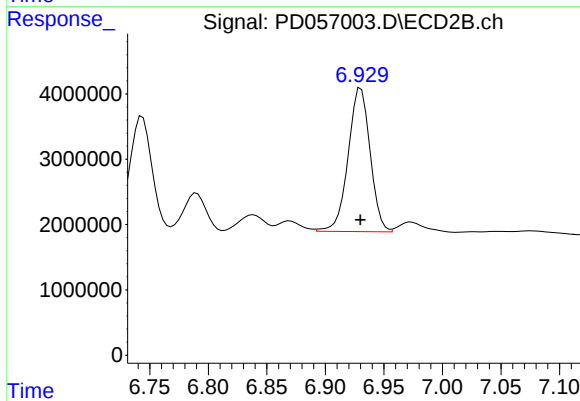

#27 Chlordane-5


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 28737944
Conc: 514.77 ng/ml

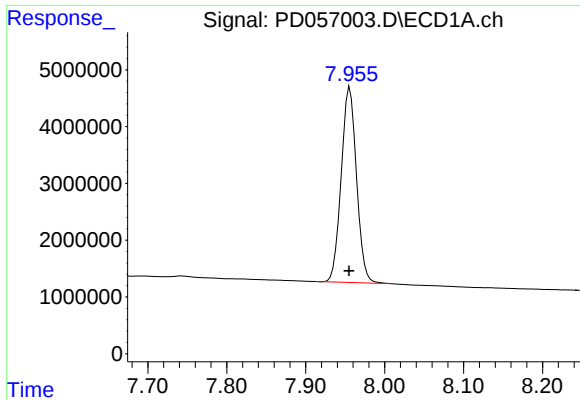

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 46240997
Conc: 47.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

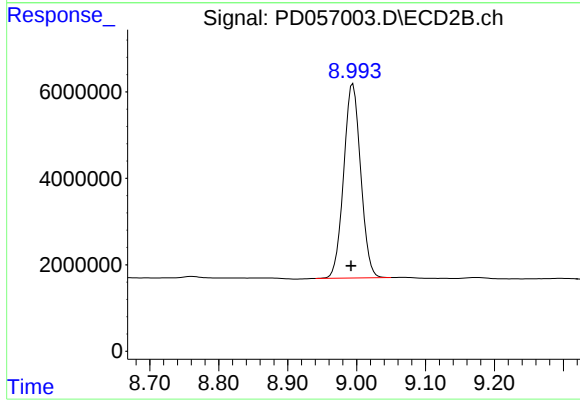

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.002 min
Response: 76942887
Conc: 46.16 ng/ml