

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012020\
 Data File : PD057012.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 14:16
 Operator : AJ\MA
 Sample : L1161-08
 Misc : CHLOR LOQ 50 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOQ-WATER-02-QT1-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:11:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	14813300	28536257	17.937	17.439
28)	SA Decachlor...	7.956	8.995	17915089	30779235	18.485	18.467
Target Compounds							
23)	Chlordane-1	4.124	4.947	1533148	3422310	55.440	52.962
24)	Chlordane-2	4.615	5.412	1977331	3949631	56.403	57.578
25)	Chlordane-3	5.169	6.056	5007187	12762676	51.133	45.233
26)	Chlordane-4	5.225	6.129	4544003	15617855	52.252	46.250
27)	Chlordane-5	6.048	6.930	1604621	2623376	46.378	46.991



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012020\
Data File : PD057012.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 14:16
Operator : AJ\MA
Sample : L1161-08
Misc : CHLOR LOQ 50 PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT1-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:11:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

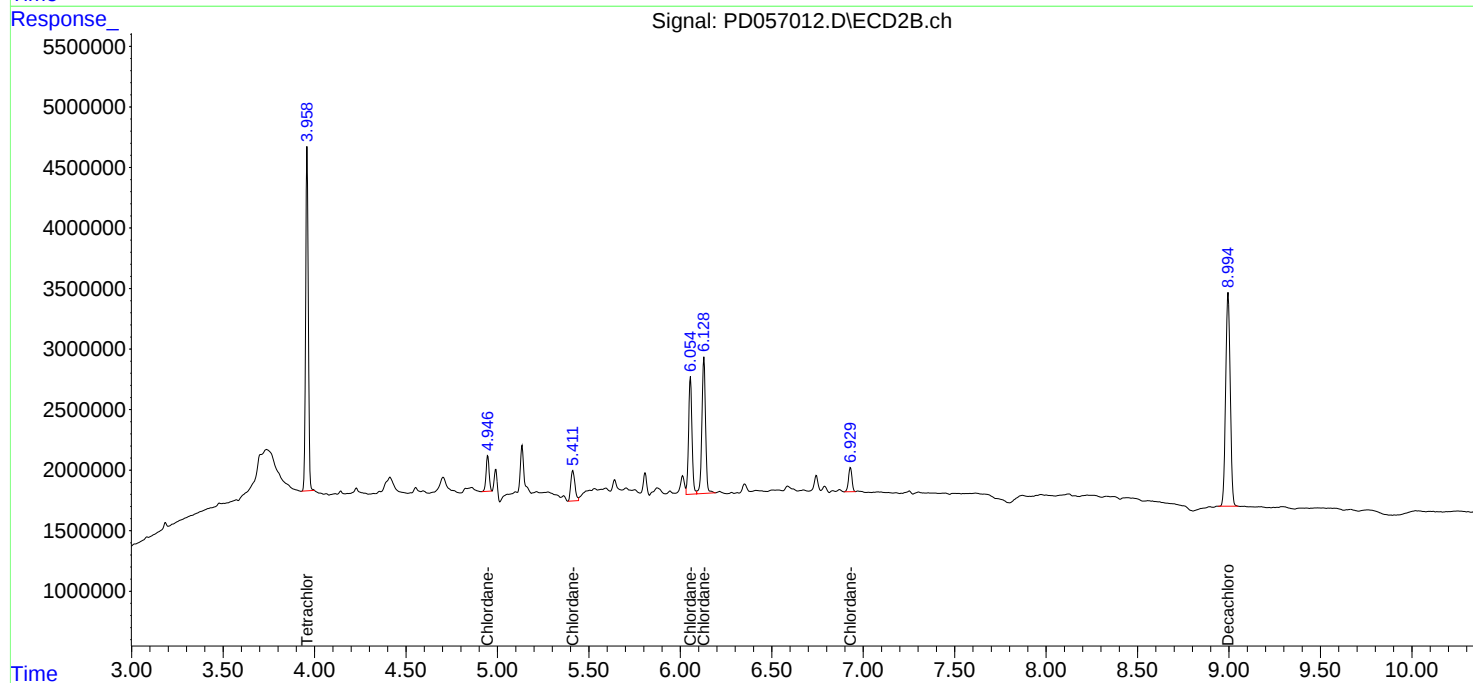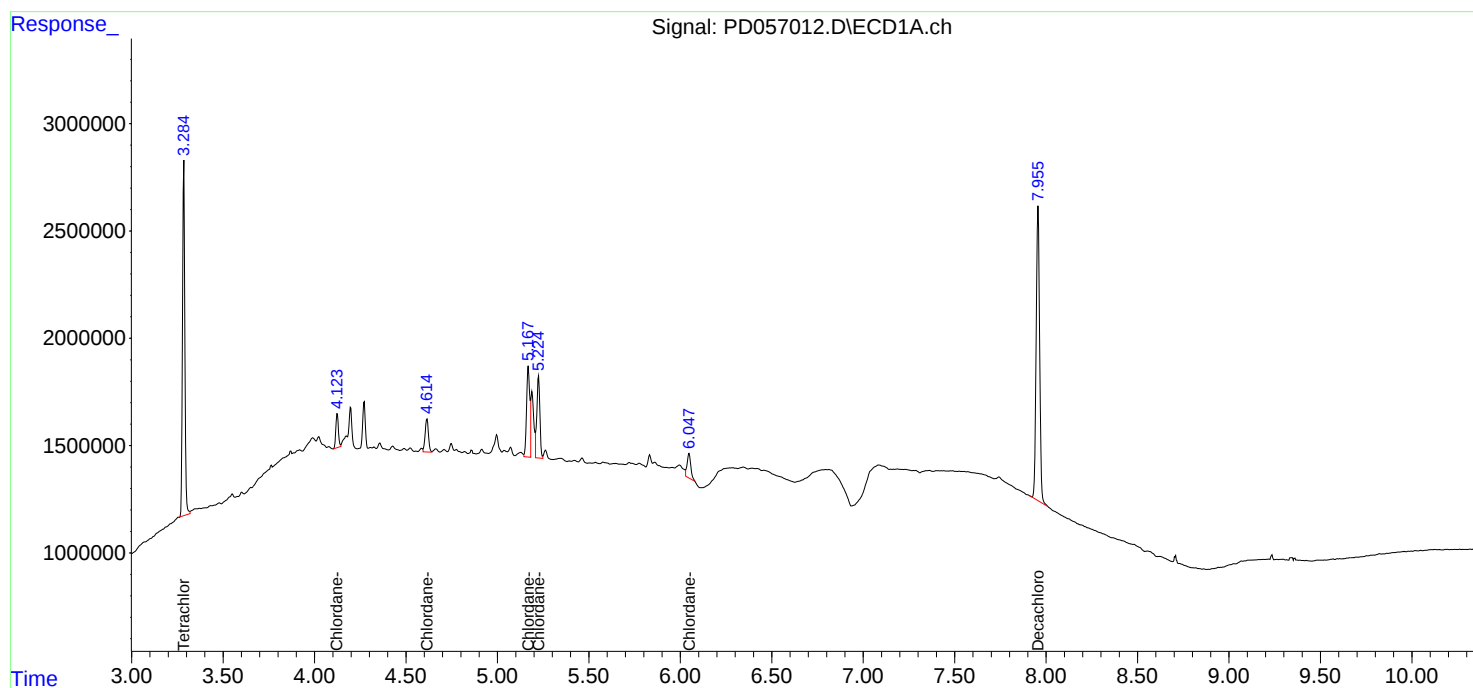


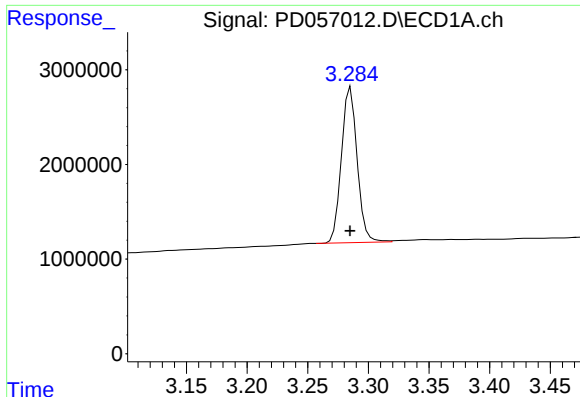

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 14813300
Conc: 17.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT1-2020

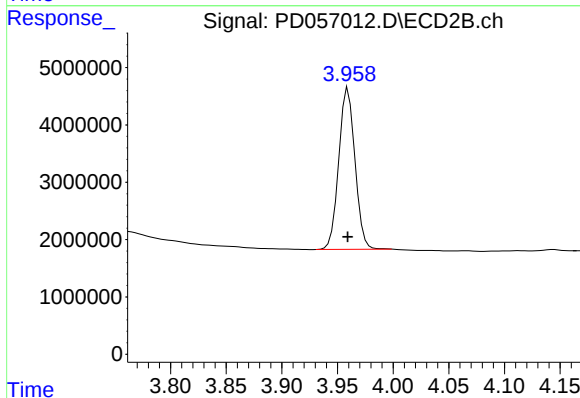


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 28536257
Conc: 17.44 ng/ml

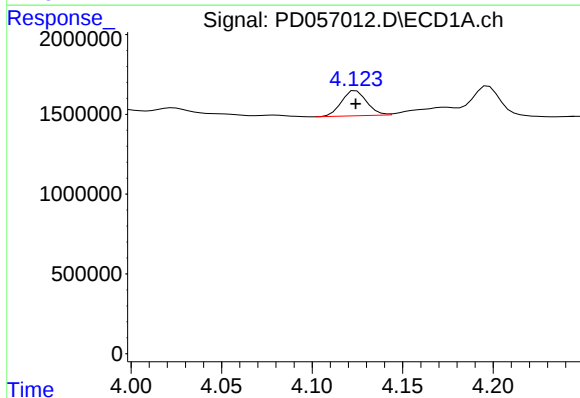


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 1533148
Conc: 55.44 ng/ml

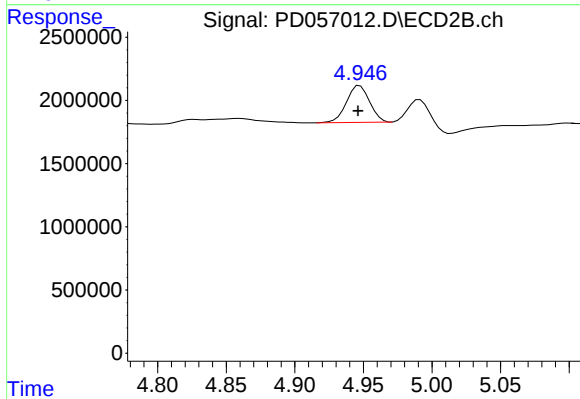

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.001 min
Response: 3422310
Conc: 52.96 ng/ml

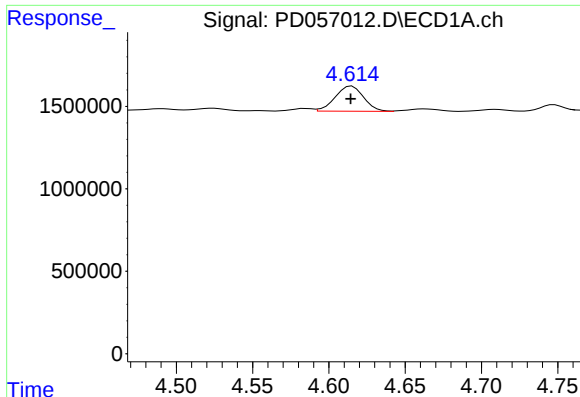

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: 0.000 min
Response: 1977331
Conc: 56.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT1-2020

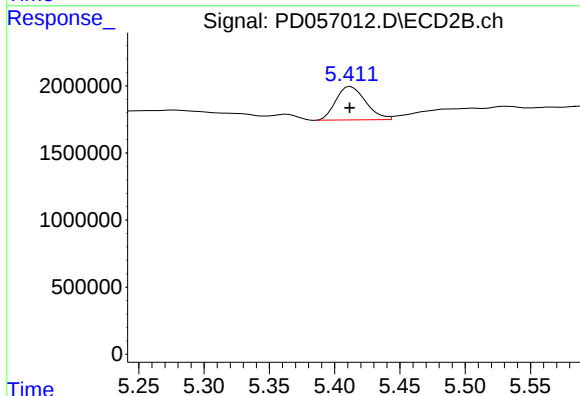


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 3949631
Conc: 57.58 ng/ml

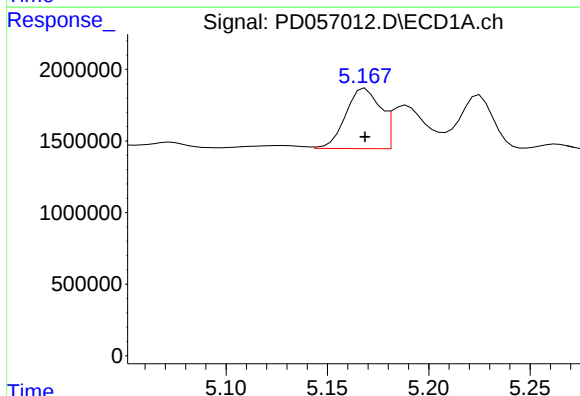


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 5007187
Conc: 51.13 ng/ml

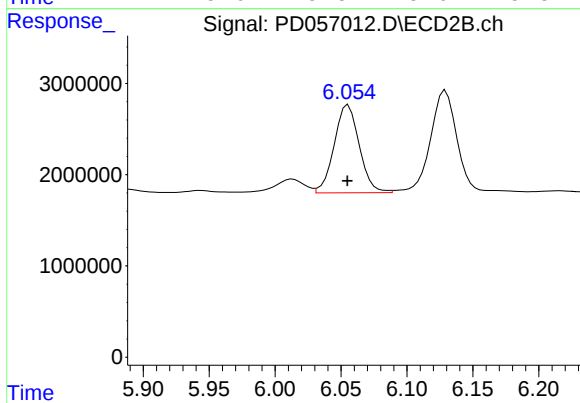

#25 Chlordane-3


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 12762676
Conc: 45.23 ng/ml

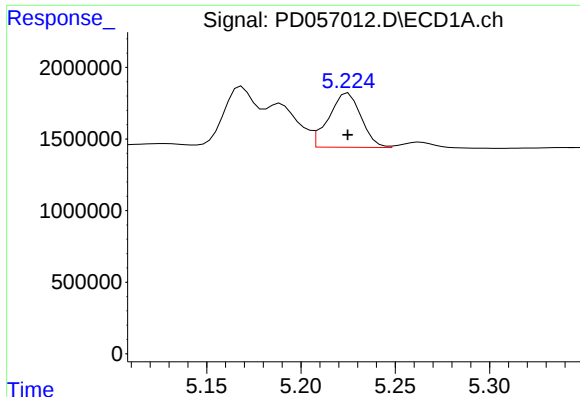

#26 Chlordane-4


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 4544003
Conc: 52.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT1-2020

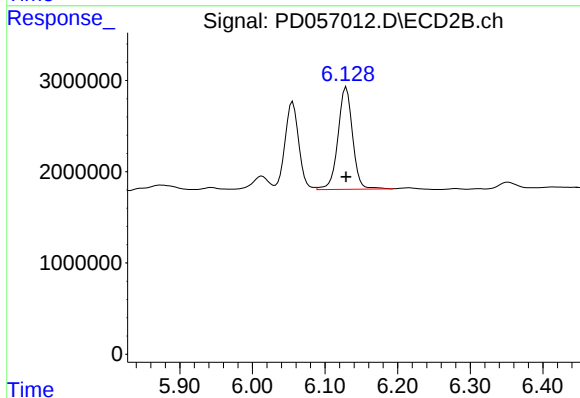


#26 Chlordane-4

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 15617855
Conc: 46.25 ng/ml

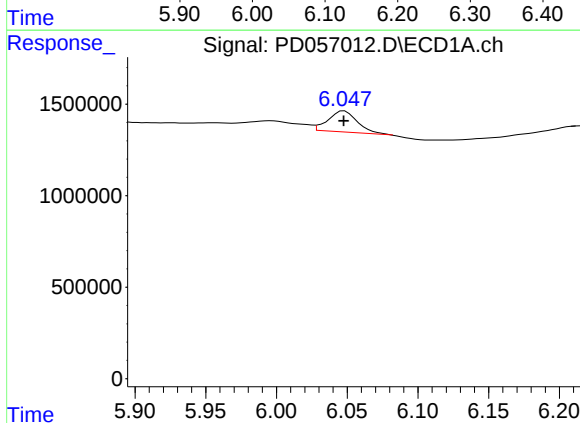


#27 Chlordane-5

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 1604621
Conc: 46.38 ng/ml

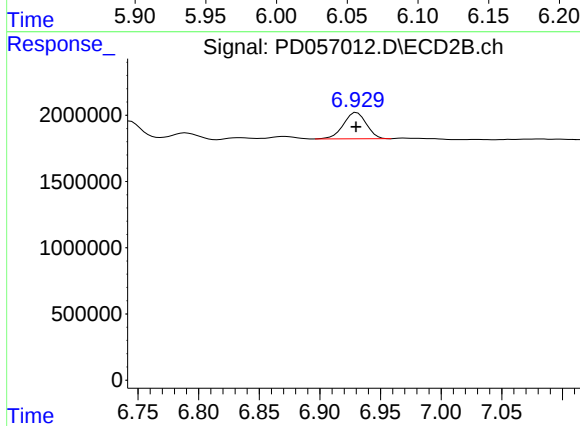

#27 Chlordane-5


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 2623376
Conc: 46.99 ng/ml

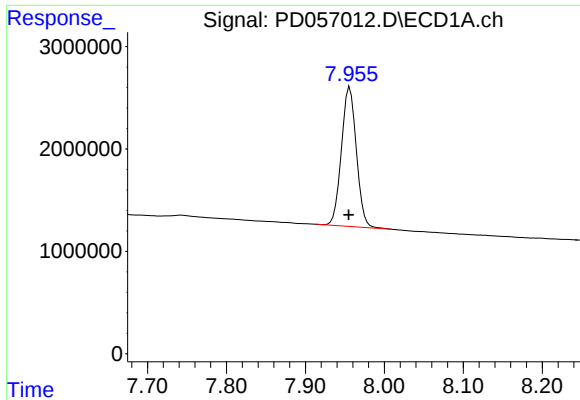

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.001 min
Response: 17915089
Conc: 18.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT1-2020

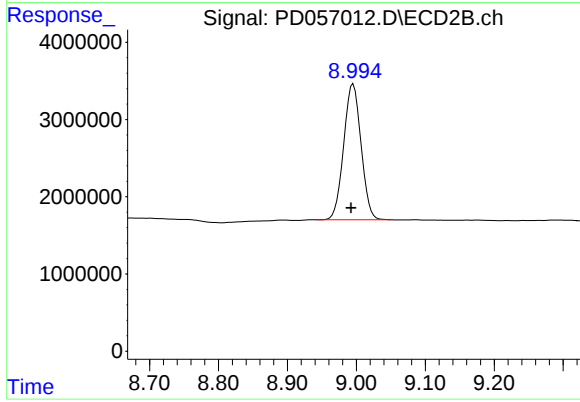

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.003 min
Response: 30779235
Conc: 18.47 ng/ml