

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012020\
 Data File : PD057014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2020 14:45
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:11:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	43189445	78302823	52.297	47.852
28)	SA Decachlor...	7.956	8.995	45300911	76001240	46.741	45.598
Target Compounds							
23)	Chlordane-1	4.124	4.947	13413439	30756305	485.042	475.973
24)	Chlordane-2	4.615	5.412	16064300	32357862	458.234	471.718
25)	Chlordane-3	5.169	6.056	45936335	134.7E6	469.098	477.511
26)	Chlordane-4	5.225	6.130	41478582	161.2E6	476.971	477.398
27)	Chlordane-5	6.049	6.930	15885448	27777787	459.132	497.567



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012020\
Data File : PD057014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2020 14:45
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:11:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

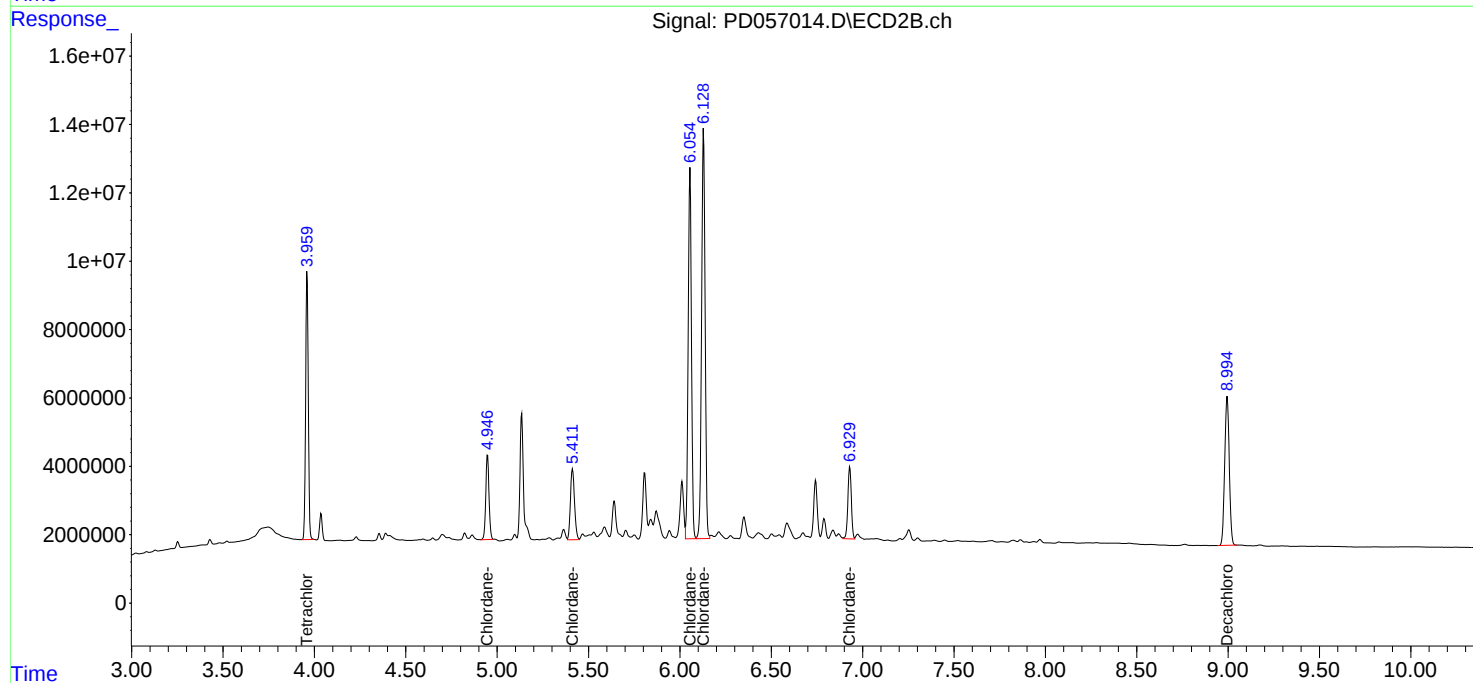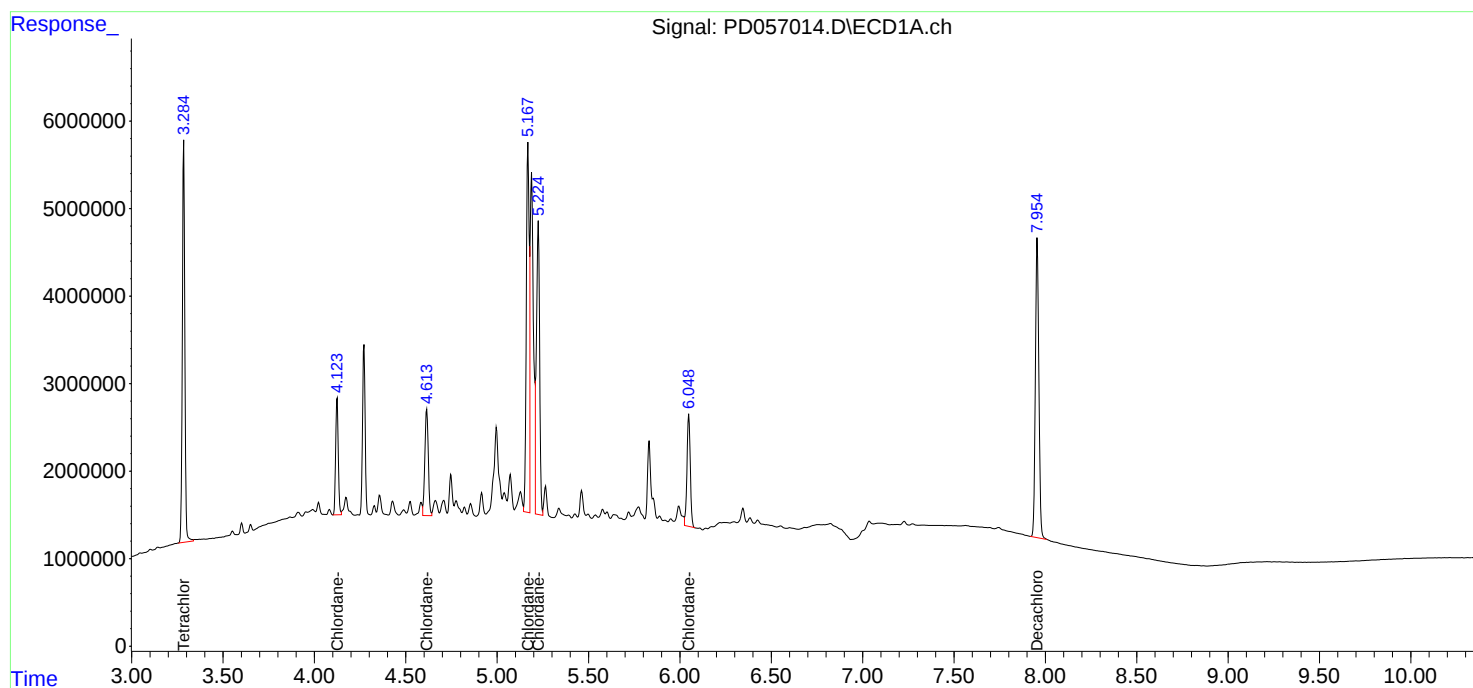


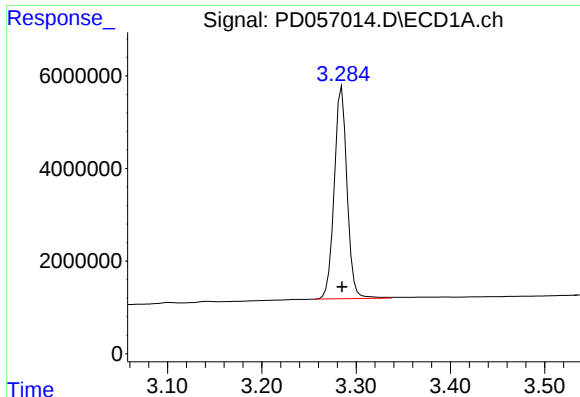

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 43189445
Conc: 52.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

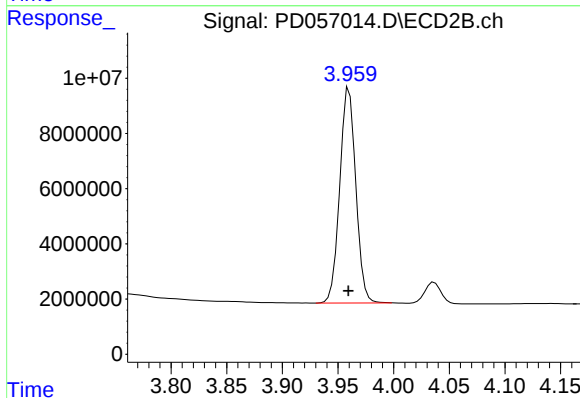


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 78302823
Conc: 47.85 ng/ml

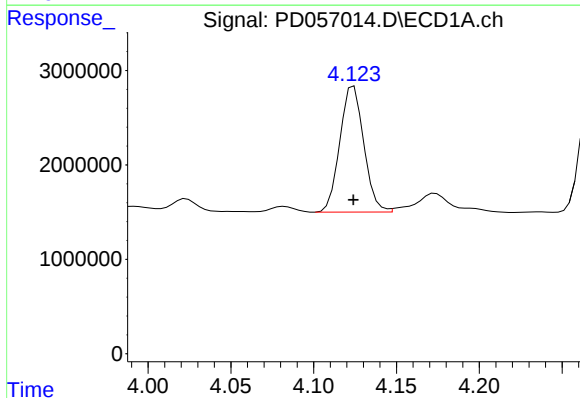


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 13413439
Conc: 485.04 ng/ml

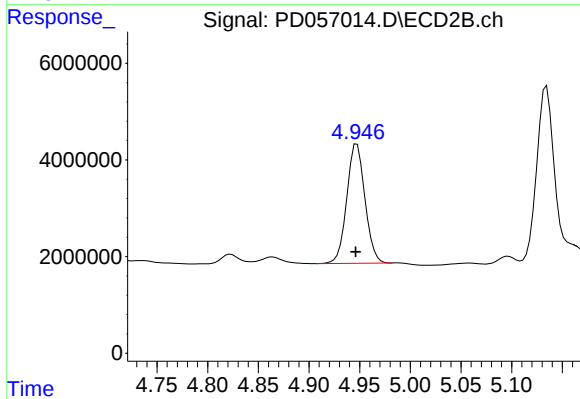

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.001 min
Response: 30756305
Conc: 475.97 ng/ml

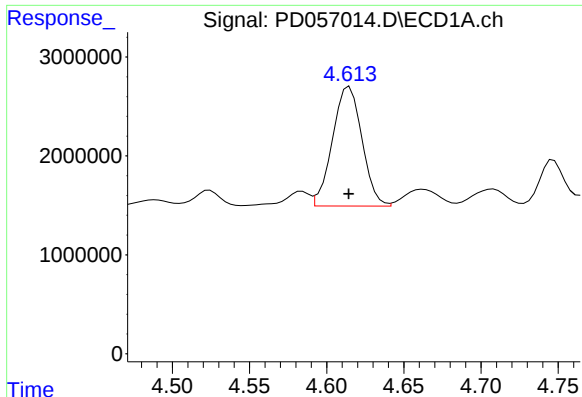

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: 0.000 min
Response: 16064300
Conc: 458.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

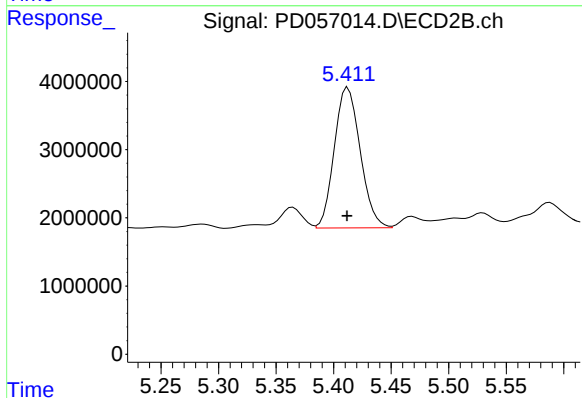


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 32357862
Conc: 471.72 ng/ml

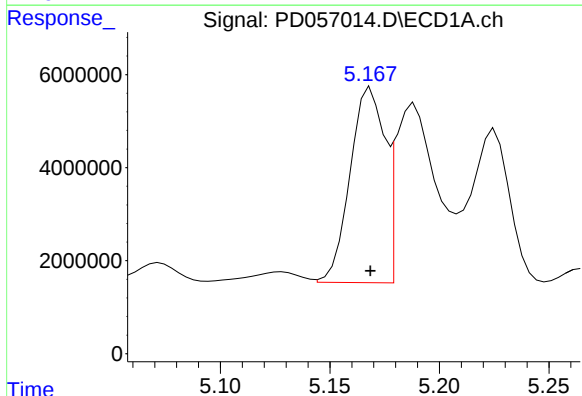


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 45936335
Conc: 469.10 ng/ml

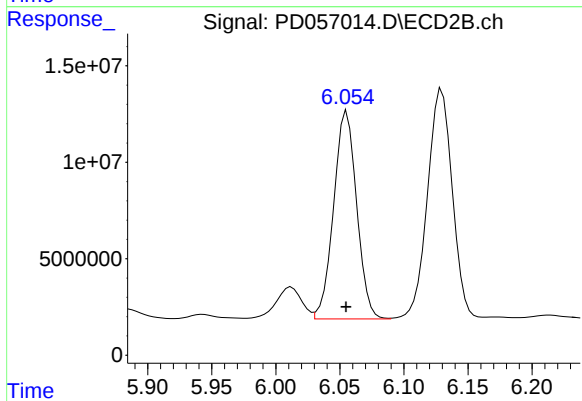

#25 Chlordane-3


R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 134730404
Conc: 477.51 ng/ml

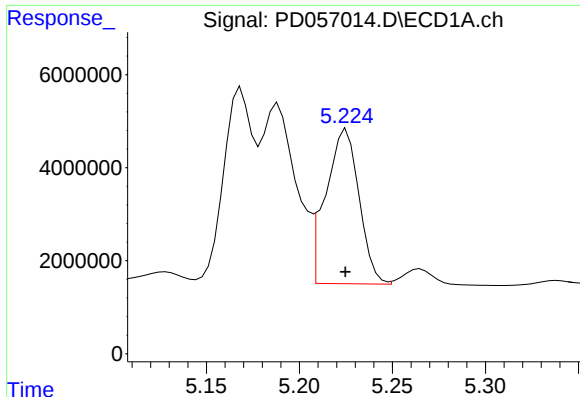

#26 Chlordane-4


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 41478582
Conc: 476.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

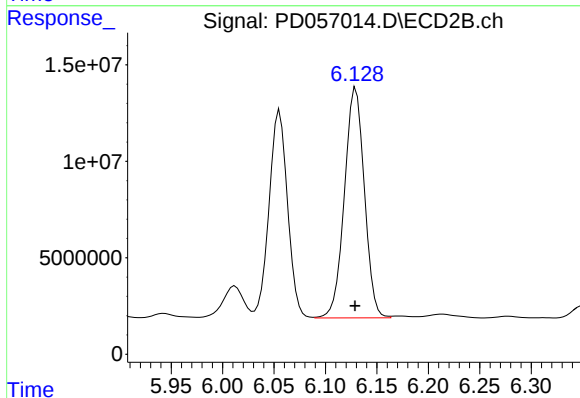


#26 Chlordane-4

R.T.: 6.130 min
Delta R.T.: 0.000 min
Response: 161208000
Conc: 477.40 ng/ml

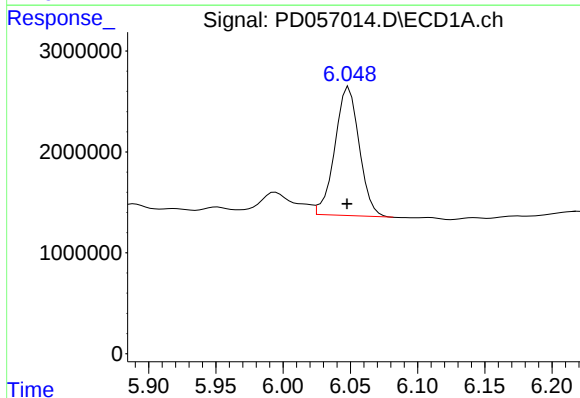


#27 Chlordane-5

R.T.: 6.049 min
Delta R.T.: 0.001 min
Response: 15885448
Conc: 459.13 ng/ml

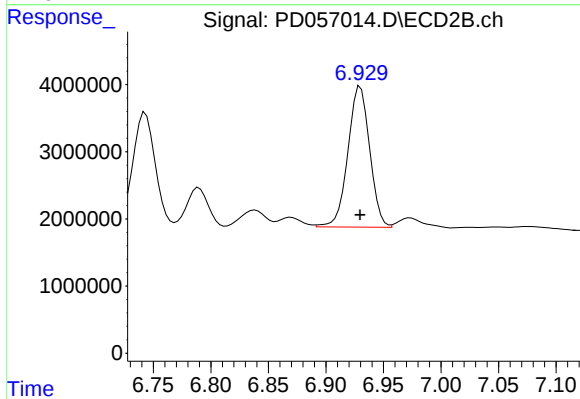

#27 Chlordane-5


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 27777787
Conc: 497.57 ng/ml

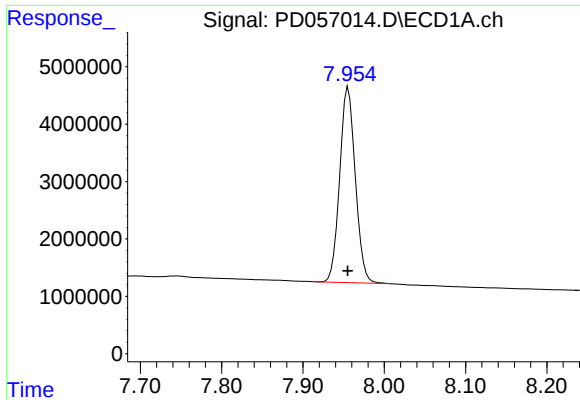

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 45300911
Conc: 46.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

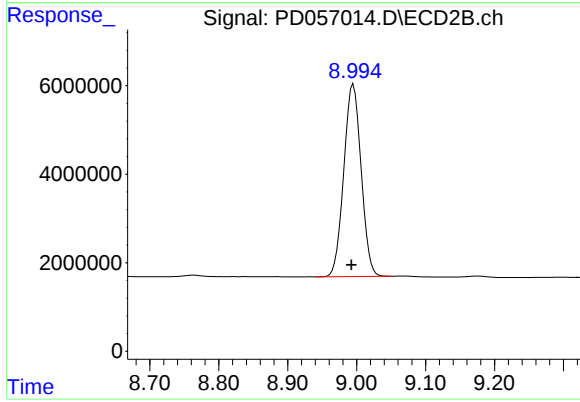

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.003 min
Response: 76001240
Conc: 45.60 ng/ml