

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012021\
 Data File : PD061018.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2021 14:40
 Operator : DD\AJ
 Sample : INDA304
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3005

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:53:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 08 03:28:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.021	22629053	149.0E6	17.048	21.457 #
27)	SA Decachlor...	8.280	9.106	53782881	242.8E6	33.424	39.369
Target Compounds							
2)	A alpha-BHC	3.938	4.411	33346313	227.2E6	17.105	21.318
3)	MA gamma-BHC...	4.223	4.697	31899624	208.9E6	17.059	21.323 #
4)	MA Heptachlor	4.529	5.208	33524093	210.1E6	16.556	21.363 #
9)	A Endosulfan I	5.566	6.260	29026210	170.0E6	16.571	21.815 #
13)	MA Dieldrin	5.811	6.517	65352734	364.8E6	33.877	43.474 #
14)	MA Endrin	6.069	6.736	50253289	265.3E6	31.785	40.854 #
16)	A 4,4'-DDD	6.193	6.855	53134406	284.5E6	37.988	48.785 #
17)	MA 4,4'-DDT	6.436	7.155	52855569	259.8E6	33.934	42.079
20)	A Methoxychlor	6.983	7.612	129.4E6	570.5E6	169.293	200.346

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012021\
Data File : PD061018.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2021 14:40
Operator : DD\AJ
Sample : INDA304
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:53:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD010721CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 08 03:28:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

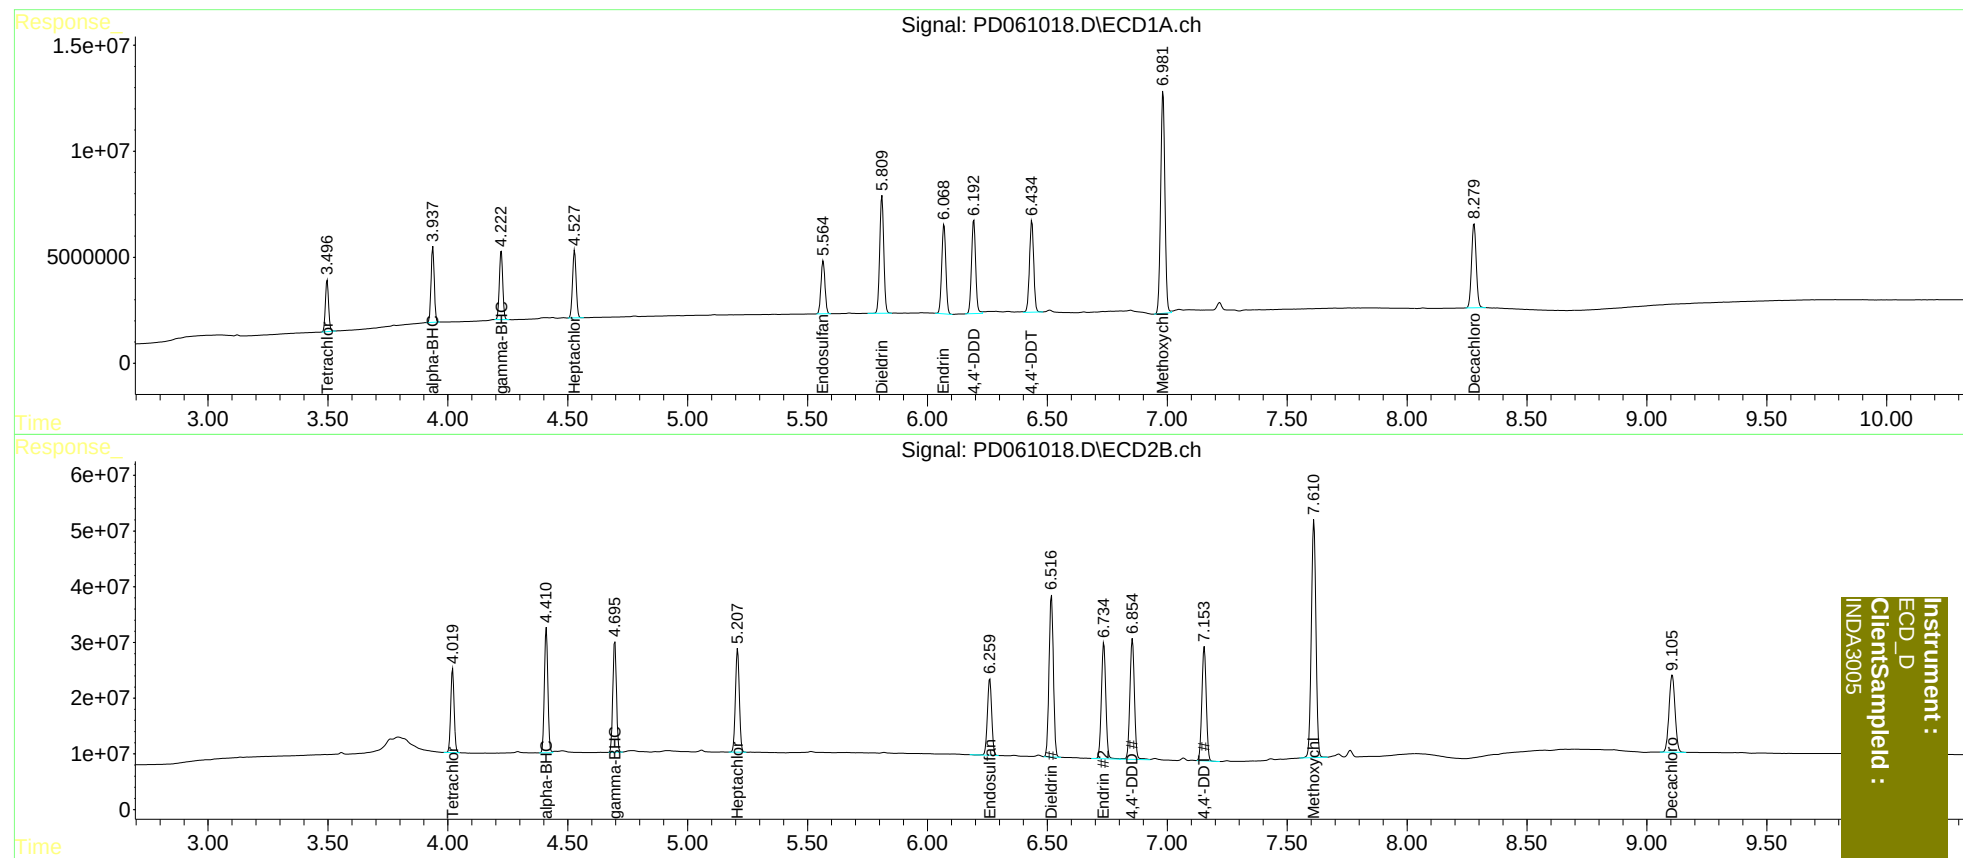

Instrument :
ECD_D
ClientSampled :
INDA3005