

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012023\
 Data File : PD073695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 16:37
 Operator : AR\AJ
 Sample : PB150361BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 21:24:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.777	43694288	23934471	18.693	18.801
28)	SA Decachlor...	9.104	7.935	58767031	23507625	20.854	20.205
Target Compounds							
4)	MA Heptachlor	4.951	0.000	1642293	0	0.442	N.D. #
7)	B delta-BHC	4.782	0.000	5720181	0	1.700	N.D. #
8)	B Heptachlo...	5.703	0.000	936252	0	0.293	N.D. #
9)	A Endosulfan I	6.106	0.000	159180	0	0.052	N.D. #
11)	B alpha-Chl...	6.031	0.000	156788	0	0.048	N.D. #
18)	B Endrin al...	6.947	0.000	303423	0	0.140	N.D. #
21)	B Endrin ke...	7.700f	0.000	1212934	0	0.401	N.D. #
26)	Chlordane-4	6.031f	0.000	156788	0	0.274	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012023\
Data File : PD073695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 16:37
Operator : AR\AJ
Sample : PB150361BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 21:24:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

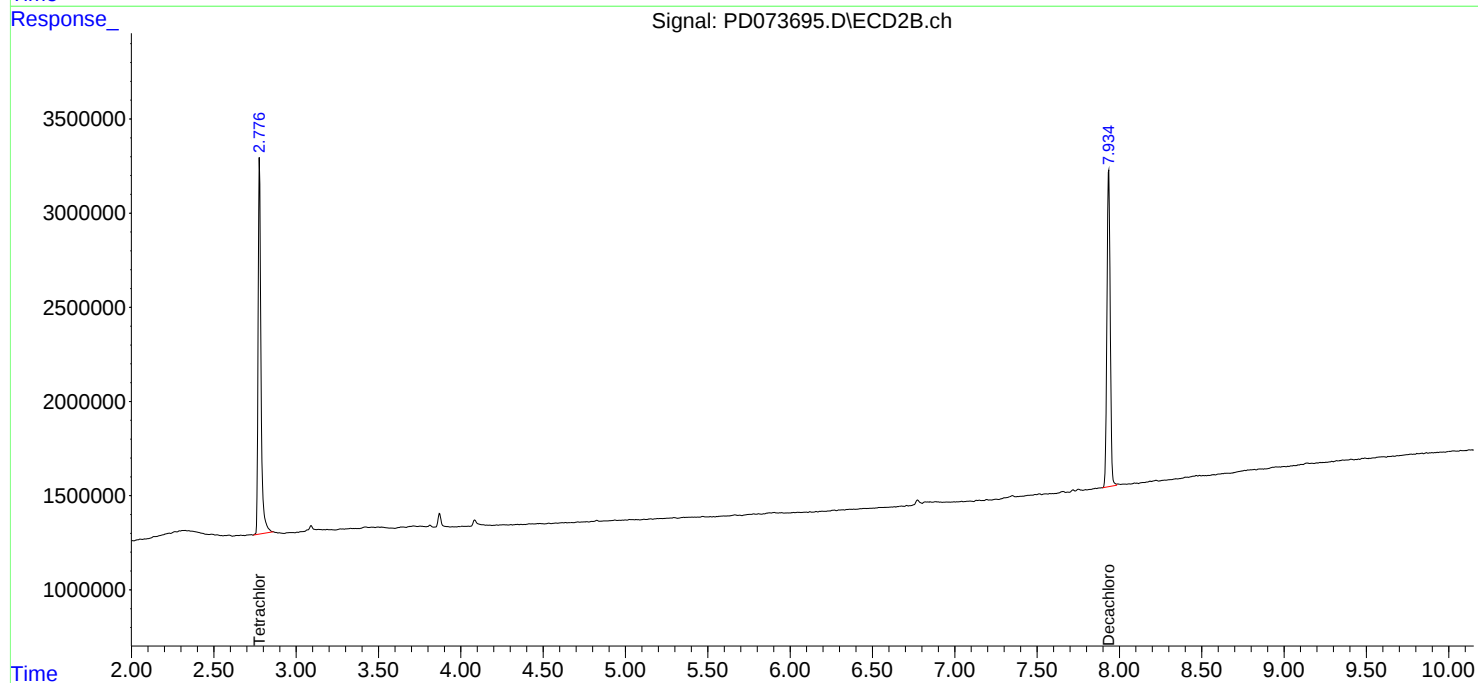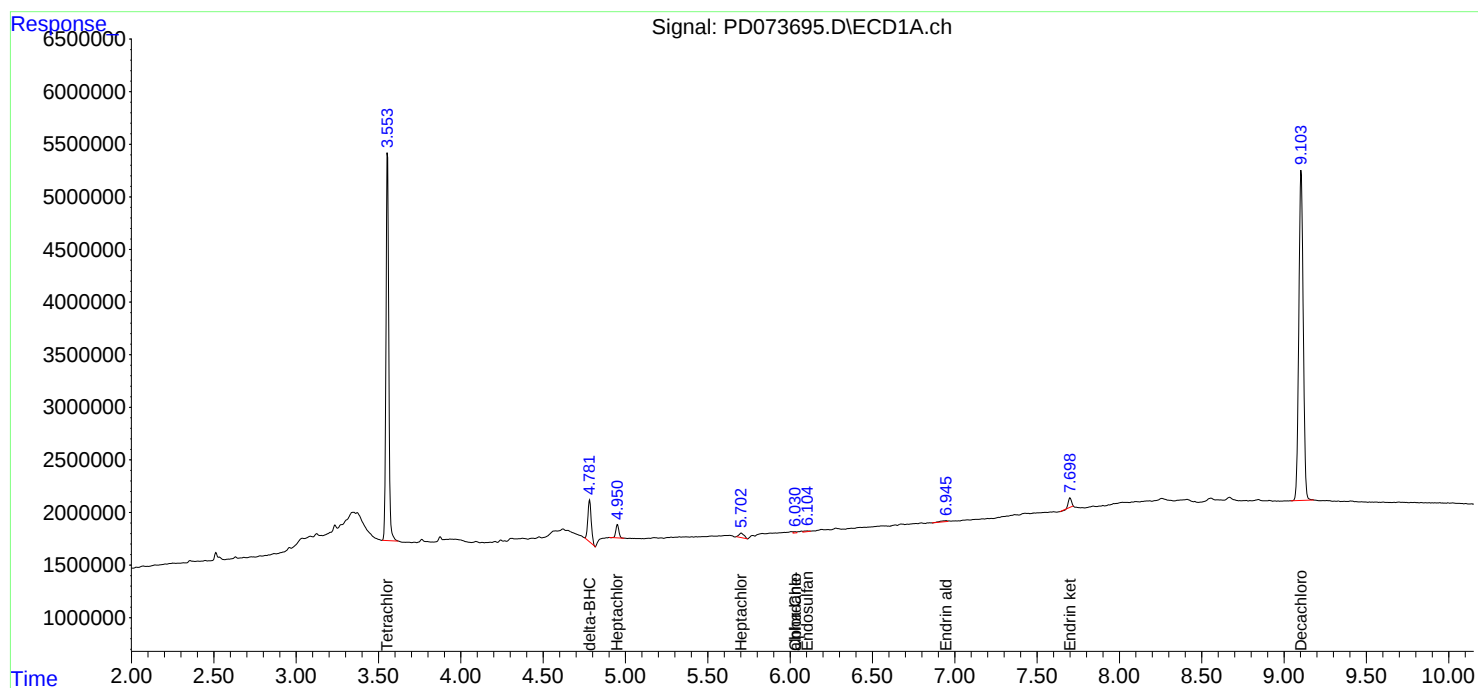


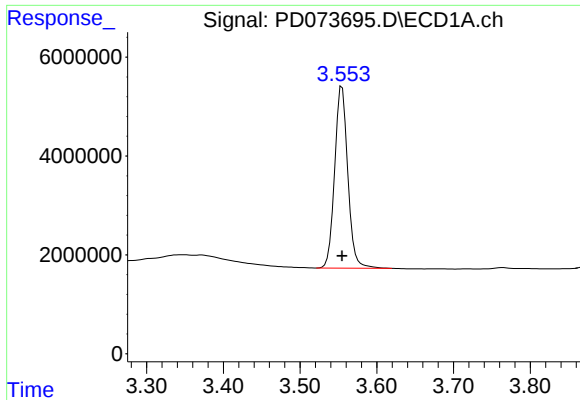

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 43694288
Conc: 18.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

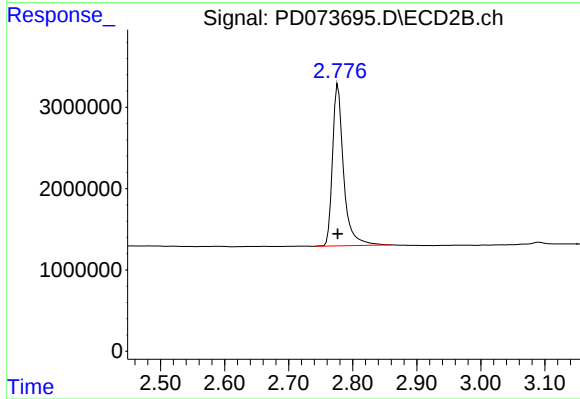


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 23934471
Conc: 18.80 ng/ml

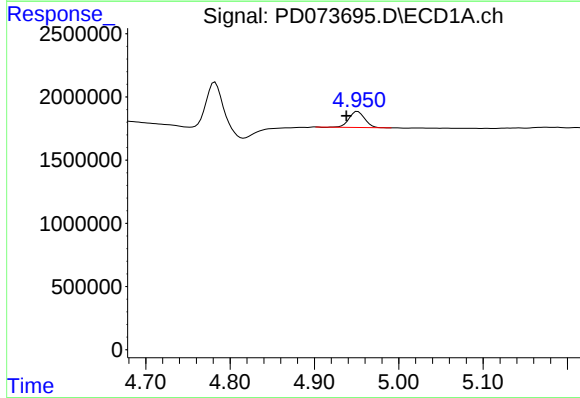


#4 Heptachlor

R.T.: 4.951 min
Delta R.T.: 0.013 min
Response: 1642293
Conc: 0.44 ng/ml

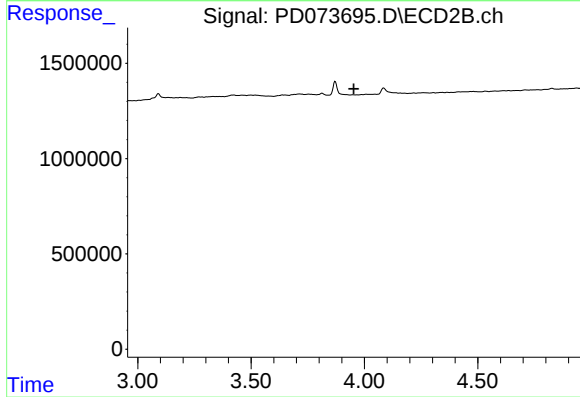

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.953 min
Response: 0
Conc: N.D.

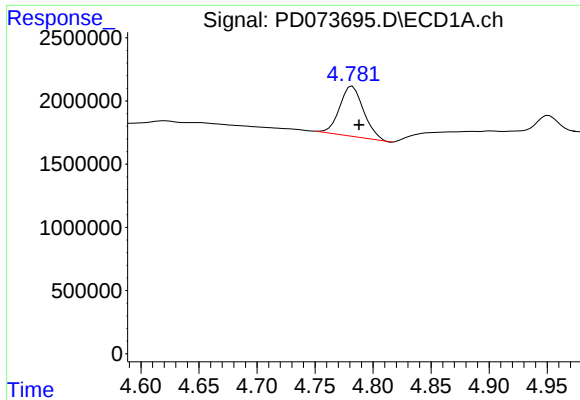

#7 delta-BHC


R.T.: 4.782 min
Delta R.T.: -0.006 min
Response: 5720181
Conc: 1.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

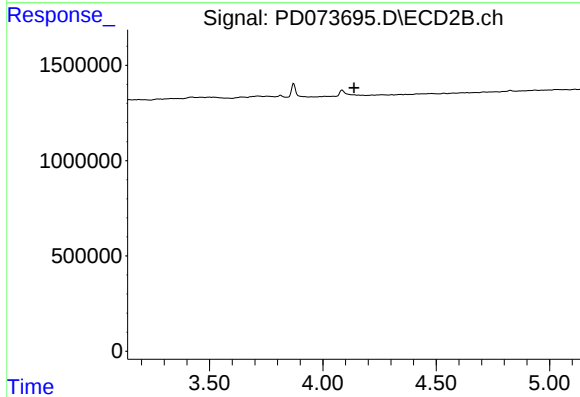


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

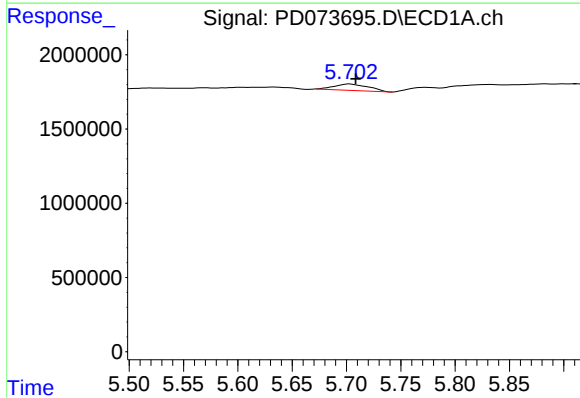


#8 Heptachlor epoxide

R.T.: 5.703 min
Delta R.T.: -0.005 min
Response: 936252
Conc: 0.29 ng/ml

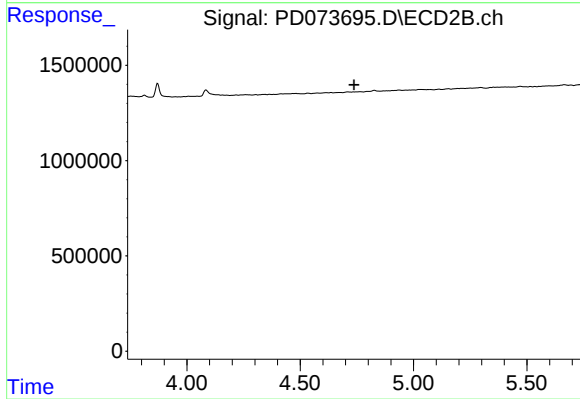

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

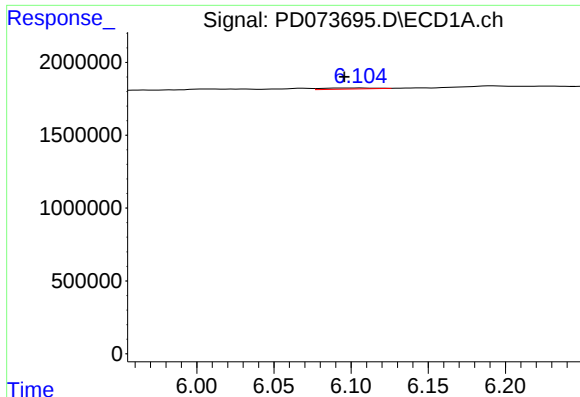

#9 Endosulfan I


R.T.: 6.106 min
Delta R.T.: 0.010 min
Response: 159180
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

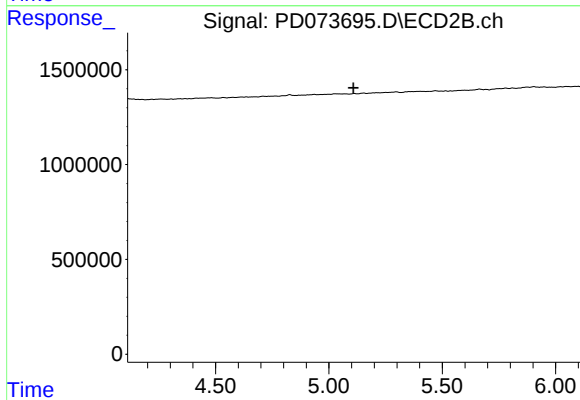


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

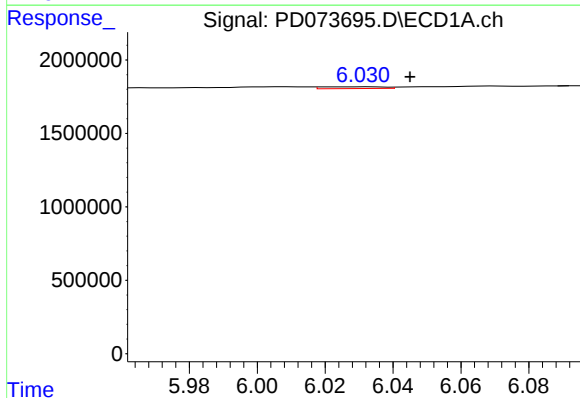


#11 alpha-Chlordane

R.T.: 6.031 min
Delta R.T.: -0.014 min
Response: 156788
Conc: 0.05 ng/ml

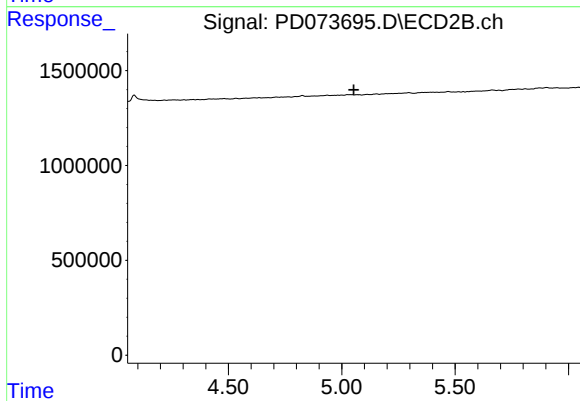

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.054 min
Response: 0
Conc: N.D.

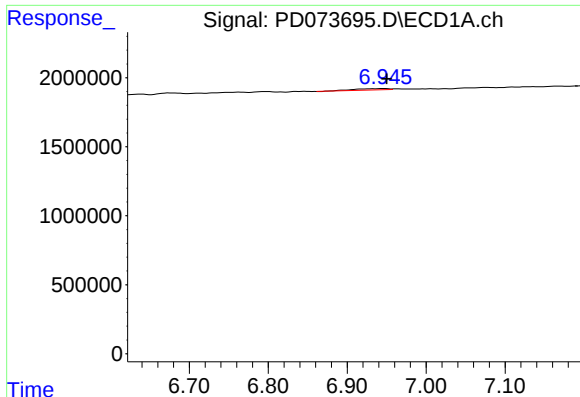

#18 Endrin aldehyde


R.T.: 6.947 min
Delta R.T.: -0.003 min
Response: 303423
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

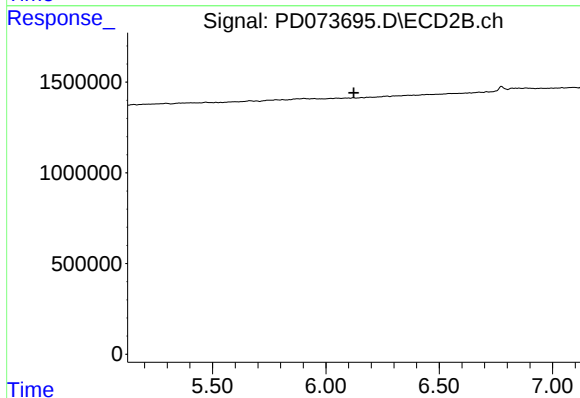


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

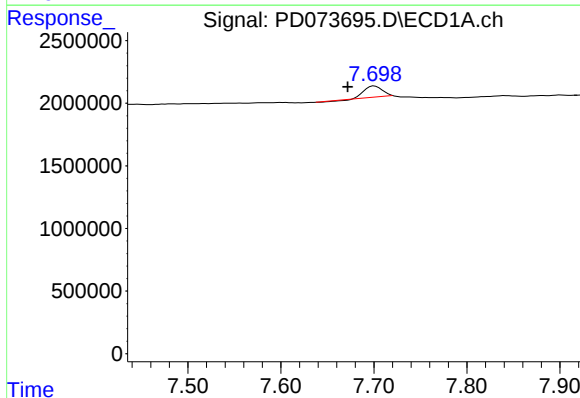


#21 Endrin ketone

R.T.: 7.700 min
Delta R.T.: 0.028 min
Response: 1212934
Conc: 0.40 ng/ml

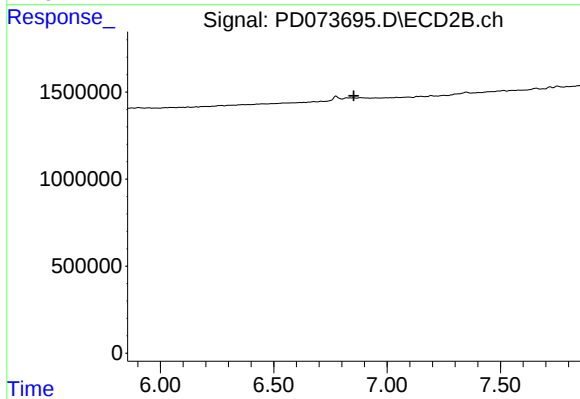

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

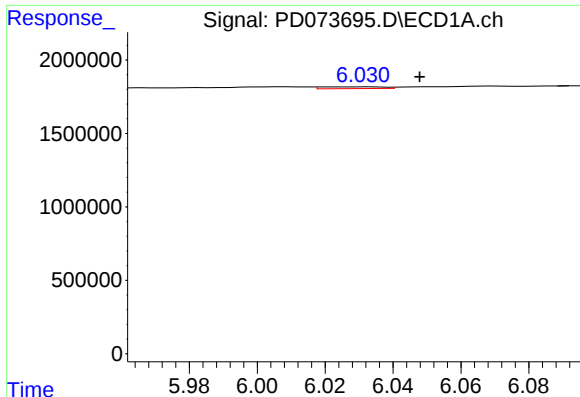

#26 Chlordane-4


R.T.: 6.031 min
Delta R.T.: -0.017 min
Response: 156788
Conc: 0.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

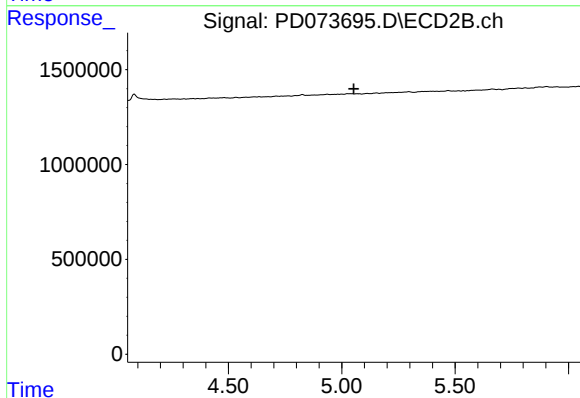


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.053 min
Response: 0
Conc: N.D.

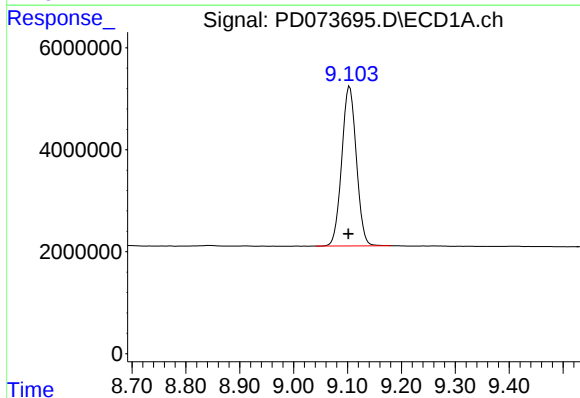

#28 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.002 min
Response: 58767031
Conc: 20.85 ng/ml

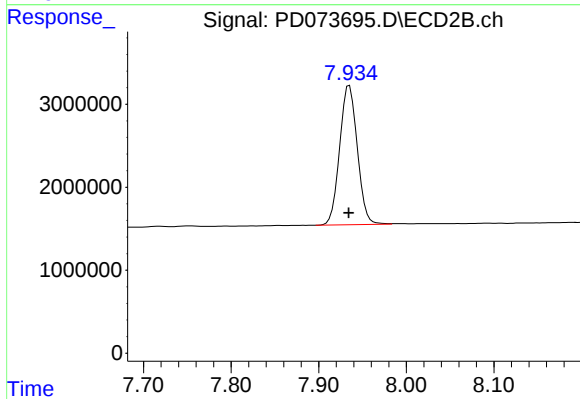

#28 Decachlorobiphenyl

R.T.: 7.935 min
Delta R.T.: 0.000 min
Response: 23507625
Conc: 20.20 ng/ml