

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012023\
 Data File : PD073678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 12:49
 Operator : AR\AJ
 Sample : 01203-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 21:14:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.776	39778465	20114636	17.018	15.800
28)	SA Decachlor...	9.104	7.936	71949776	19275574	25.532	16.567 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012023\
Data File : PD073678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 12:49
Operator : AR\AJ
Sample : 01203-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 21:14:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

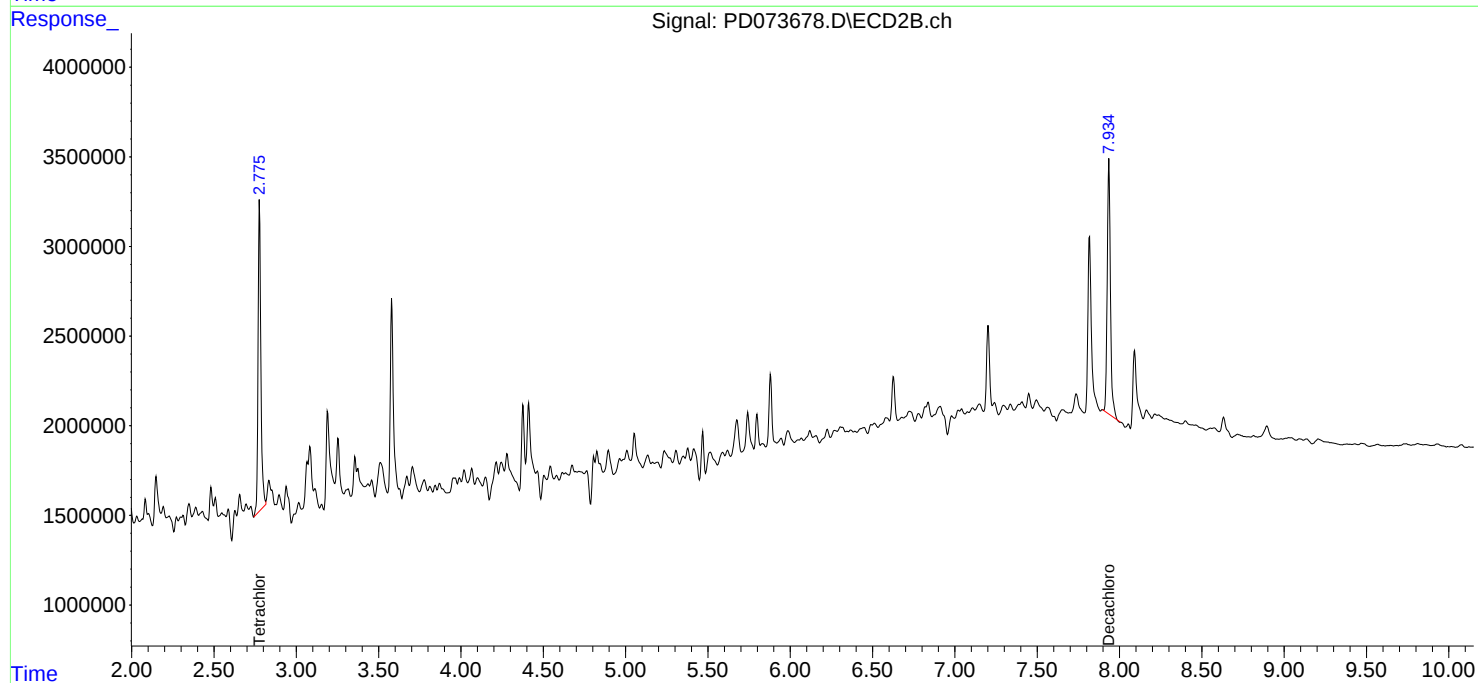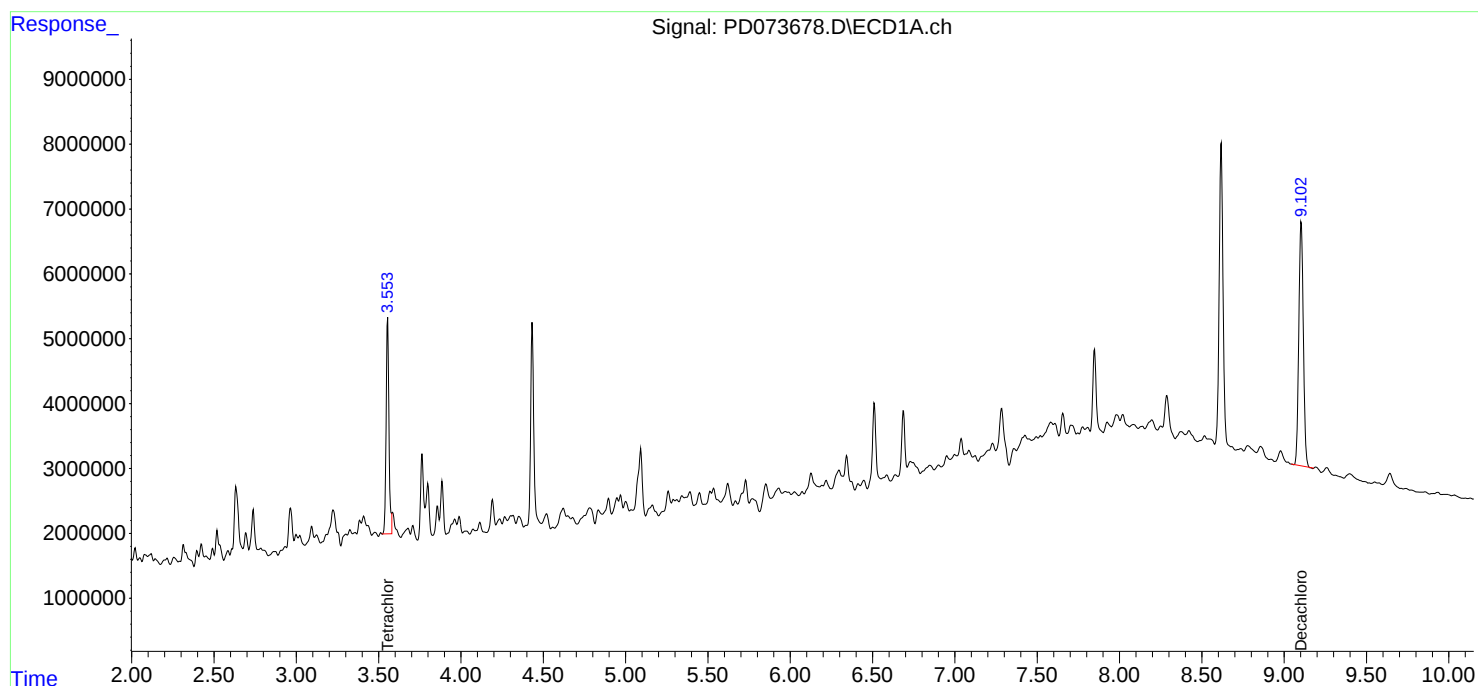


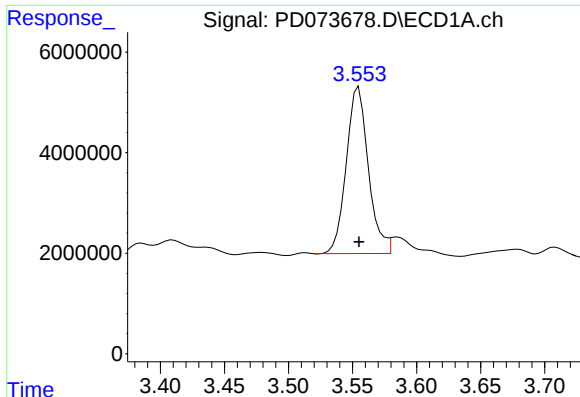

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 39778465
Conc: 17.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT

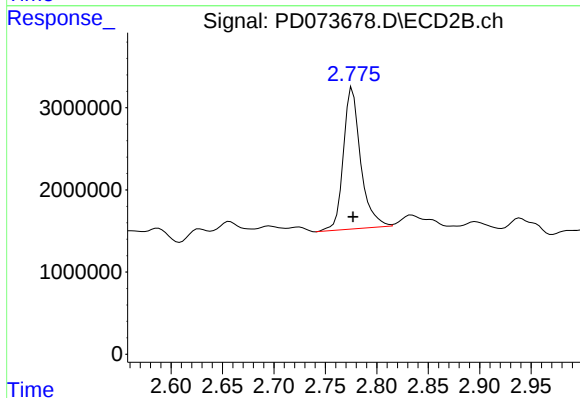


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 20114636
Conc: 15.80 ng/ml

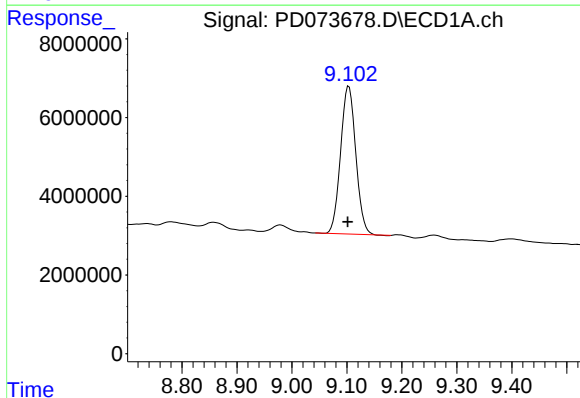

#28 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.002 min
Response: 71949776
Conc: 25.53 ng/ml

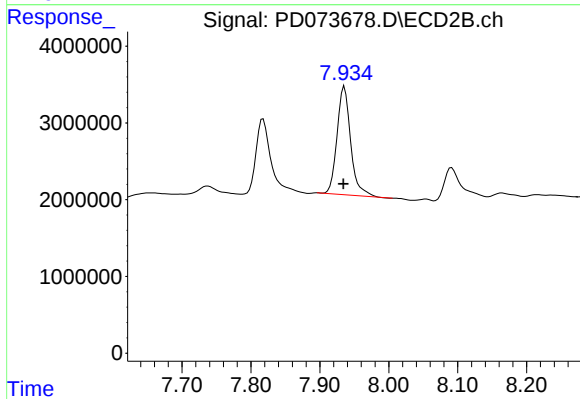

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.001 min
Response: 19275574
Conc: 16.57 ng/ml