

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012025\
 Data File : PD087448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2025 18:20
 Operator : AR\AJ
 Sample : Q1088-06MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B01MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/21/2025
 Supervised By : Ankita Jodhani 01/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 22:44:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.882	34322839	220.5E6	16.842	17.831
27)	SA Decachlor...	9.081	8.081	58922013	251.9E6	17.624	17.389
Target Compounds							
2)	A alpha-BHC	4.004	3.396	215.0E6	920.7E6	51.762	46.497
3)	MA gamma-BHC...	4.335	3.733	208.7E6	898.9E6	51.881	49.077
4)	MA Heptachlor	4.936	4.087	208.1E6	825.7E6	50.899	44.241
5)	MB Aldrin	5.277	4.373	195.8E6	824.7E6	48.884	45.629
6)	B beta-BHC	4.519	4.028	78243002	360.7E6	43.564	42.287
7)	B delta-BHC	4.768	4.265	211.0E6	852.2E6	51.057	45.662
8)	B Heptachlo...	5.697	4.877	180.2E6	747.6E6	48.235	44.172
9)	A Endosulfan I	6.079	5.252	167.0E6	750.7E6	47.928m	47.294
10)	B trans-Chl...	5.950	5.131	173.1E6	787.2E6	46.986m	43.790
11)	B cis-Chlor...	6.031	5.196	183.0E6	766.3E6	49.217m	44.276
12)	B 4,4'-DDE	6.201	5.381	354.1E6	1438.8E6	100.534m	87.846
13)	MA Dieldrin	6.352	5.518	382.4E6	1477.5E6	100.308m	88.524
14)	MA Endrin	6.581	5.794	320.5E6	1319.5E6	98.742	88.309
15)	B Endosulfa...	6.792	6.086	303.1E6	1283.0E6	94.144	86.606
16)	A 4,4'-DDD	6.711	5.935	271.6E6	1180.1E6	98.786	88.270
17)	MA 4,4'-DDT	7.025	6.190	290.5E6	1265.4E6	100.245m	91.822
18)	B Endrin al...	6.920	6.264	231.9E6	975.5E6	92.036	84.609
19)	B Endosulfa...	7.154	6.488	300.0E6	1278.4E6	97.185	87.940
20)	A Methoxychlor	7.499	6.761	741.2E6	2464.5E6	467.801	400.134
21)	B Endrin ke...	7.634	6.997	330.5E6	1372.8E6	96.002m	86.438

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012025\
Data File : PD087448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2025 18:20
Operator : AR\AJ
Sample : Q1088-06MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 22:44:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

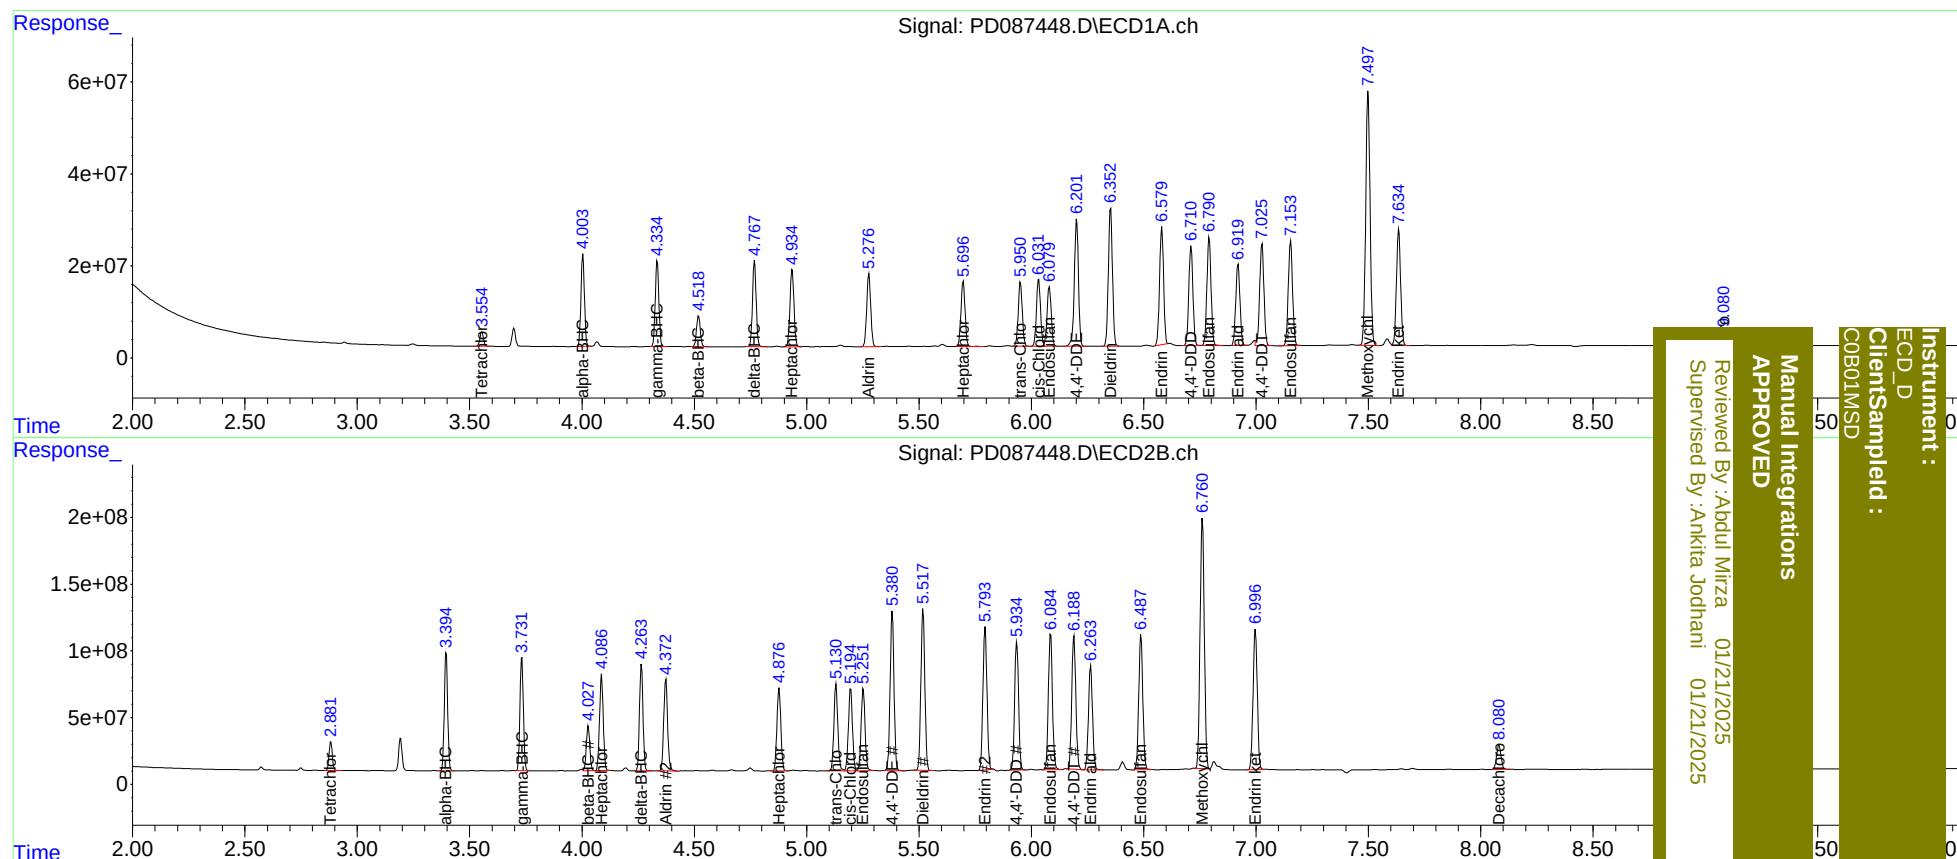

0806
Reviewed By: Abdul Mirza 01/21/2025
Supervised By: Ankita Jodhani 01/21/2025

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C0B01MSD