

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012025\
 Data File : PD087447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2025 18:06
 Operator : AR\AJ
 Sample : Q1088-05MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B01MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/21/2025
 Supervised By : Ankita Jodhani 01/21/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 20 22:44:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 16 13:39:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.882	34560840	224.5E6	16.958	18.151
2)	SA Decachlor...	9.081	8.081	59816514	255.4E6	17.891	17.634
Target Compounds							
2)	A alpha-BHC	4.004	3.396	217.3E6	933.3E6	52.296	47.135
3)	MA gamma-BHC...	4.335	3.732	210.7E6	900.9E6	52.371	49.186
4)	MA Heptachlor	4.935	4.087	210.8E6	836.1E6	51.567	44.799
5)	MB Aldrin	5.277	4.373	198.2E6	833.2E6	49.487	46.100
6)	B beta-BHC	4.520	4.028	78773993	367.6E6	43.860	43.090
7)	B delta-BHC	4.768	4.265	212.5E6	861.4E6	51.421	46.153
8)	B Heptachlo...	5.697	4.877	182.9E6	755.8E6	48.942	44.655
9)	A Endosulfan I	6.079	5.252	168.7E6	759.5E6	48.427m	47.851
10)	B trans-Chl...	5.952	5.131	174.9E6	794.1E6	47.485	44.173
11)	B cis-Chlor...	6.032	5.196	185.7E6	775.2E6	49.954m	44.792
12)	B 4,4'-DDE	6.200	5.381	358.5E6	1456.6E6	101.791m	88.934
13)	MA Dieldrin	6.352	5.518	386.6E6	1493.2E6	101.419m	89.465
14)	MA Endrin	6.581	5.794	324.2E6	1329.9E6	99.881	89.001
15)	B Endosulfa...	6.792	6.086	307.3E6	1295.6E6	95.444	87.457
16)	A 4,4'-DDD	6.711	5.935	275.5E6	1191.0E6	100.203	89.084
17)	MA 4,4'-DDT	7.026	6.190	293.1E6	1279.9E6	101.126m	92.878
18)	B Endrin al...	6.921	6.264	234.3E6	982.4E6	92.977	85.209
19)	B Endosulfa...	7.154	6.488	303.5E6	1289.8E6	98.294	88.722
20)	A Methoxychlor	7.499	6.761	750.8E6	2480.5E6	473.870	402.725
21)	B Endrin ke...	7.636	6.997	327.6E6	1383.6E6	95.150	87.115

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012025\
Data File : PD087447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2025 18:06
Operator : AR\AJ
Sample : Q1088-05MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 20 22:44:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011625CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jan 16 13:39:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

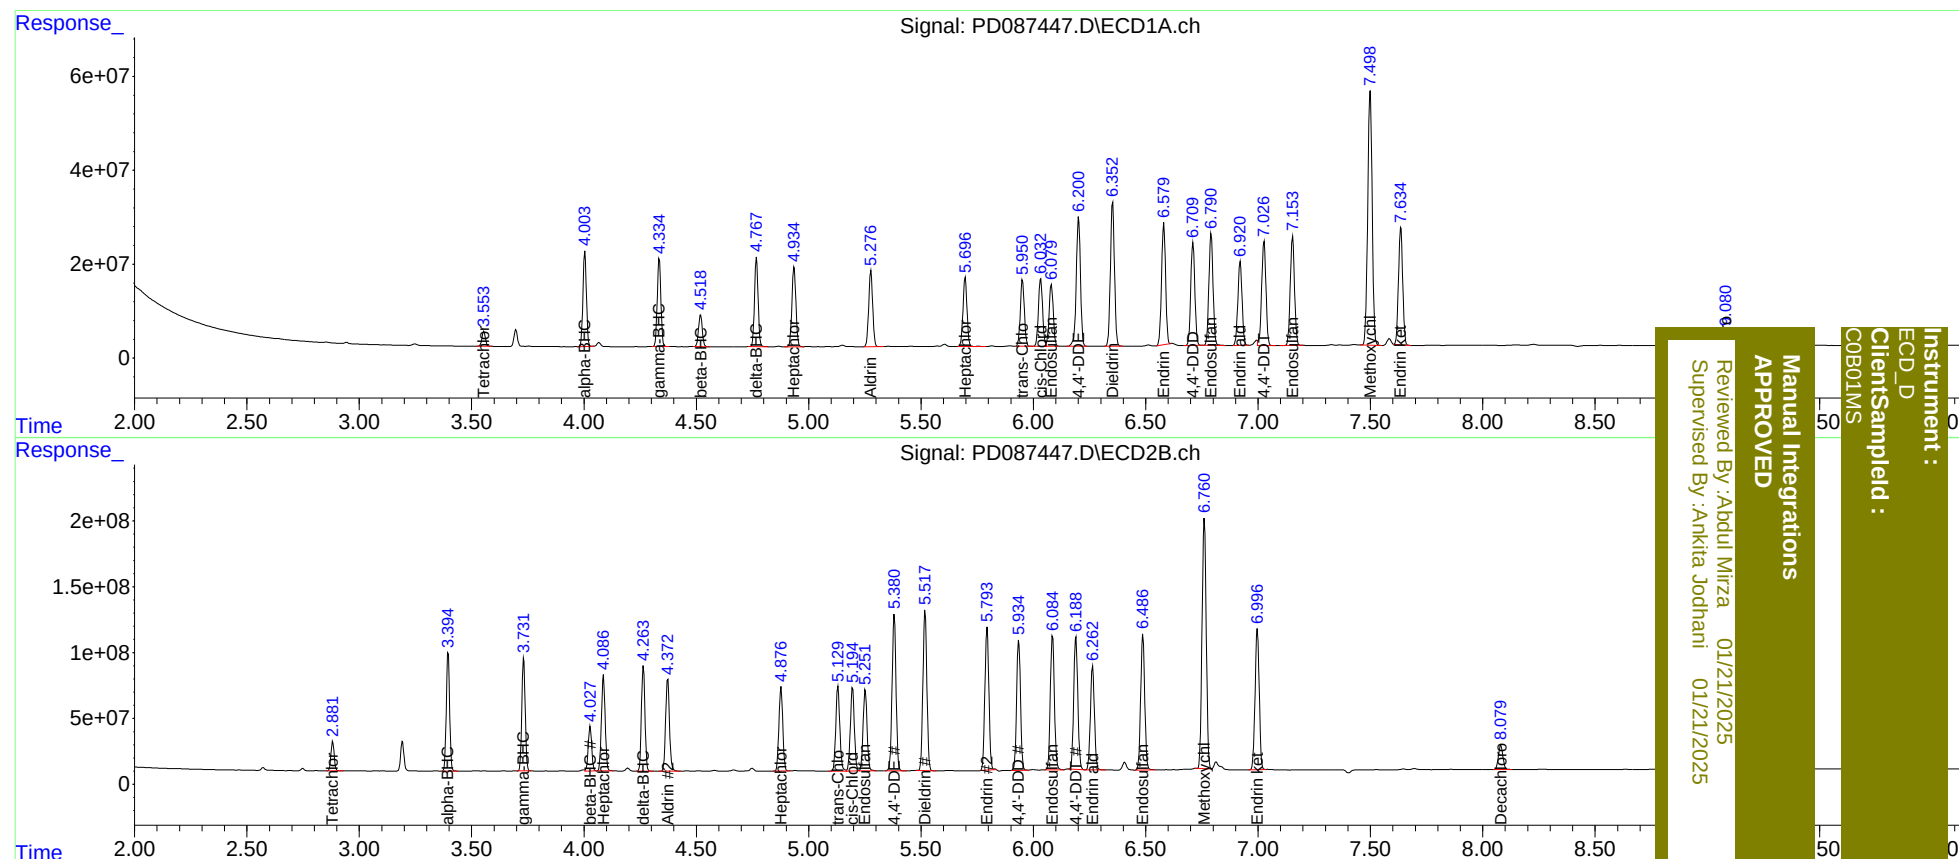

0801MS
Reviewed By: Abdul Mirza 01/21/2025
Supervised By: Ankita Jodhani 01/21/2025

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
COB01MS