

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
 Data File : PD057016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 00:11
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:29:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) MA	gamma-BHC...	3.983	0.000	269449	0	0.202	N.D. #
6) B	beta-BHC	4.206f	0.000	38019	0	0.074	N.D. #
12) B	4,4'-DDE	5.396	0.000	159240	0	0.169	N.D. #
17) MA	4,4'-DDT	6.138	0.000	158811	0	0.221	N.D. #
18) B	Endrin al...	6.217	0.000	1330968	0	1.574	N.D. #
19) B	Endosulfa...	6.404f	0.000	904649	0	0.987	N.D. #
20) A	Methoxychlor	6.694	0.000	227600	0	0.580	N.D. #
22)	Mirex	7.084	0.000	599136	0	0.713	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
Data File : PD057016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 00:11
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:29:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

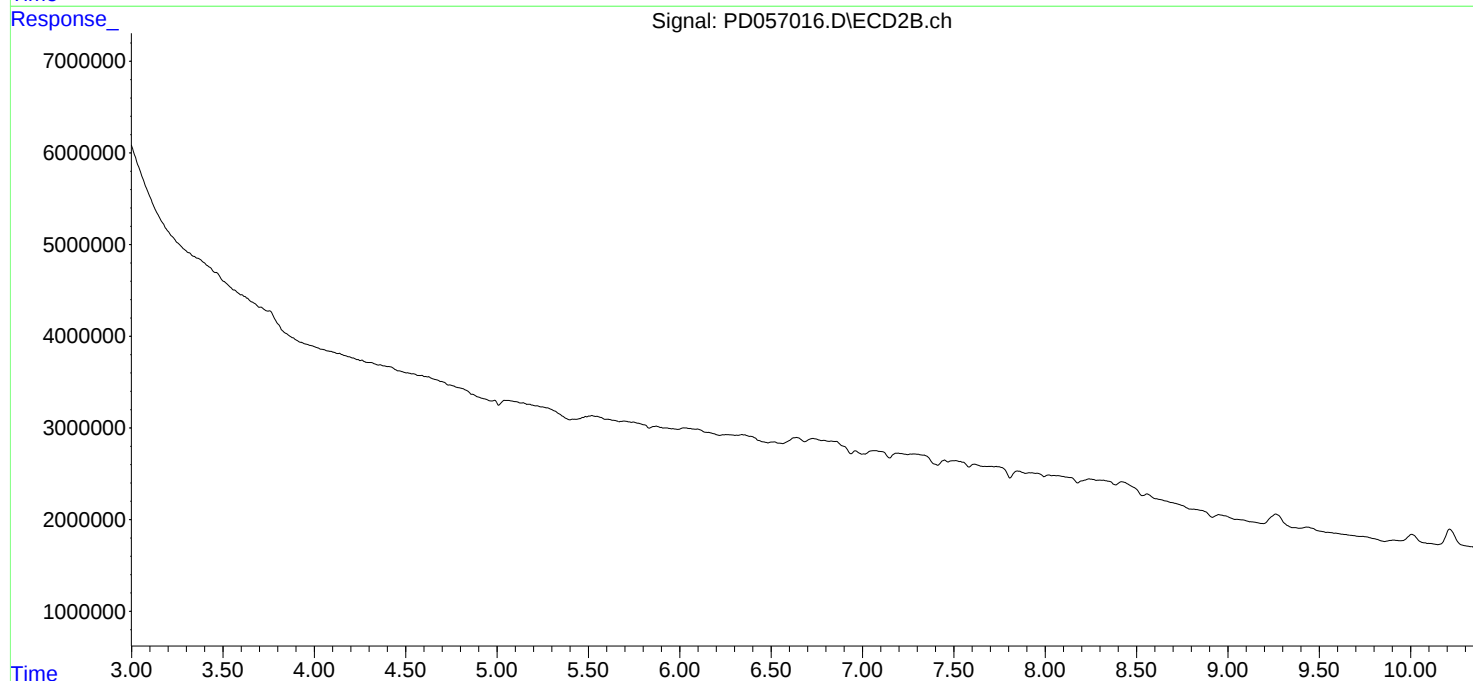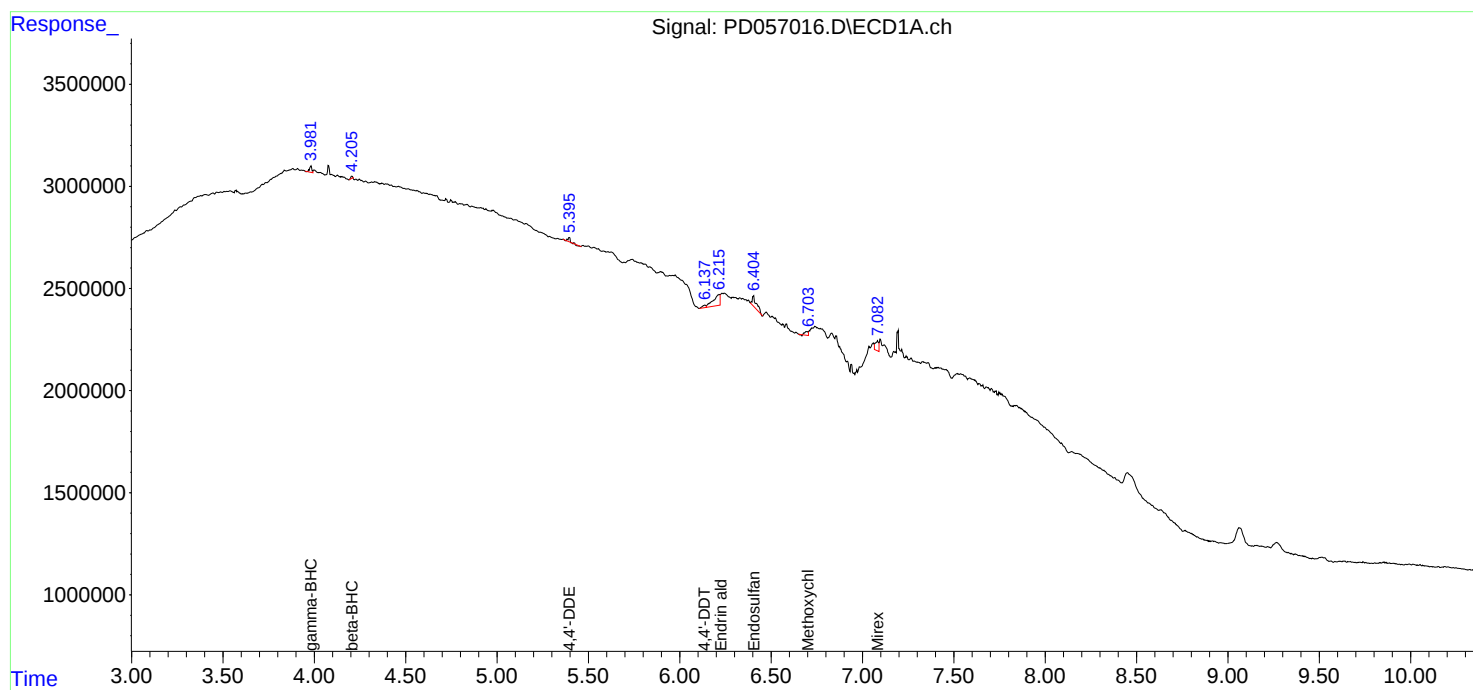


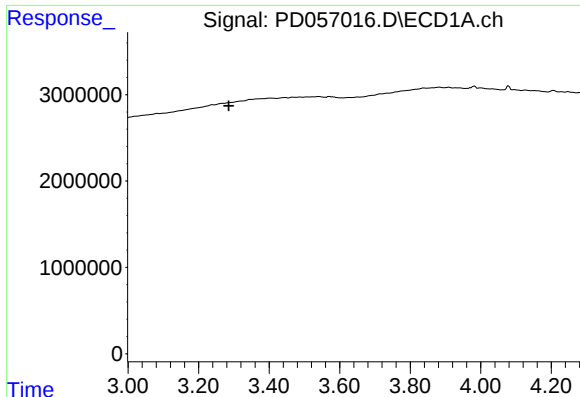

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.285 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

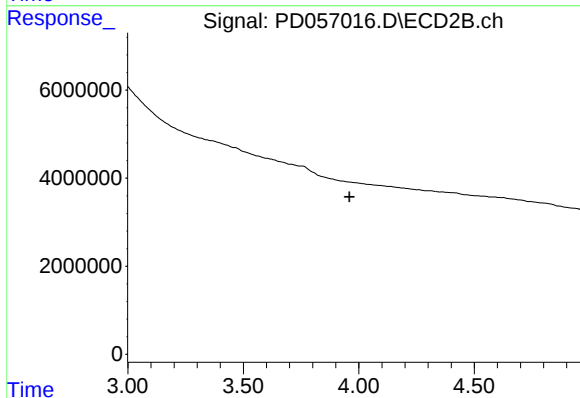


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.959 min
Response: 0
Conc: N.D.

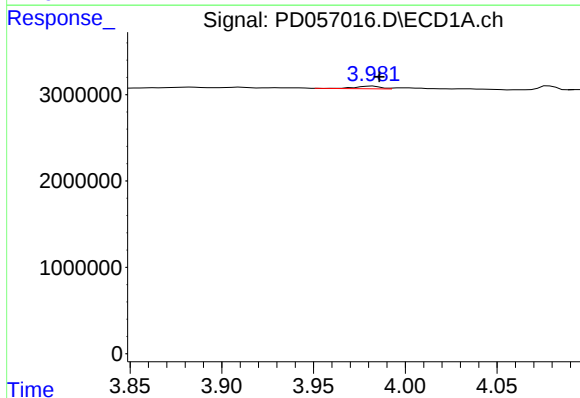


#3 gamma-BHC (Lindane)

R.T.: 3.983 min
Delta R.T.: -0.003 min
Response: 269449
Conc: 0.20 ng/ml

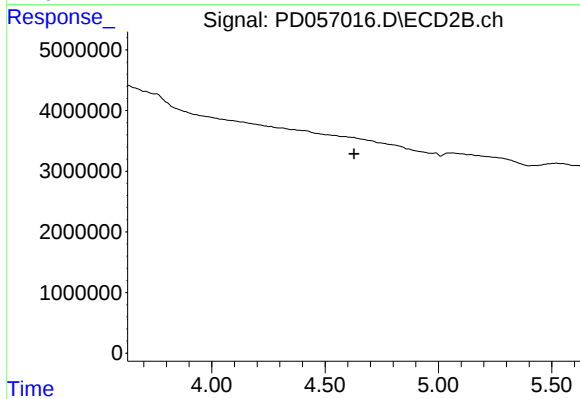

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.628 min
Response: 0
Conc: N.D.

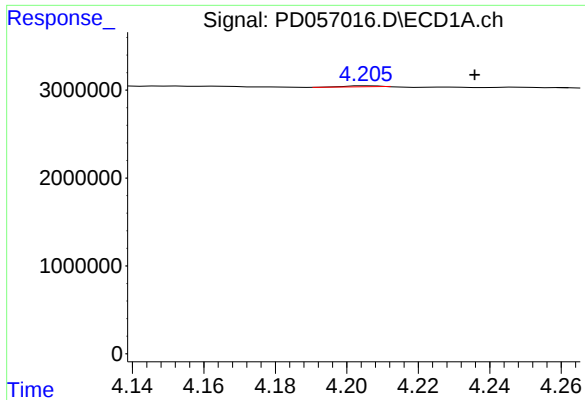

#6 beta-BHC


R.T.: 4.206 min
Delta R.T.: -0.030 min
Response: 38019
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :

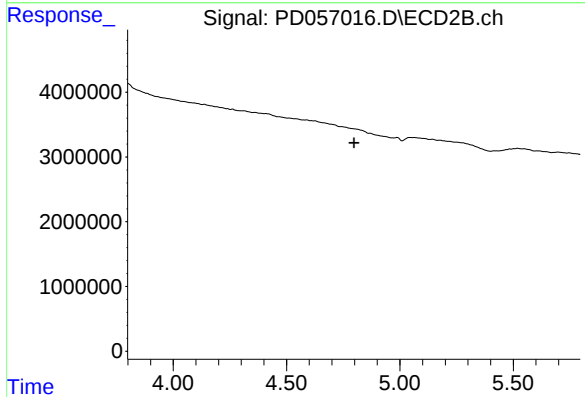


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.797 min
Response: 0
Conc: N.D.

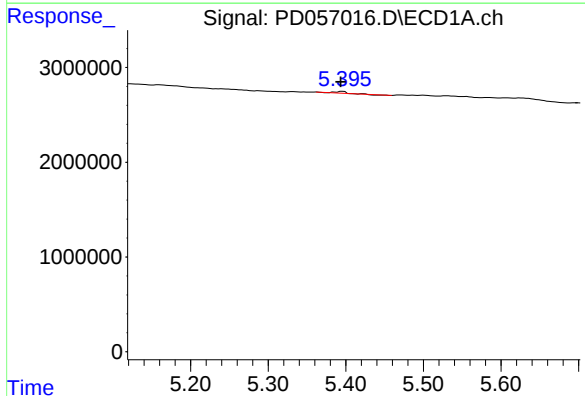


#12 4,4'-DDE

R.T.: 5.396 min
Delta R.T.: 0.003 min
Response: 159240
Conc: 0.17 ng/ml

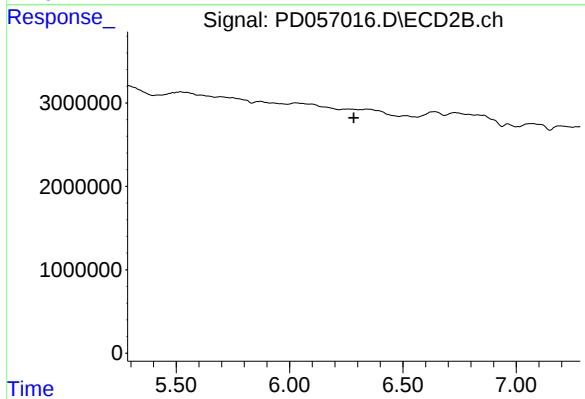

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.284 min
Response: 0
Conc: N.D.

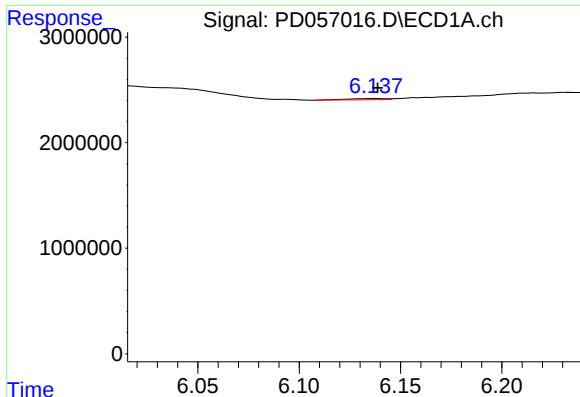

#17 4,4'-DDT


R.T.: 6.138 min
Delta R.T.: 0.000 min
Response: 158811
Conc: 0.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

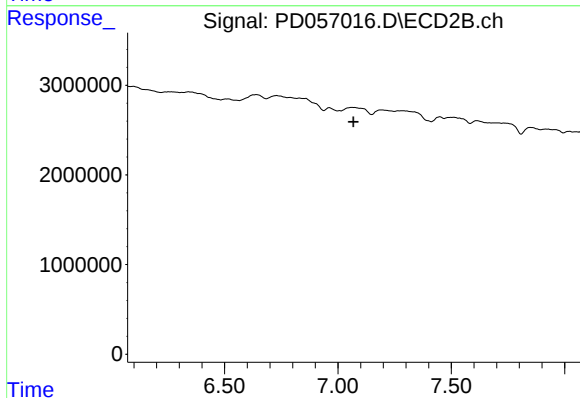

#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.069 min
Response: 0
Conc: N.D.

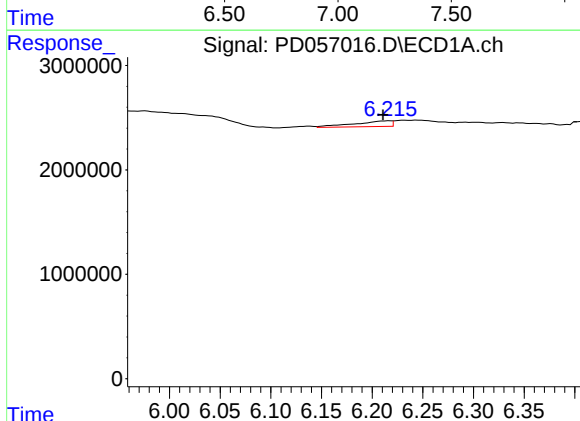


#18 Endrin aldehyde

R.T.: 6.217 min
Delta R.T.: 0.006 min
Response: 1330968
Conc: 1.57 ng/ml

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.980 min
Response: 0
Conc: N.D.

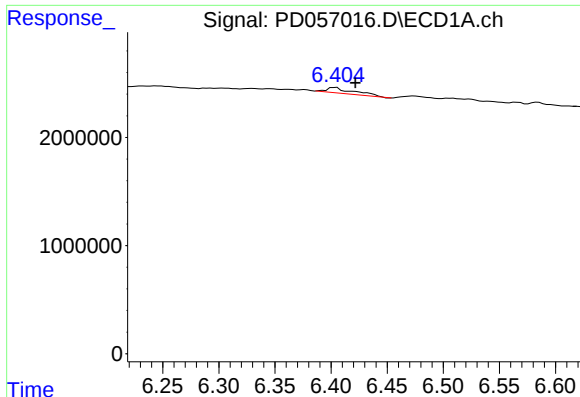

#19 Endosulfan Sulfate


R.T.: 6.404 min
Delta R.T.: -0.017 min
Response: 904649
Conc: 0.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

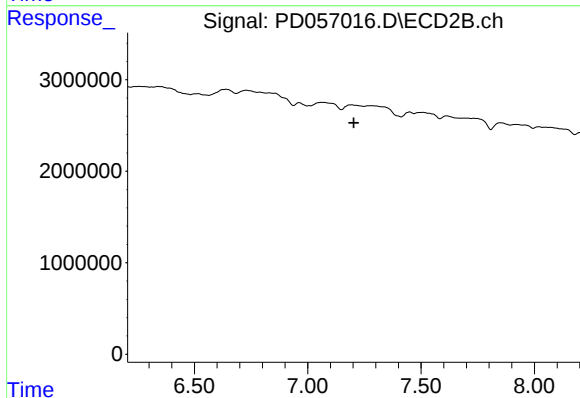


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.203 min
Response: 0
Conc: N.D.

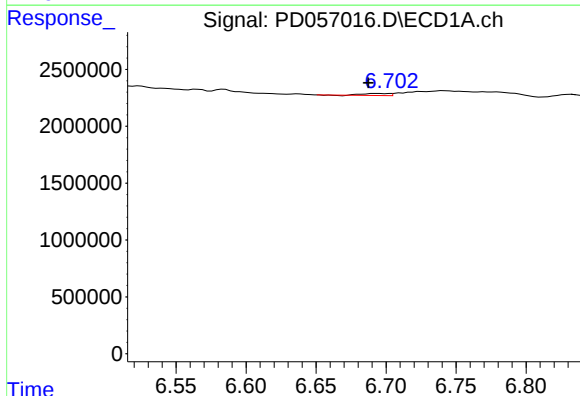


#20 Methoxychlor

R.T.: 6.694 min
Delta R.T.: 0.006 min
Response: 227600
Conc: 0.58 ng/ml

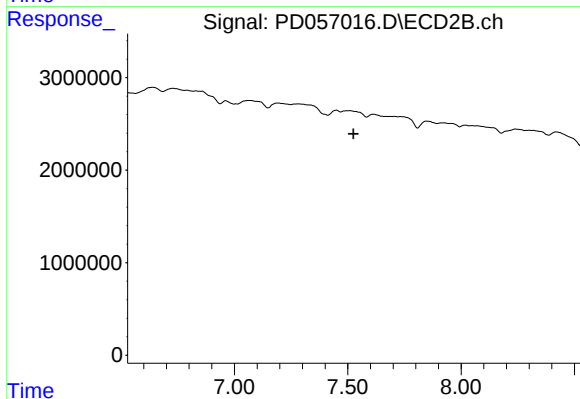

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.526 min
Response: 0
Conc: N.D.

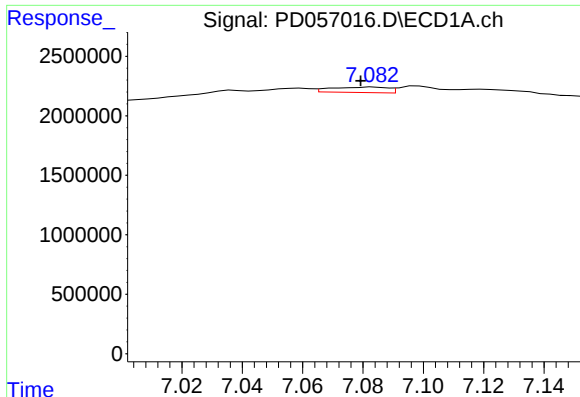

#22 Mirex


R.T.: 7.084 min
Delta R.T.: 0.005 min
Response: 599136
Conc: 0.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

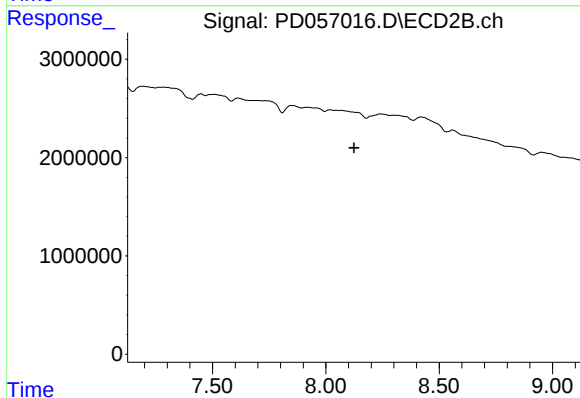


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.125 min
Response: 0
Conc: N.D.

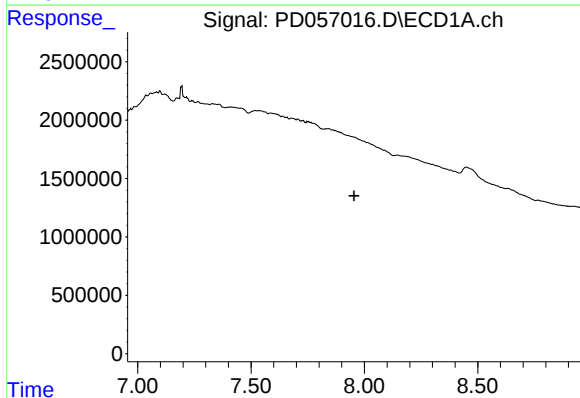

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.955 min
Response: 0
Conc: N.D.

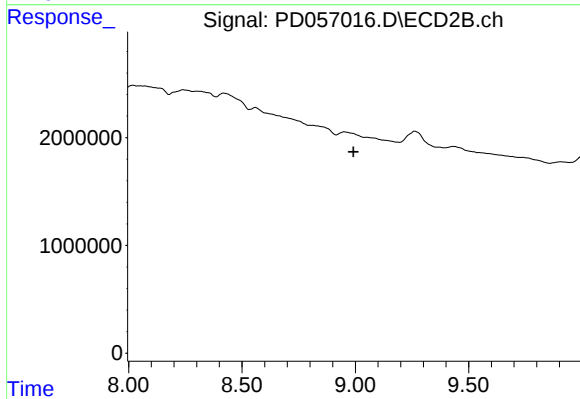

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.992 min
Response: 0
Conc: N.D.