

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
 Data File : PD057022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 01:35
 Operator : AJ\MA
 Sample : PB126211BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:30:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	23862974	47029389	28.895	28.740
28)	SA Decachlor...	7.955	8.993	27531334	46034710	28.407	27.619
Target Compounds							
3)	MA gamma-BHC...	3.995	0.000	2954055	0	2.215	N.D. #
7)	B delta-BHC	0.000	4.990f	0	1346979	N.D.	0.602 #
8)	B Heptachlo...	0.000	5.818	0	8433220	N.D.	3.884 #
9)	A Endosulfan I	5.293f	0.000	891831	0	0.907	N.D. #
11)	B alpha-Chl...	0.000	6.107f	0	5862418	N.D.	2.633 #
14)	MA Endrin	5.788f	6.655	341641	3295221	0.384	1.915 #
22)	Mirex	7.093	0.000	1508283	0	1.795	N.D. #
24)	Chlordane-2	4.594f	0.000	2976328	0	84.900	N.D. #
26)	Chlordane-4	0.000	6.107f	0	5862418	N.D.	17.361 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
Data File : PD057022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 01:35
Operator : AJ\MA
Sample : PB126211BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:30:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

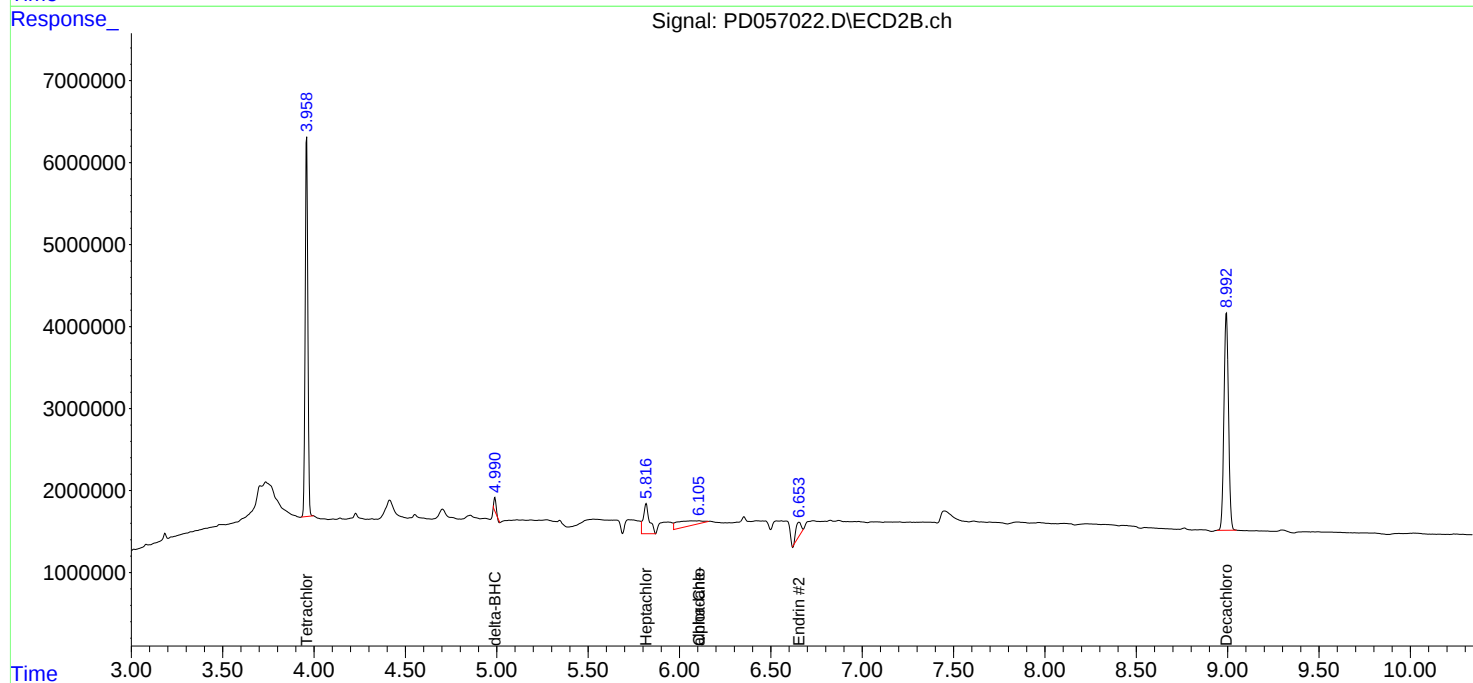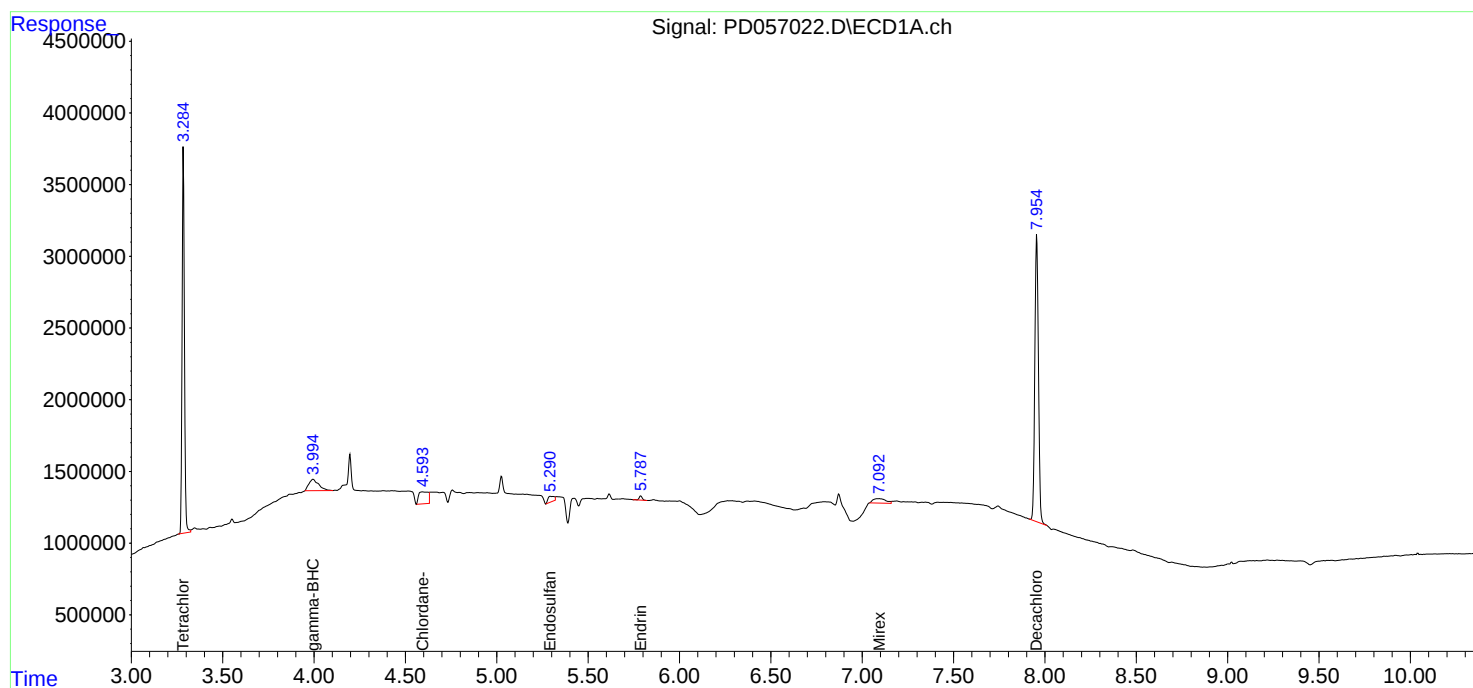


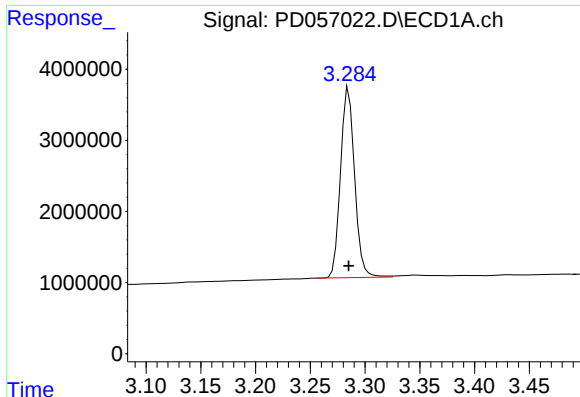

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 23862974
Conc: 28.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

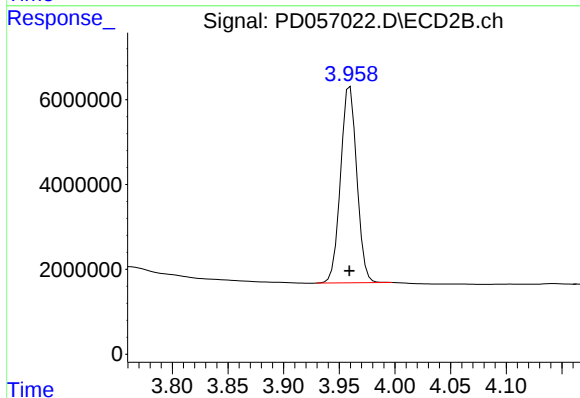


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 47029389
Conc: 28.74 ng/ml

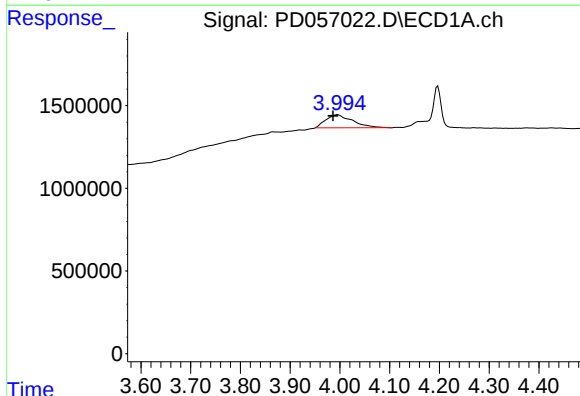


#3 gamma-BHC (Lindane)

R.T.: 3.995 min
Delta R.T.: 0.009 min
Response: 2954055
Conc: 2.21 ng/ml

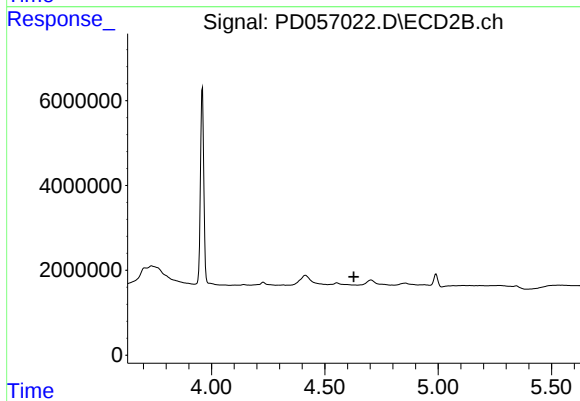

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.628 min
Response: 0
Conc: N.D.

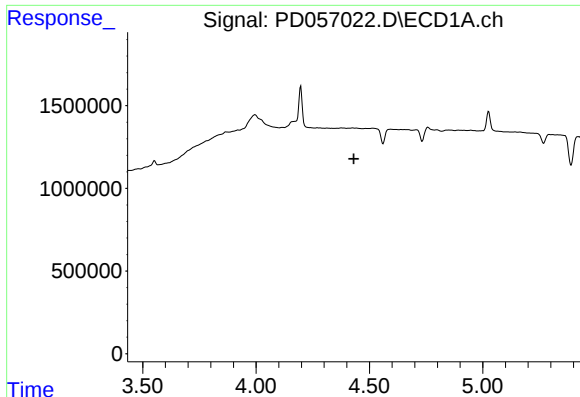

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

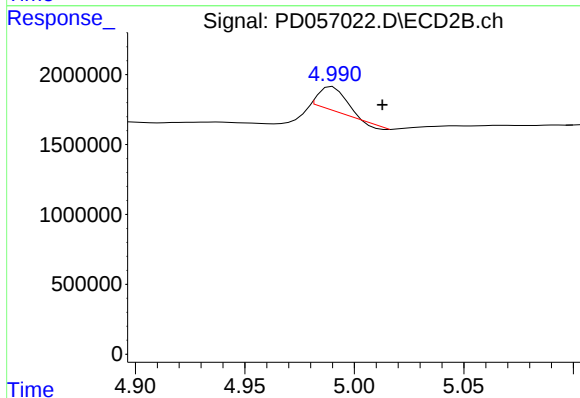


#7 delta-BHC

R.T.: 4.990 min
Delta R.T.: -0.023 min
Response: 1346979
Conc: 0.60 ng/ml

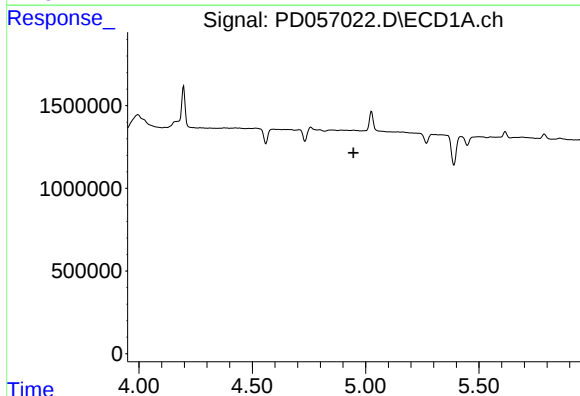


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.947 min
Response: 0
Conc: N.D.

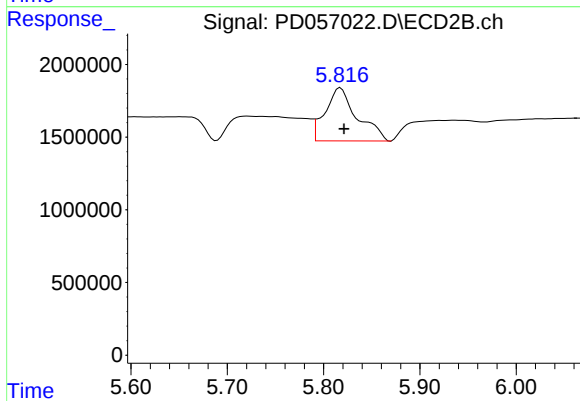

#8 Heptachlor epoxide


R.T.: 5.818 min
Delta R.T.: -0.004 min
Response: 8433220
Conc: 3.88 ng/ml

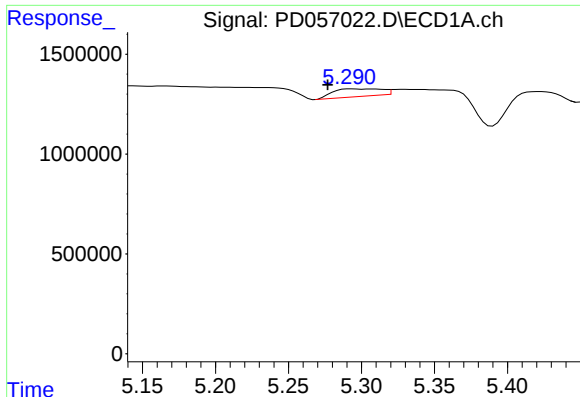

#9 Endosulfan I


R.T.: 5.293 min
Delta R.T.: 0.017 min
Response: 891831
Conc: 0.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

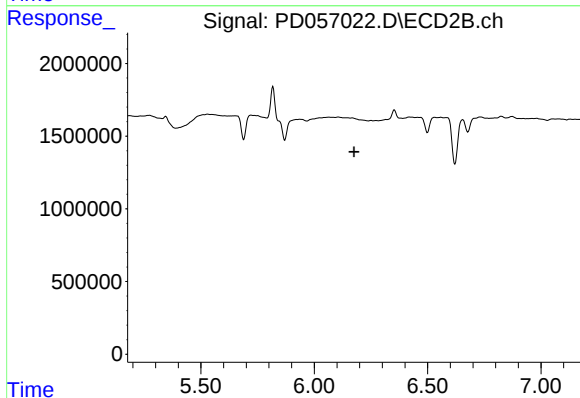


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

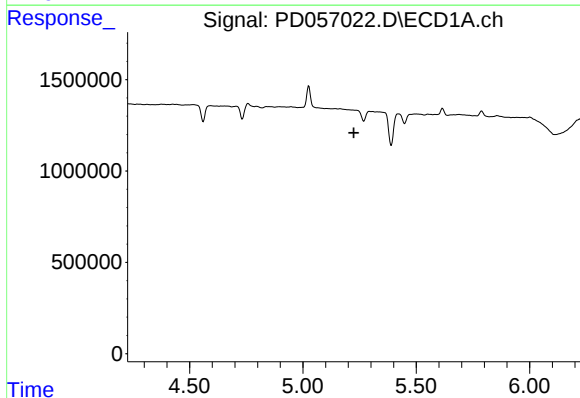


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.225 min
Response: 0
Conc: N.D.

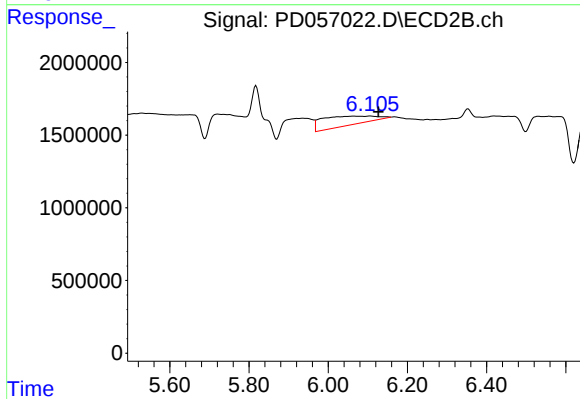

#11 alpha-Chlordane


R.T.: 6.107 min
Delta R.T.: -0.020 min
Response: 5862418
Conc: 2.63 ng/ml

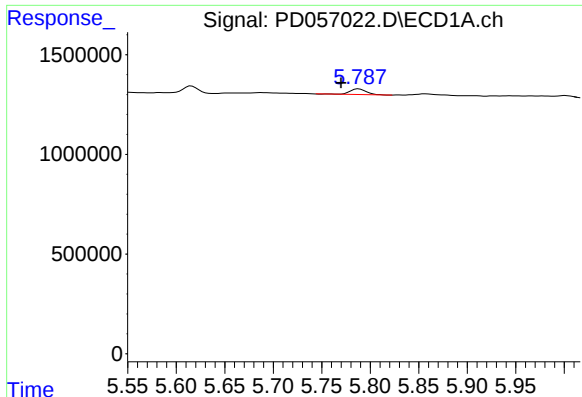

#14 Endrin


R.T.: 5.788 min
Delta R.T.: 0.019 min
Response: 341641
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

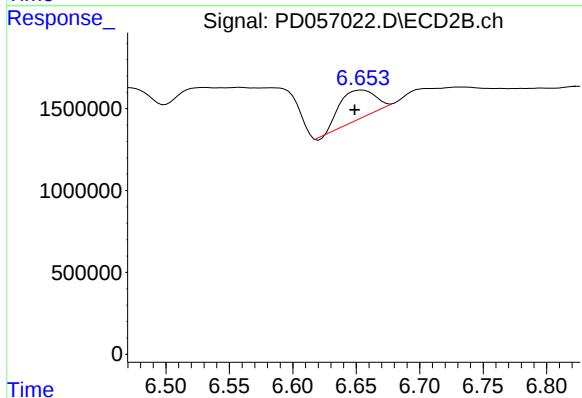


#14 Endrin

R.T.: 6.655 min
Delta R.T.: 0.006 min
Response: 3295221
Conc: 1.91 ng/ml

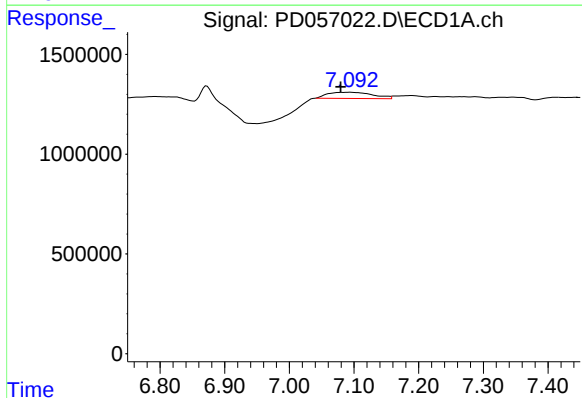


#22 Mirex

R.T.: 7.093 min
Delta R.T.: 0.014 min
Response: 1508283
Conc: 1.79 ng/ml

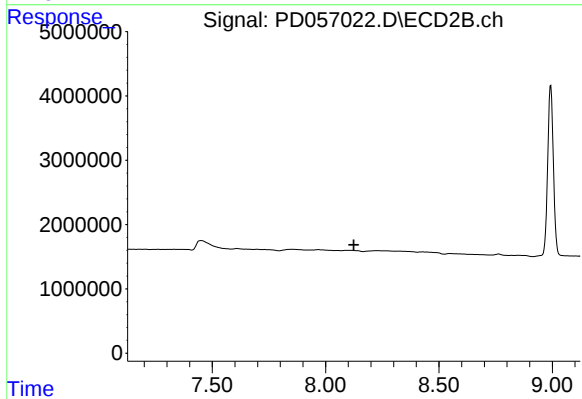

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.125 min
Response: 0
Conc: N.D.

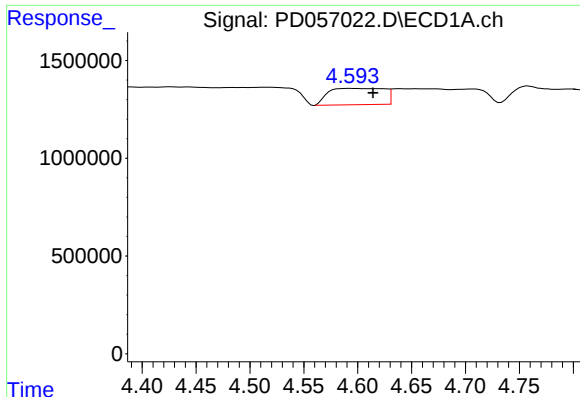

#24 Chlordane-2


R.T.: 4.594 min
Delta R.T.: -0.020 min
Response: 2976328
Conc: 84.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

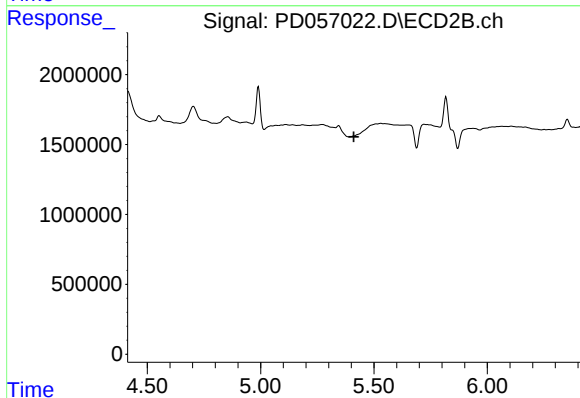


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.412 min
Response: 0
Conc: N.D.

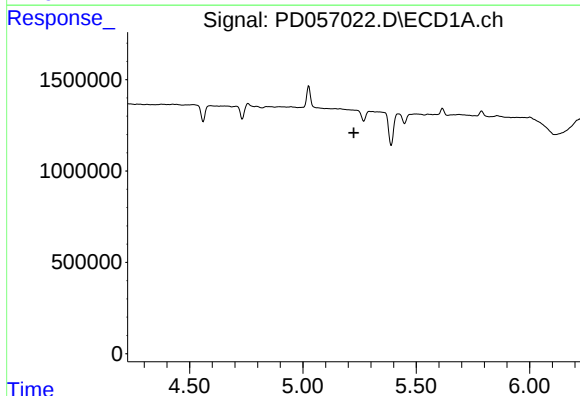


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.225 min
Response: 0
Conc: N.D.

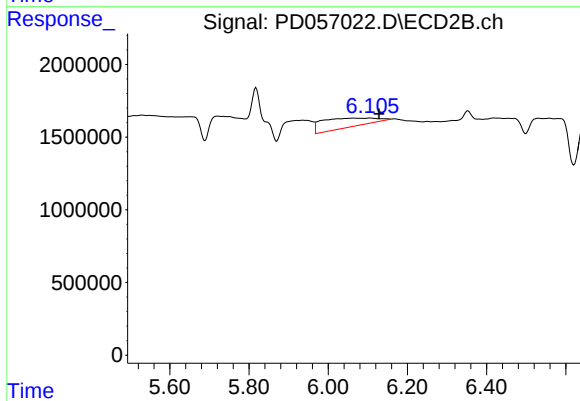

#26 Chlordane-4


R.T.: 6.107 min
Delta R.T.: -0.022 min
Response: 5862418
Conc: 17.36 ng/ml

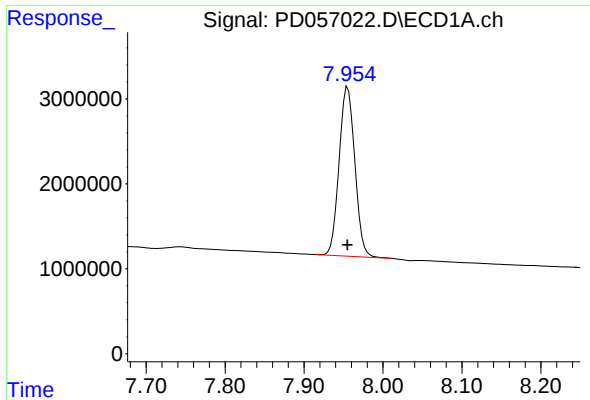

#28 Decachlorobiphenyl

R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 27531334
Conc: 28.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

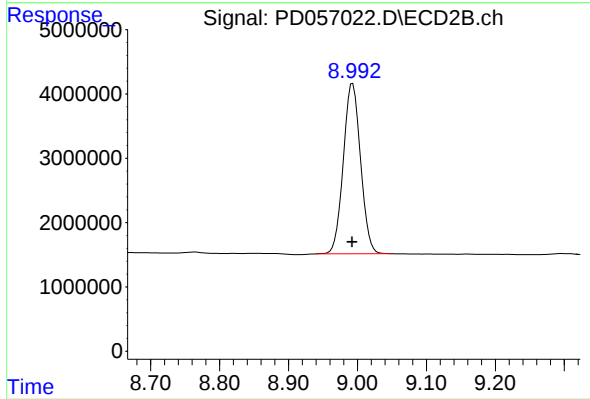

#28 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: 0.000 min
Response: 46034710
Conc: 27.62 ng/ml