

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
 Data File : PD057030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 03:28
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:31:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	17353825	34293542	21.013	20.957
28)	SA Decachlor...	7.955	8.994	20212619	34334051	20.855	20.599
Target Compounds							
3)	MA gamma-BHC...	3.994	0.000	1676493	0	1.257	N.D. #
22)	Mirex	7.101f	0.000	879048	0	1.046	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
Data File : PD057030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 03:28
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:31:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

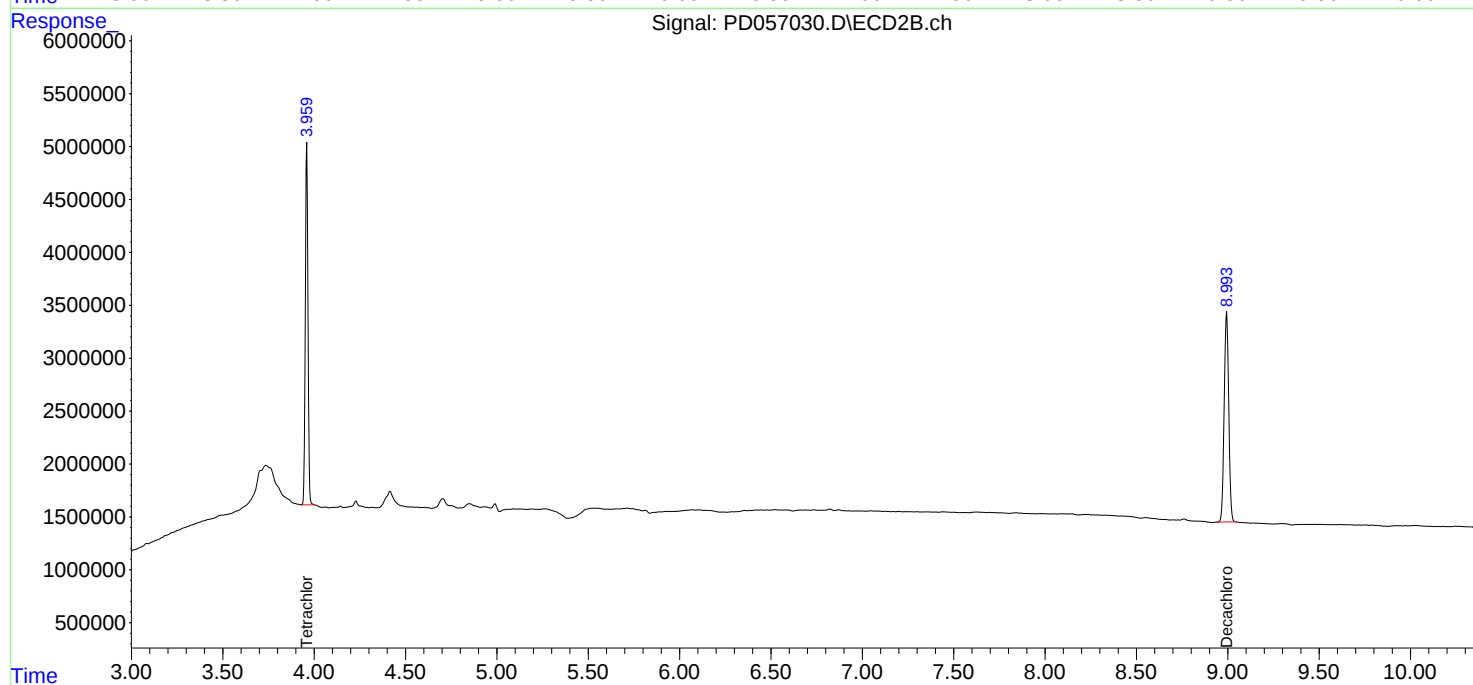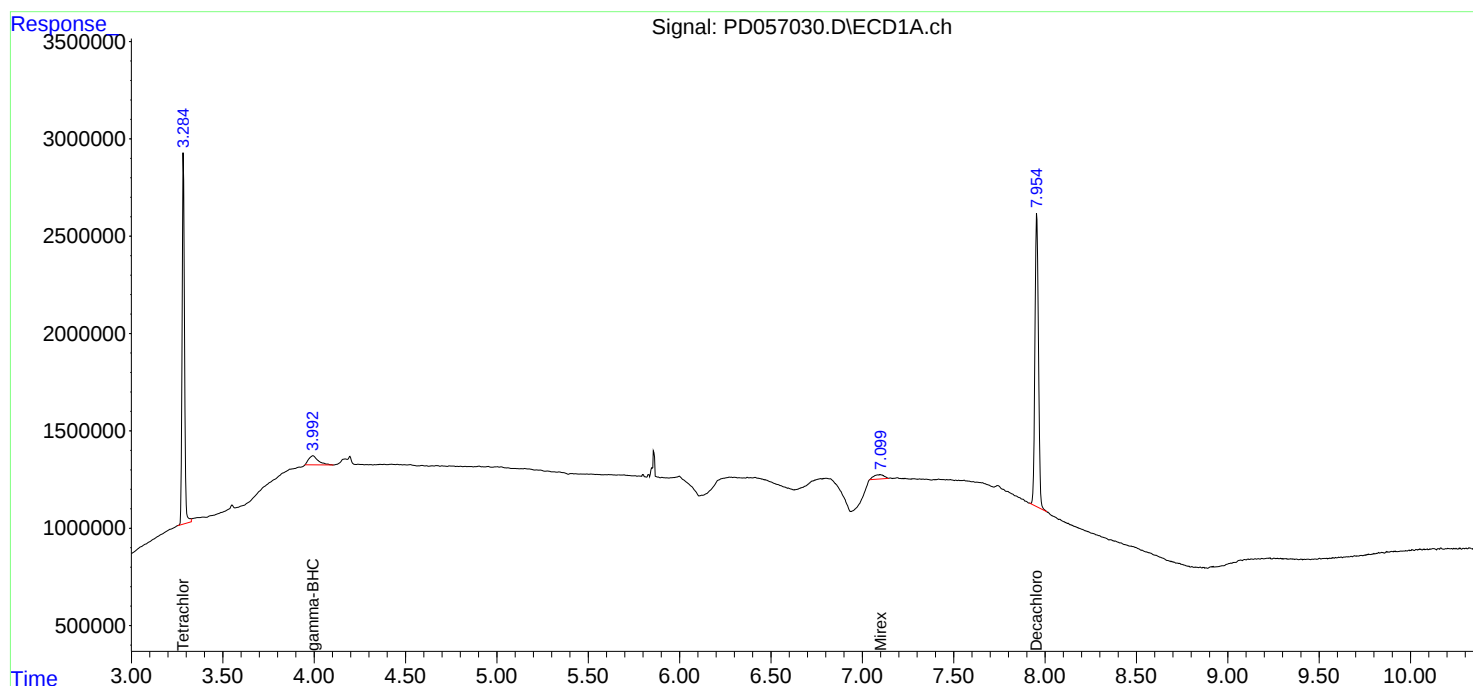


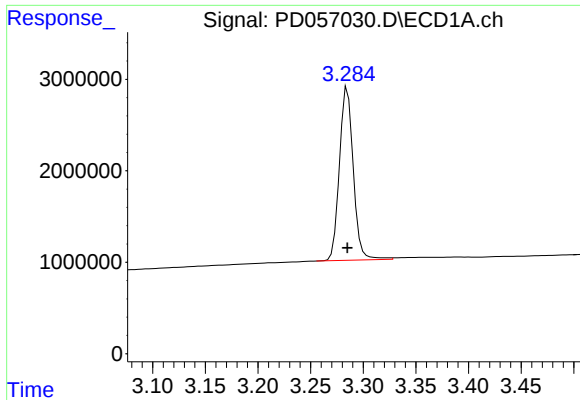

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 17353825
Conc: 21.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

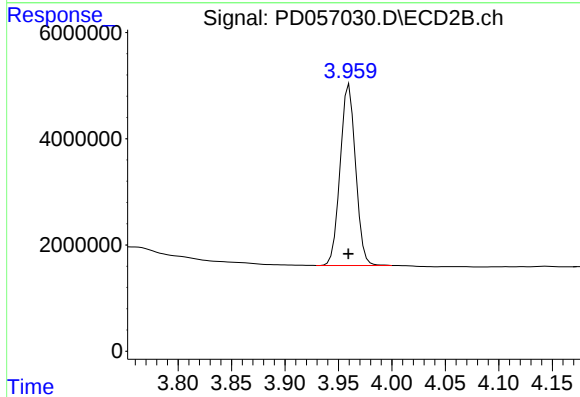


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 34293542
Conc: 20.96 ng/ml

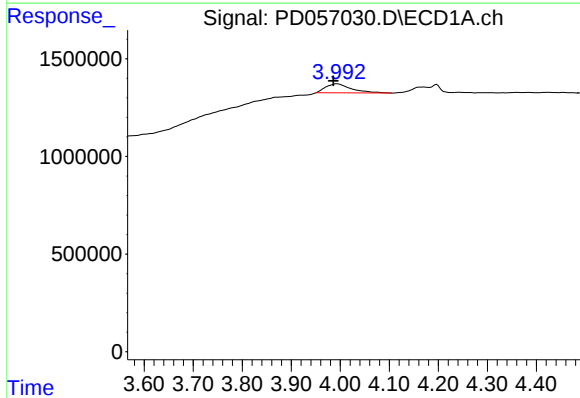


#3 gamma-BHC (Lindane)

R.T.: 3.994 min
Delta R.T.: 0.008 min
Response: 1676493
Conc: 1.26 ng/ml

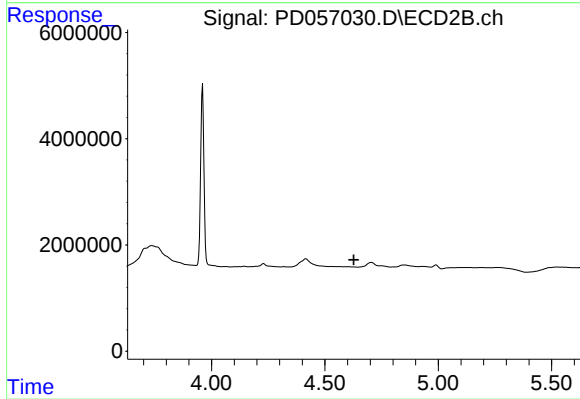

#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.628 min
Response: 0
Conc: N.D.

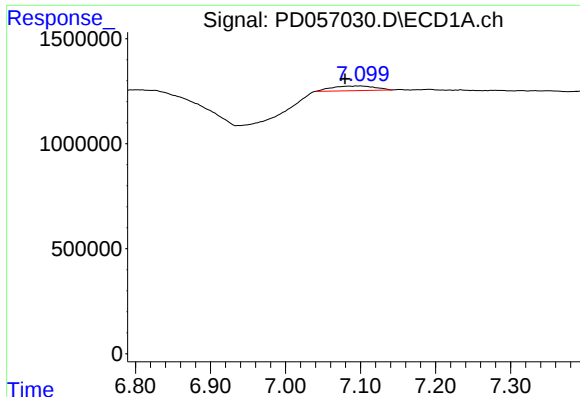

#22 Mirex


R.T.: 7.101 min

Delta R.T.: 0.022 min

Response: 879048

Conc: 1.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

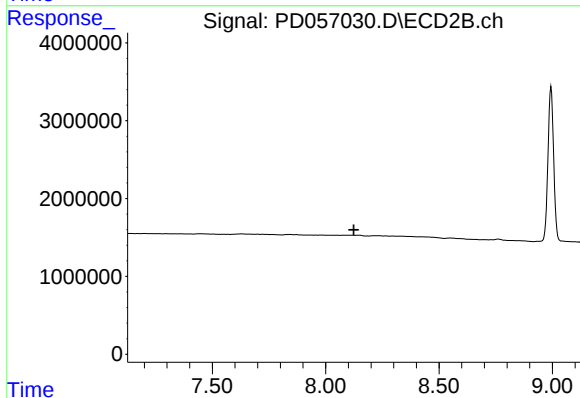


#22 Mirex

R.T.: 0.000 min

Exp R.T. : 8.125 min

Response: 0

Conc: N.D.

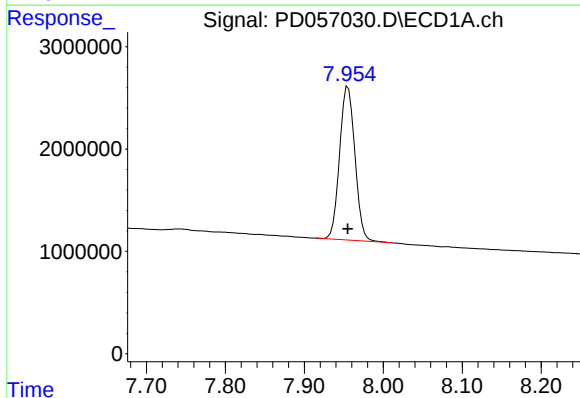


#28 Decachlorobiphenyl

R.T.: 7.955 min

Delta R.T.: 0.000 min

Response: 20212619

Conc: 20.86 ng/ml

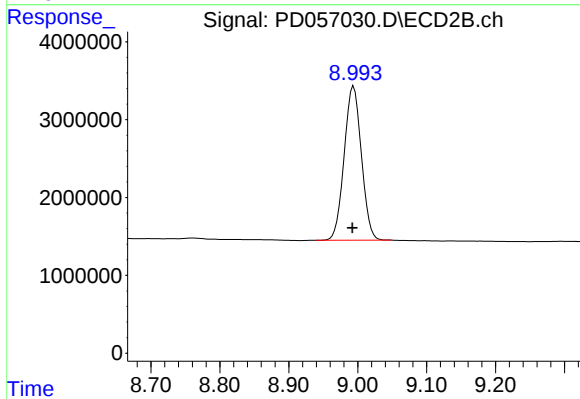

#28 Decachlorobiphenyl

R.T.: 8.994 min

Delta R.T.: 0.002 min

Response: 34334051

Conc: 20.60 ng/ml