

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
 Data File : PD057020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 01:07
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:30:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	45031751	82295330	54.528	50.292
28)	SA Decachlor...	7.956	8.994	46688474	76549583	48.173	45.927
Target Compounds							
23)	Chlordane-1	4.124	4.947	13894146	32455155	502.425	502.264
24)	Chlordane-2	4.615	5.412	16539632	34532294	471.793	503.417
25)	Chlordane-3	5.170	6.055	48176840	140.4E6	491.978	497.642
26)	Chlordane-4	5.225	6.129	42825875	167.5E6	492.463	495.885
27)	Chlordane-5	6.048	6.930	16171344	29265249	467.395	524.211



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
Data File : PD057020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 01:07
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:30:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

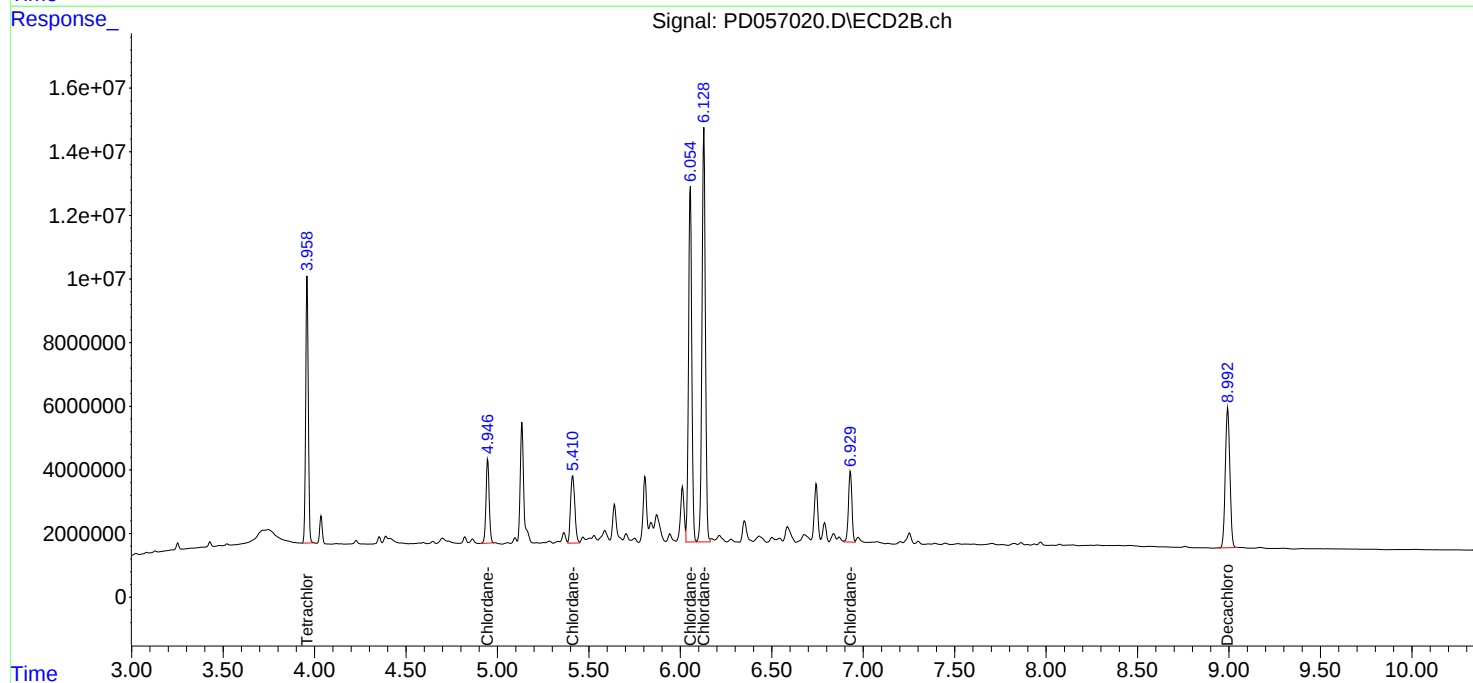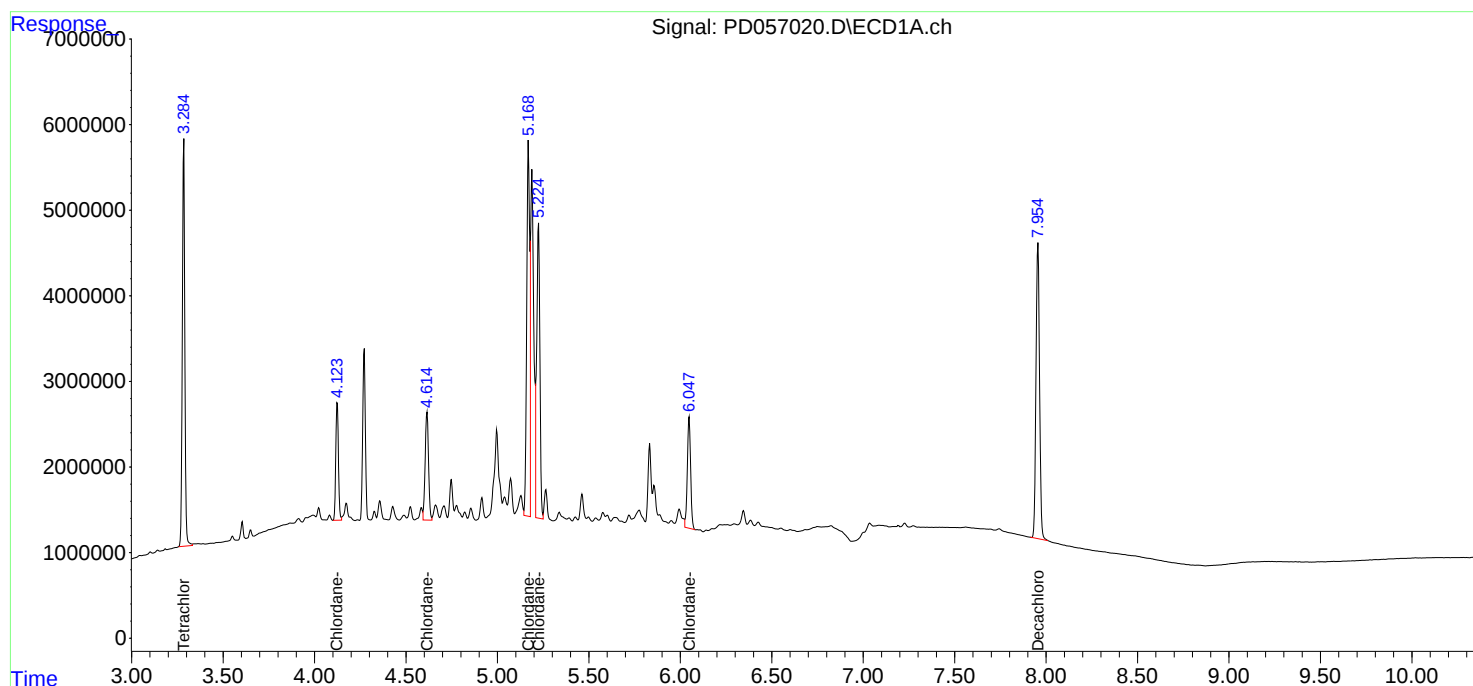


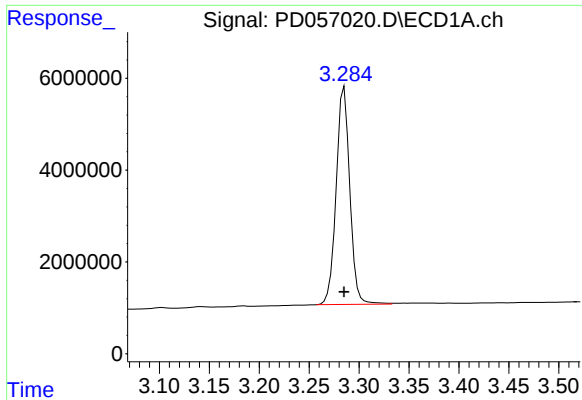

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 45031751
Conc: 54.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

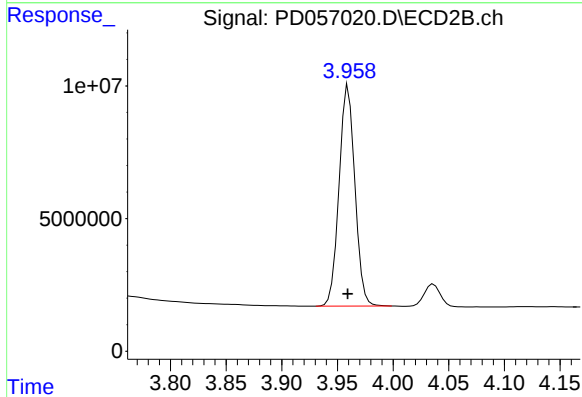


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 82295330
Conc: 50.29 ng/ml

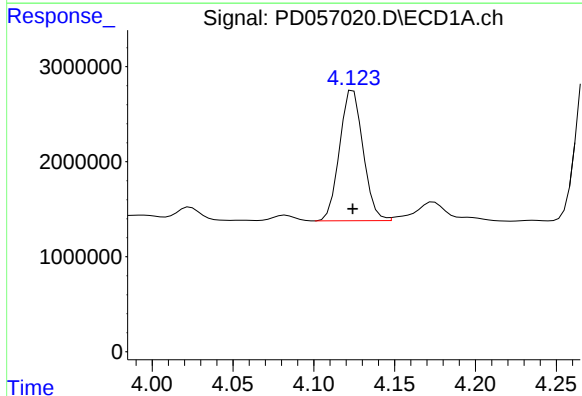


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 13894146
Conc: 502.42 ng/ml

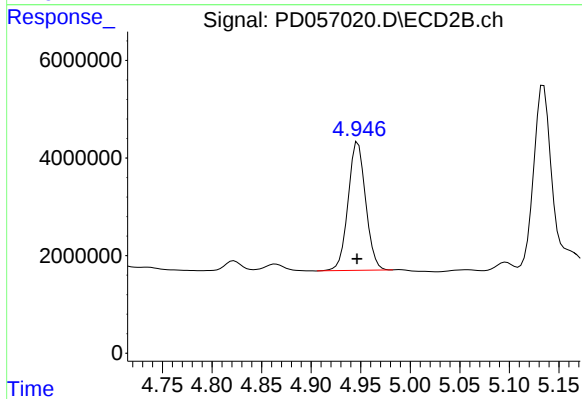

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.001 min
Response: 32455155
Conc: 502.26 ng/ml

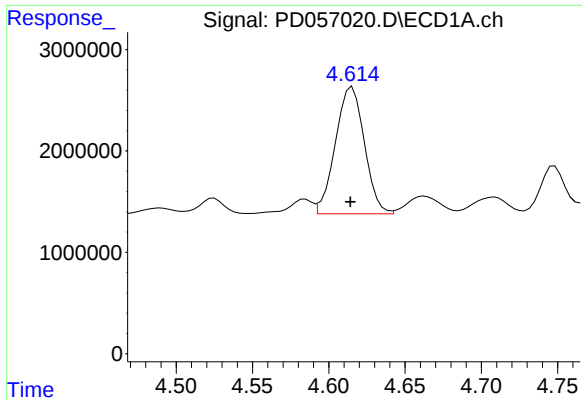

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: 0.001 min
Response: 16539632
Conc: 471.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

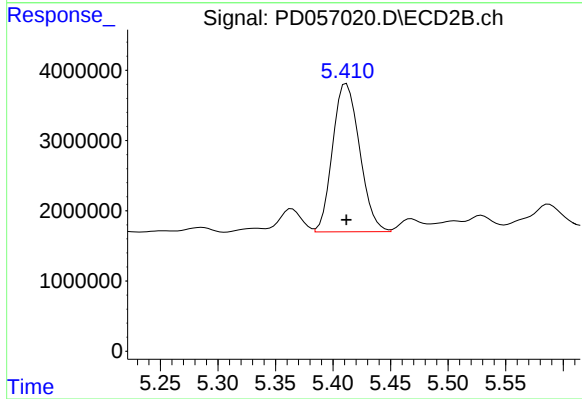


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 34532294
Conc: 503.42 ng/ml

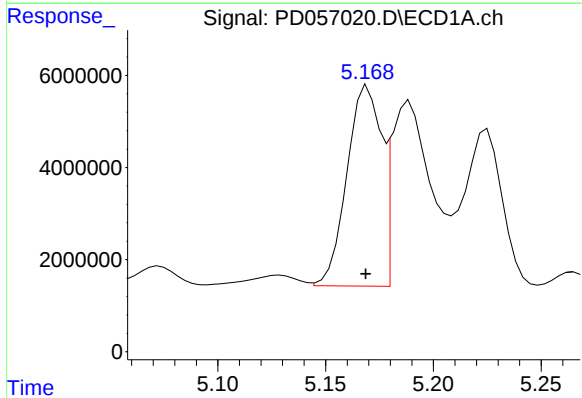


#25 Chlordane-3

R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 48176840
Conc: 491.98 ng/ml

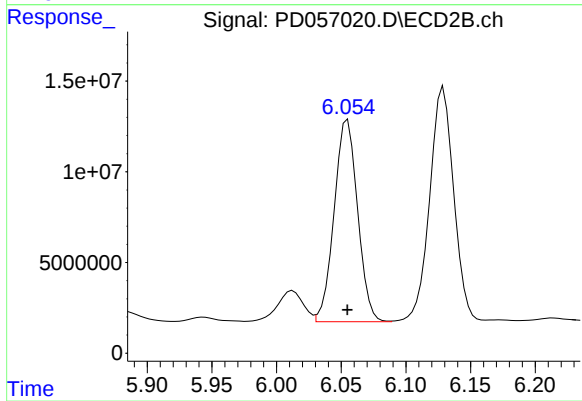

#25 Chlordane-3


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 140410551
Conc: 497.64 ng/ml

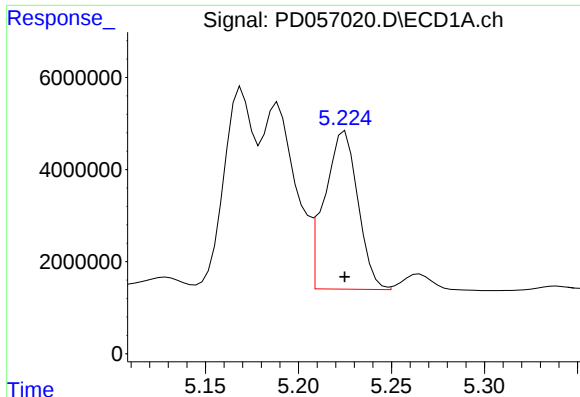

#26 Chlordane-4


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 42825875
Conc: 492.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

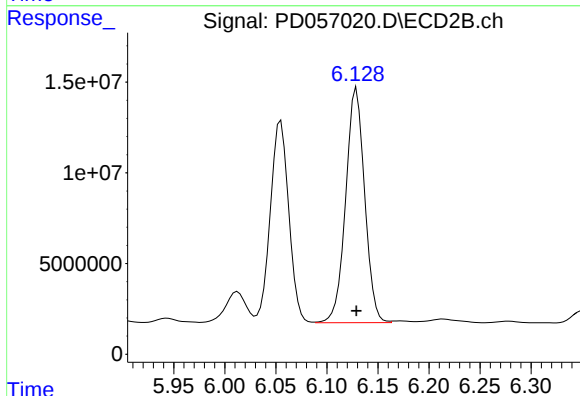


#26 Chlordane-4

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 167450938
Conc: 495.89 ng/ml

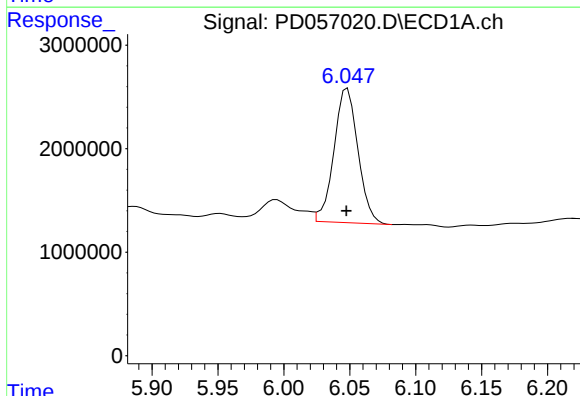


#27 Chlordane-5

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 16171344
Conc: 467.39 ng/ml

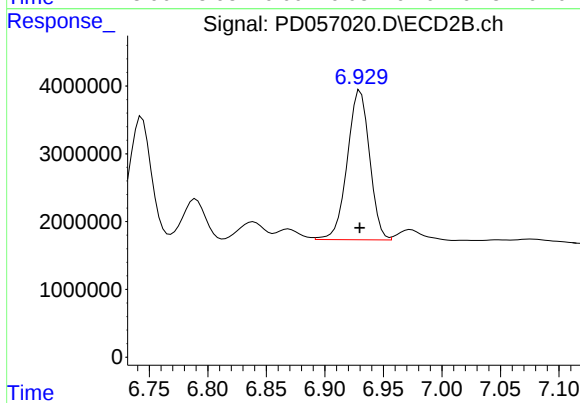

#27 Chlordane-5


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 29265249
Conc: 524.21 ng/ml

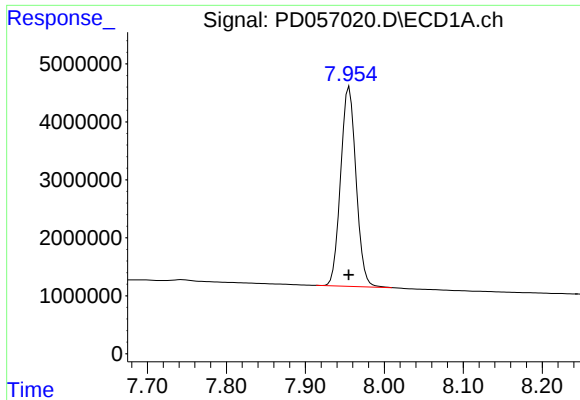

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 46688474
Conc: 48.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

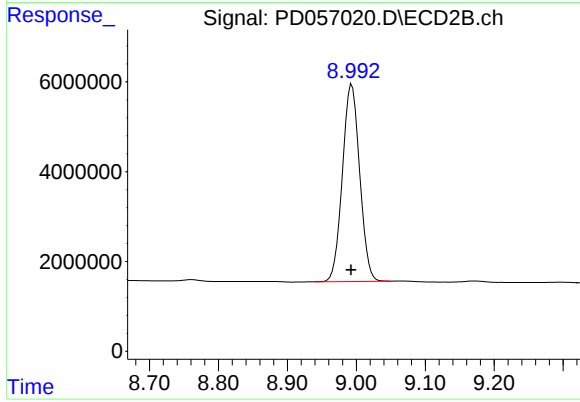

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.001 min
Response: 76549583
Conc: 45.93 ng/ml