

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
 Data File : PD057027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 02:45
 Operator : AJ\MA
 Sample : L1161-09
 Misc : CHLOR MDL 25 PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:31:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	13691263	27294830	16.578	16.680
28)	SA Decachlor...	7.956	8.994	16431553	28196327	16.954	16.917
Target Compounds							
23)	Chlordane-1	4.124	4.947	643001	1765826	23.251	27.327
24)	Chlordane-2	4.614	5.412	1039439	1970597	29.650	28.728
25)	Chlordane-3	5.168	6.055	2258746	6770158	23.066	23.995
26)	Chlordane-4	5.225	6.129	2071449	8414016	23.820	24.917
27)	Chlordane-5	6.047	6.930	865368	1271840	25.011	22.782



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
Data File : PD057027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 02:45
Operator : AJ\MA
Sample : L1161-09
Misc : CHLOR MDL 25 PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT1-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:31:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

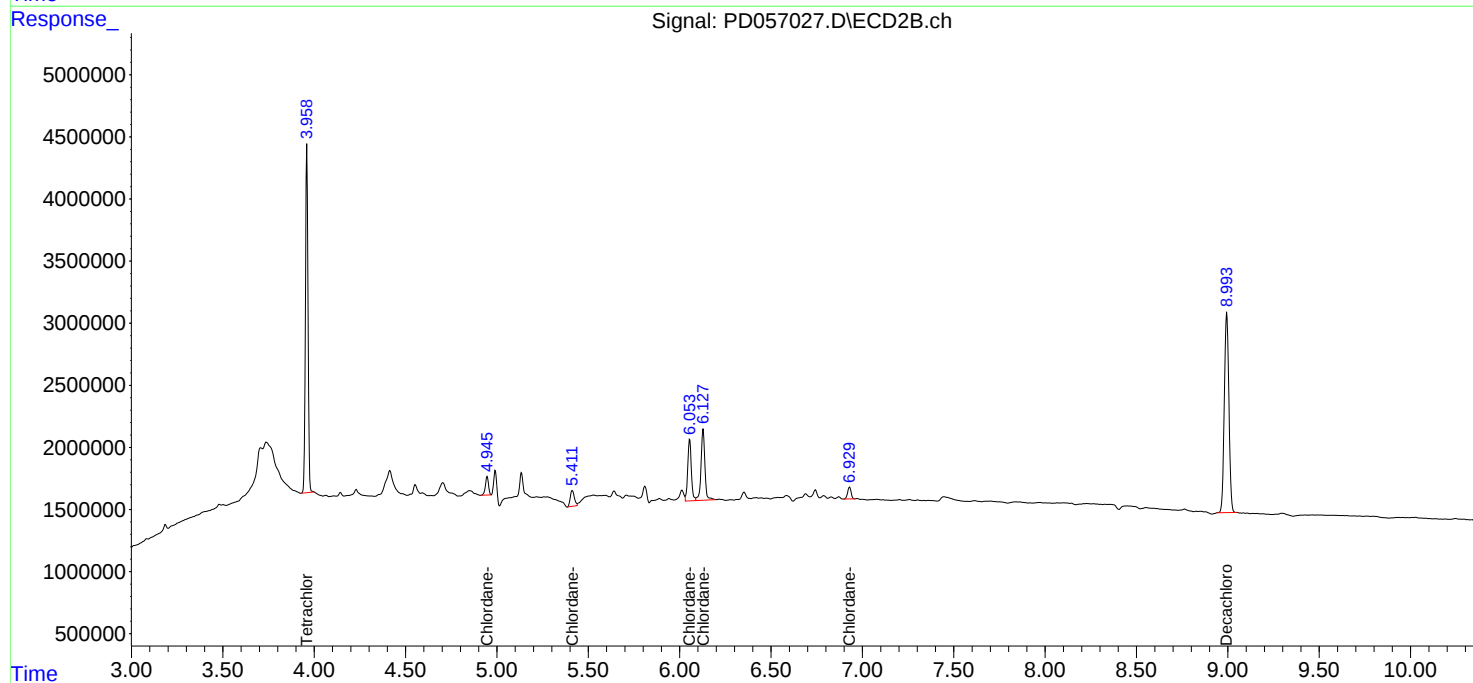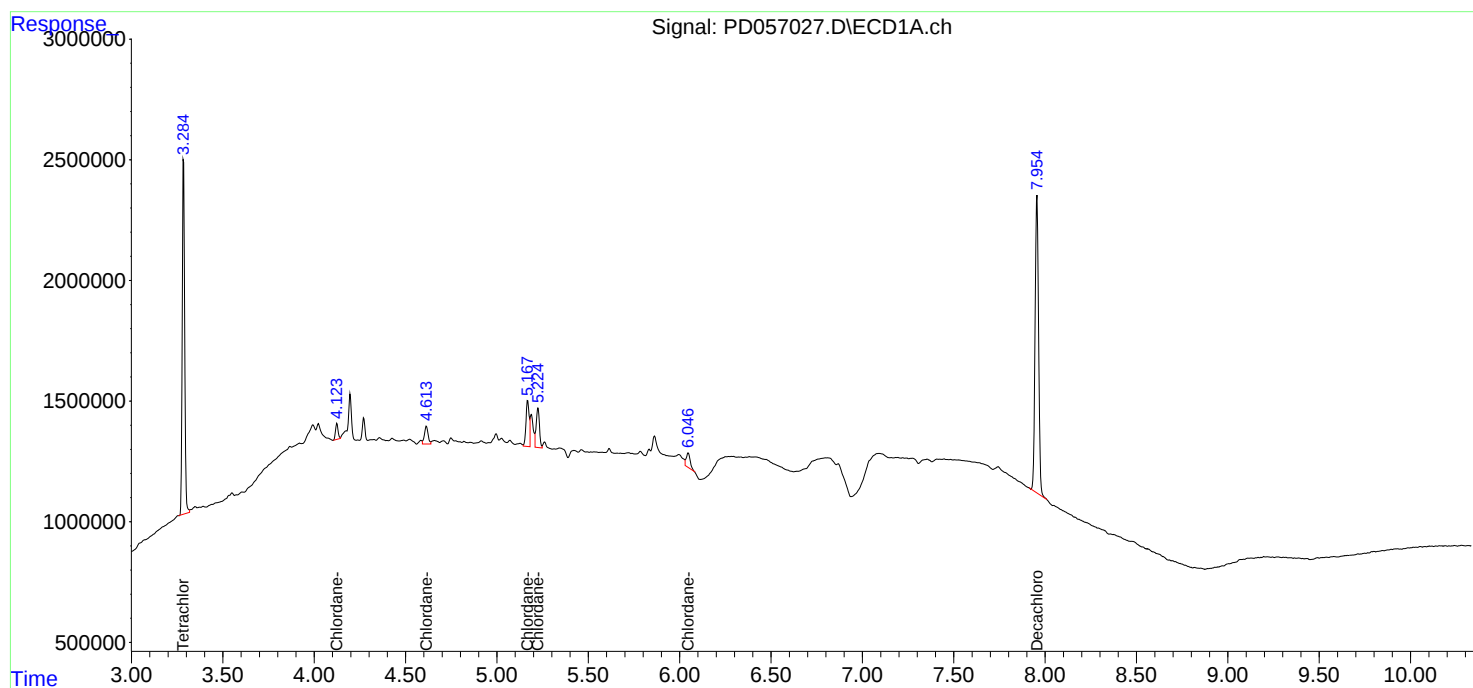


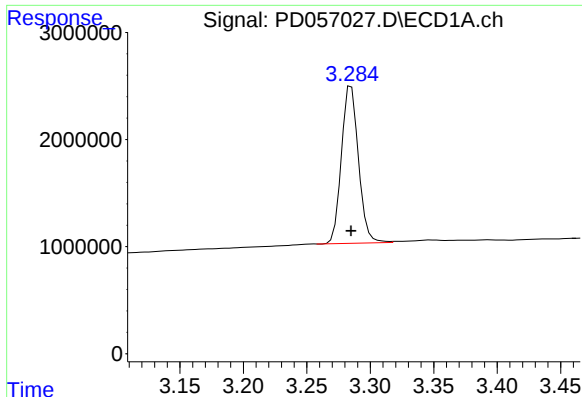

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 13691263
Conc: 16.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT1-2020

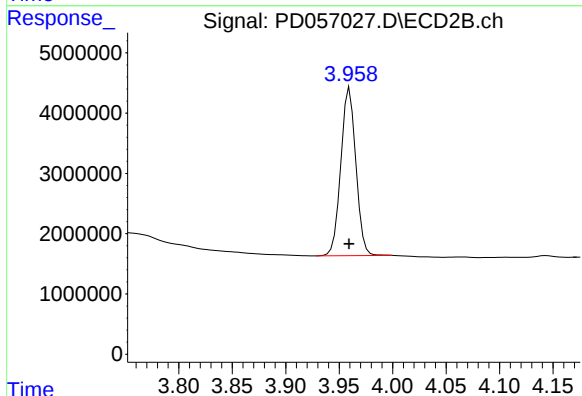


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 27294830
Conc: 16.68 ng/ml

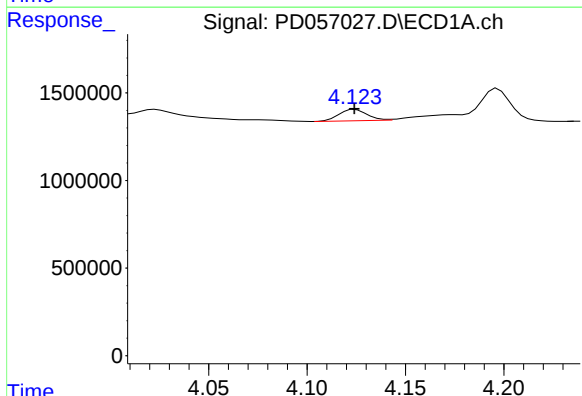


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 643001
Conc: 23.25 ng/ml

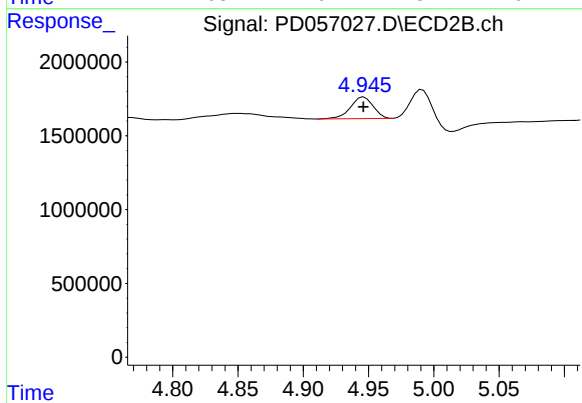

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 1765826
Conc: 27.33 ng/ml

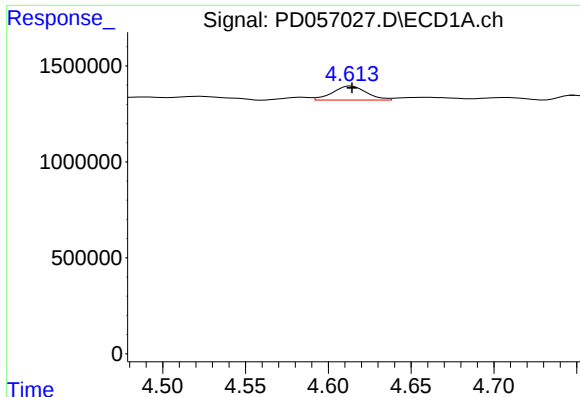

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 1039439
Conc: 29.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT1-2020

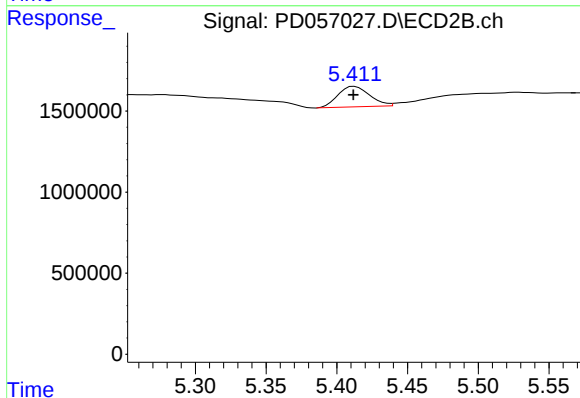


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 1970597
Conc: 28.73 ng/ml

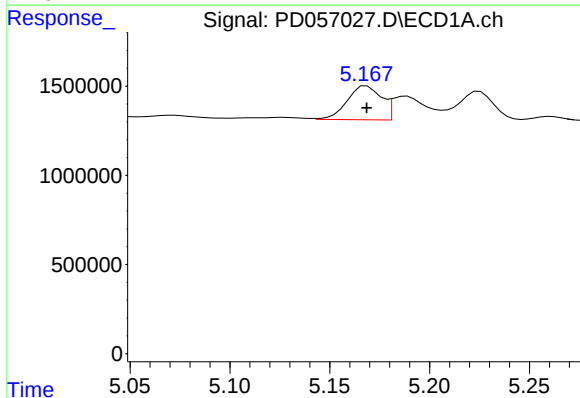


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 2258746
Conc: 23.07 ng/ml

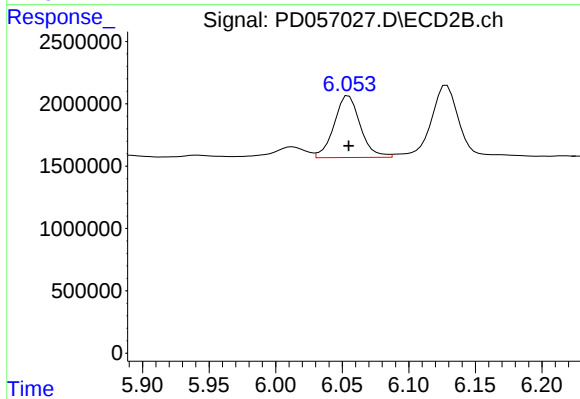

#25 Chlordane-3


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 6770158
Conc: 23.99 ng/ml

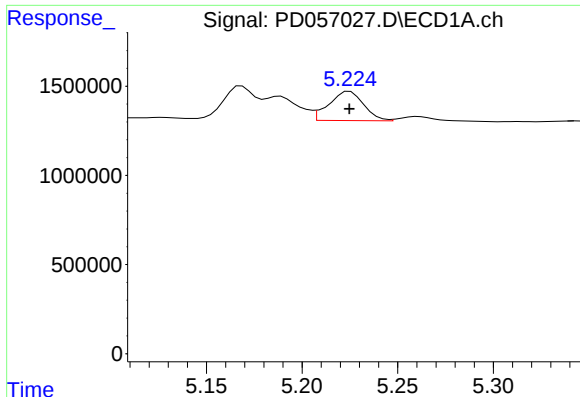

#26 Chlordane-4


R.T.: 5.225 min
Delta R.T.: 0.000 min
Response: 2071449
Conc: 23.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT1-2020

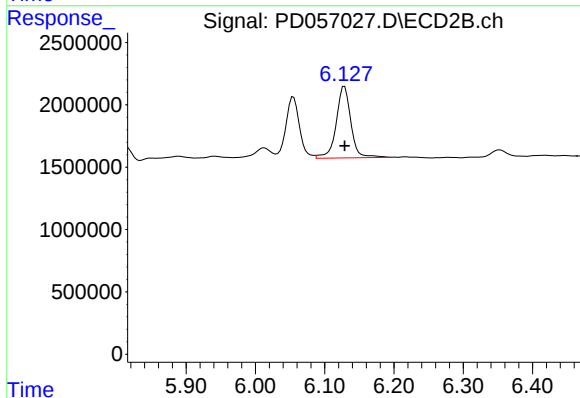


#26 Chlordane-4

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 8414016
Conc: 24.92 ng/ml

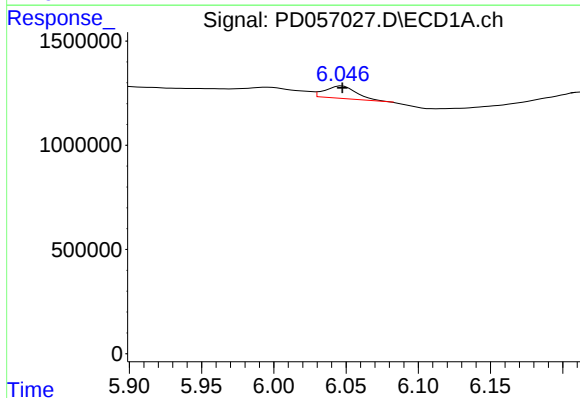


#27 Chlordane-5

R.T.: 6.047 min
Delta R.T.: 0.000 min
Response: 865368
Conc: 25.01 ng/ml

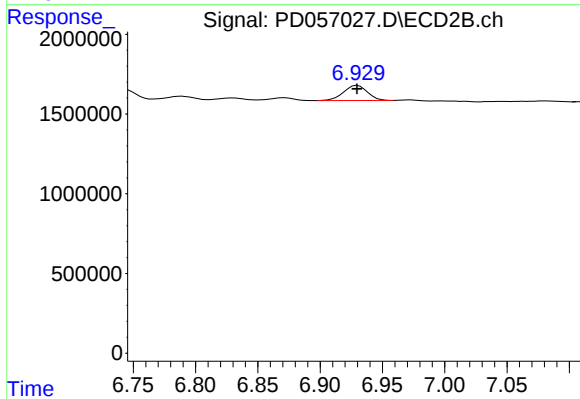

#27 Chlordane-5


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 1271840
Conc: 22.78 ng/ml

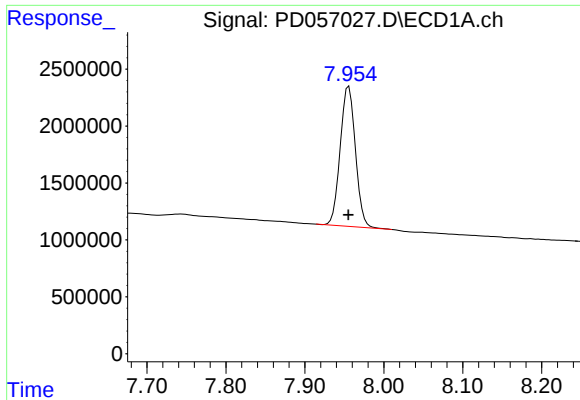

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 16431553
Conc: 16.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
MDL-WATER-03-QT1-2020

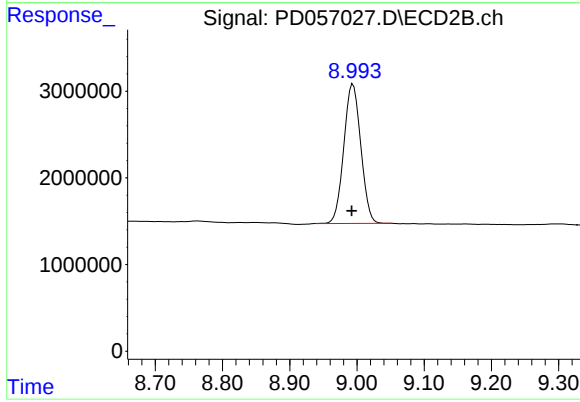

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 28196327
Conc: 16.92 ng/ml