

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
 Data File : PD057032.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2020 03:56
 Operator : AJ\MA
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 04:32:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 20 05:43:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.959	44797492	82211643	54.244	50.241
28)	SA Decachlor...	7.956	8.994	46733357	77980926	48.219	46.786
Target Compounds							
23)	Chlordane-1	4.124	4.947	13809319	32570817	499.358	504.054
24)	Chlordane-2	4.615	5.412	16525947	34613800	471.403	504.606
25)	Chlordane-3	5.168	6.055	48016306	141.0E6	490.339	499.857
26)	Chlordane-4	5.224	6.129	41696949	168.6E6	479.482	499.261
27)	Chlordane-5	6.048	6.929	16525922	29257242	477.643	524.068



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012120\
Data File : PD057032.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2020 03:56
Operator : AJ\MA
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 04:32:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011820.M
Quant Title : GC Extractables
QLast Update : Mon Jan 20 05:43:46 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

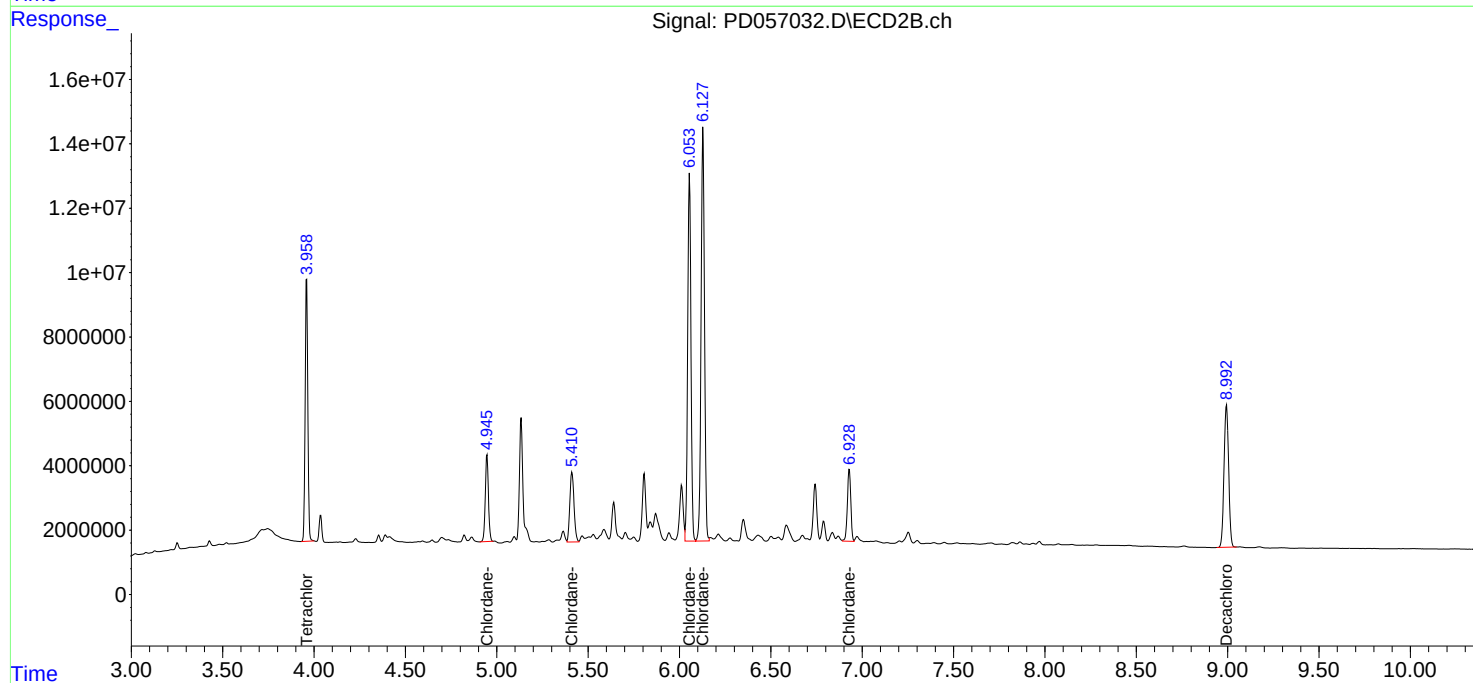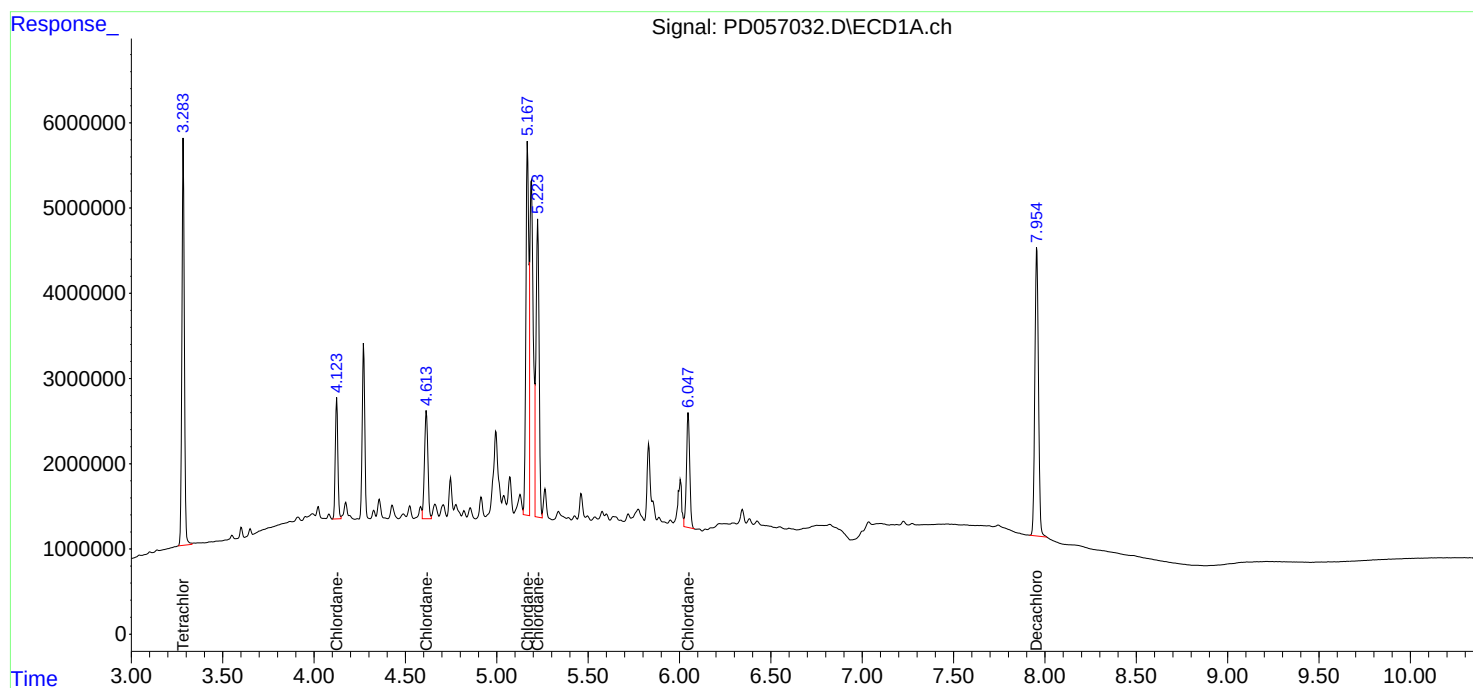


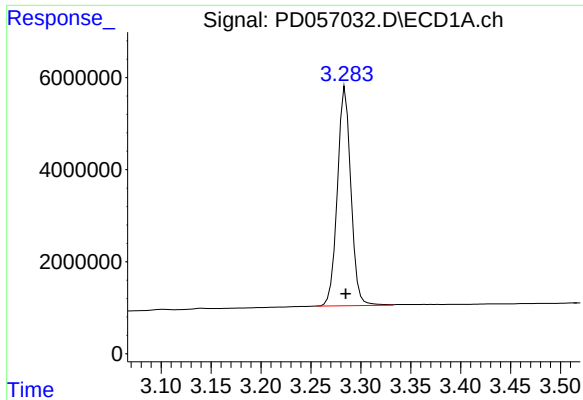

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 44797492
Conc: 54.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

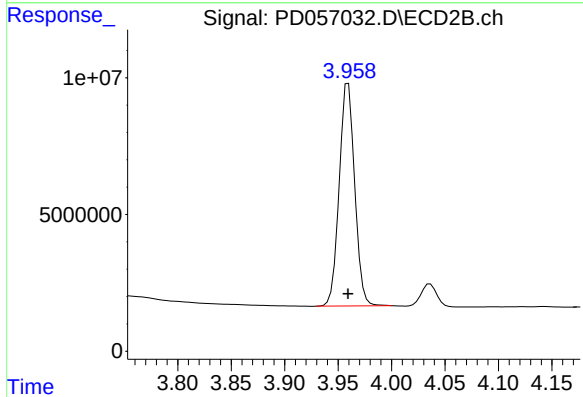


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 82211643
Conc: 50.24 ng/ml

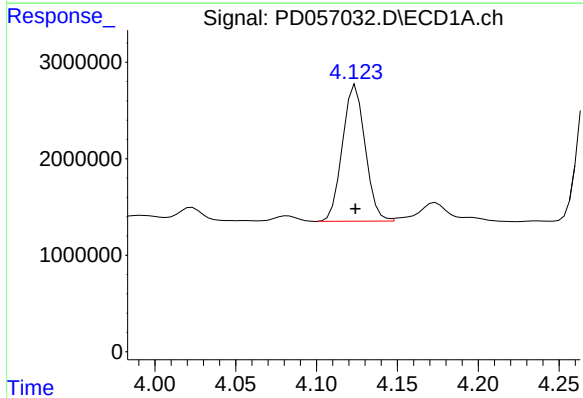


#23 Chlordane-1

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 13809319
Conc: 499.36 ng/ml

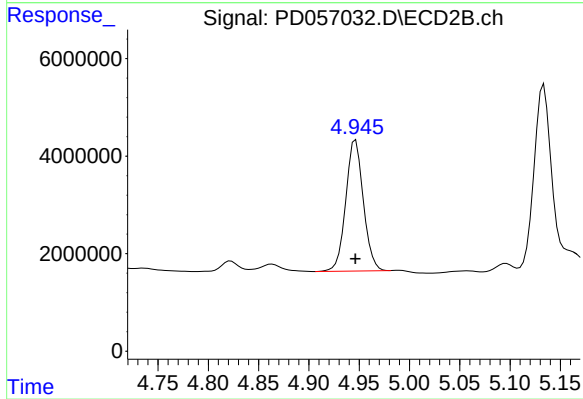

#23 Chlordane-1


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 32570817
Conc: 504.05 ng/ml

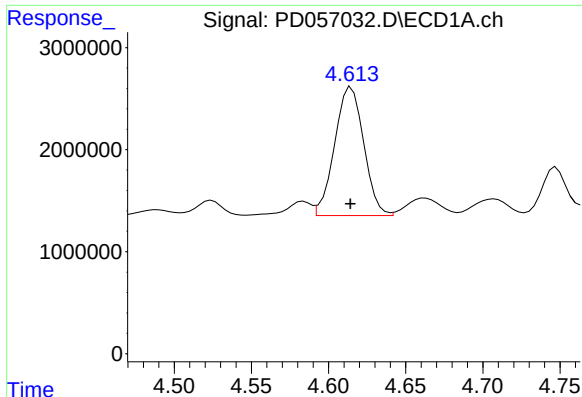

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: 0.000 min
Response: 16525947
Conc: 471.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

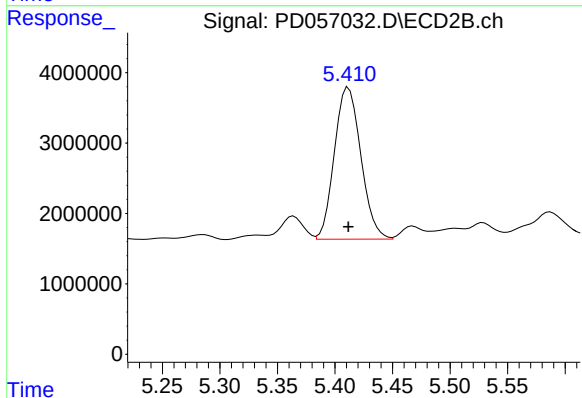


#24 Chlordane-2

R.T.: 5.412 min
Delta R.T.: 0.000 min
Response: 34613800
Conc: 504.61 ng/ml

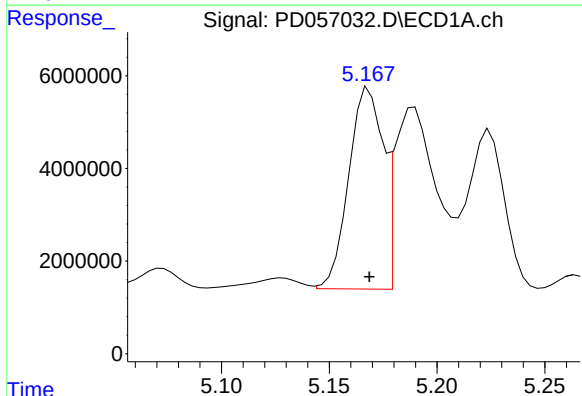


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 48016306
Conc: 490.34 ng/ml

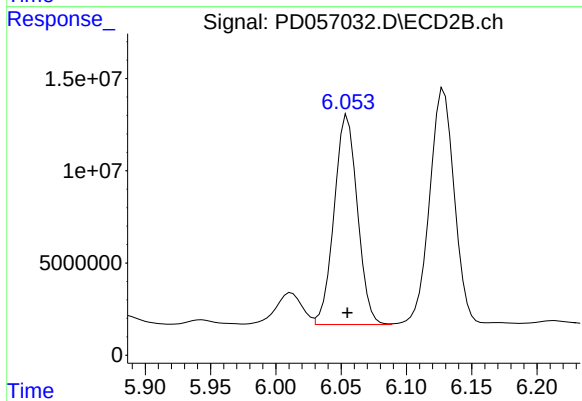

#25 Chlordane-3


R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 141035461
Conc: 499.86 ng/ml

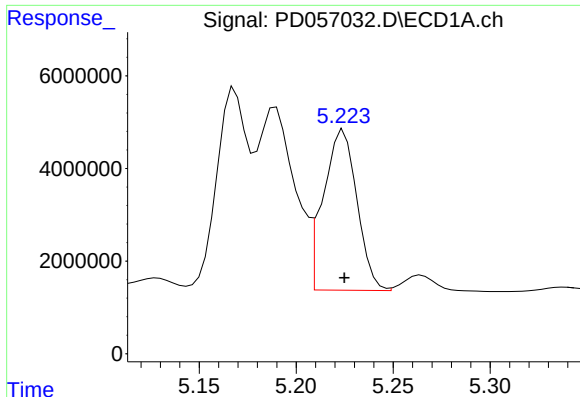

#26 Chlordane-4


R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 41696949
Conc: 479.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

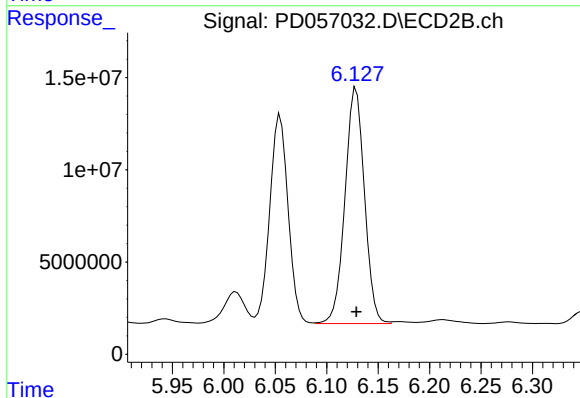


#26 Chlordane-4

R.T.: 6.129 min
Delta R.T.: 0.000 min
Response: 168591017
Conc: 499.26 ng/ml

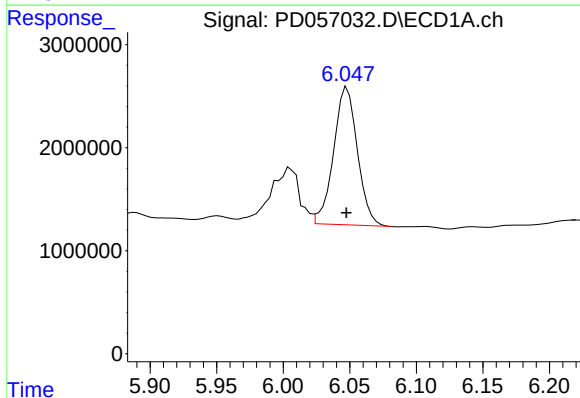


#27 Chlordane-5

R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 16525922
Conc: 477.64 ng/ml

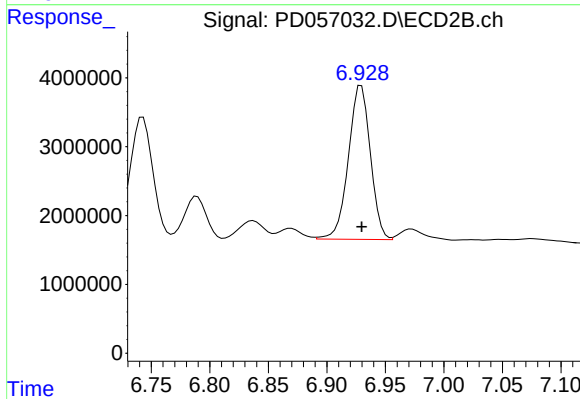

#27 Chlordane-5


R.T.: 6.929 min
Delta R.T.: 0.000 min
Response: 29257242
Conc: 524.07 ng/ml

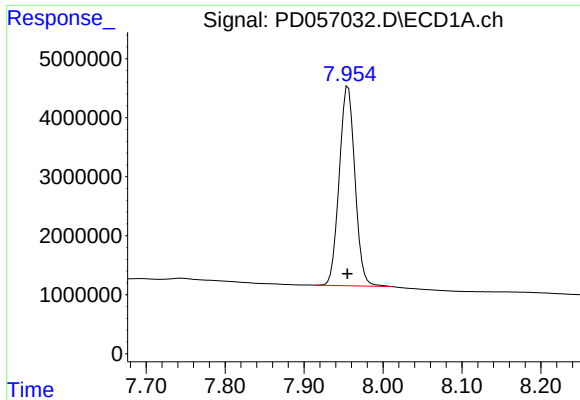

#28 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 46733357
Conc: 48.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

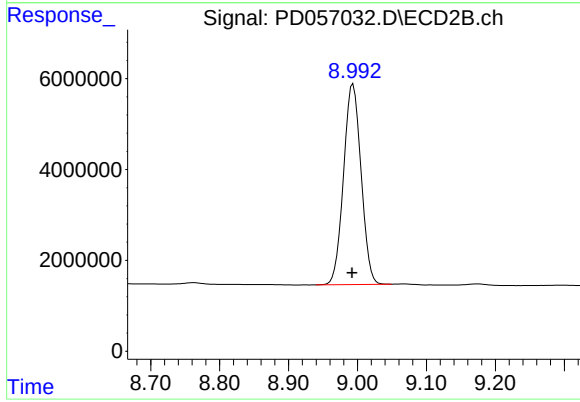

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.001 min
Response: 77980926
Conc: 46.79 ng/ml