

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012122\
 Data File : PD067750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 10:54
 Operator : AR\AJ
 Sample : N1196-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/24/2022
 Supervised By :Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 23:55:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.436	3.957	33319819	66603741	18.335	10.094m#
2) SA Decachlor...	8.153	9.007	9692948	16070437	10.912m	3.381m#
Target Compounds						
14) MA Endrin	5.971	6.670	18588117	43966308	8.849m	7.931m
20) A Methoxychlor	6.881	7.552	2705598	45382624	3.187m	15.641 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012122\
Data File : PD067750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 10:54
Operator : AR\AJ
Sample : N1196-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/24/2022
Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 23:55:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

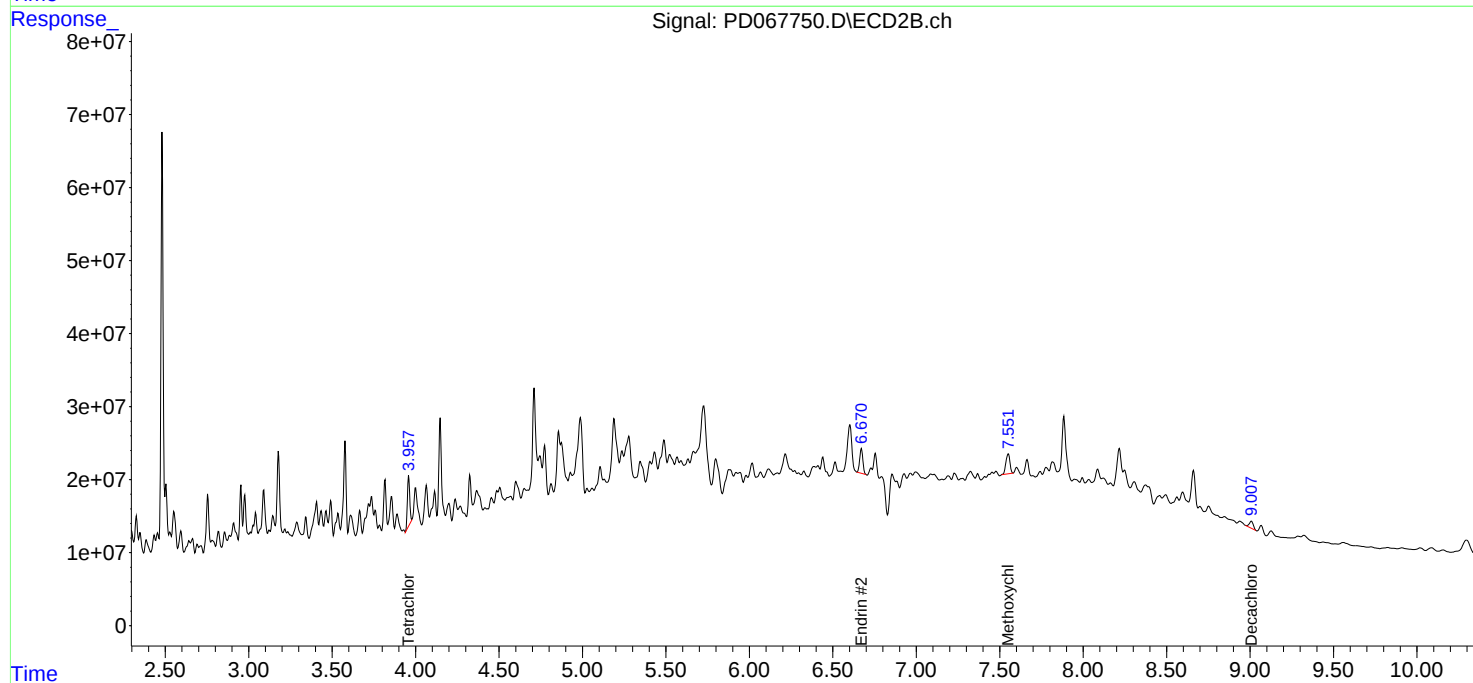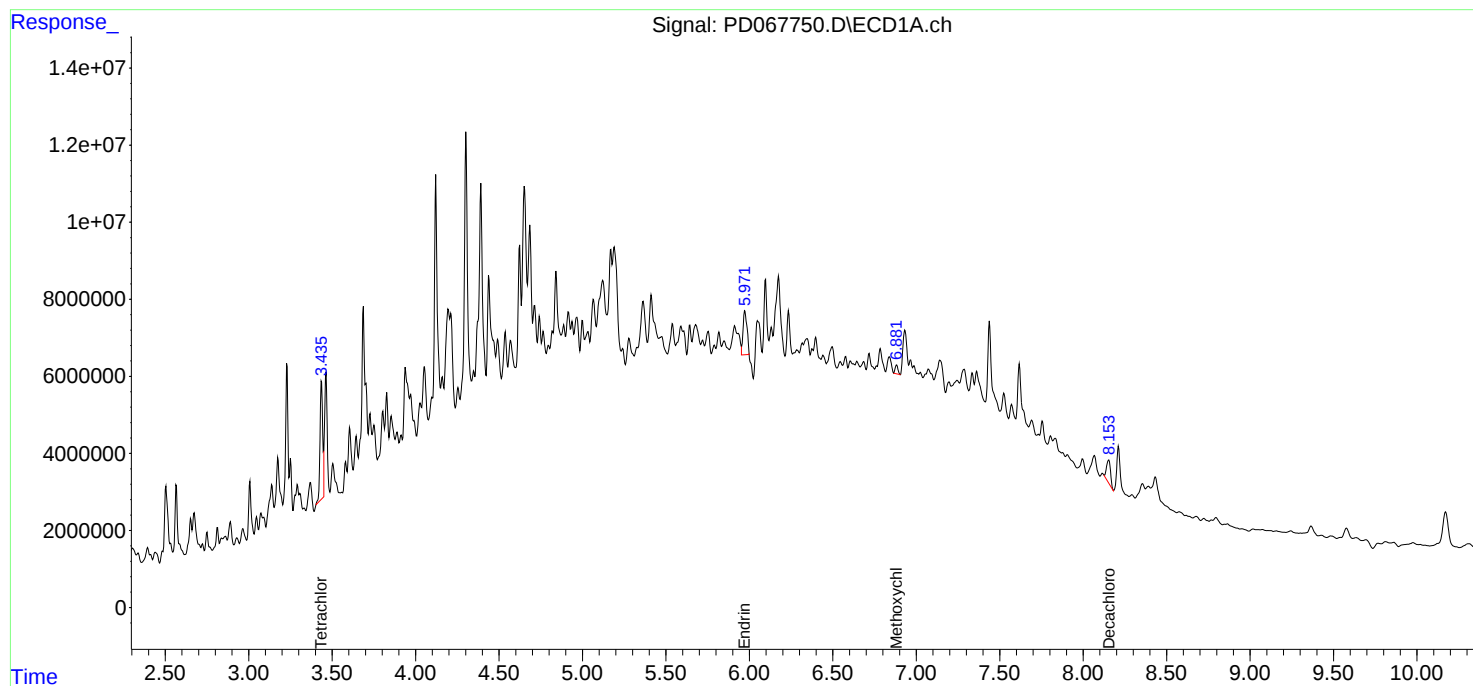

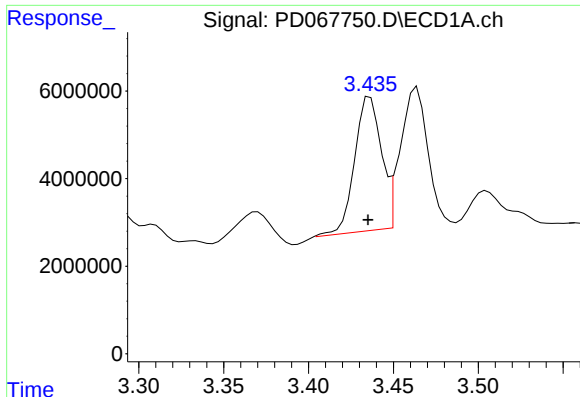


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: 0.001 min
Response: 33319819
Conc: 18.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2022
Supervised By :Ankita Jodhani 01/25/2022

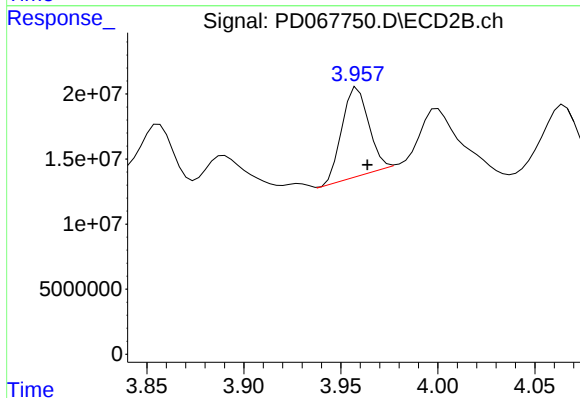


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.006 min
Response: 66603741
Conc: 10.09 ng/ml m

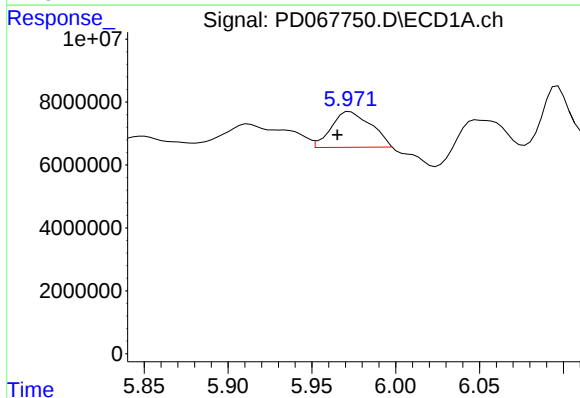


#14 Endrin

R.T.: 5.971 min
Delta R.T.: 0.006 min
Response: 18588117
Conc: 8.85 ng/ml m

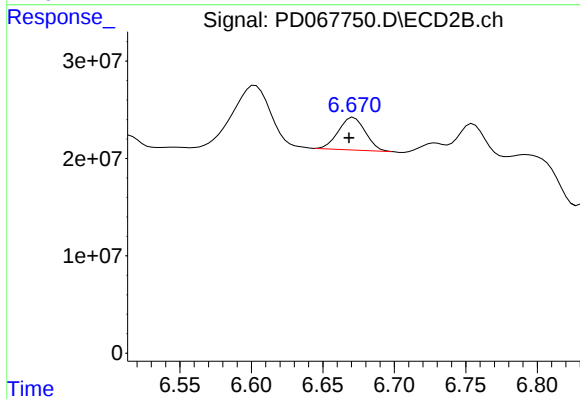

#14 Endrin

R.T.: 6.670 min
Delta R.T.: 0.002 min
Response: 43966308
Conc: 7.93 ng/ml m

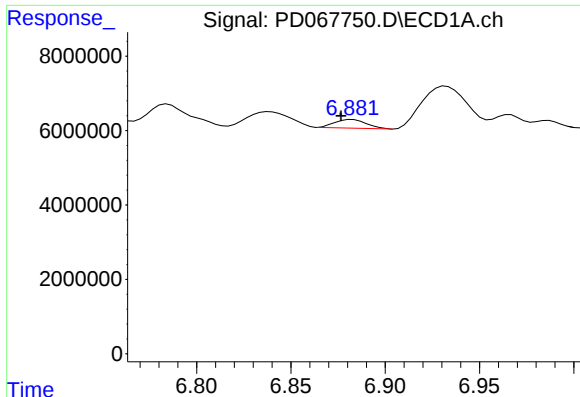


#20 Methoxychlor

R.T.: 6.881 min
Delta R.T.: 0.005 min
Response: 2705598
Conc: 3.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2022
Supervised By :Ankita Jodhani 01/25/2022

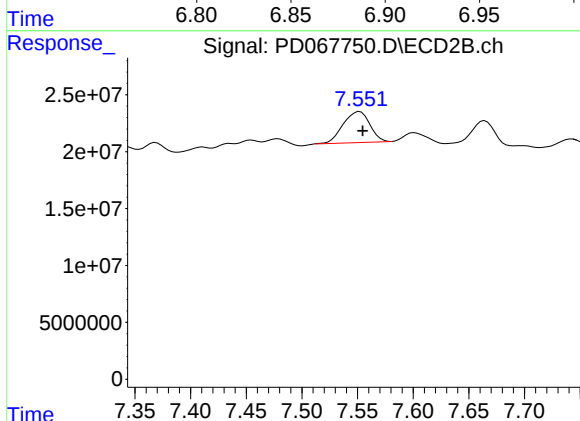


#20 Methoxychlor

R.T.: 7.552 min
Delta R.T.: -0.003 min
Response: 45382624
Conc: 15.64 ng/ml

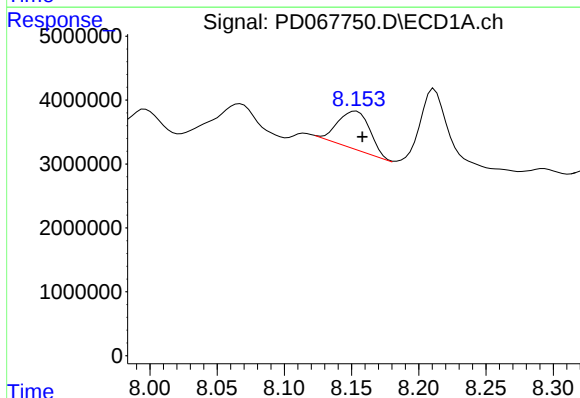

#28 Decachlorobiphenyl

R.T.: 8.153 min
Delta R.T.: -0.005 min
Response: 9692948
Conc: 10.91 ng/ml m

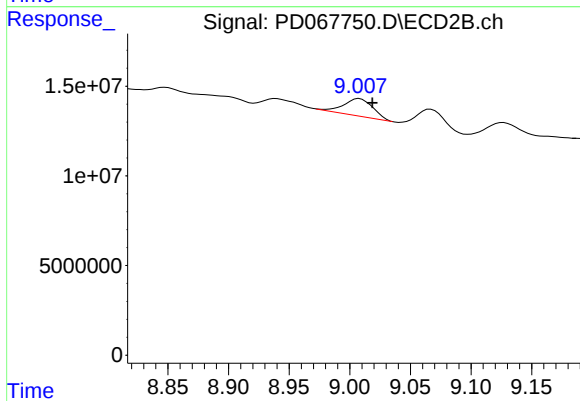

#28 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.012 min
Response: 16070437
Conc: 3.38 ng/ml m