

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012122\
 Data File : PD067751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 11:08
 Operator : AR\AJ
 Sample : N1196-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-DECANTRE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/24/2022
 Supervised By :Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 23:56:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.432	3.958	33922056	68111375	18.667	10.323m#
2) SA Decachlor...	8.145	9.007	8461446	11819456	9.526m	2.487m#
Target Compounds						
14) MA Endrin	5.963	6.670	21309270	55550226	10.144m	10.020m
20) A Methoxychlor	6.875	7.548	3195898	47302911	3.765m	16.303 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012122\
Data File : PD067751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 11:08
Operator : AR\AJ
Sample : N1196-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/24/2022
Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 23:56:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

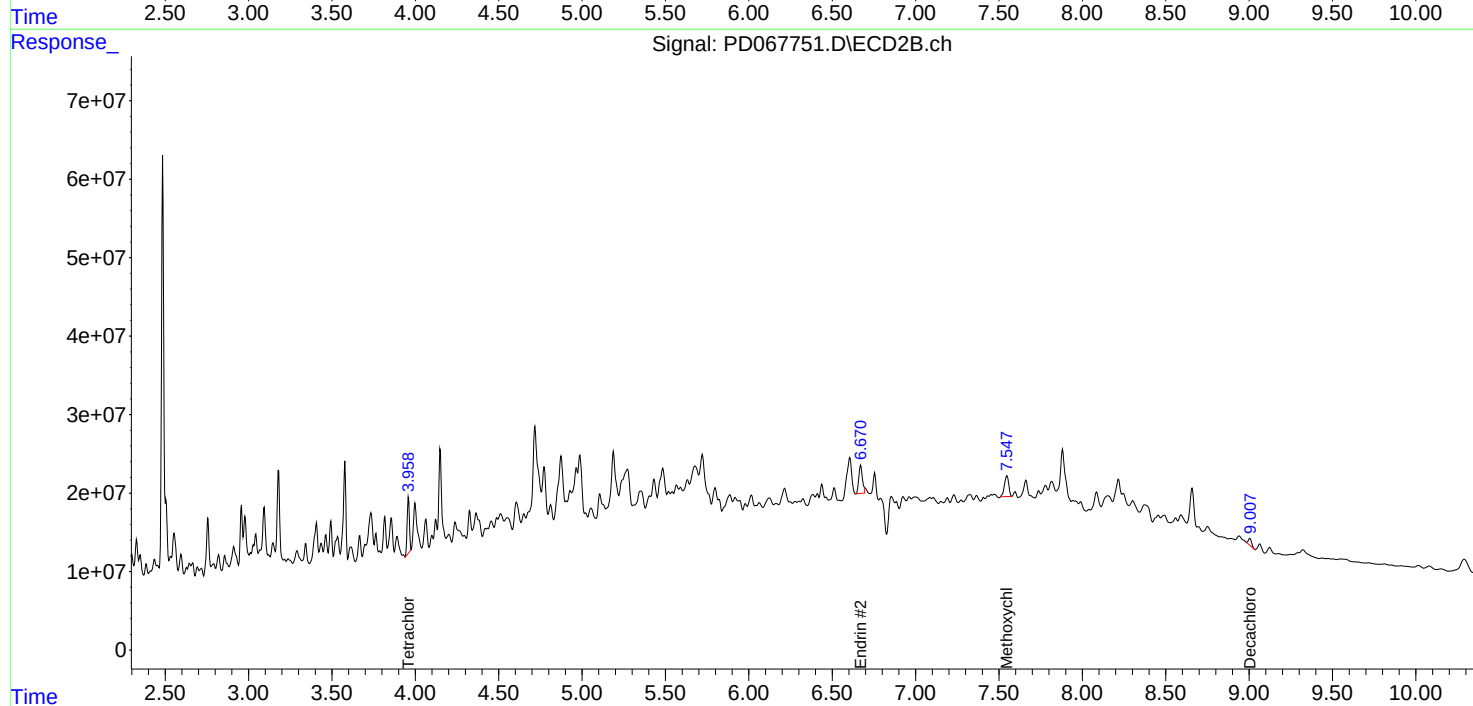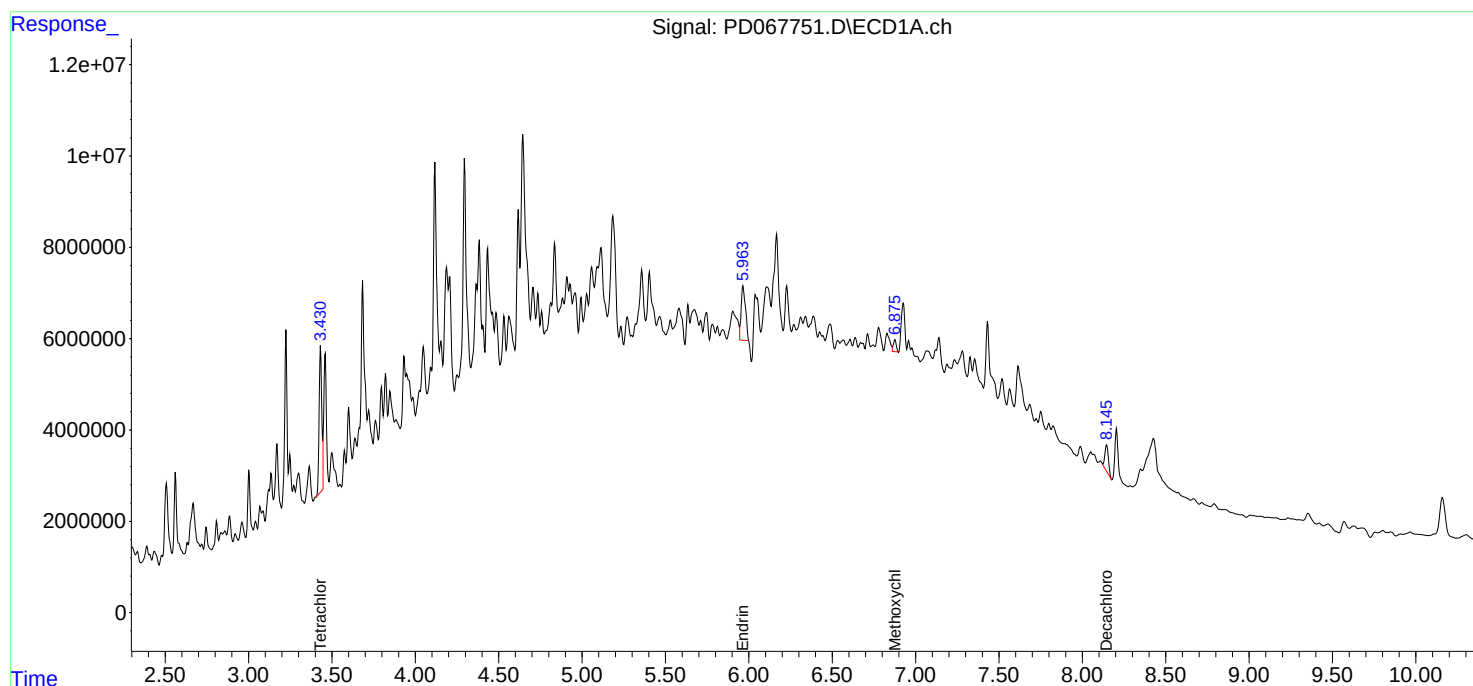

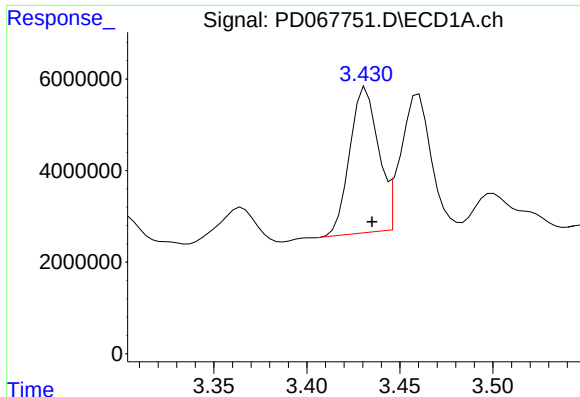


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: -0.003 min
Response: 33922056
Conc: 18.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2022
Supervised By :Ankita Jodhani 01/25/2022

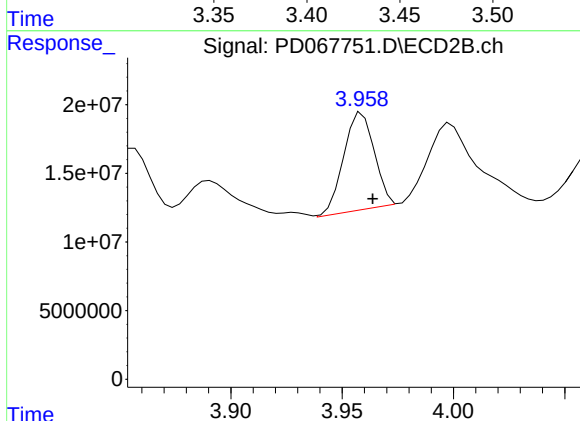


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: -0.006 min
Response: 68111375
Conc: 10.32 ng/ml m

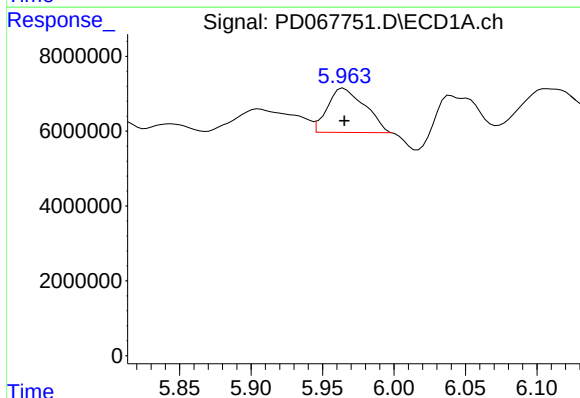


#14 Endrin

R.T.: 5.963 min
Delta R.T.: -0.002 min
Response: 21309270
Conc: 10.14 ng/ml m

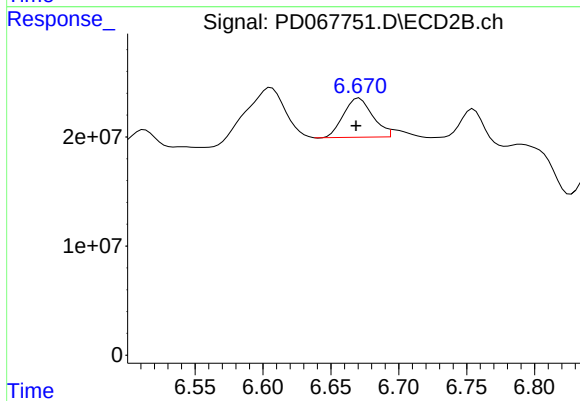

#14 Endrin

R.T.: 6.670 min
Delta R.T.: 0.001 min
Response: 55550226
Conc: 10.02 ng/ml m

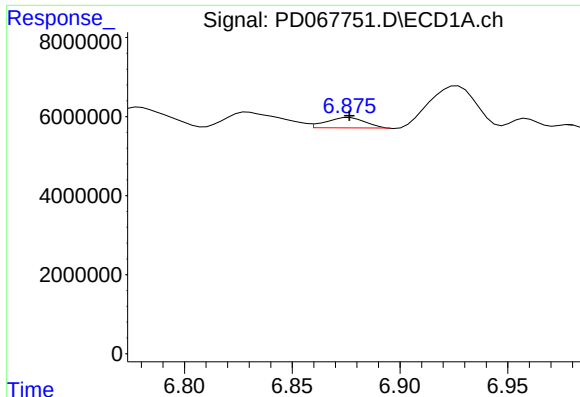


#20 Methoxychlor

R.T.: 6.875 min
Delta R.T.: -0.001 min
Response: 3195898
Conc: 3.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2022
Supervised By :Ankita Jodhani 01/25/2022

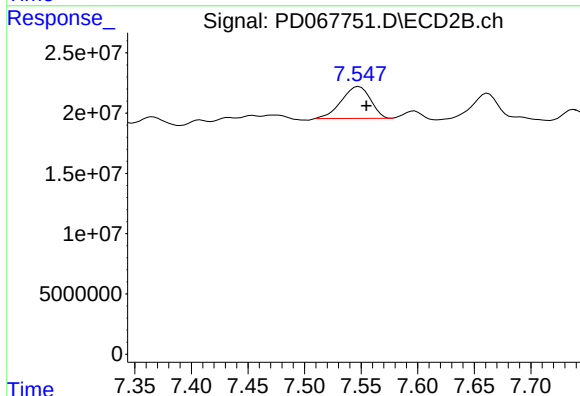


#20 Methoxychlor

R.T.: 7.548 min
Delta R.T.: -0.007 min
Response: 47302911
Conc: 16.30 ng/ml

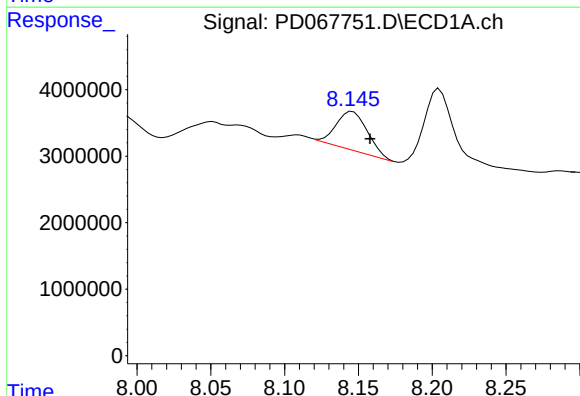

#28 Decachlorobiphenyl

R.T.: 8.145 min
Delta R.T.: -0.013 min
Response: 8461446
Conc: 9.53 ng/ml m

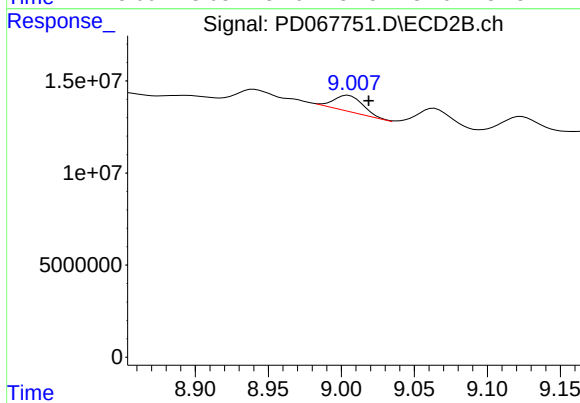

#28 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.012 min
Response: 11819456
Conc: 2.49 ng/ml m