

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012122\
 Data File : PD067752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2022 11:27
 Operator : AR\AJ
 Sample : N1197-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/24/2022
 Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 23:56:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 03:00:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.434	3.957	33625341	104.3E6	18.504	15.802m
28) SA Decachlor...	8.153	9.007	5751436	30575359	6.475	6.433
Target Compounds						
16) A 4,4'-DDD	6.099	6.789	16843519	36238871	9.804	7.239m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012122\
Data File : PD067752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2022 11:27
Operator : AR\AJ
Sample : N1197-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/24/2022
Supervised By : Ankita Jodhani 01/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 23:56:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PD122821.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 03:00:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

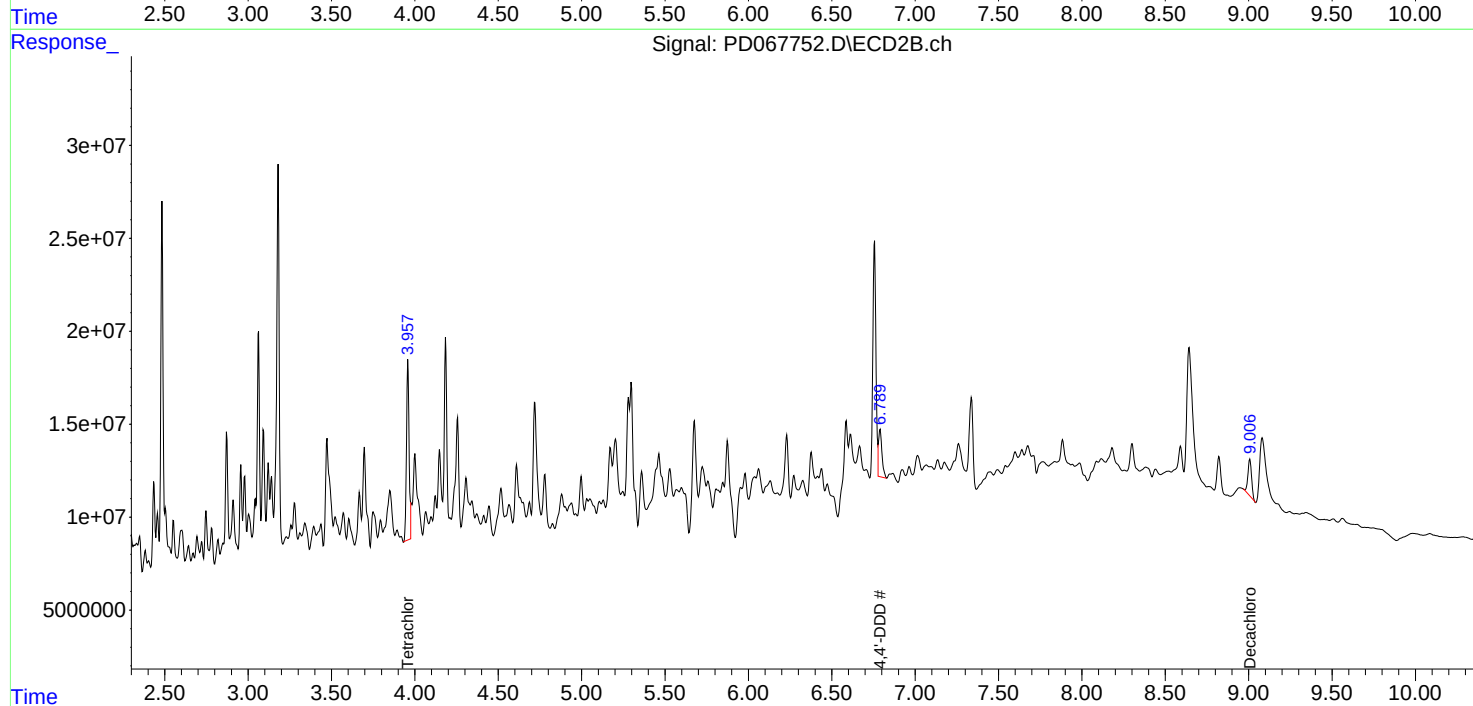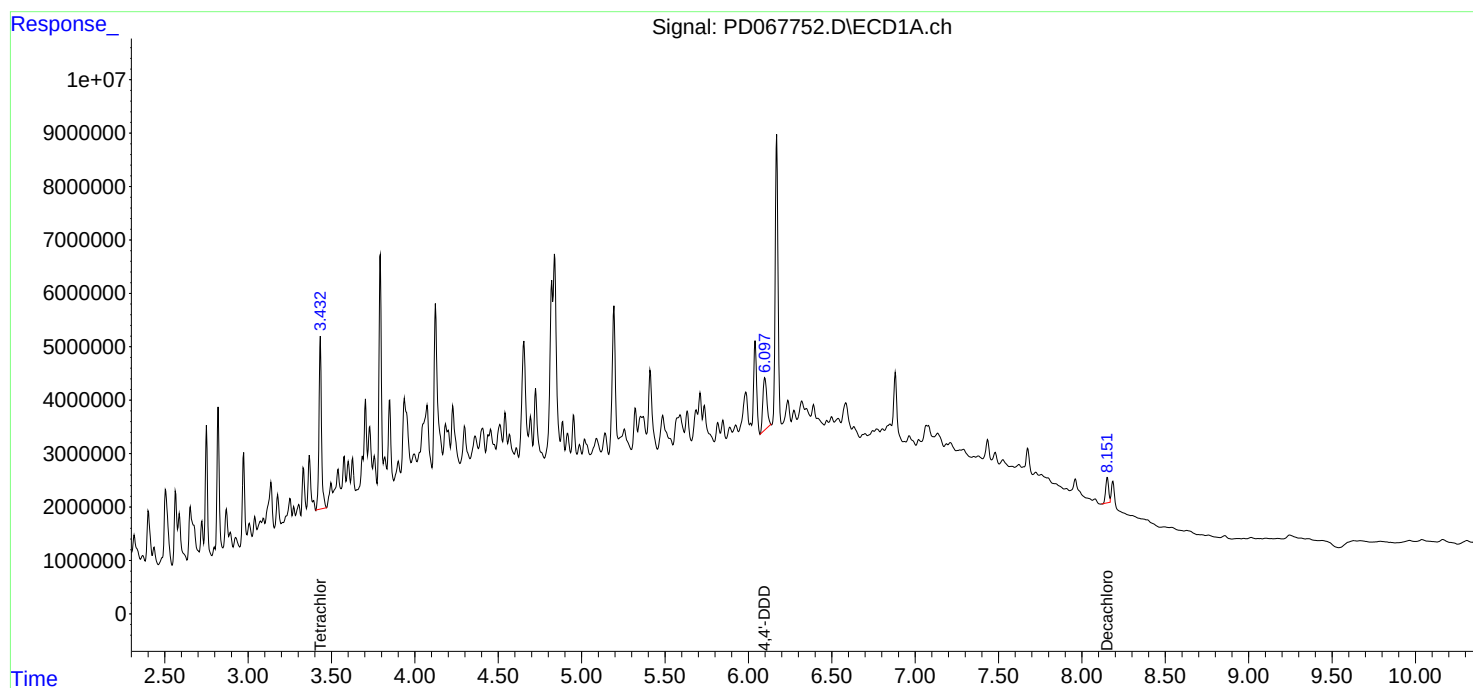

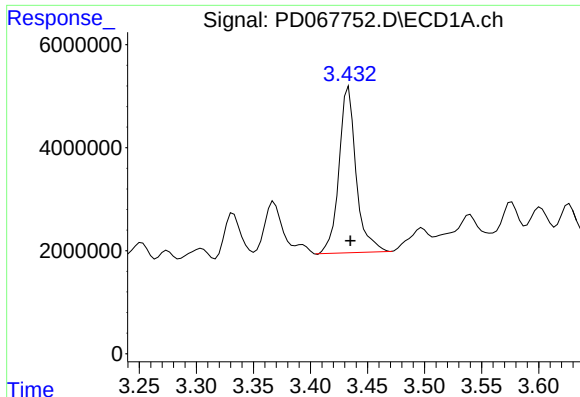


#1 Tetrachloro-m-xylene

R.T.: 3.434 min
Delta R.T.: -0.001 min
Response: 33625341
Conc: 18.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2022
Supervised By :Ankita Jodhani 01/25/2022

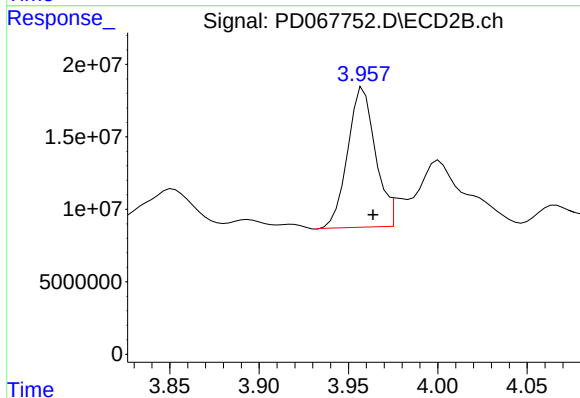


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.007 min
Response: 104263074
Conc: 15.80 ng/ml m

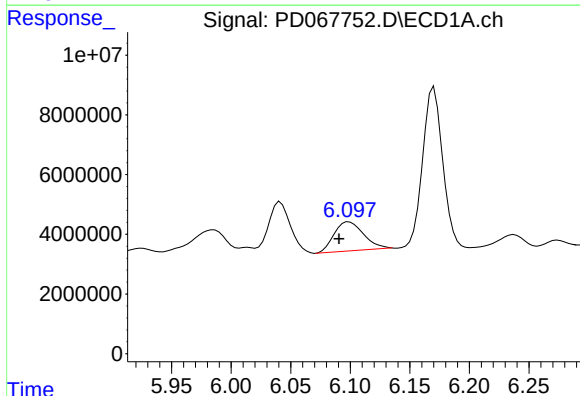


#16 4,4'-DDD

R.T.: 6.099 min
Delta R.T.: 0.008 min
Response: 16843519
Conc: 9.80 ng/ml

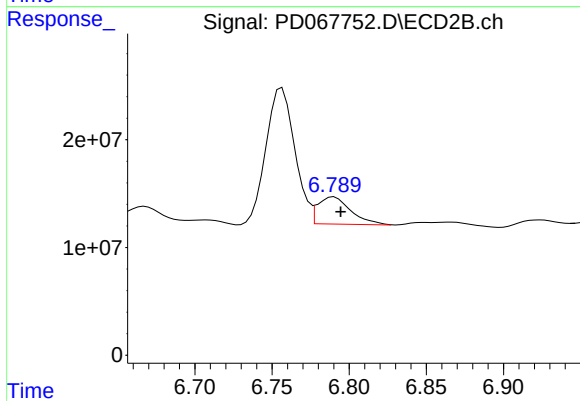

#16 4,4'-DDD

R.T.: 6.789 min
Delta R.T.: -0.006 min
Response: 36238871
Conc: 7.24 ng/ml m

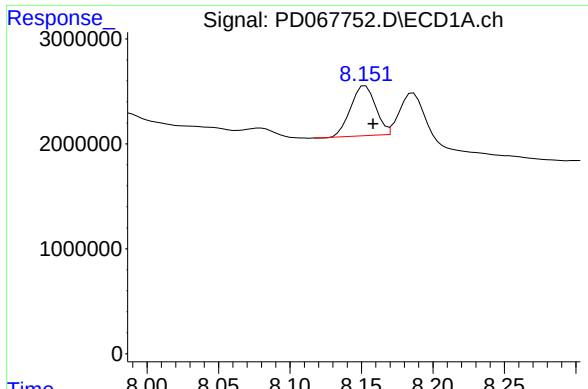


#28 Decachlorobiphenyl

R.T.: 8.153 min
Delta R.T.: -0.005 min
Response: 5751436
Conc: 6.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENT

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/24/2022
Supervised By :Ankita Jodhani 01/25/2022

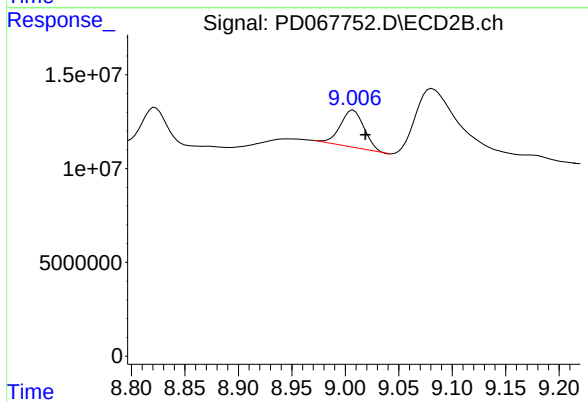

#28 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: -0.011 min
Response: 30575359
Conc: 6.43 ng/ml