

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012320\
 Data File : PD057062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2020 17:31
 Operator : AJ\MA
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA301

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 08:18:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 24 08:15:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	18062049	37083563	20.000	20.000
27)	SA Decachlor...	7.956	8.995	43098700	74570338	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.712	4.346	26311200	53042924	20.000	20.000
3)	MA gamma-BHC...	3.987	4.629	25797157	51159015	20.000	20.000
4)	MA Heptachlor	4.272	5.134	24395000	52522579	20.000	20.000
9)	A Endosulfan I	5.278	6.178	20797880	43527204	20.000	20.000
13)	MA Dieldrin	5.518	6.433	47060693	95499361	40.000	40.000
14)	MA Endrin	5.770	6.650	39736426	77771581	40.000	40.000
16)	A 4,4'-DDD	5.905	6.772	35333590	74148344	40.000	40.000
17)	MA 4,4'-DDT	6.140	7.070	34730665	75890013	40.000	40.000
20)	A Methoxychlor	6.688	7.527	94493382	204.1E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012320\
Data File : PD057062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2020 17:31
Operator : AJ\MA
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA301

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 08:18:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 24 08:15:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

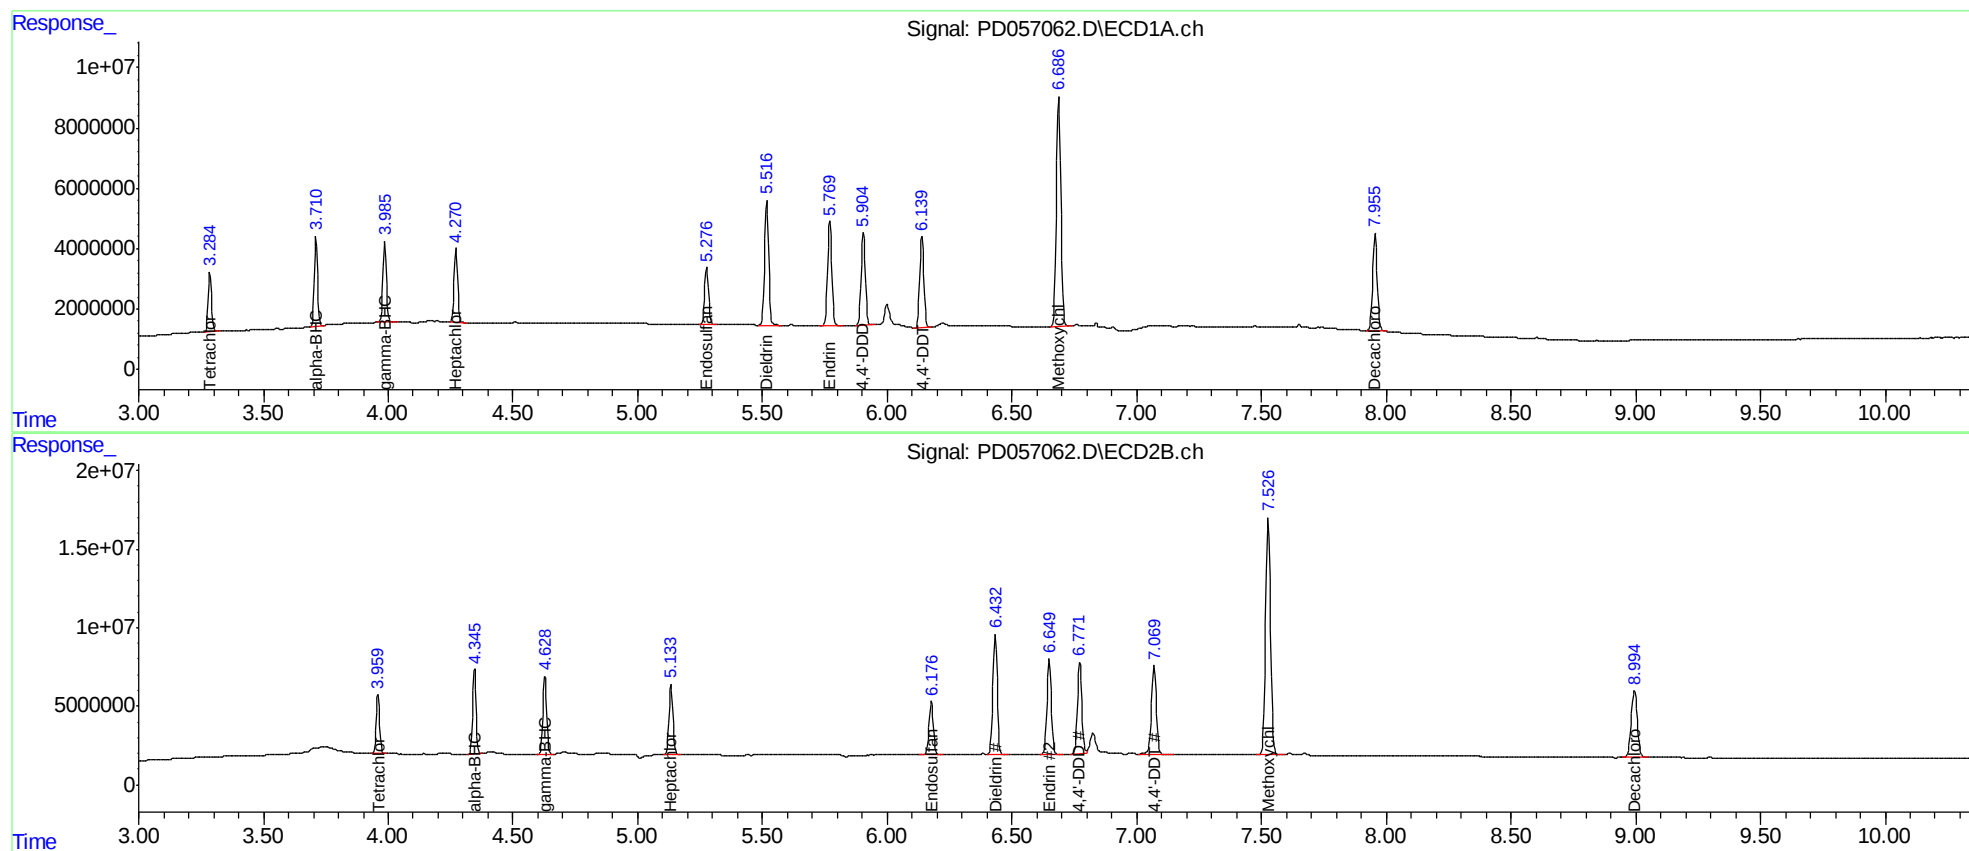


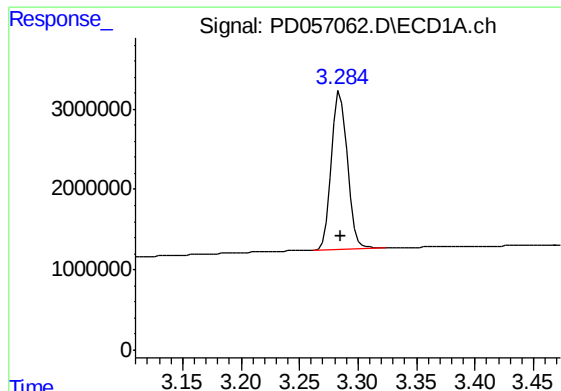

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 18062049
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

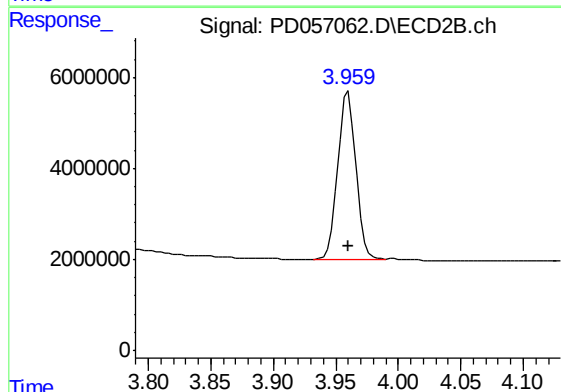


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 37083563
Conc: 20.00 ng/ml

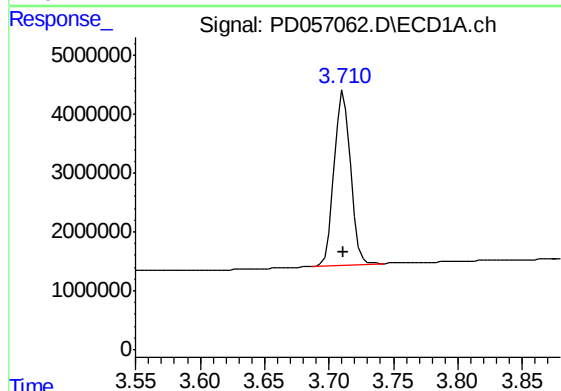


#2 alpha-BHC

R.T.: 3.712 min
Delta R.T.: 0.000 min
Response: 26311200
Conc: 20.00 ng/ml

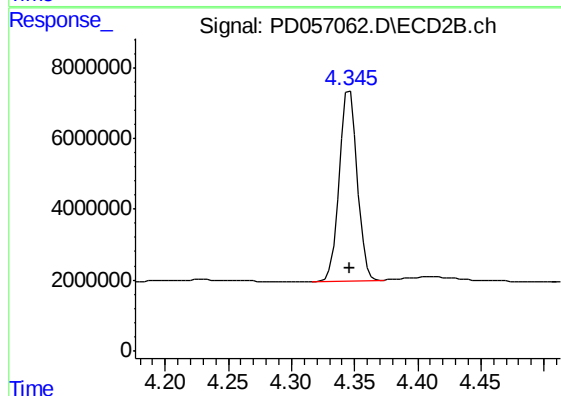

#2 alpha-BHC


R.T.: 4.346 min
Delta R.T.: 0.000 min
Response: 53042924
Conc: 20.00 ng/ml

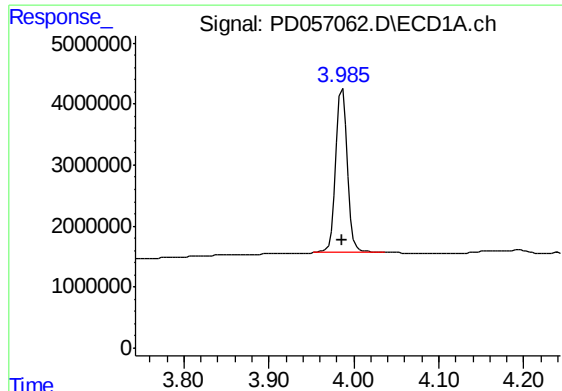

#3 gamma-BHC (Lindane)


R.T.: 3.987 min
Delta R.T.: 0.000 min
Response: 25797157
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

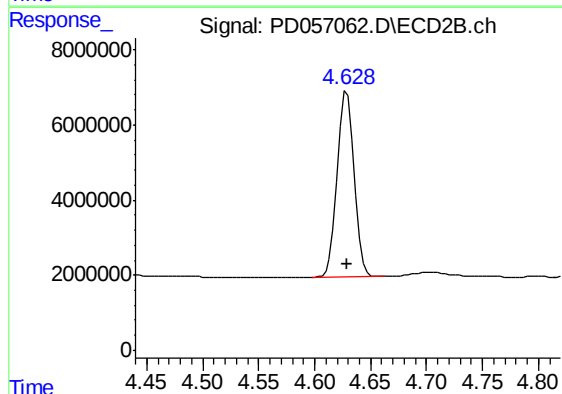


#3 gamma-BHC (Lindane)

R.T.: 4.629 min
Delta R.T.: 0.000 min
Response: 51159015
Conc: 20.00 ng/ml

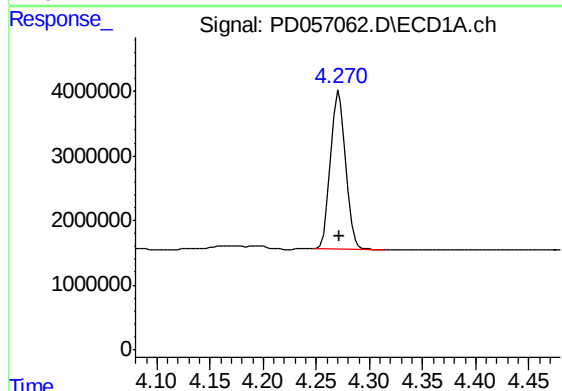


#4 Heptachlor

R.T.: 4.272 min
Delta R.T.: 0.000 min
Response: 24395000
Conc: 20.00 ng/ml

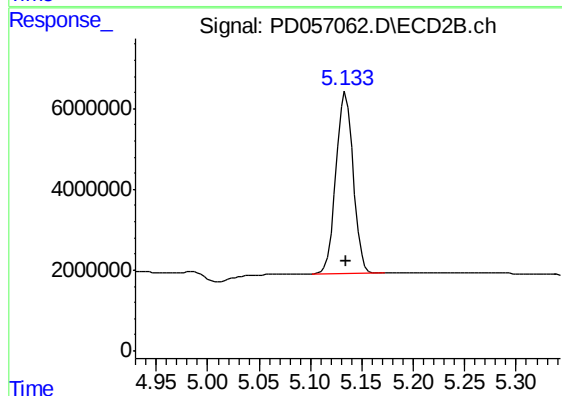

#4 Heptachlor


R.T.: 5.134 min
Delta R.T.: 0.000 min
Response: 52522579
Conc: 20.00 ng/ml

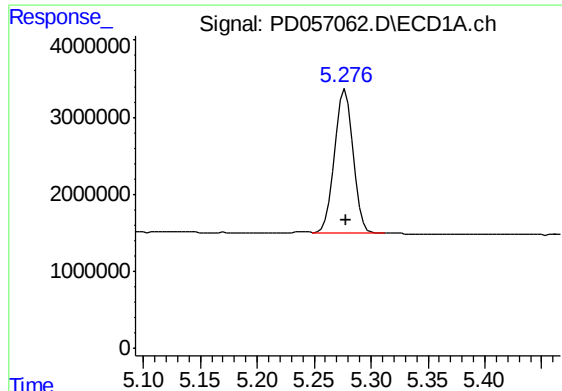

#9 Endosulfan I


R.T.: 5.278 min
Delta R.T.: 0.000 min
Response: 20797880
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

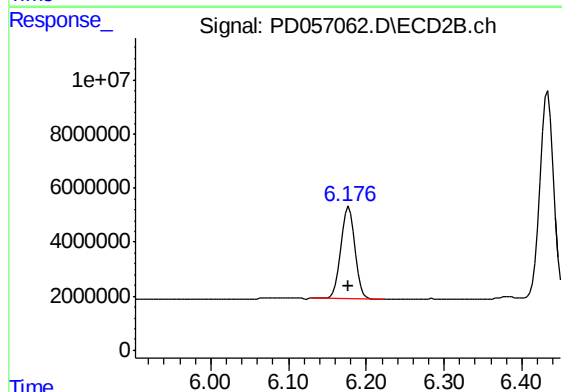


#9 Endosulfan I

R.T.: 6.178 min
Delta R.T.: 0.000 min
Response: 43527204
Conc: 20.00 ng/ml

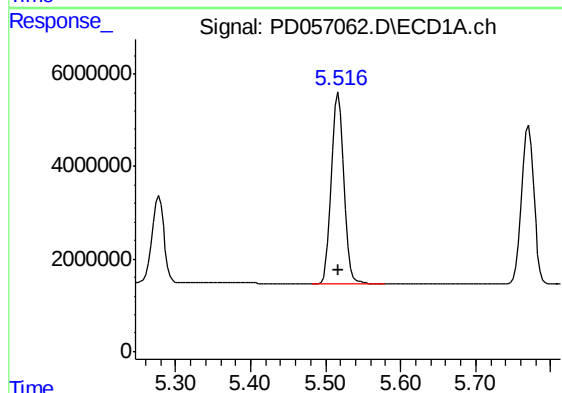


#13 Dieldrin

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 47060693
Conc: 40.00 ng/ml

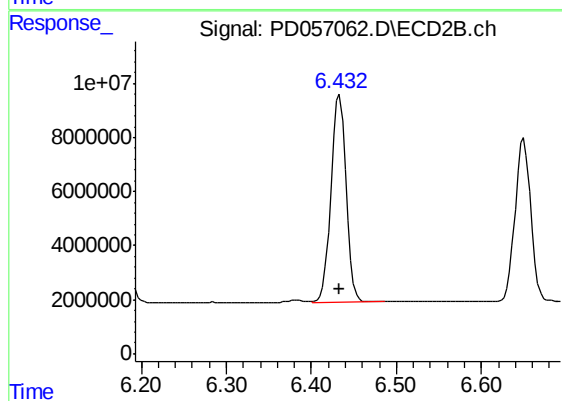

#13 Dieldrin


R.T.: 6.433 min
Delta R.T.: 0.000 min
Response: 95499361
Conc: 40.00 ng/ml

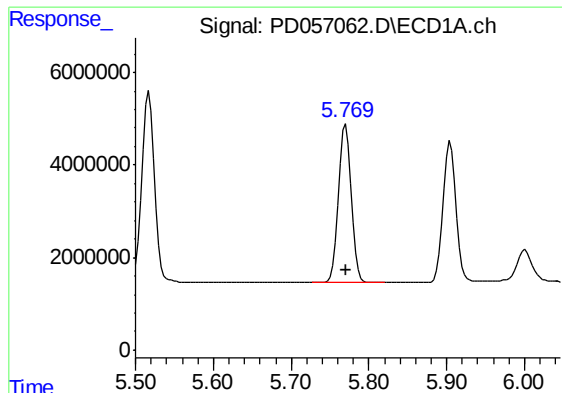

#14 Endrin


R.T.: 5.770 min
Delta R.T.: 0.000 min
Response: 39736426
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

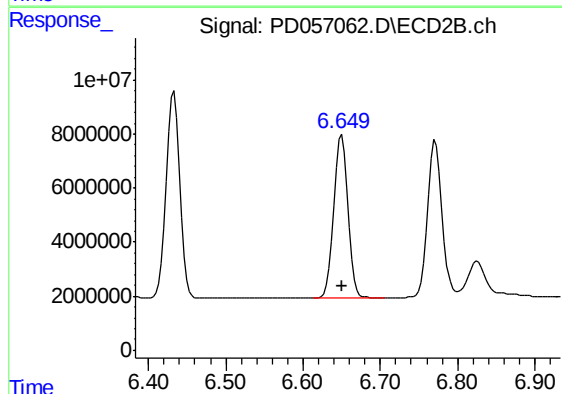


#14 Endrin

R.T.: 6.650 min
Delta R.T.: 0.000 min
Response: 77771581
Conc: 40.00 ng/ml

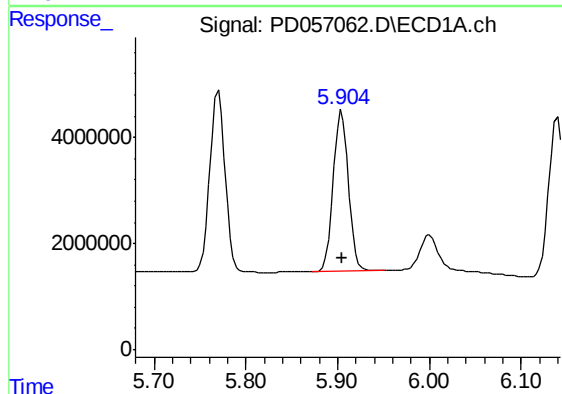


#16 4,4'-DDD

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 35333590
Conc: 40.00 ng/ml

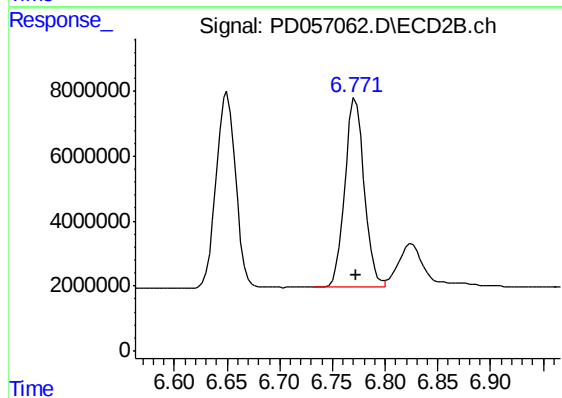

#16 4,4'-DDD


R.T.: 6.772 min
Delta R.T.: 0.000 min
Response: 74148344
Conc: 40.00 ng/ml

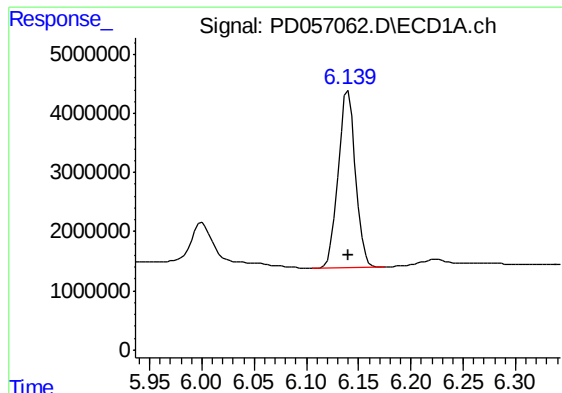

#17 4,4'-DDT


R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 34730665
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

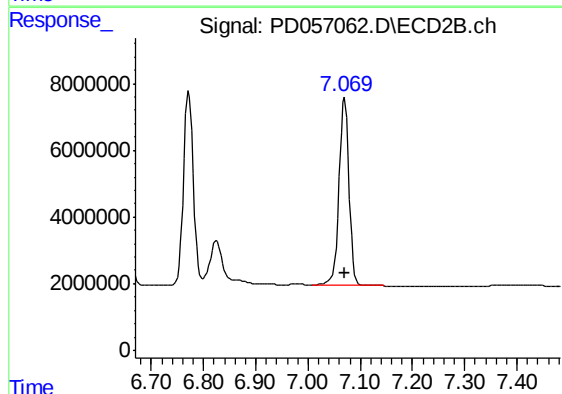


#17 4,4'-DDT

R.T.: 7.070 min
Delta R.T.: 0.000 min
Response: 75890013
Conc: 40.00 ng/ml

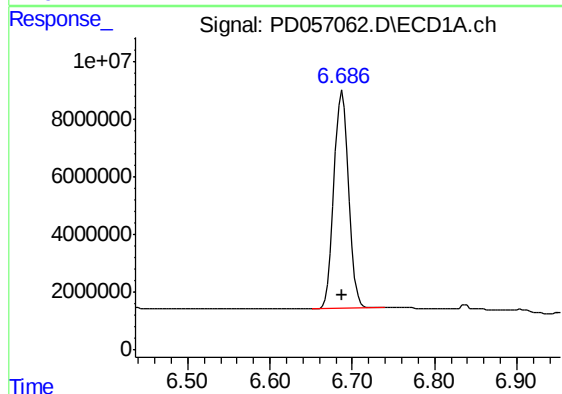


#20 Methoxychlor

R.T.: 6.688 min
Delta R.T.: 0.000 min
Response: 94493382
Conc: 200.00 ng/ml

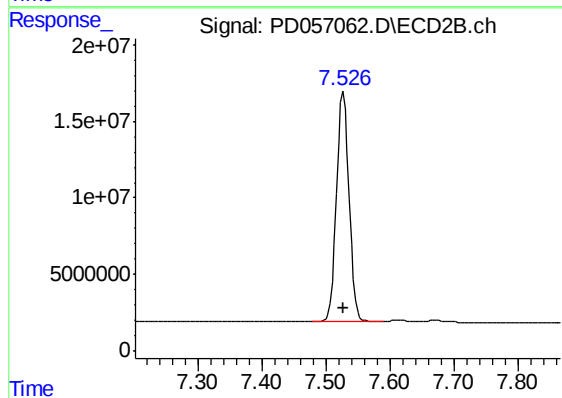

#20 Methoxychlor


R.T.: 7.527 min
Delta R.T.: 0.000 min
Response: 204085296
Conc: 200.00 ng/ml

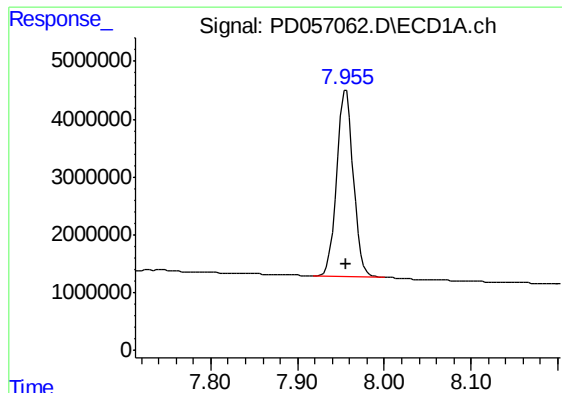

#27 Decachlorobiphenyl

R.T.: 7.956 min
Delta R.T.: 0.000 min
Response: 43098700
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA301

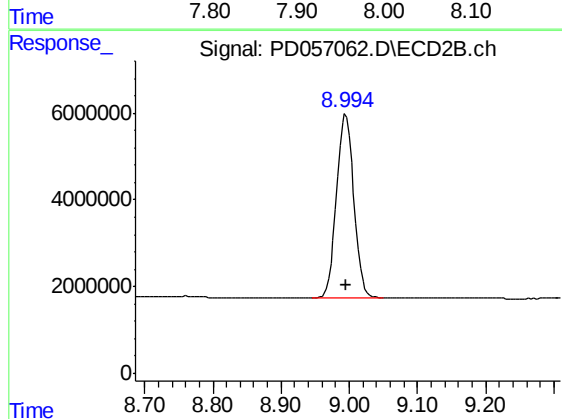

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.000 min
Response: 74570338
Conc: 40.00 ng/ml