

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012320\
 Data File : PD057066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2020 18:27
 Operator : AJ\MA
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 08:19:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 24 08:15:19 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.960	70444843	143.1E6	78.003	77.191
27)	SA Decachlor...	7.957	8.995	158.7E6	265.7E6	147.301	142.541
Target Compounds							
2)	A alpha-BHC	3.712	4.347	112.1E6	222.7E6	85.225	83.976
3)	MA gamma-BHC...	3.987	4.630	104.6E6	210.3E6	81.112	82.227
4)	MA Heptachlor	4.272	5.135	99166547	209.4E6	81.301	79.731
9)	A Endosulfan I	5.277	6.178	82853012	170.7E6	79.674	78.428
13)	MA Dieldrin	5.518	6.434	194.6E6	388.1E6	165.398	162.552
14)	MA Endrin	5.771	6.651	158.6E6	313.1E6	159.613	161.032
16)	A 4,4'-DDD	5.905	6.773	145.5E6	297.0E6	164.687	160.218
17)	MA 4,4'-DDT	6.140	7.071	154.5E6	313.2E6	177.976	165.071
20)	A Methoxychlor	6.688	7.528	351.5E6	742.0E6	743.905	727.169


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012320\
Data File : PD057066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2020 18:27
Operator : AJ\MA
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA501

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 08:19:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012320CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 24 08:15:19 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

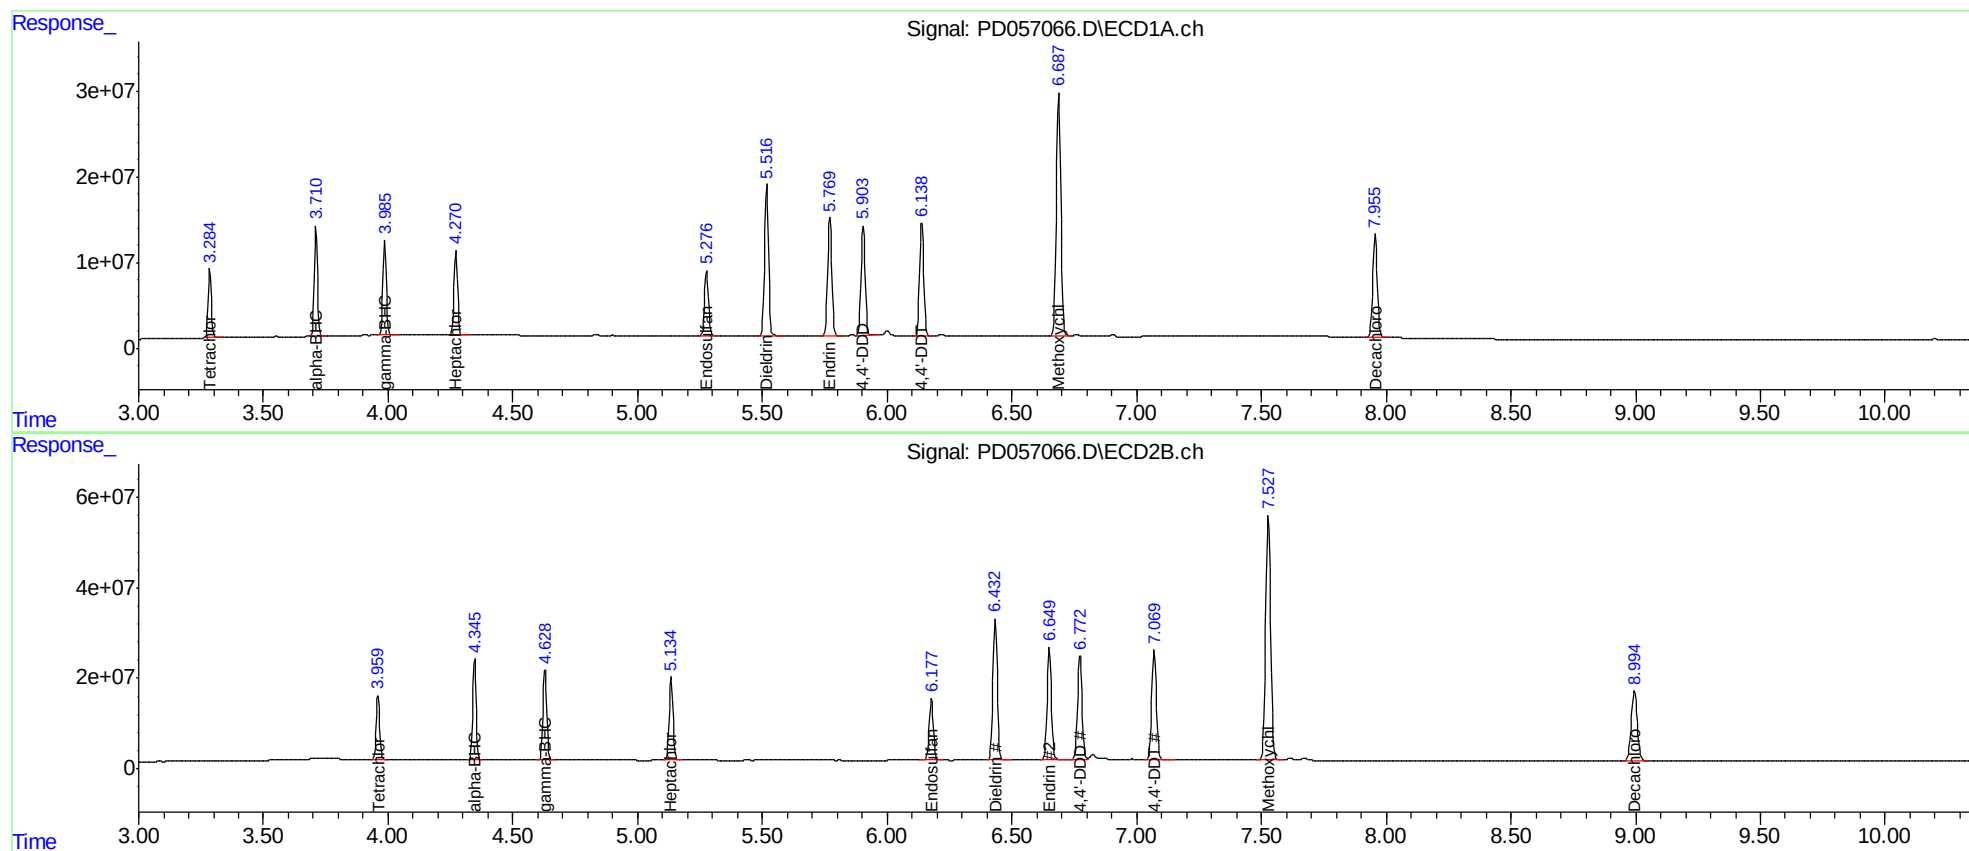


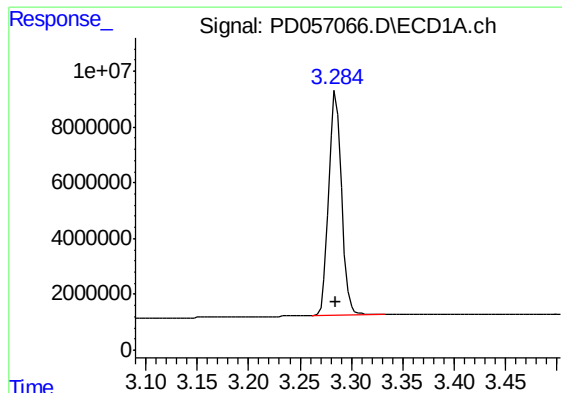

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: 0.000 min
Response: 70444843
Conc: 78.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

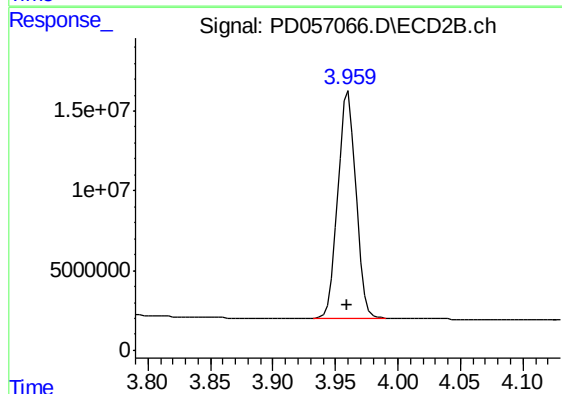


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 143126120
Conc: 77.19 ng/ml

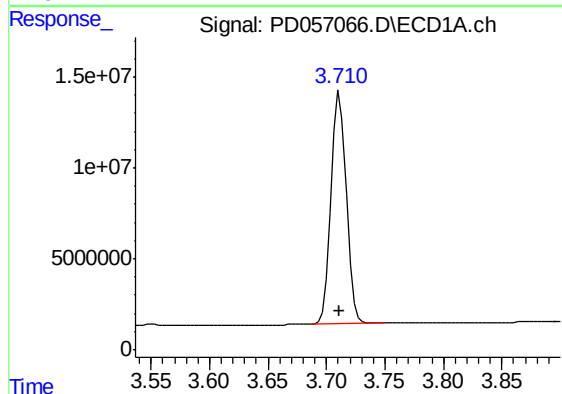


#2 alpha-BHC

R.T.: 3.712 min
Delta R.T.: 0.000 min
Response: 112118175
Conc: 85.22 ng/ml

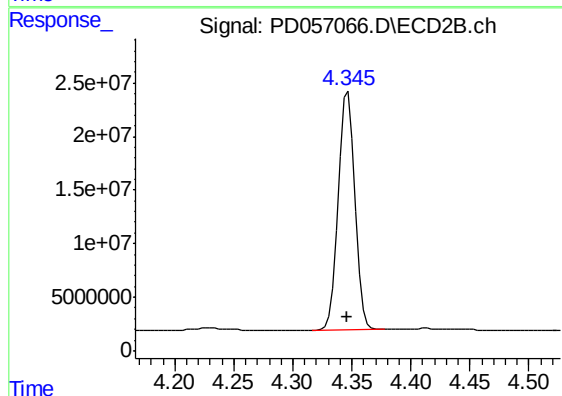

#2 alpha-BHC


R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 222716454
Conc: 83.98 ng/ml

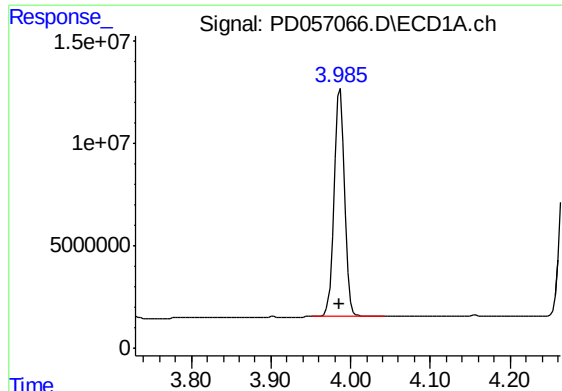

#3 gamma-BHC (Lindane)


R.T.: 3.987 min
Delta R.T.: 0.000 min
Response: 104623212
Conc: 81.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

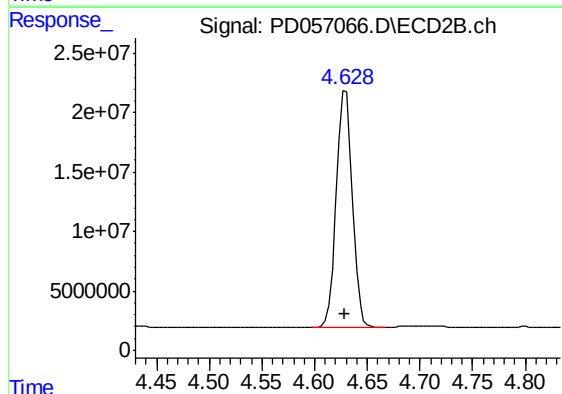


#3 gamma-BHC (Lindane)

R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 210333498
Conc: 82.23 ng/ml

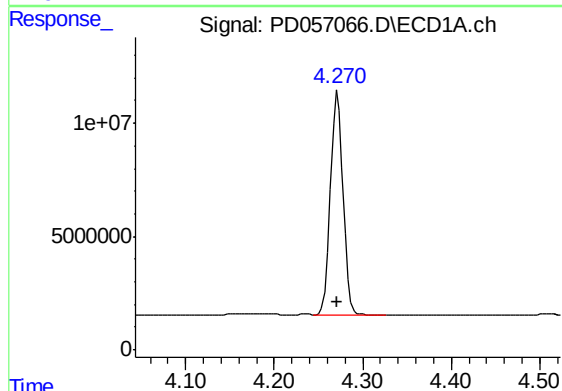


#4 Heptachlor

R.T.: 4.272 min
Delta R.T.: 0.000 min
Response: 99166547
Conc: 81.30 ng/ml

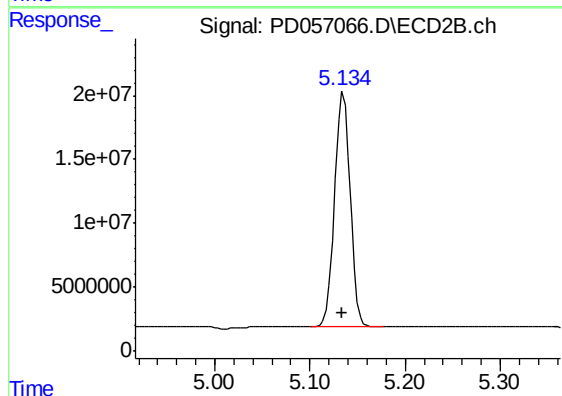

#4 Heptachlor


R.T.: 5.135 min
Delta R.T.: 0.000 min
Response: 209383776
Conc: 79.73 ng/ml

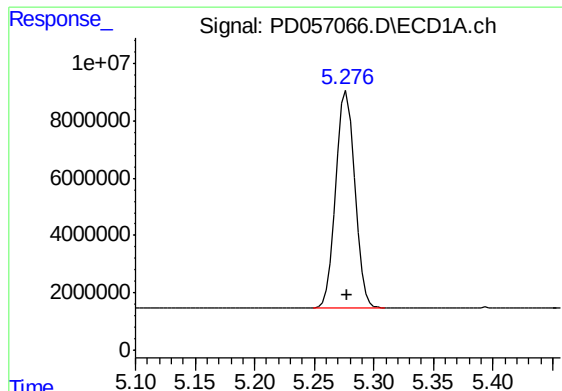

#9 Endosulfan I


R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 82853012
Conc: 79.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

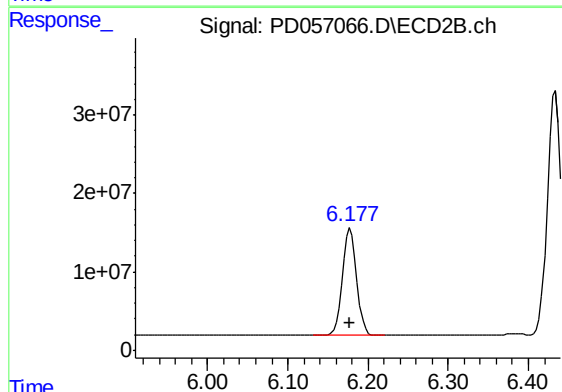


#9 Endosulfan I

R.T.: 6.178 min
Delta R.T.: 0.000 min
Response: 170688038
Conc: 78.43 ng/ml

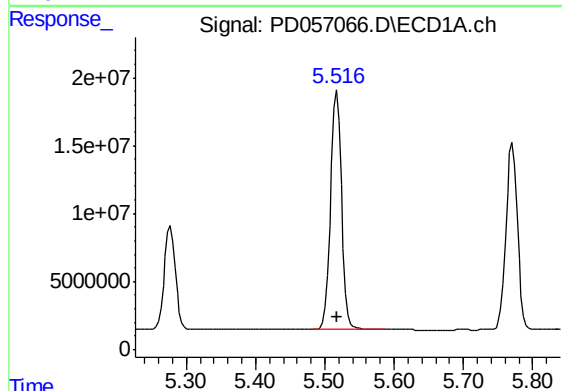


#13 Dieldrin

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 194593465
Conc: 165.40 ng/ml

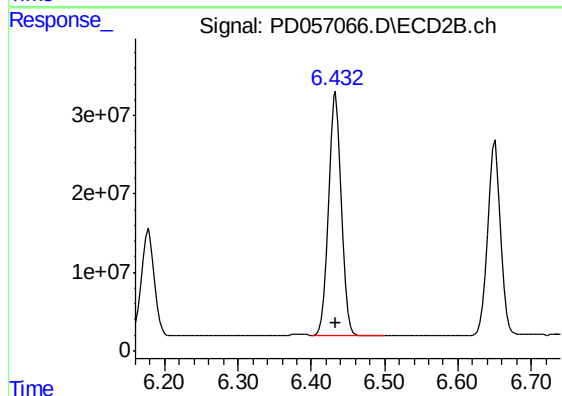

#13 Dieldrin


R.T.: 6.434 min
Delta R.T.: 0.000 min
Response: 388090083
Conc: 162.55 ng/ml

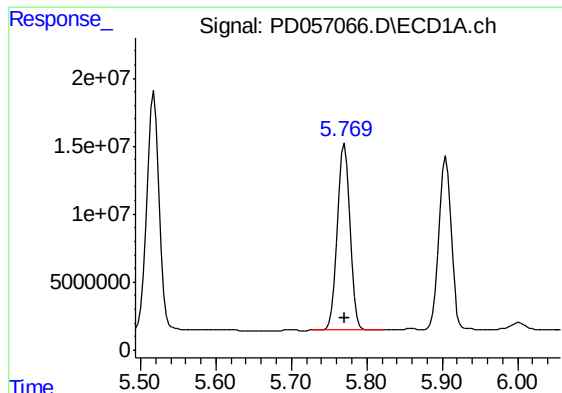

#14 Endrin


R.T.: 5.771 min
Delta R.T.: 0.000 min
Response: 158561611
Conc: 159.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

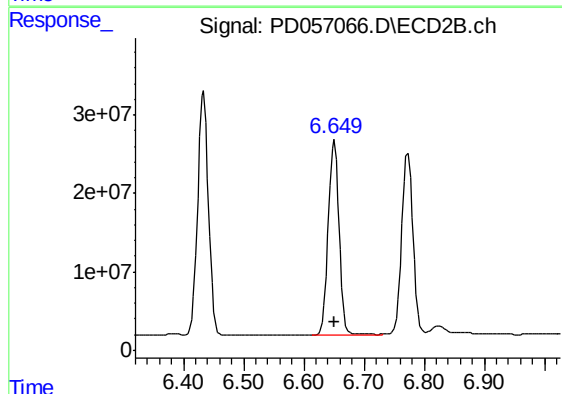


#14 Endrin

R.T.: 6.651 min
Delta R.T.: 0.000 min
Response: 313093238
Conc: 161.03 ng/ml

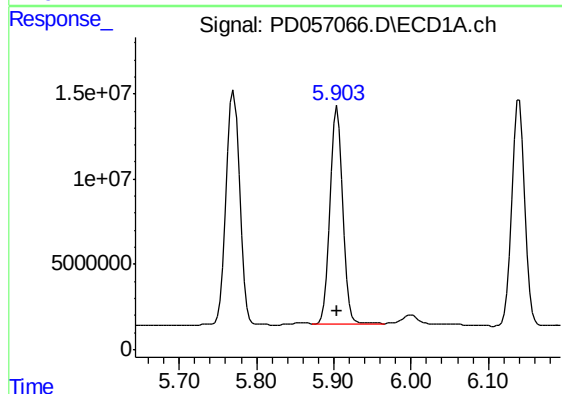


#16 4,4'-DDD

R.T.: 5.905 min
Delta R.T.: 0.000 min
Response: 145474155
Conc: 164.69 ng/ml

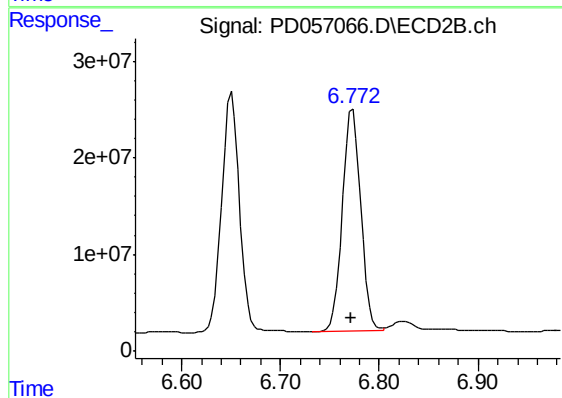

#16 4,4'-DDD


R.T.: 6.773 min
Delta R.T.: 0.001 min
Response: 296997606
Conc: 160.22 ng/ml

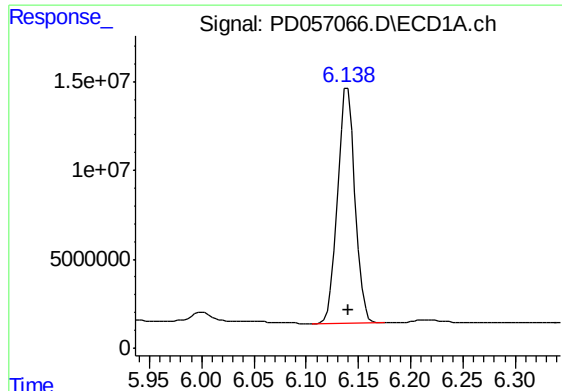

#17 4,4'-DDT


R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 154530942
Conc: 177.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

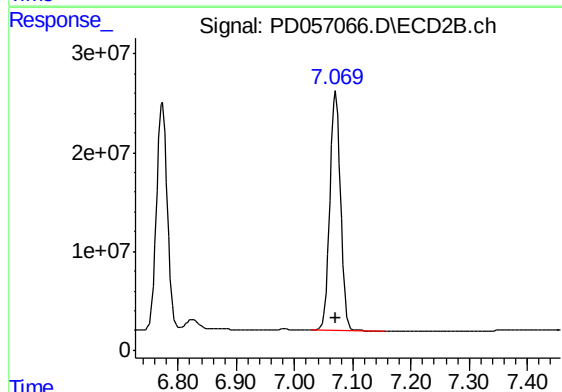


#17 4,4'-DDT

R.T.: 7.071 min
Delta R.T.: 0.000 min
Response: 313181000
Conc: 165.07 ng/ml

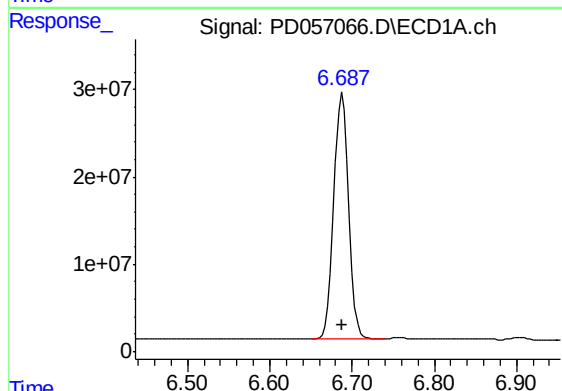


#20 Methoxychlor

R.T.: 6.688 min
Delta R.T.: 0.000 min
Response: 351470721
Conc: 743.91 ng/ml

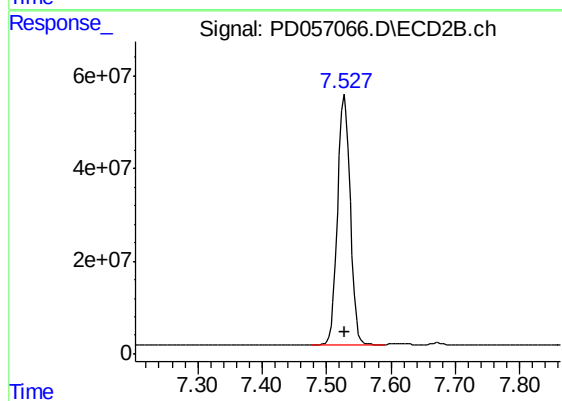

#20 Methoxychlor


R.T.: 7.528 min
Delta R.T.: 0.000 min
Response: 742022446
Conc: 727.17 ng/ml

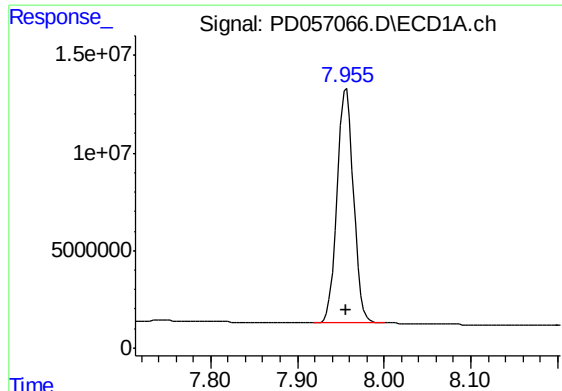

#27 Decachlorobiphenyl

R.T.: 7.957 min
Delta R.T.: 0.000 min
Response: 158712416
Conc: 147.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA501

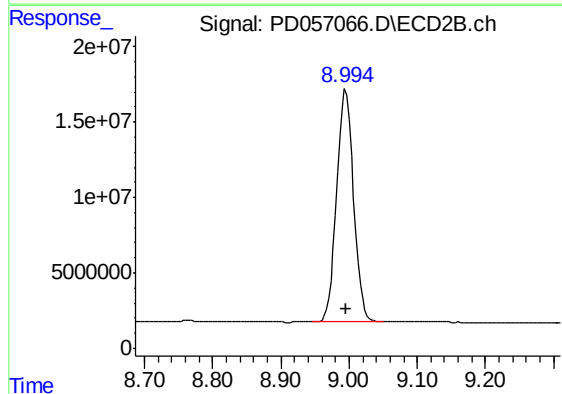

#27 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.000 min
Response: 265732507
Conc: 142.54 ng/ml