

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012323\
 Data File : PD073715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2023 15:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 21:00:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.776	52591598	28949053	22.499	22.740
28)	SA Decachlor...	9.104	7.935	58850023	25097352	20.883	21.571
Target Compounds							
4)	MA Heptachlor	4.924	0.000	275722	0	0.074	N.D. #
6)	B beta-BHC	4.509f	3.916	120872	82900	0.078	0.125 #
7)	B delta-BHC	4.780	0.000	2602631	0	0.773	N.D. #
8)	B Heptachlo...	5.700	0.000	1204076	0	0.377	N.D. #
9)	A Endosulfan I	6.100	0.000	203874	0	0.066	N.D. #
10)	B gamma-Chl...	5.959	0.000	349167	0	0.106	N.D. #
15)	B Endosulfa...	6.845f	0.000	535832	0	0.202	N.D. #
21)	B Endrin ke...	7.701f	0.000	583015	0	0.193	N.D. #
24)	Chlordane-2	0.000	4.358	0	215684	N.D.	4.319 #
25)	Chlordane-3	5.959	0.000	349167	0	0.746	N.D. #
27)	Chlordane-5	0.000	5.976f	0	201385	N.D.	4.008 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012323\
Data File : PD073715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2023 15:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 21:00:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

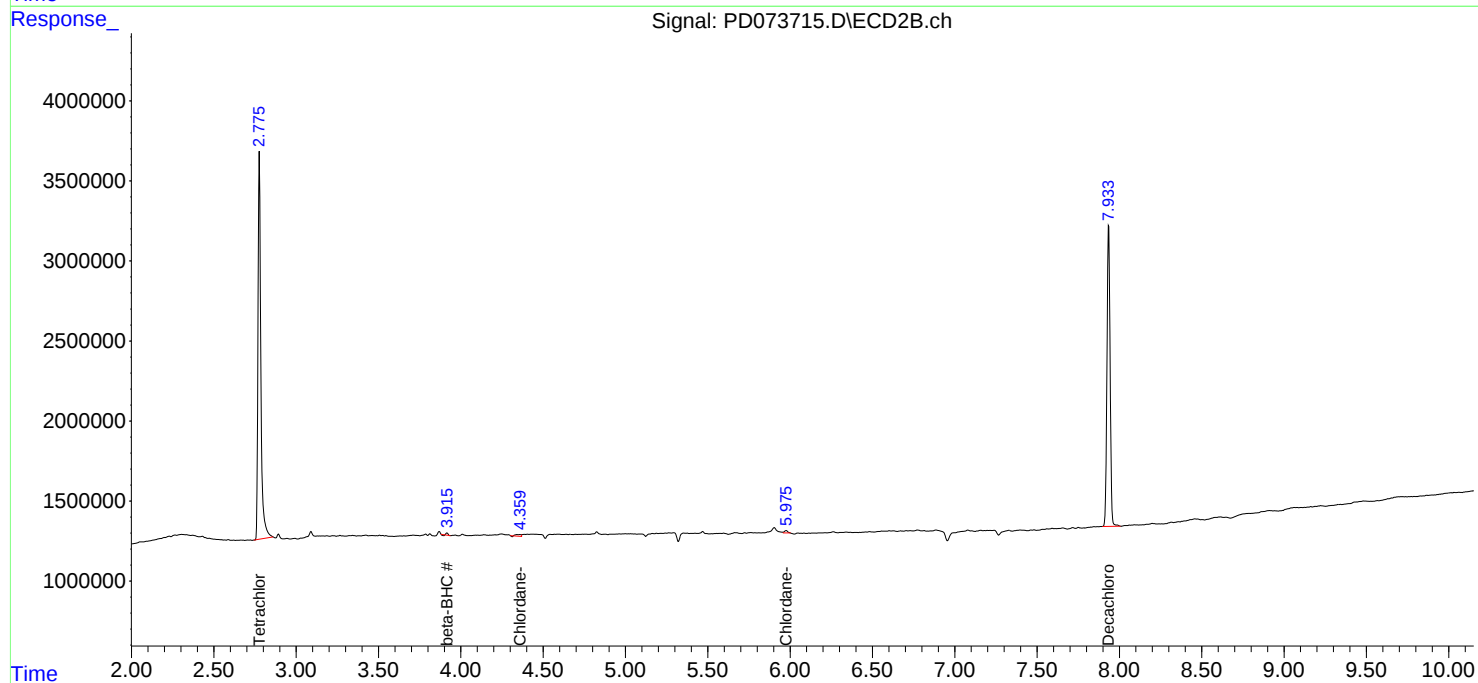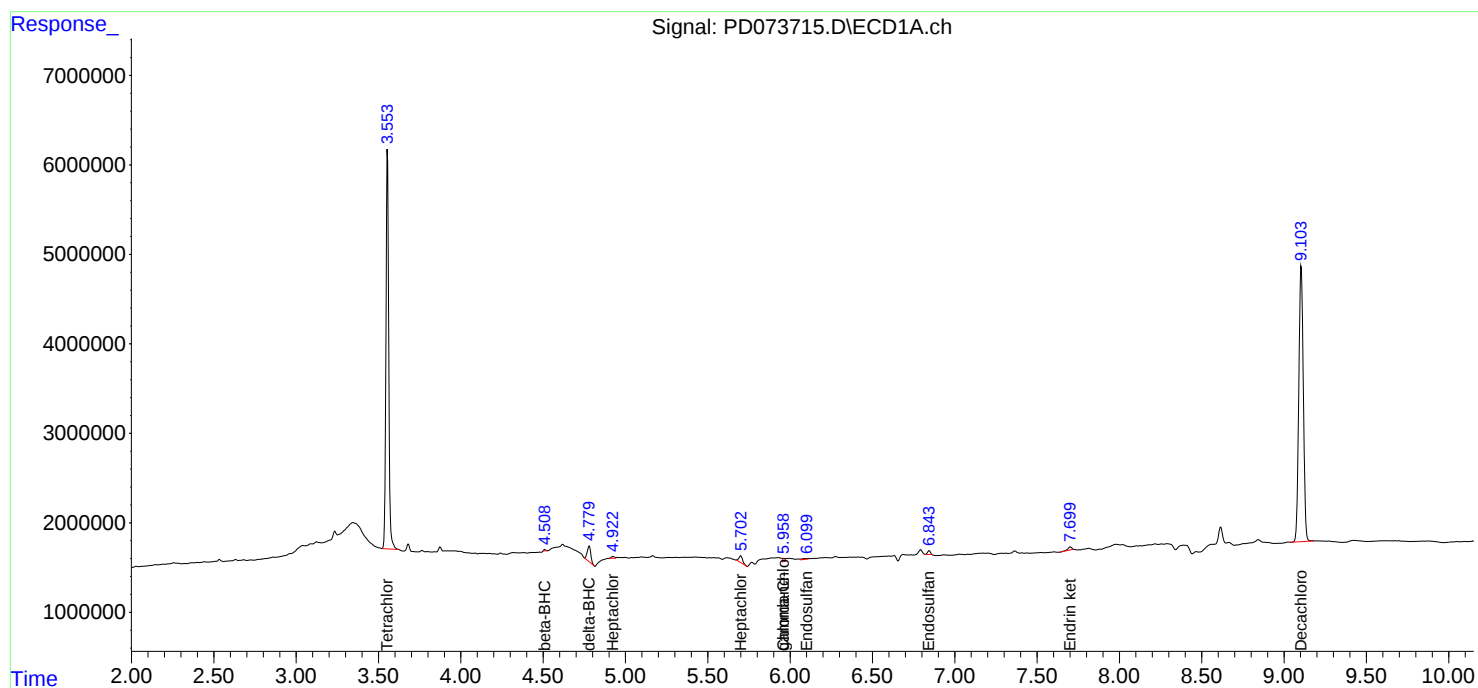


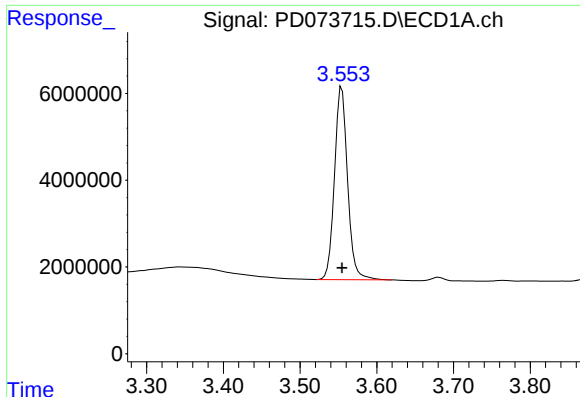

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 52591598
Conc: 22.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

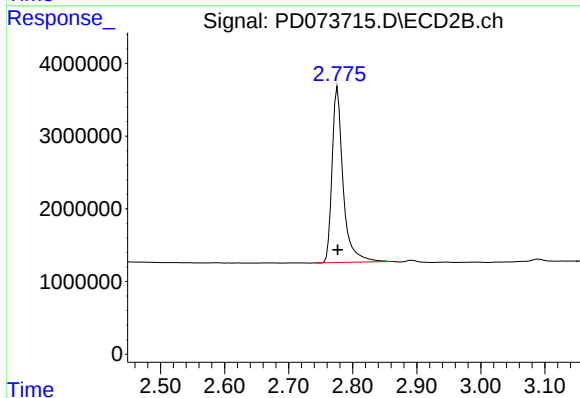


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 28949053
Conc: 22.74 ng/ml

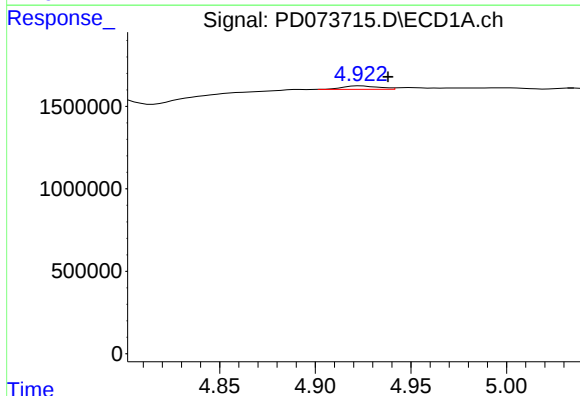


#4 Heptachlor

R.T.: 4.924 min
Delta R.T.: -0.014 min
Response: 275722
Conc: 0.07 ng/ml

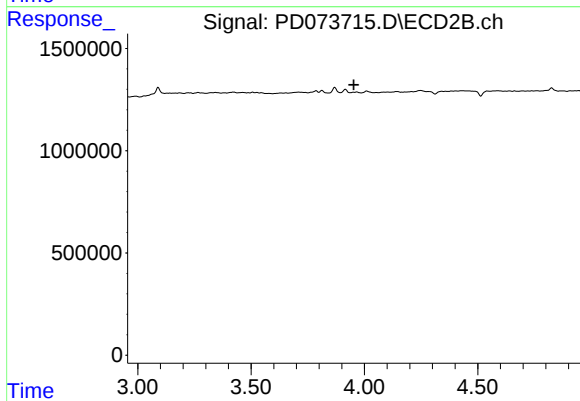

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.953 min
Response: 0
Conc: N.D.

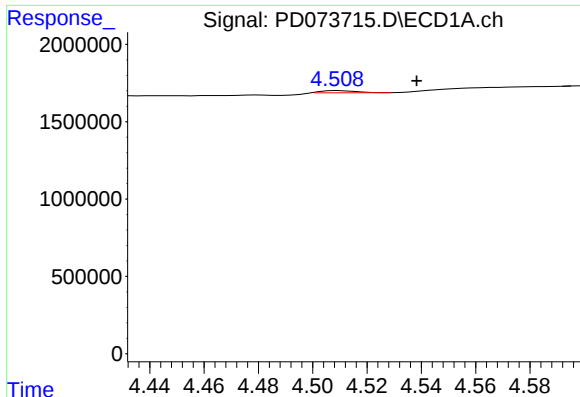

#6 beta-BHC


R.T.: 4.509 min
Delta R.T.: -0.029 min
Response: 120872
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

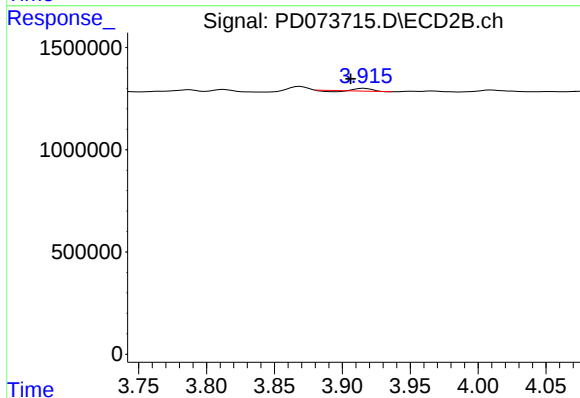


#6 beta-BHC

R.T.: 3.916 min
Delta R.T.: 0.010 min
Response: 82900
Conc: 0.13 ng/ml

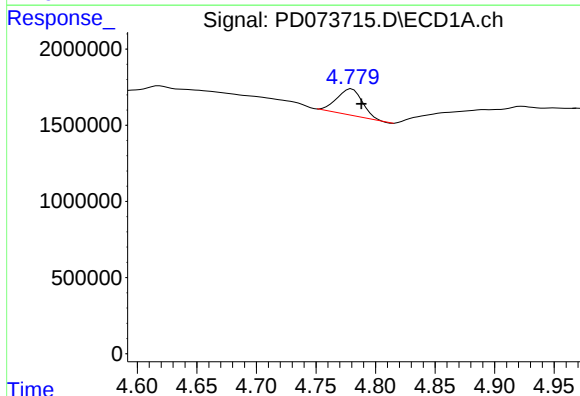


#7 delta-BHC

R.T.: 4.780 min
Delta R.T.: -0.008 min
Response: 2602631
Conc: 0.77 ng/ml

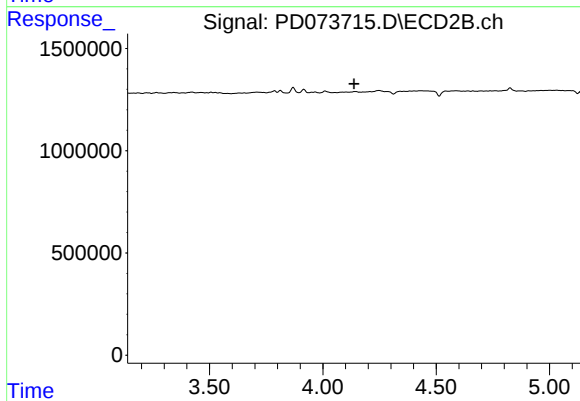

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

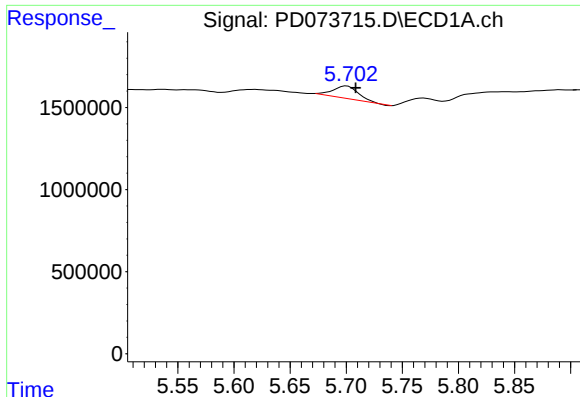

#8 Heptachlor epoxide


R.T.: 5.700 min
Delta R.T.: -0.008 min
Response: 1204076
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

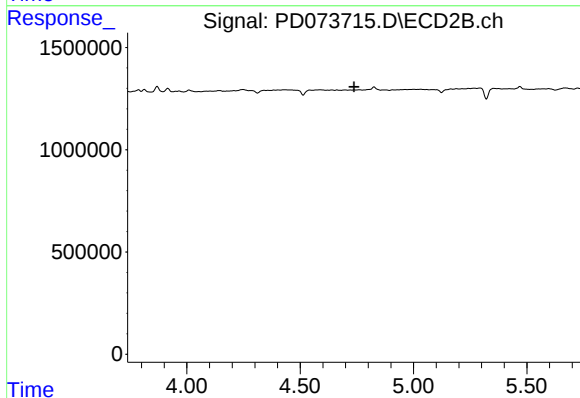


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

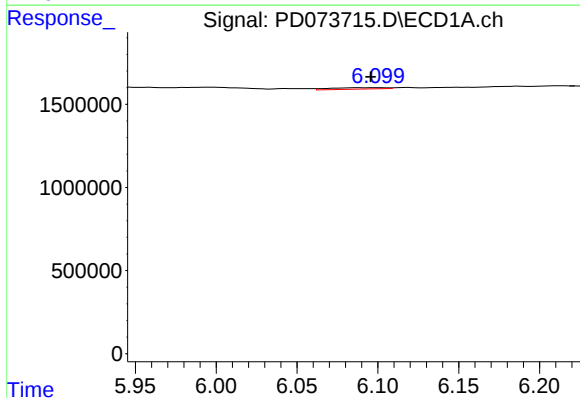


#9 Endosulfan I

R.T.: 6.100 min
Delta R.T.: 0.004 min
Response: 203874
Conc: 0.07 ng/ml

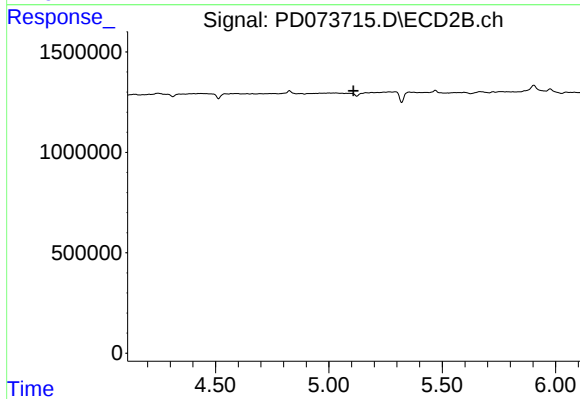

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.109 min
Response: 0
Conc: N.D.

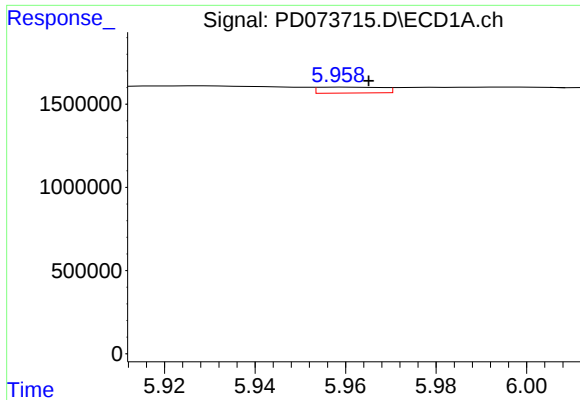

#10 gamma-Chlordane


R.T.: 5.959 min
Delta R.T.: -0.006 min
Response: 349167
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

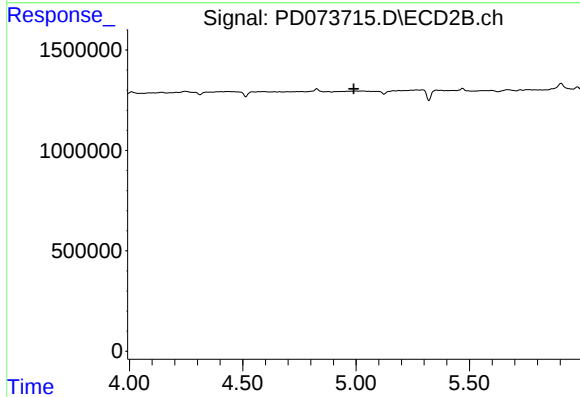


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

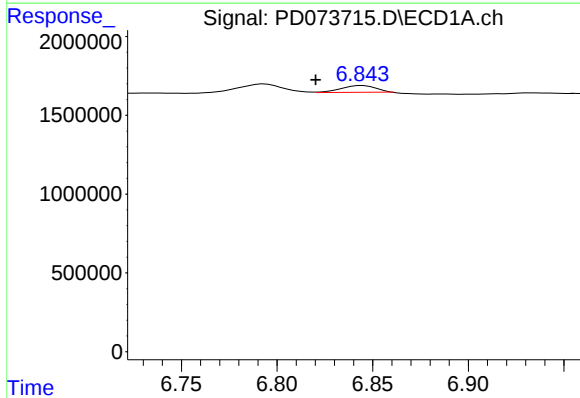


#15 Endosulfan II

R.T.: 6.845 min
Delta R.T.: 0.024 min
Response: 535832
Conc: 0.20 ng/ml

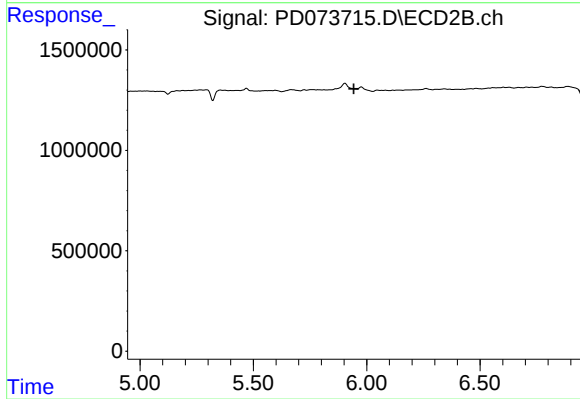

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

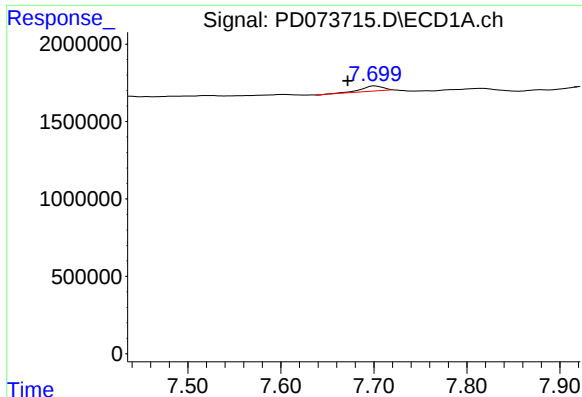

#21 Endrin ketone


R.T.: 7.701 min
Delta R.T.: 0.029 min
Response: 583015
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

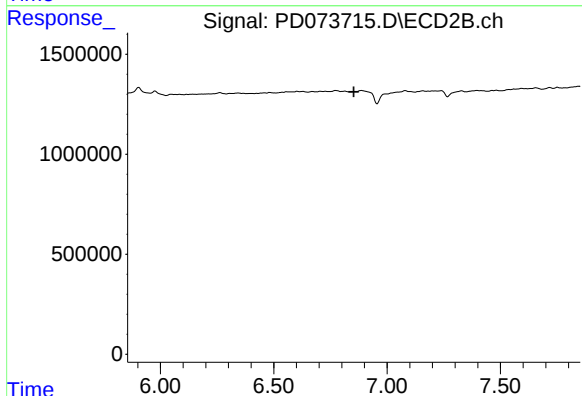


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

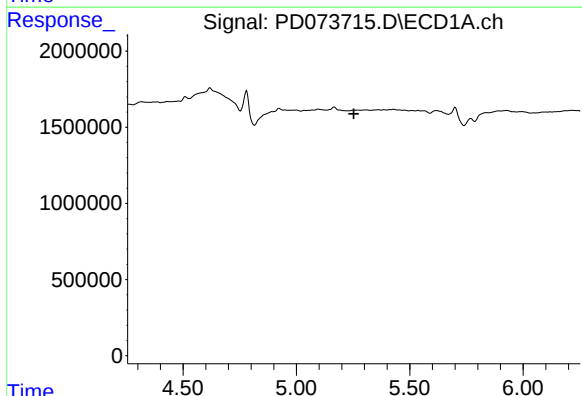


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.253 min
Response: 0
Conc: N.D.

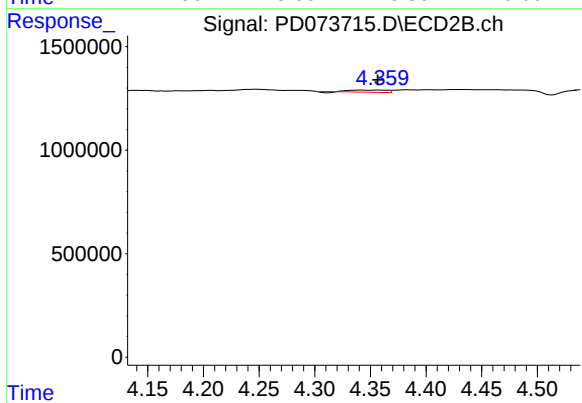

#24 Chlordane-2


R.T.: 4.358 min
Delta R.T.: 0.002 min
Response: 215684
Conc: 4.32 ng/ml

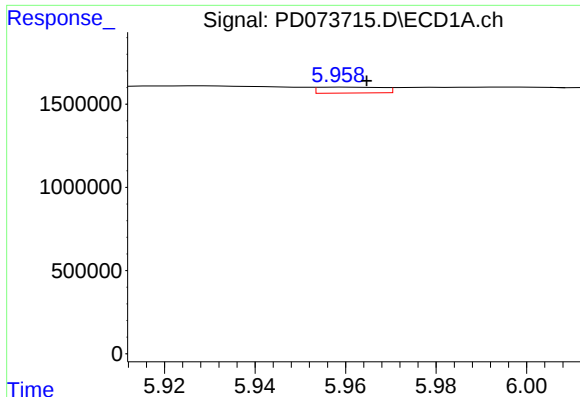

#25 Chlordane-3


R.T.: 5.959 min
Delta R.T.: -0.006 min
Response: 349167
Conc: 0.75 ng/ml

Instrument :
ECD_D
ClientSampleId :

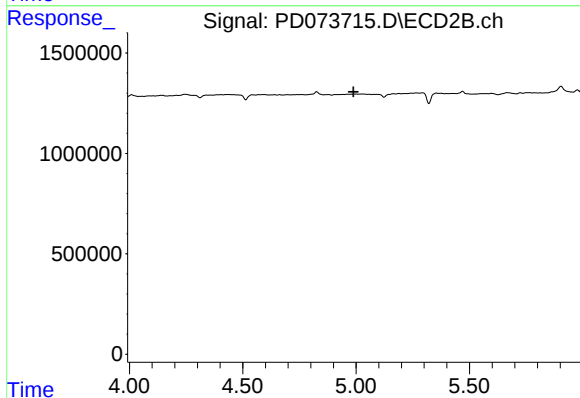


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

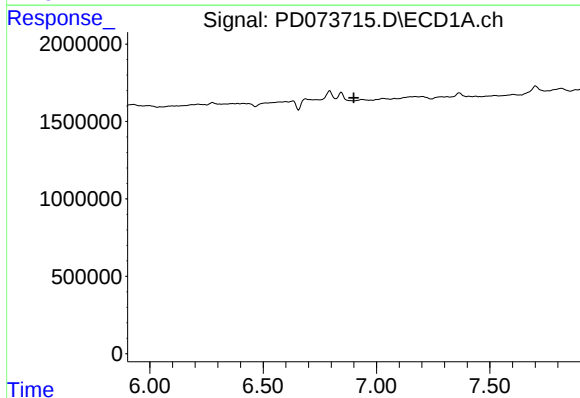


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.900 min
Response: 0
Conc: N.D.

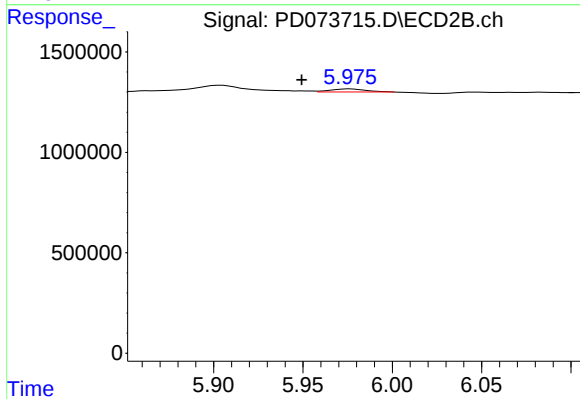

#27 Chlordane-5


R.T.: 5.976 min
Delta R.T.: 0.027 min
Response: 201385
Conc: 4.01 ng/ml

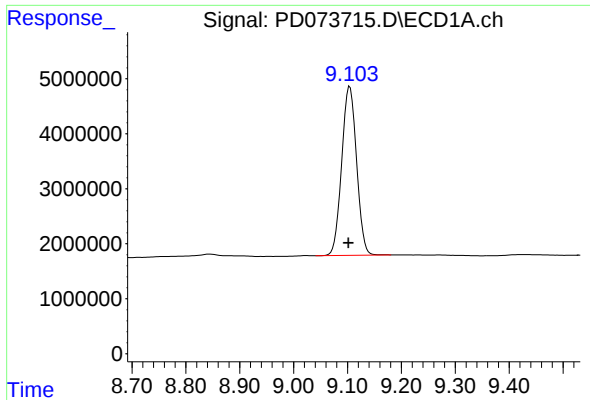

#28 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: 0.003 min
Response: 58850023
Conc: 20.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

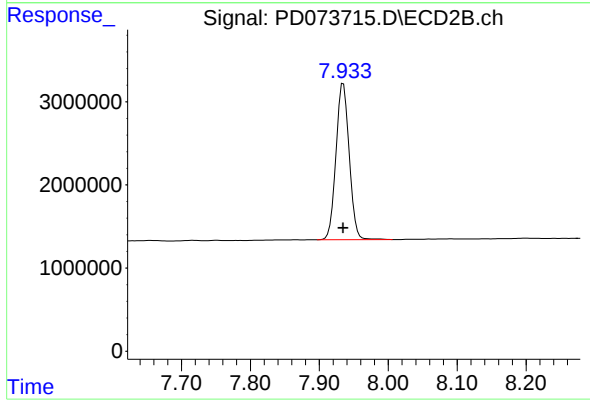

#28 Decachlorobiphenyl

R.T.: 7.935 min
Delta R.T.: 0.000 min
Response: 25097352
Conc: 21.57 ng/ml