

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012324\
 Data File : PD080823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2024 10:23
 Operator : AR\AJ
 Sample : P1197-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEST-GPC-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 21:38:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 10 14:12:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	0.000	2.786	0	214779	N.D.	<MDL
Target Compounds						
3) MA gamma-BHC...	0.000	3.641	0	103233	N.D.	<MDL
4) MA Heptachlor	0.000	3.957	0	30095	N.D.	<MDL
6) B beta-BHC	0.000	3.929	0	21942	N.D.	<MDL
8) B Heptachlo...	0.000	4.791f	0	181549	N.D.	<MDL
14) MA Endrin	0.000	5.675	0	109531	N.D.	<MDL
15) B Endosulfa...	0.000	5.935	0	29329	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012324\
Data File : PD080823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2024 10:23
Operator : AR\AJ
Sample : P1197-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 21:38:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jan 10 14:12:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

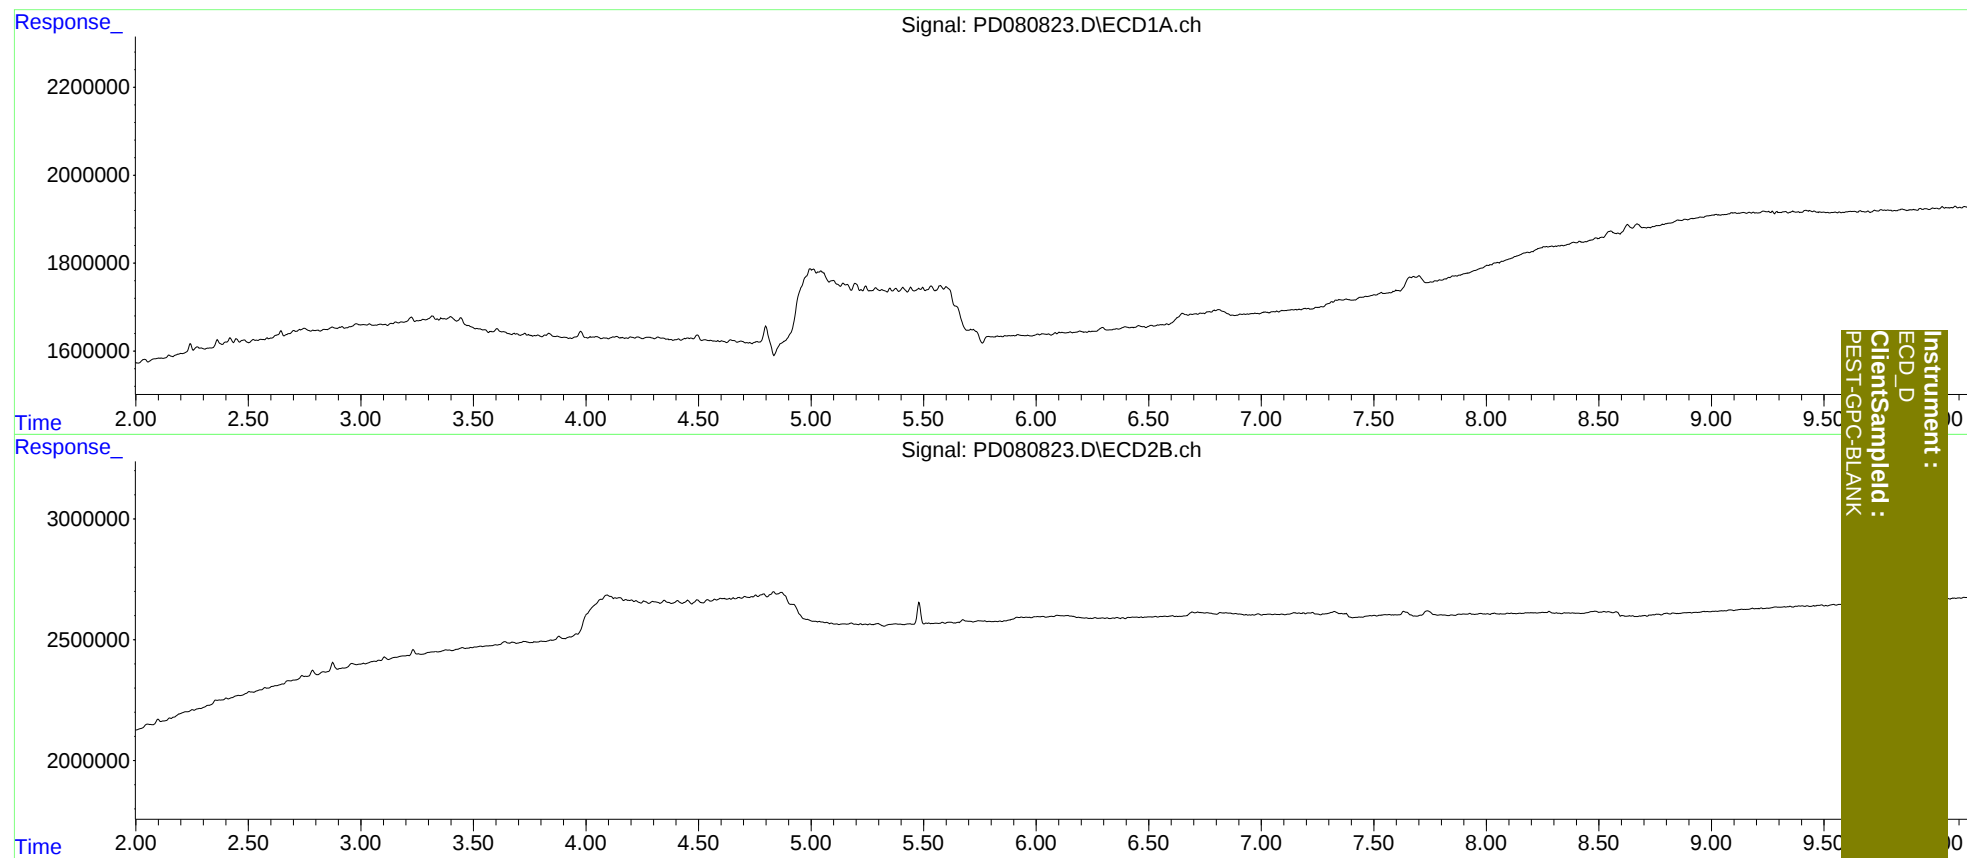


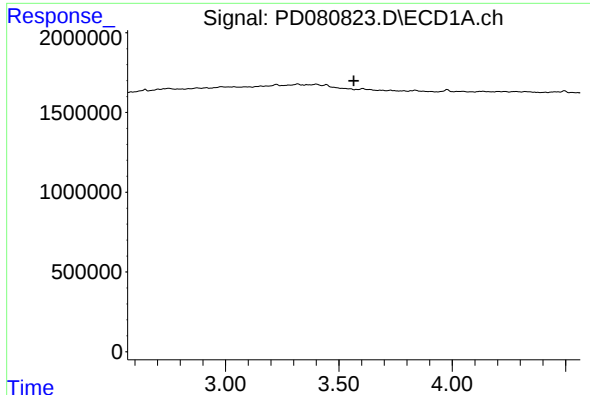

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PEST-GPC-BLANK

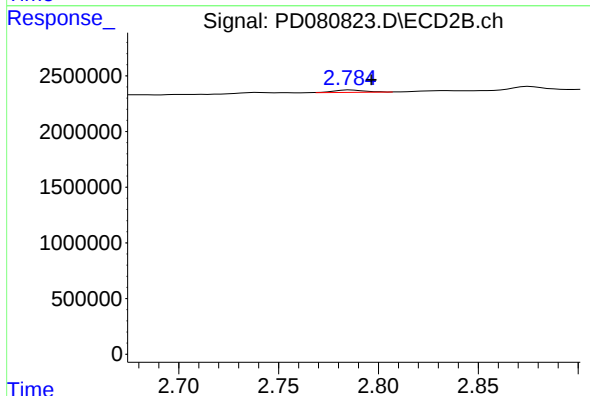


#1 Tetrachloro-m-xylene

R.T.: 2.786 min
Delta R.T.: -0.010 min
Response: 214779
Conc: N.D.

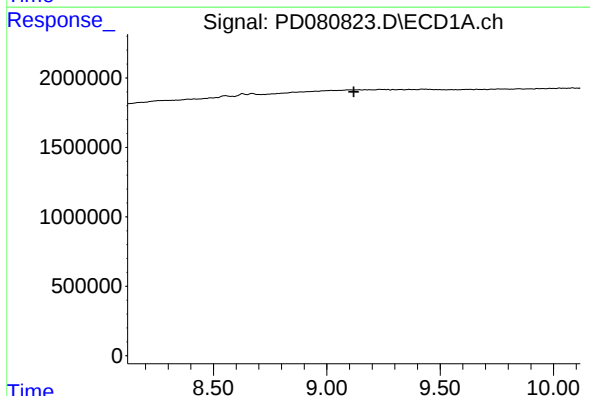

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.119 min
Response: 0
Conc: N.D.

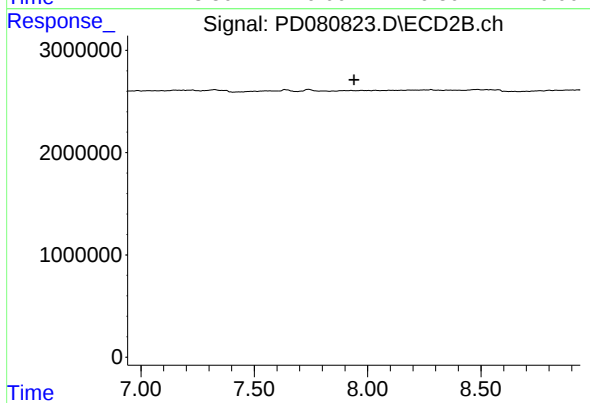

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.941 min
Response: 0
Conc: N.D.