

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012325\
 Data File : PD087503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2025 13:15
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 14:18:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012325.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 22 14:13:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.881	141.3E6	982.6E6	74.735	74.821
28)	SA Decachlor...	9.079	8.080	204.3E6	956.7E6	74.520	74.234
Target Compounds							
23)	Chlordane-1	4.720	3.909	94366454	384.4E6	751.949	747.431
24)	Chlordane-2	5.246	4.491	93765680	399.4E6	744.646	746.115
25)	Chlordane-3	5.951	5.131	376.9E6	1207.6E6	748.837	747.492
26)	Chlordane-4	6.037	5.195	447.7E6	1014.0E6	747.608	748.092
27)	Chlordane-5	6.876	6.095	77489558	454.9E6	746.421	743.898



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012325\
Data File : PD087503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2025 13:15
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 14:18:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012325.M
Quant Title : GC Extractables
QLast Update : Wed Jan 22 14:13:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

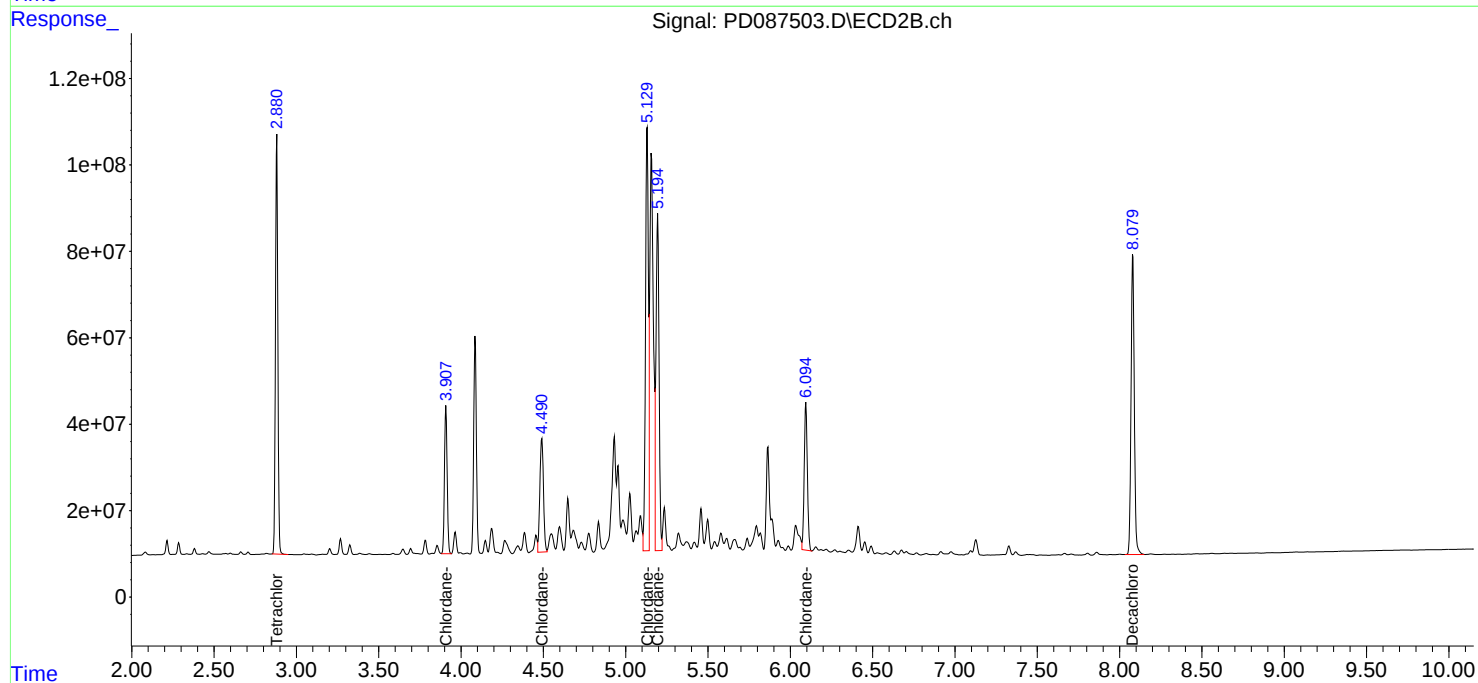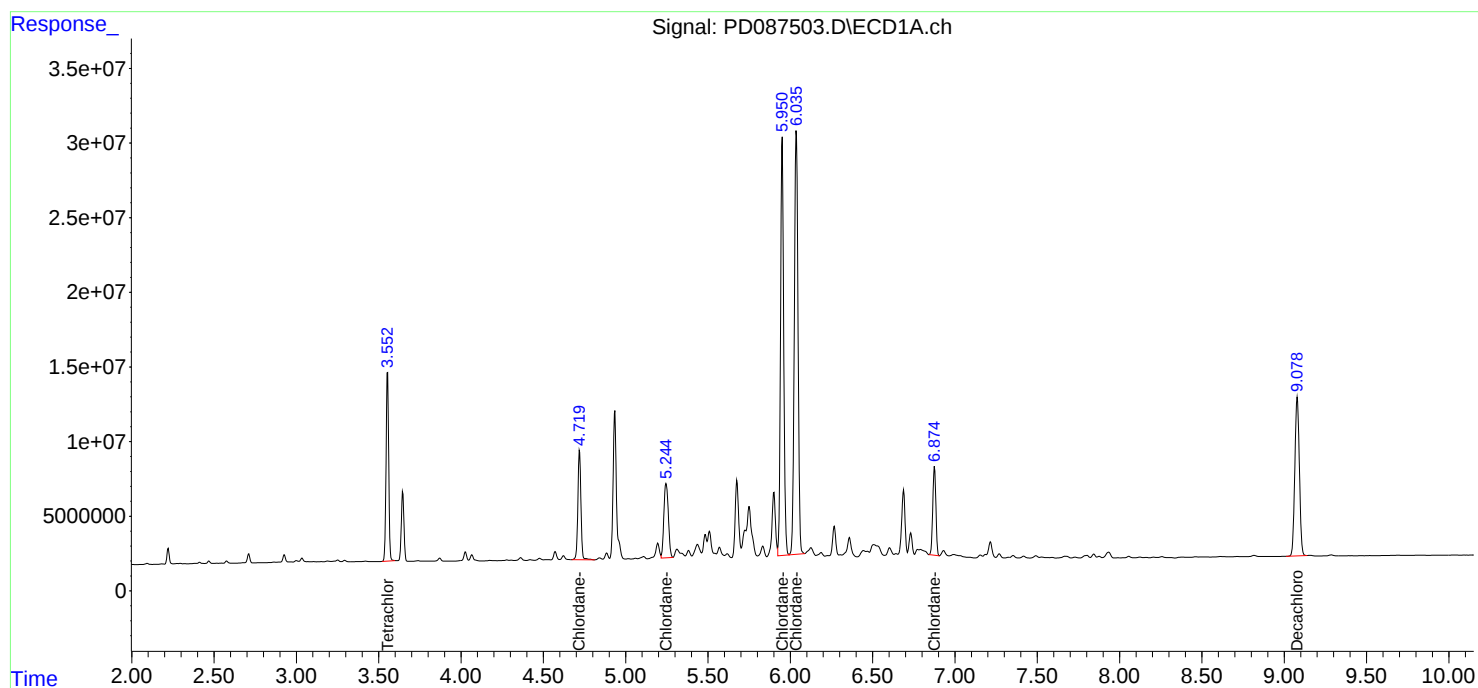


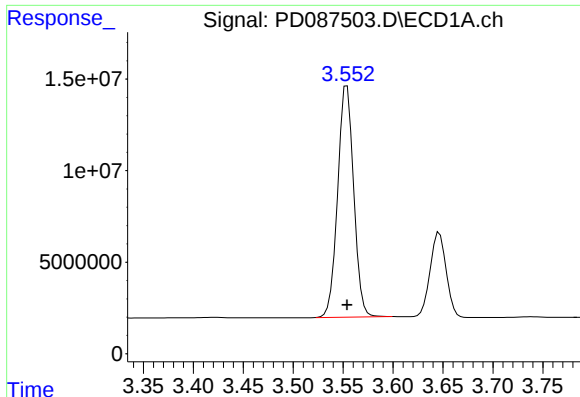

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 141344928
Conc: 74.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

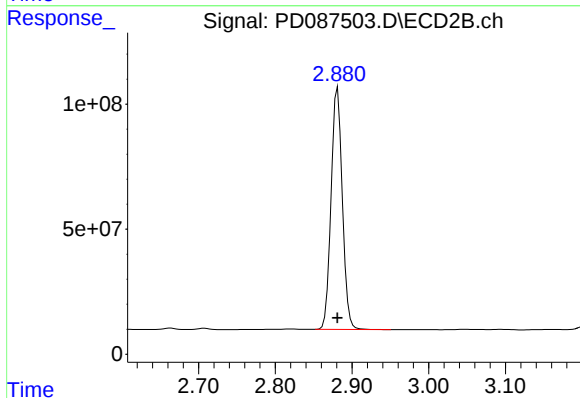


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 982598528
Conc: 74.82 ng/ml

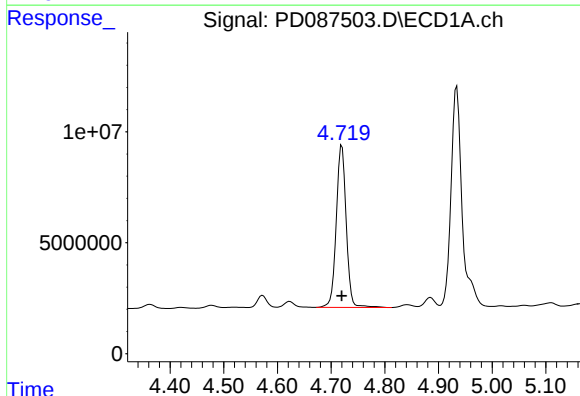


#23 Chlordane-1

R.T.: 4.720 min
Delta R.T.: 0.000 min
Response: 94366454
Conc: 751.95 ng/ml

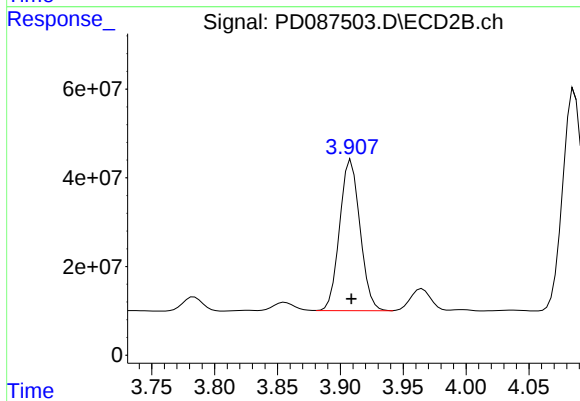

#23 Chlordane-1


R.T.: 3.909 min
Delta R.T.: 0.000 min
Response: 384440006
Conc: 747.43 ng/ml

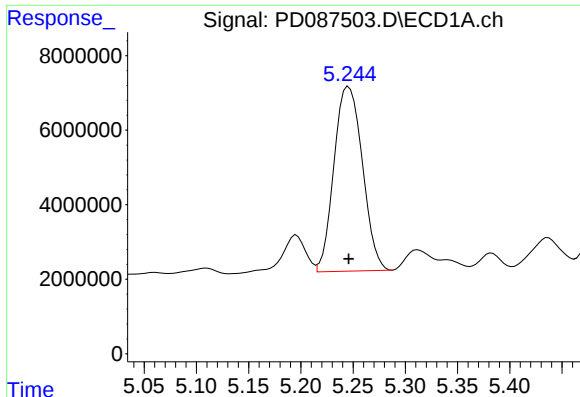

#24 Chlordane-2


R.T.: 5.246 min
Delta R.T.: 0.000 min
Response: 93765680
Conc: 744.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

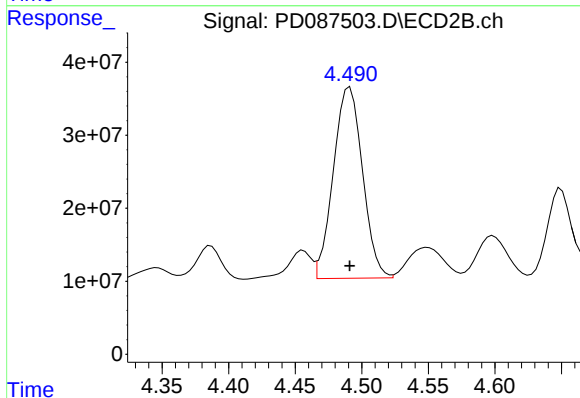


#24 Chlordane-2

R.T.: 4.491 min
Delta R.T.: 0.000 min
Response: 399385056
Conc: 746.12 ng/ml

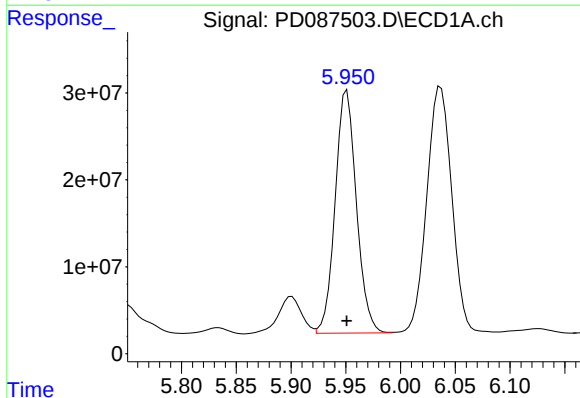


#25 Chlordane-3

R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 376945530
Conc: 748.84 ng/ml

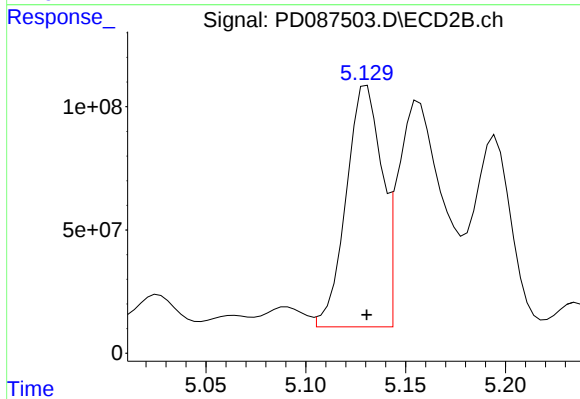

#25 Chlordane-3


R.T.: 5.131 min
Delta R.T.: 0.000 min
Response: 1207558179
Conc: 747.49 ng/ml

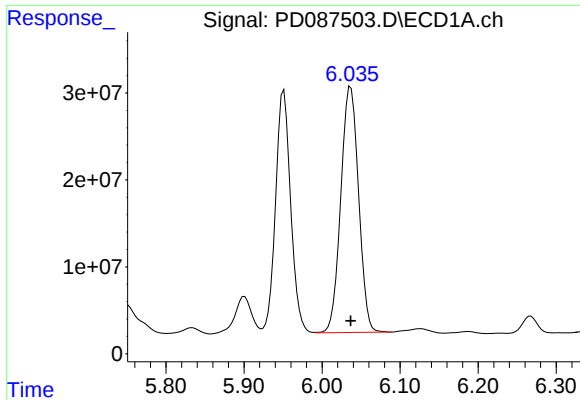

#26 Chlordane-4


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 447726969
Conc: 747.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

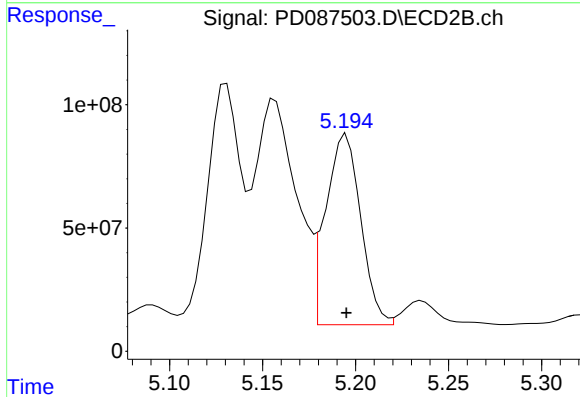


#26 Chlordane-4

R.T.: 5.195 min
Delta R.T.: 0.000 min
Response: 1013997280
Conc: 748.09 ng/ml

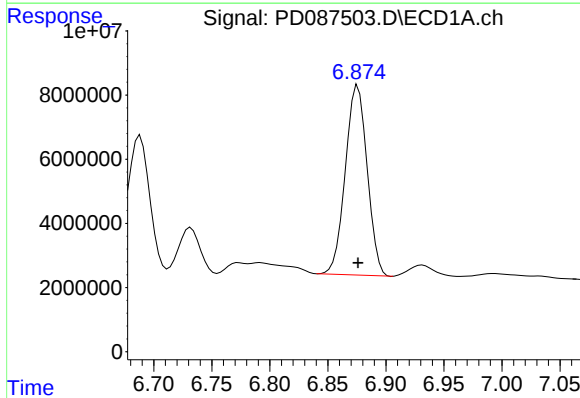


#27 Chlordane-5

R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 77489558
Conc: 746.42 ng/ml

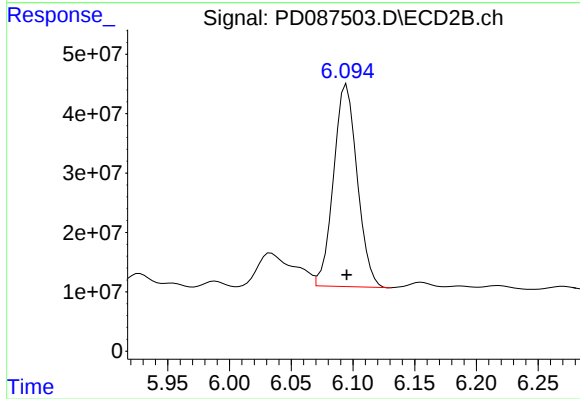

#27 Chlordane-5

R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 454896581
Conc: 743.90 ng/ml

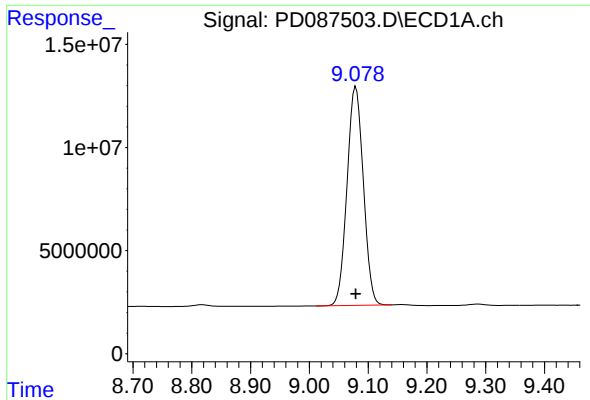

#28 Decachlorobiphenyl


R.T.: 9.079 min

Delta R.T.: 0.000 min

Response: 204330103

Conc: 74.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

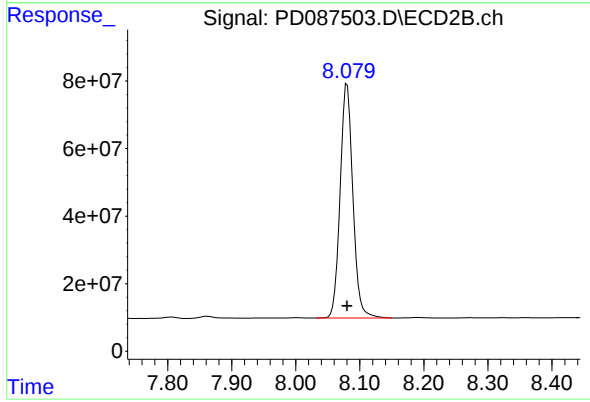

#28 Decachlorobiphenyl

R.T.: 8.080 min

Delta R.T.: 0.000 min

Response: 956731674

Conc: 74.23 ng/ml