

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012325\
 Data File : PD087496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2025 11:37
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 13:01:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012325.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 22 12:58:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.881	38202520	240.1E6	19.175	19.963
28)	SA Decachlor...	9.080	8.080	58676121	280.3E6	19.238	19.837
Target Compounds							
9)	A Endosulfan I	6.079	5.251	27956039	146.5E6	8.875	9.827
10)	B gamma-Chl...	5.951	5.130	30586355	168.9E6	9.254	10.386
12)	B 4,4'-DDE	6.201	5.381	55922228	313.3E6	18.533	19.910
13)	MA Dieldrin	6.353	5.518	61194101	317.4E6	18.120	19.483
19)	B Endosulfa...	7.154	6.487	51299260	280.1E6	18.711	19.701
20)	A Methoxychlor	7.498	6.761	128.4E6	629.3E6	87.455	82.343
21)	B Endrin ke...	7.635	6.996	56126879	302.8E6	18.253	19.405



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012325\
Data File : PD087496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2025 11:37
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 13:01:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012325.M
Quant Title : GC Extractables
QLast Update : Wed Jan 22 12:58:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

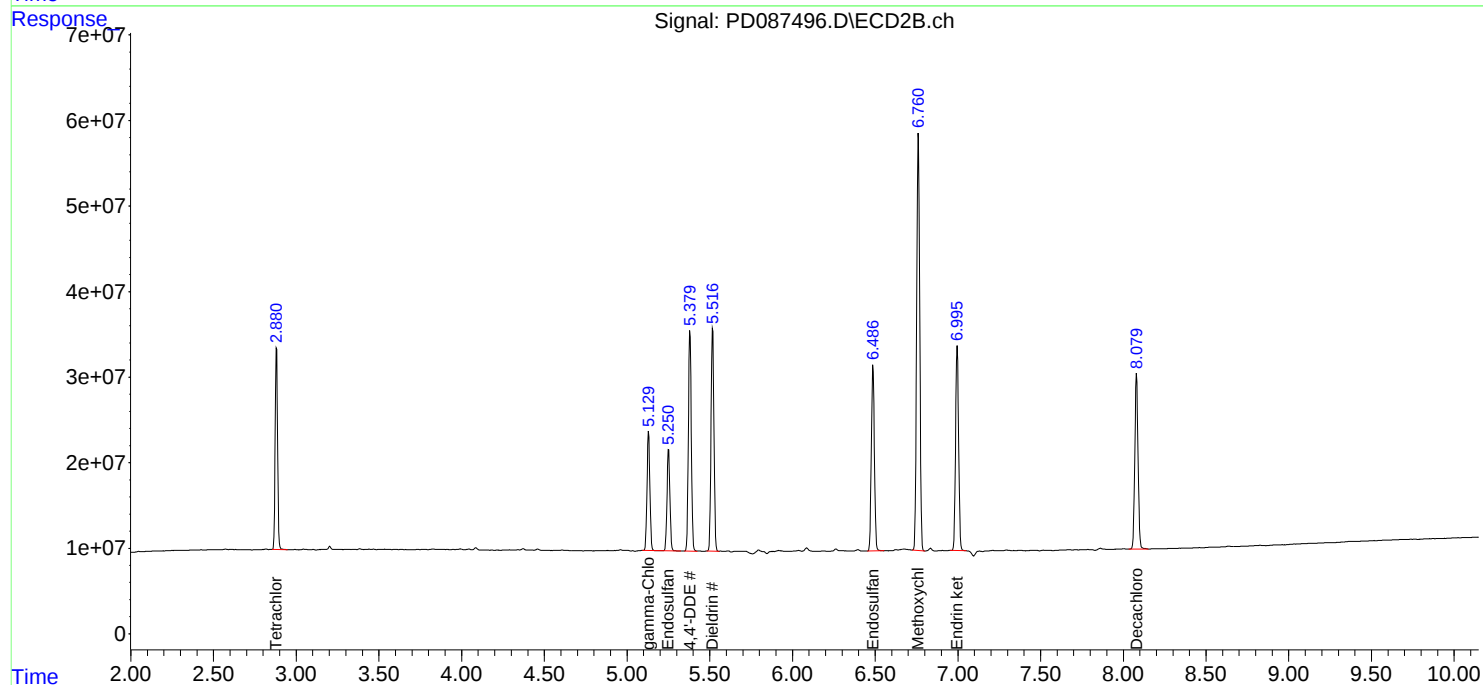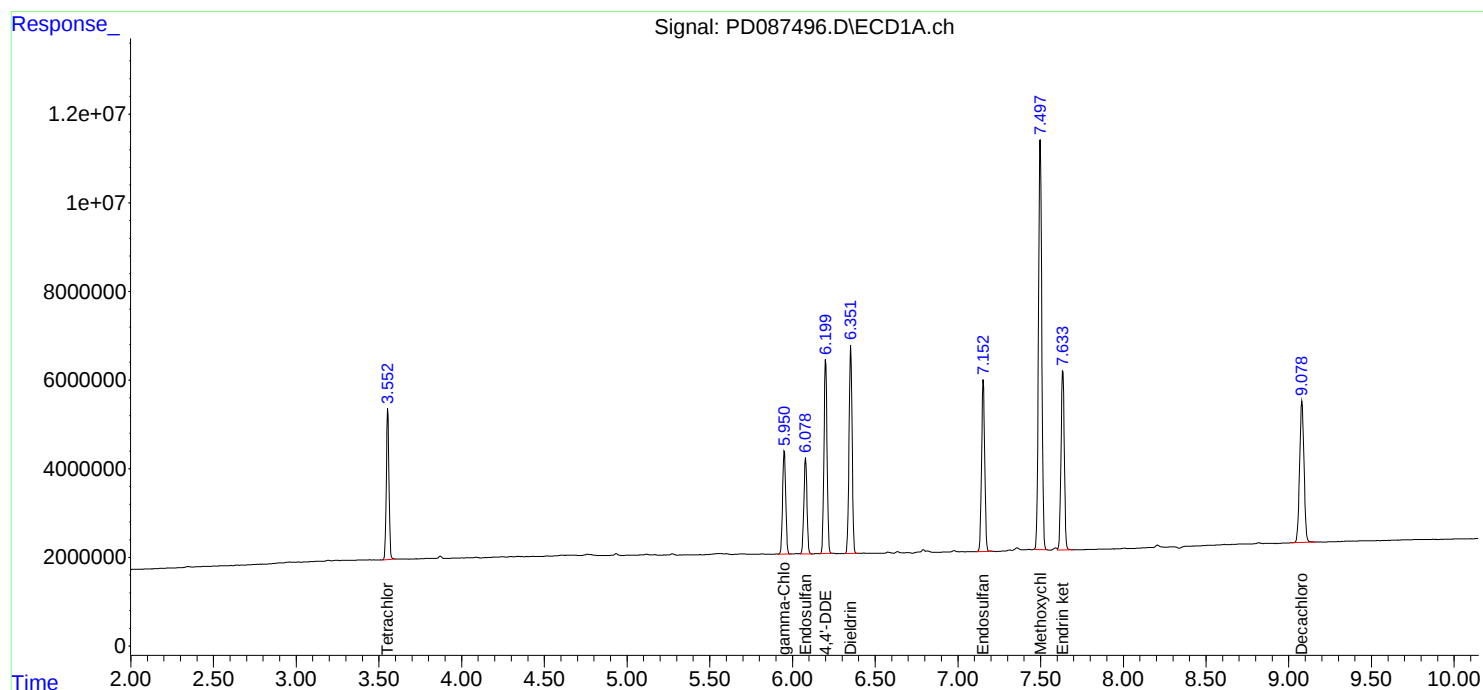


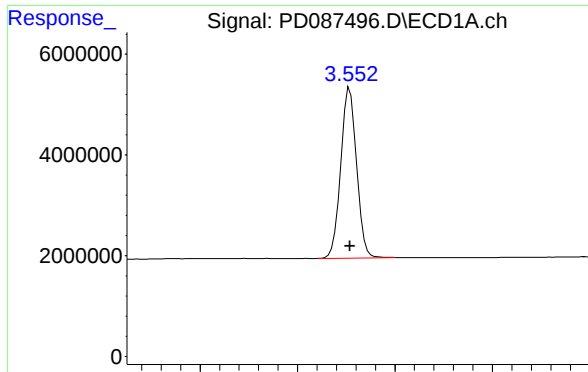

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.000 min
Response: 38202520
Conc: 19.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

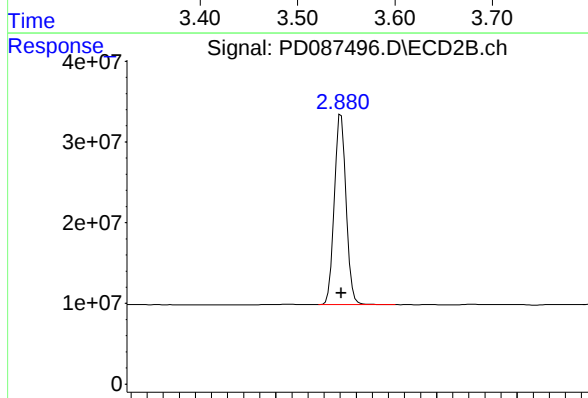


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 240087938
Conc: 19.96 ng/ml

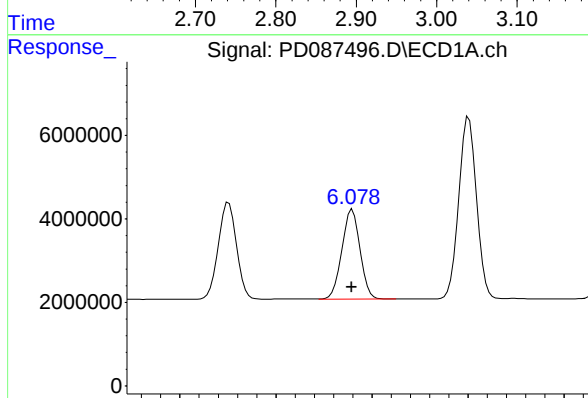


#9 Endosulfan I

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 27956039
Conc: 8.87 ng/ml

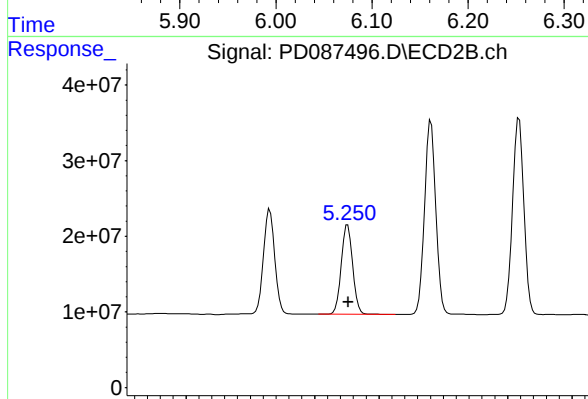

#9 Endosulfan I


R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 146461952
Conc: 9.83 ng/ml

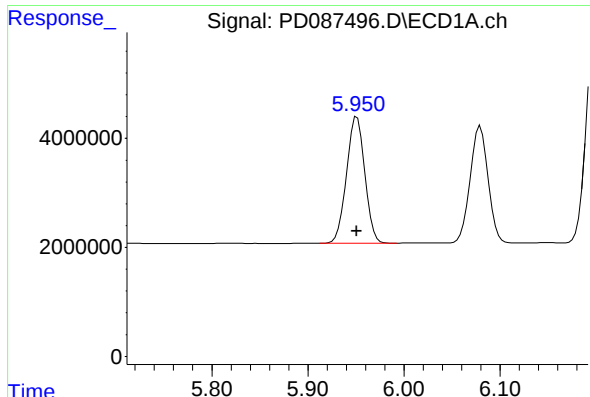

#10 gamma-Chlordane


R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 30586355
Conc: 9.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

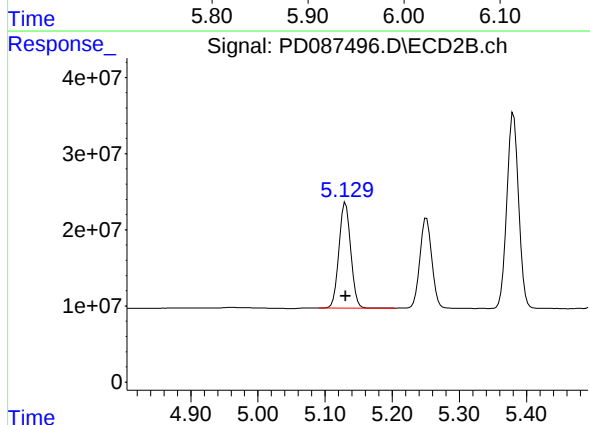


#10 gamma-Chlordane

R.T.: 5.130 min
Delta R.T.: 0.000 min
Response: 168923227
Conc: 10.39 ng/ml

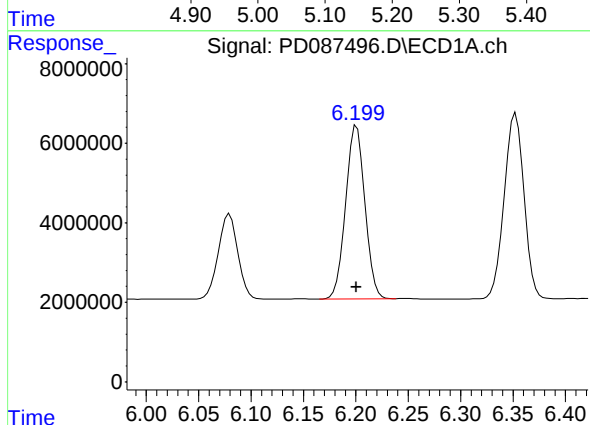


#12 4,4'-DDE

R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 55922228
Conc: 18.53 ng/ml

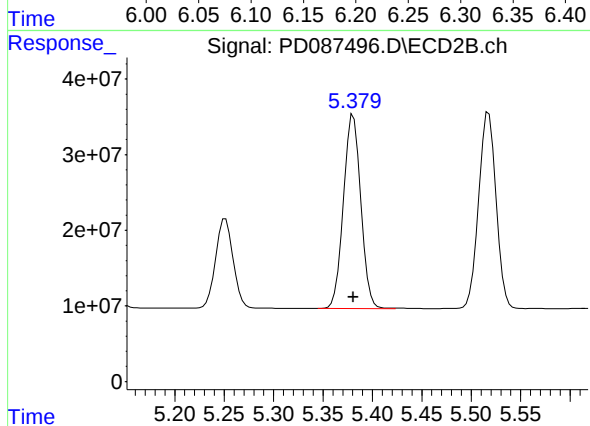

#12 4,4'-DDE


R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 313263790
Conc: 19.91 ng/ml

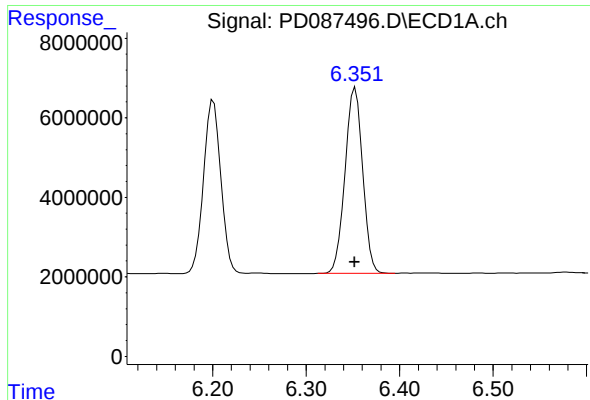

#13 Dieldrin


R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 61194101
Conc: 18.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

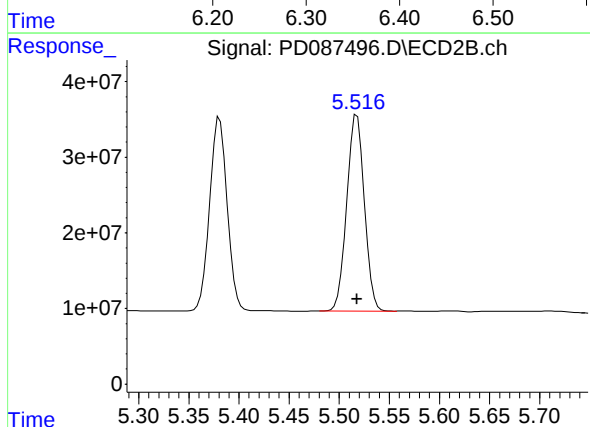


#13 Dieldrin

R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 317396123
Conc: 19.48 ng/ml

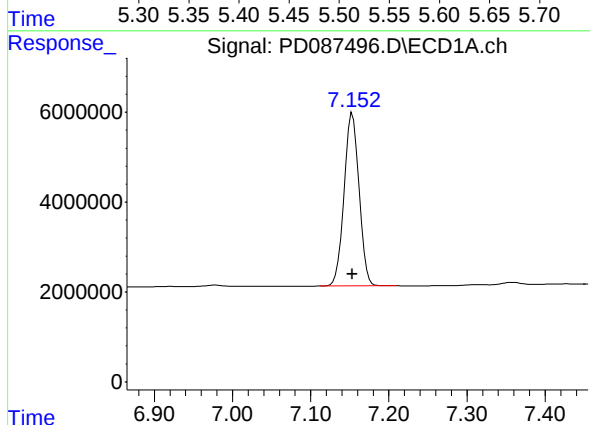


#19 Endosulfan Sulfate

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 51299260
Conc: 18.71 ng/ml

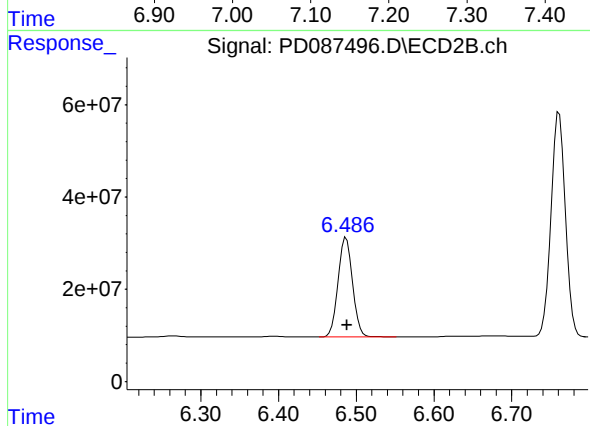

#19 Endosulfan Sulfate


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 280105331
Conc: 19.70 ng/ml

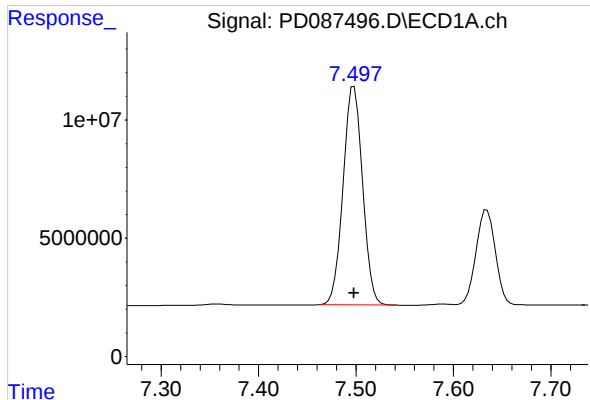

#20 Methoxychlor


R.T.: 7.498 min
Delta R.T.: 0.000 min
Response: 128370071
Conc: 87.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

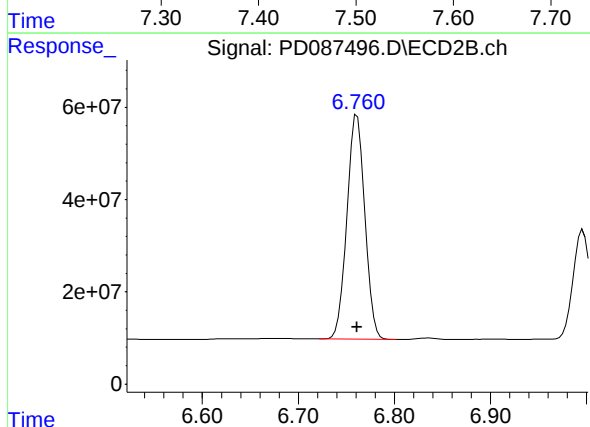


#20 Methoxychlor

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 629304469
Conc: 82.34 ng/ml

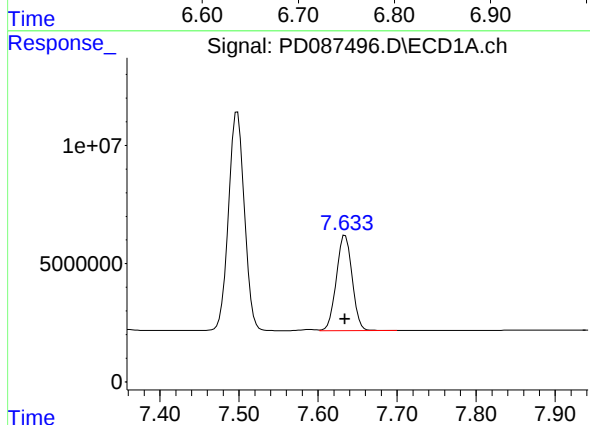


#21 Endrin ketone

R.T.: 7.635 min
Delta R.T.: 0.000 min
Response: 56126879
Conc: 18.25 ng/ml

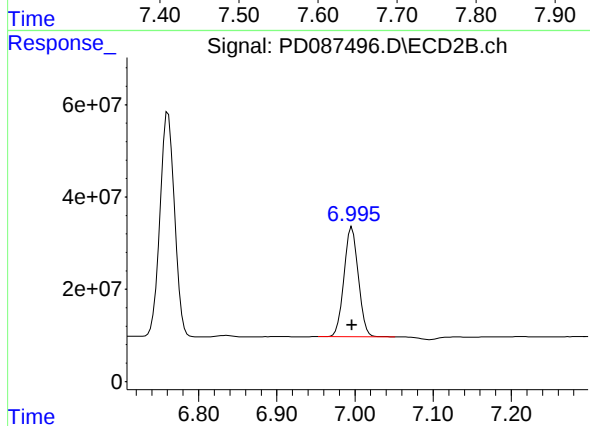

#21 Endrin ketone


R.T.: 6.996 min
Delta R.T.: 0.000 min
Response: 302795884
Conc: 19.41 ng/ml

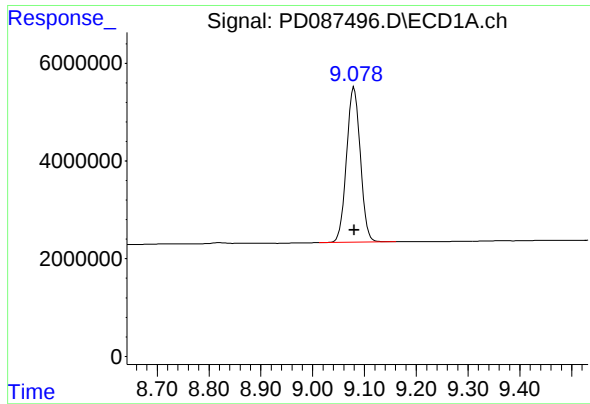

#28 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: 0.000 min
Response: 58676121
Conc: 19.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

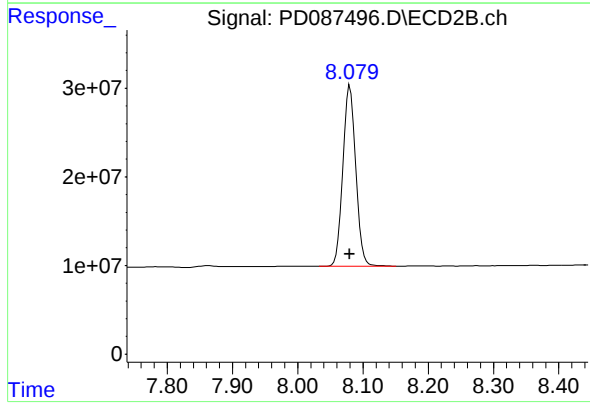

#28 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: 0.000 min
Response: 280344534
Conc: 19.84 ng/ml