

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012325\
 Data File : PD087504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jan 2025 13:30
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 14:14:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012325.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 22 14:13:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.881	93831064	662.2E6	50.000	50.000
28)	SA Decachlor...	9.082	8.081	140.1E6	661.6E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.722	3.909	61210584	261.9E6	500.000	500.000
24)	Chlordane-2	5.247	4.491	64262360	276.5E6	500.000	500.000
25)	Chlordane-3	5.953	5.131	245.2E6	819.1E6	500.000	500.000
26)	Chlordane-4	6.039	5.196	293.8E6	688.3E6	500.000	500.000
27)	Chlordane-5	6.878	6.095	51437816	314.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012325\
Data File : PD087504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jan 2025 13:30
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 14:14:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012325.M
Quant Title : GC Extractables
QLast Update : Wed Jan 22 14:13:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

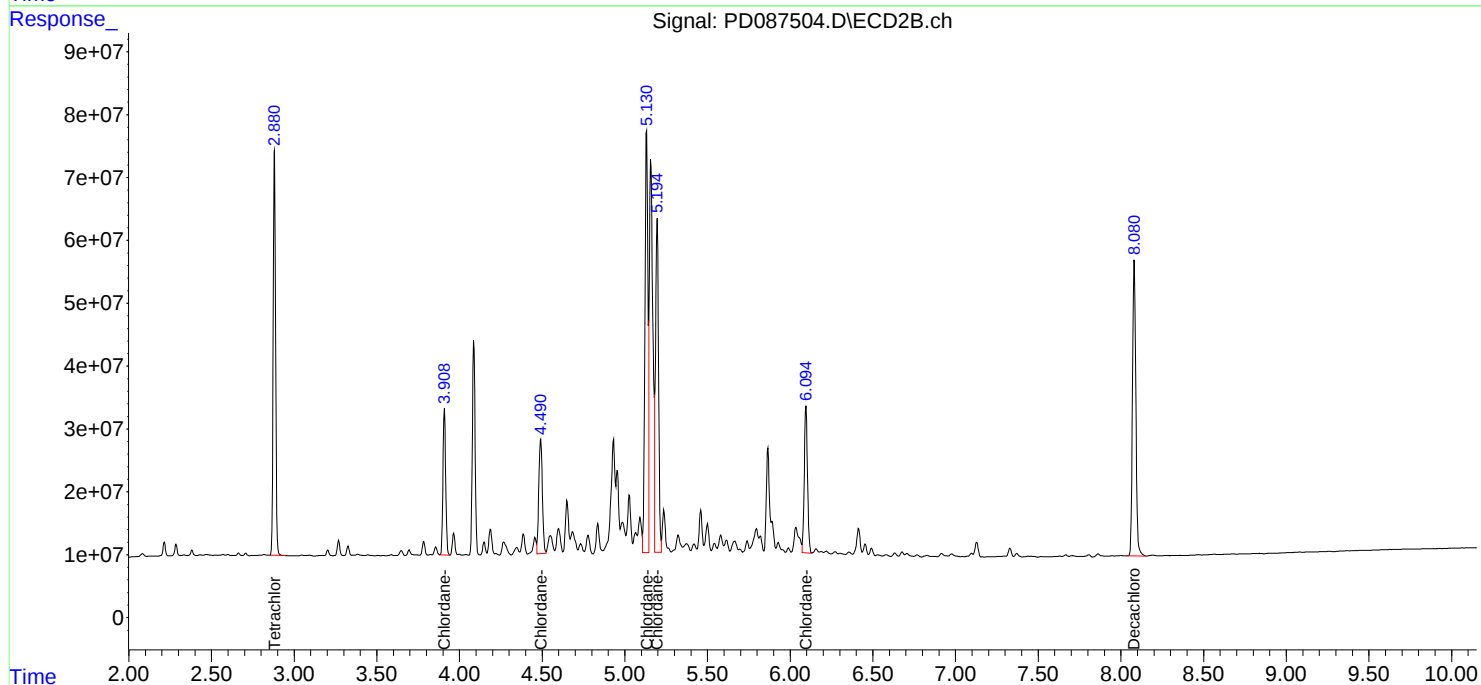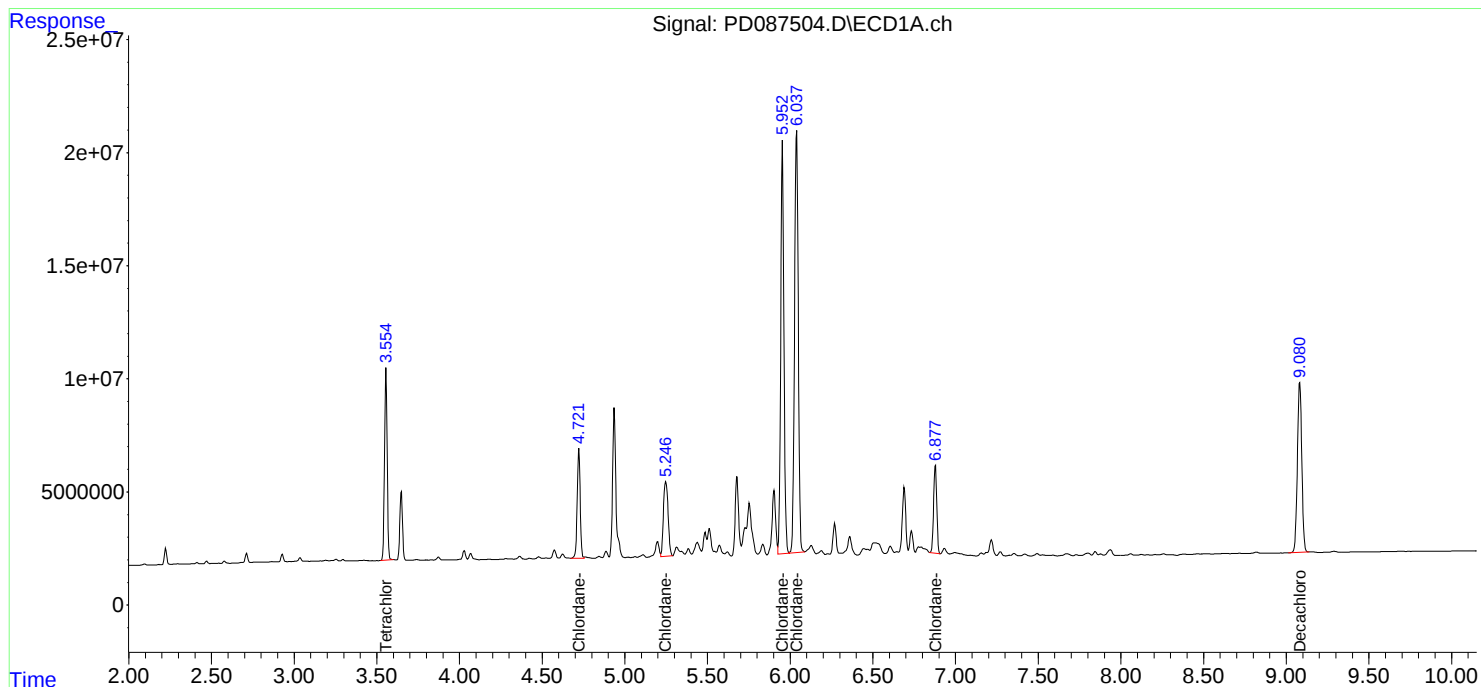


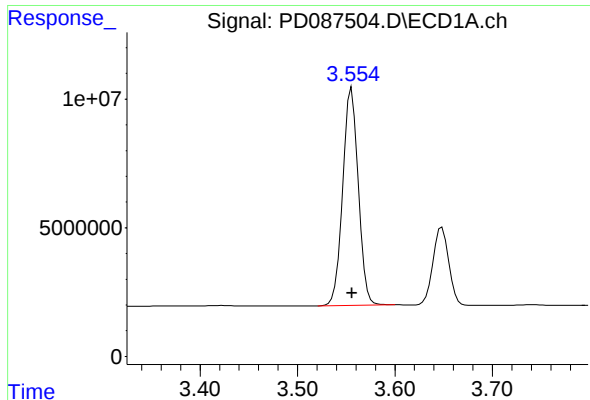

#1 Tetrachloro-m-xylene


R.T.: 3.556 min
Delta R.T.: 0.000 min
Response: 93831064
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

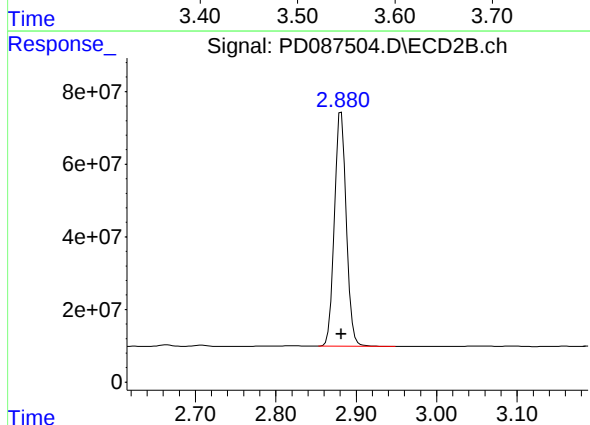


#1 Tetrachloro-m-xylene

R.T.: 2.881 min
Delta R.T.: 0.000 min
Response: 662219381
Conc: 50.00 ng/ml

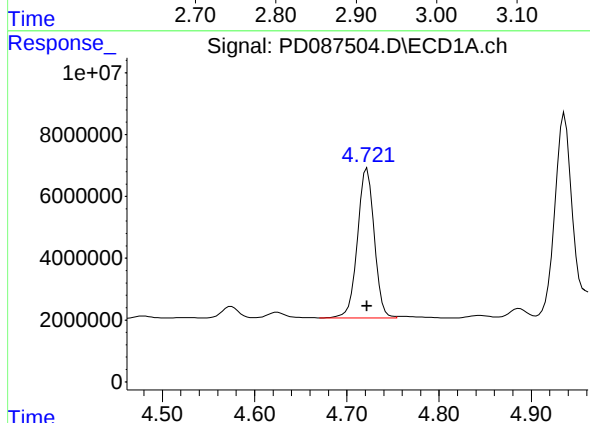


#23 Chlordane-1

R.T.: 4.722 min
Delta R.T.: 0.000 min
Response: 61210584
Conc: 500.00 ng/ml

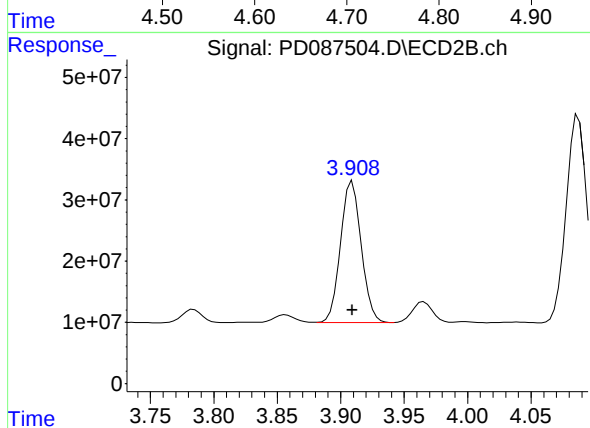

#23 Chlordane-1


R.T.: 3.909 min
Delta R.T.: 0.000 min
Response: 261926465
Conc: 500.00 ng/ml

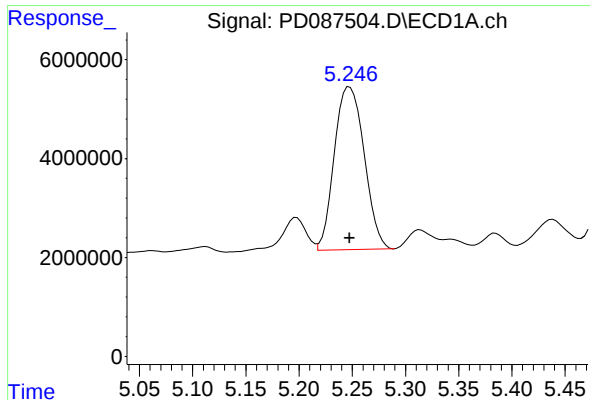

#24 Chlordane-2


R.T.: 5.247 min
Delta R.T.: 0.000 min
Response: 64262360
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

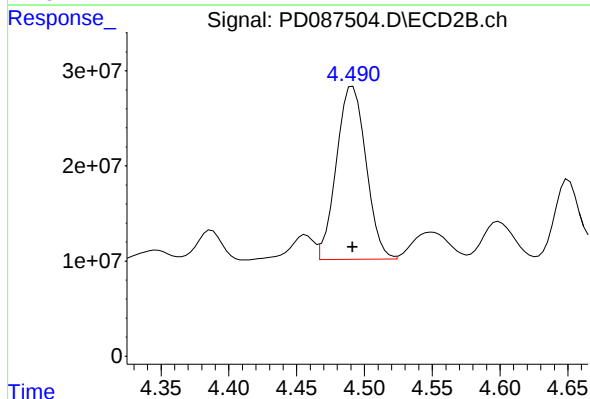


#24 Chlordane-2

R.T.: 4.491 min
Delta R.T.: 0.000 min
Response: 276495095
Conc: 500.00 ng/ml

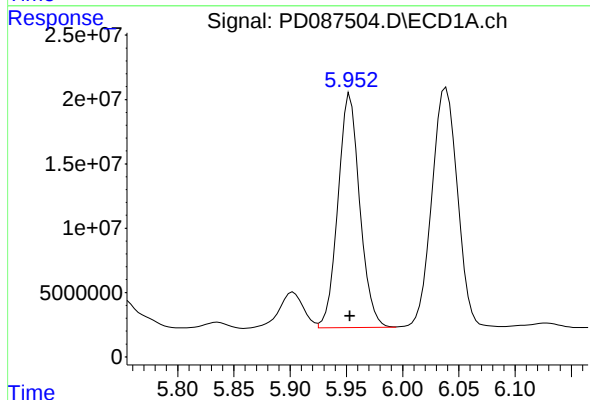


#25 Chlordane-3

R.T.: 5.953 min
Delta R.T.: 0.000 min
Response: 245233976
Conc: 500.00 ng/ml

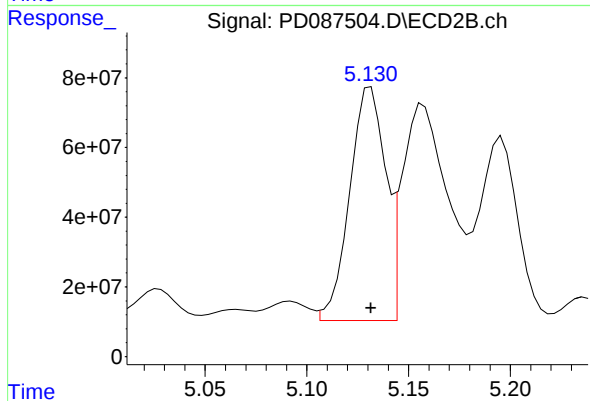

#25 Chlordane-3


R.T.: 5.131 min
Delta R.T.: 0.000 min
Response: 819131665
Conc: 500.00 ng/ml

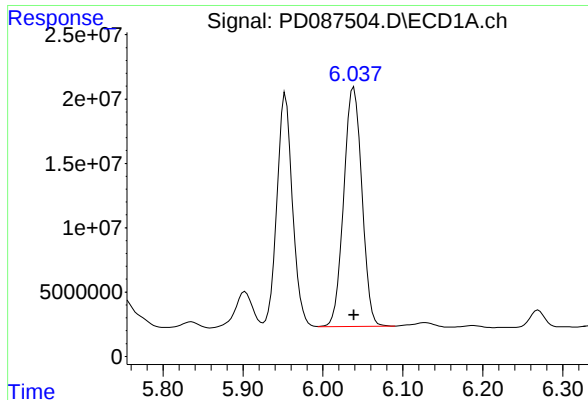

#26 Chlordane-4


R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 293820527
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

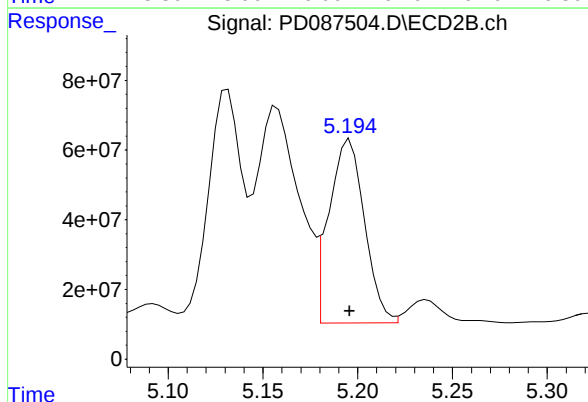


#26 Chlordane-4

R.T.: 5.196 min
Delta R.T.: 0.000 min
Response: 688333824
Conc: 500.00 ng/ml

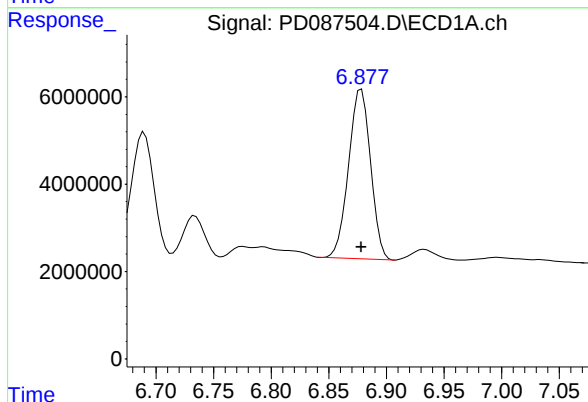


#27 Chlordane-5

R.T.: 6.878 min
Delta R.T.: 0.000 min
Response: 51437816
Conc: 500.00 ng/ml

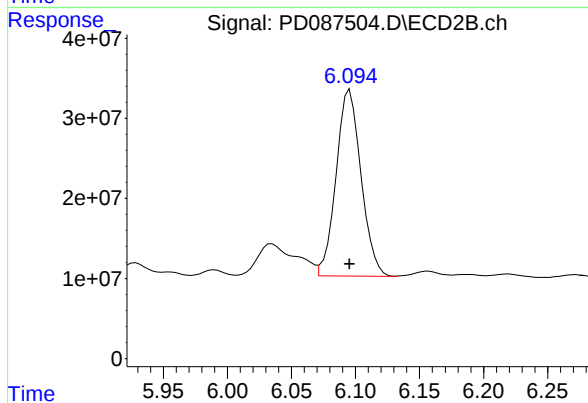

#27 Chlordane-5


R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 314410872
Conc: 500.00 ng/ml

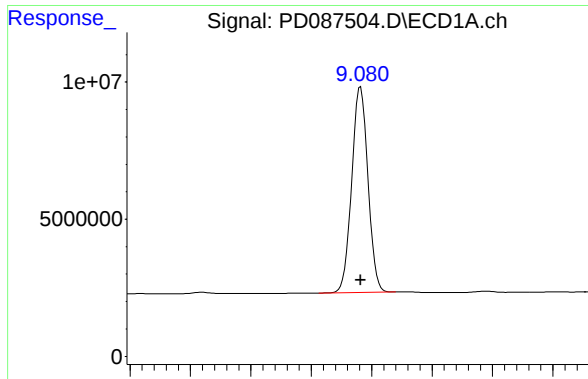

#28 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: 0.000 min
Response: 140136332
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

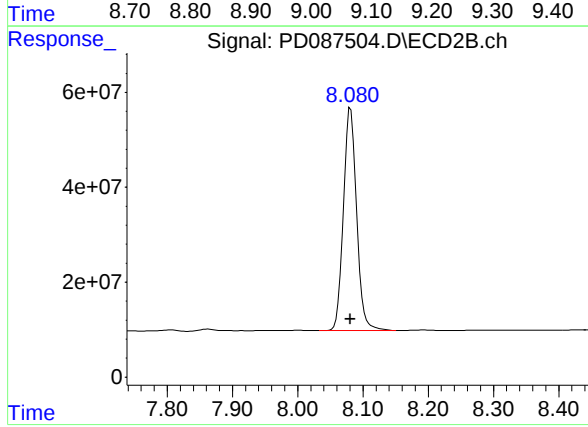

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: 0.000 min
Response: 661598145
Conc: 50.00 ng/ml