

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012419\
 Data File : PD051215.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2019 15:17
 Operator : AJ\SJ
 Sample : J6002-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 X2E84

Manual Integrations
 APPROVED

Sohil
 1/25/2019 9:36:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 03:50:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 25 03:30:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.225	4.044	28467003	805.1E6	20.400	28.239 #
27)	SA Decachlor...	7.831	9.164	47043308	785.2E6	38.506	42.220
Target Compounds							
2)	A alpha-BHC	3.646	4.439	180.8E6	2730.1E6	83.749	62.819
3)	MA gamma-BHC...	3.914	4.726	130.3E6	2099.2E6	62.543	53.106
4)	MA Heptachlor	4.192	5.240	108.3E6	1672.3E6	50.315	41.558
5)	MB Aldrin	4.425	5.547	64231912	1041.4E6	31.508	28.287
6)	B beta-BHC	4.160	4.895	45295431	776.8E6	48.331	42.082
7)	B delta-BHC	4.349	5.114	37155712	509.9E6	17.429	14.181m
8)	B Heptachlo...	4.853	5.935	78971887	1063.5E6	39.235	31.574
9)	A Endosulfan I	5.175	6.294	134.9E6	1785.9E6	69.168	57.017
10)	B trans-Chl...	5.069	6.170	98164630	1375.7E6	47.425m	40.696
11)	B cis-Chlor...	5.126	6.244	134.7E6	1747.0E6	66.554	53.664
12)	B 4,4'-DDE	5.296	6.399	177.8E6	2311.9E6	87.249	74.651
13)	MA Dieldrin	5.409	6.553	124.1E6	1693.6E6	56.690m	53.450
14)	MA Endrin	5.661	6.771	310.5E6	1737.8E6	158.273m	68.397m#
16)	A 4,4'-DDD	5.798	6.891	105.7E6	1455.8E6	61.692	58.346
17)	MA 4,4'-DDT	6.030	7.192	238.1E6	2644.3E6	132.392	115.801
19)	B Endosulfa...	6.303	7.330	62218726	884.0E6	34.873	35.548

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012419\
Data File : PD051215.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2019 15:17
Operator : AJ\SJ
Sample : J6002-09
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 03:50:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jan 25 03:30:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

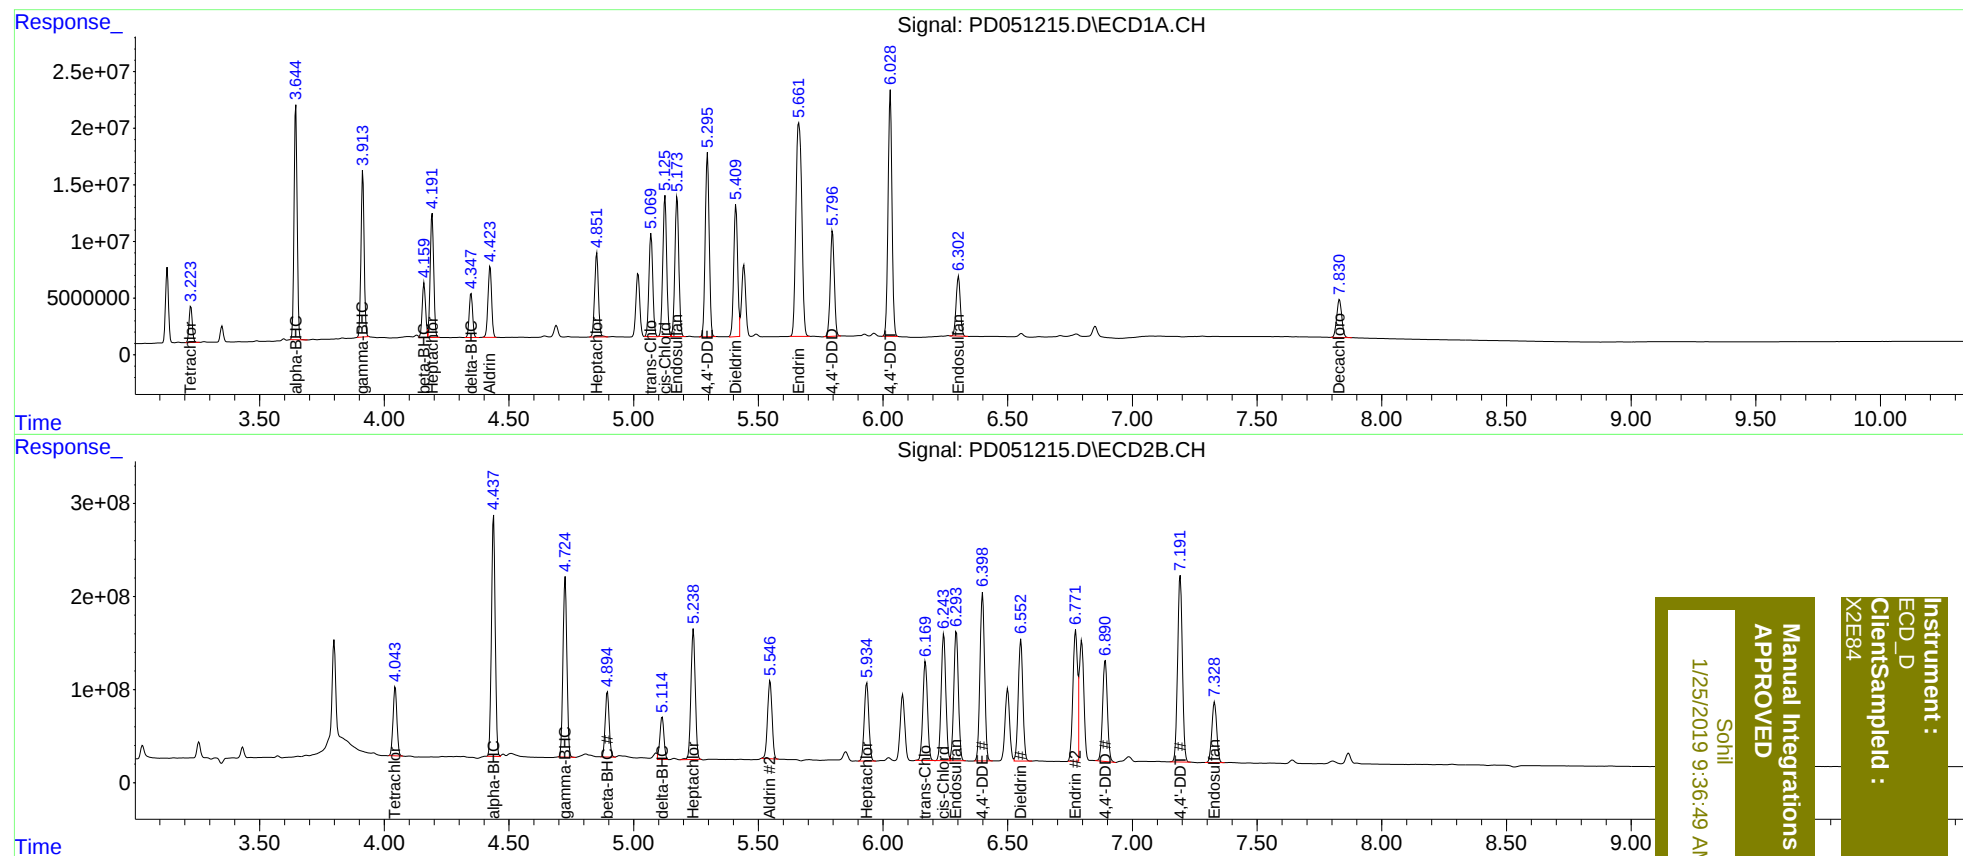

Manual Integrations
APPROVED

Sohil
1/25/2019 9:36:49 AM

Instrument :
ECD_D
ClientSampled :
X2E84

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012419\
 Data File : PD051215.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2019 15:17
 Operator : AJ\SJ
 Sample : J6002-09
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 X2E84

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 03:50:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012419CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 25 03:30:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Manual Integrations
 APPROVED

Sohil
 1/25/2019 9:36:49 AM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.225	4.044	28467003	805.1E6	20.400	28.239 #
27) SA Decachlor...	7.831	9.164	47043308	785.2E6	38.506	42.220
Target Compounds						
2) A alpha-BHC	3.646	4.439	180.8E6	2730.1E6	83.749	62.819
3) MA gamma-BHC...	3.914	4.726	130.3E6	2099.2E6	62.543	53.106
4) MA Heptachlor	4.192	5.240	108.3E6	1672.3E6	50.315	41.558
5) MB Aldrin	4.425	5.547	64231912	1041.4E6	31.508	28.287
6) B beta-BHC	4.160	4.895	45295431	776.8E6	48.331	42.082
7) B delta-BHC	4.349	5.114	37155712	509.9E6	17.429	14.181m
8) B Heptachlo...	4.853	5.935	78971887	1063.5E6	39.235	31.574
9) A Endosulfan I	5.175	6.294	134.9E6	1785.9E6	69.168	57.017
10) B trans-Chl...	5.069	6.170	98164630	1375.7E6	47.425m	40.696
11) B cis-Chlor...	5.126	6.244	134.7E6	1747.0E6	66.554	53.664
12) B 4,4'-DDE	5.296	6.399	177.8E6	2311.9E6	87.249	74.651
13) MA Dieldrin	5.409	6.553	124.1E6	1693.6E6	56.690m	53.450
14) MA Endrin	5.661	6.771	310.5E6	1737.8E6	158.273m	68.397m#
16) A 4,4'-DDD	5.798	6.891	105.7E6	1455.8E6	61.692	58.346
17) MA 4,4'-DDT	6.030	7.192	238.1E6	2644.3E6	132.392	115.801
19) B Endosulfa...	6.303	7.330	62218726	884.0E6	34.873	35.548

5.9
 01/25/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.