

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012422\
 Data File : PD067759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 10:29
 Operator : AR\AJ
 Sample : PB142200BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 05:31:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	3.960	40052356	156.3E6	17.678	19.279
27)	SA Decachlor...	8.155	9.015	35109736	170.1E6	36.658	33.669
Target Compounds							
2)	A alpha-BHC	0.000	4.381	0	1481891	N.D.	0.141
6)	B beta-BHC	0.000	4.822	0	3169393	N.D.	0.685
7)	B delta-BHC	0.000	4.998f	0	1245985	N.D.	0.133


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012422\
Data File : PD067759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 10:29
Operator : AR\AJ
Sample : PB142200BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 05:31:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

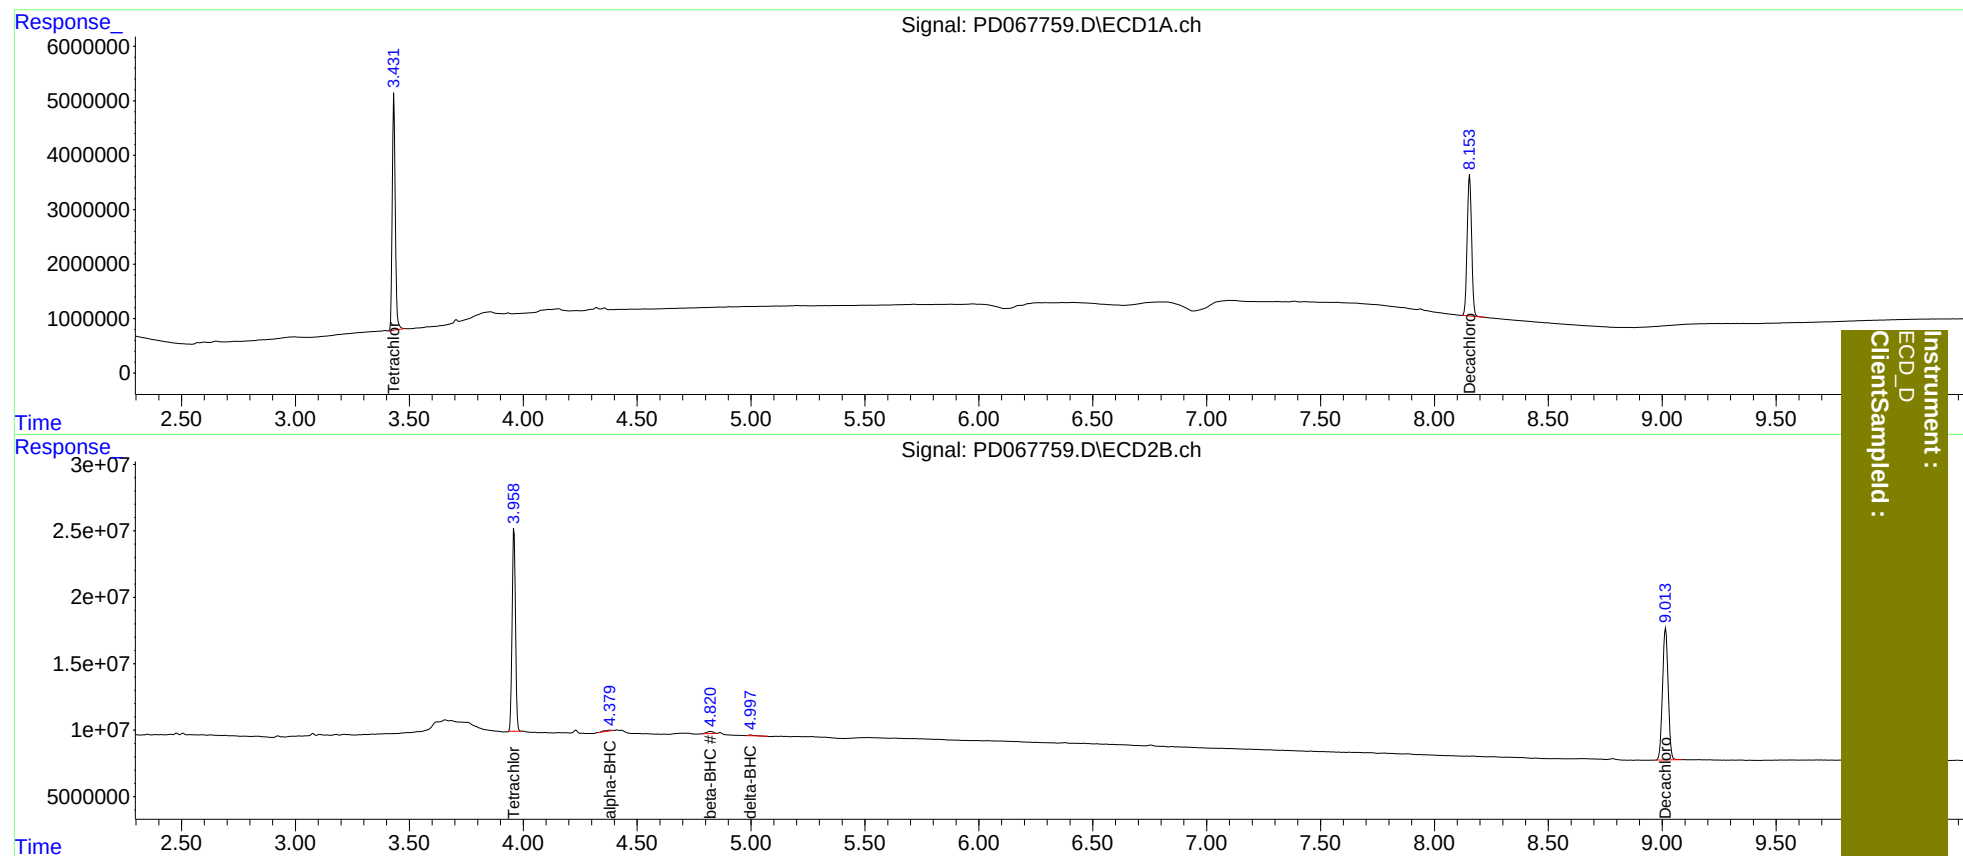


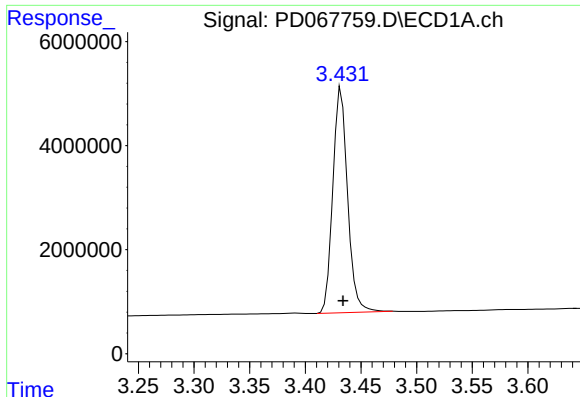

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: -0.002 min
Response: 40052356
Conc: 17.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

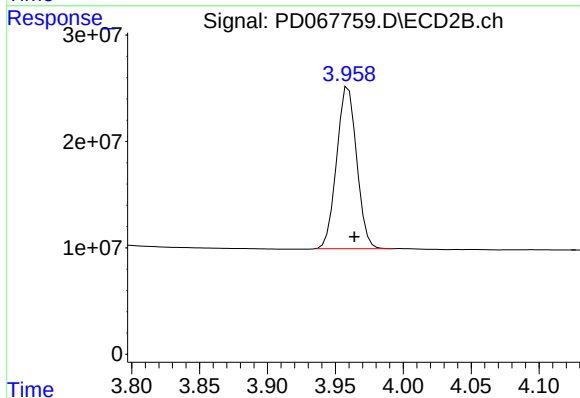


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.005 min
Response: 156255439
Conc: 19.28 ng/ml

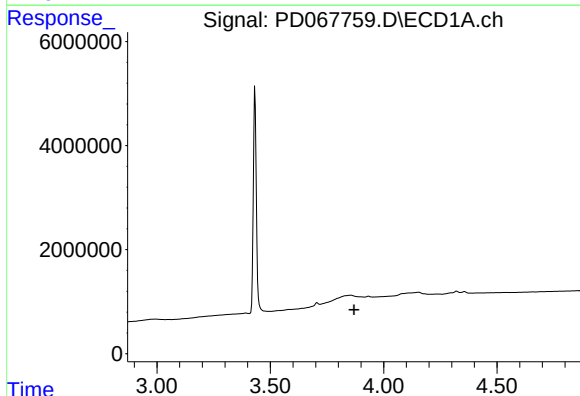


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.870 min
Response: 0
Conc: N.D.

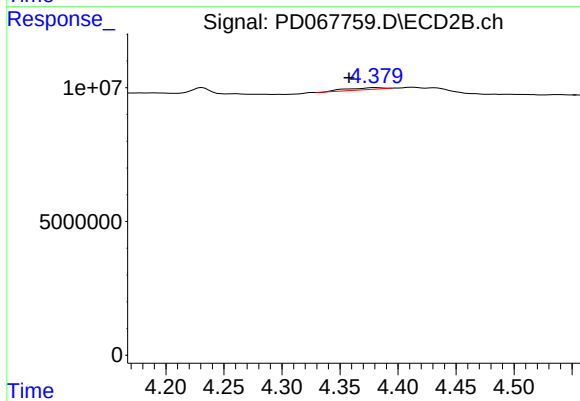

#2 alpha-BHC


R.T.: 4.381 min
Delta R.T.: 0.023 min
Response: 1481891
Conc: 0.14 ng/ml

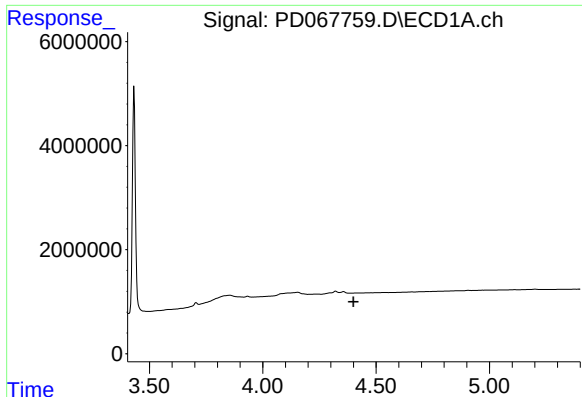

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

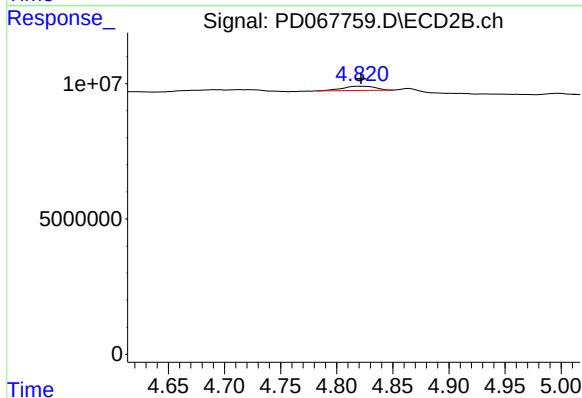


#6 beta-BHC

R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 3169393
Conc: 0.69 ng/ml

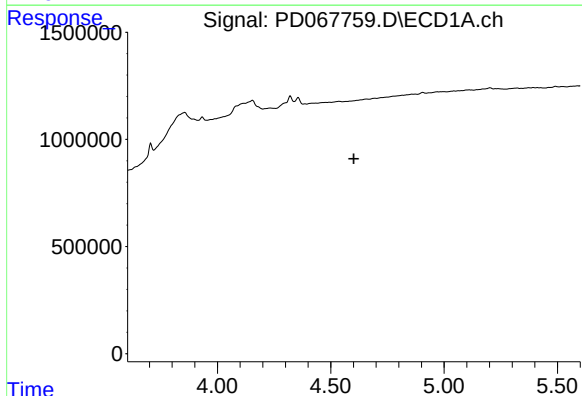


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.602 min
Response: 0
Conc: N.D.

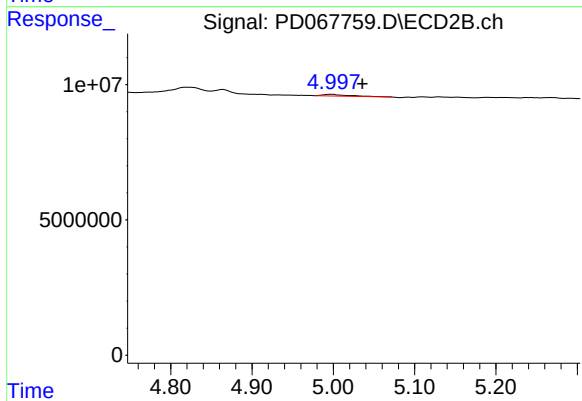

#7 delta-BHC


R.T.: 4.998 min
Delta R.T.: -0.038 min
Response: 1245985
Conc: 0.13 ng/ml

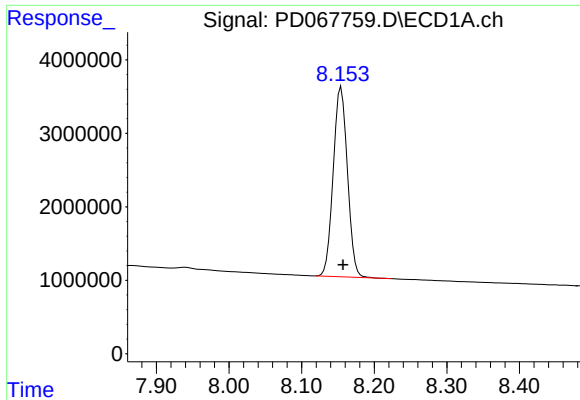

#27 Decachlorobiphenyl

R.T.: 8.155 min
Delta R.T.: -0.003 min
Response: 35109736
Conc: 36.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

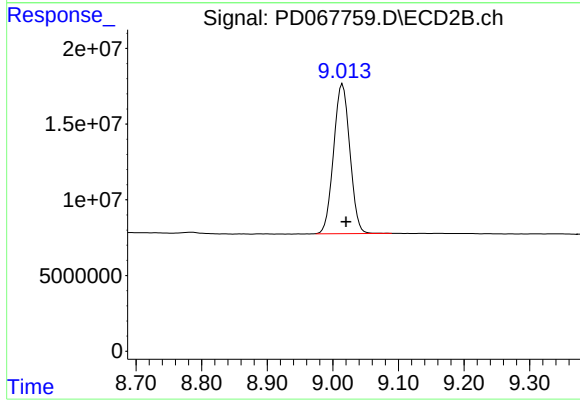

#27 Decachlorobiphenyl

R.T.: 9.015 min
Delta R.T.: -0.005 min
Response: 170132369
Conc: 33.67 ng/ml