

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012422\
 Data File : PD067769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 12:55
 Operator : AR\AJ
 Sample : N1199-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0F37

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/25/2022
 Supervised By : Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 05:34:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	3.959	45813576	173.7E6	20.221	21.427m
2)	SA Decachlor...	8.151	9.013	32834739	171.8E6	34.283m	34.002m
Target Compounds							
13)	MA Dieldrin	5.702	6.444	2259903	5995506	0.802m	0.797m
17)	MA 4,4'-DDT	6.332	7.081	6199977	3019186	3.011m	0.520 #
21)	B Endrin ke...	7.105	7.699	1464360	5557448	0.770	0.839m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012422\
Data File : PD067769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 12:55
Operator : AR\AJ
Sample : N1199-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 05:34:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

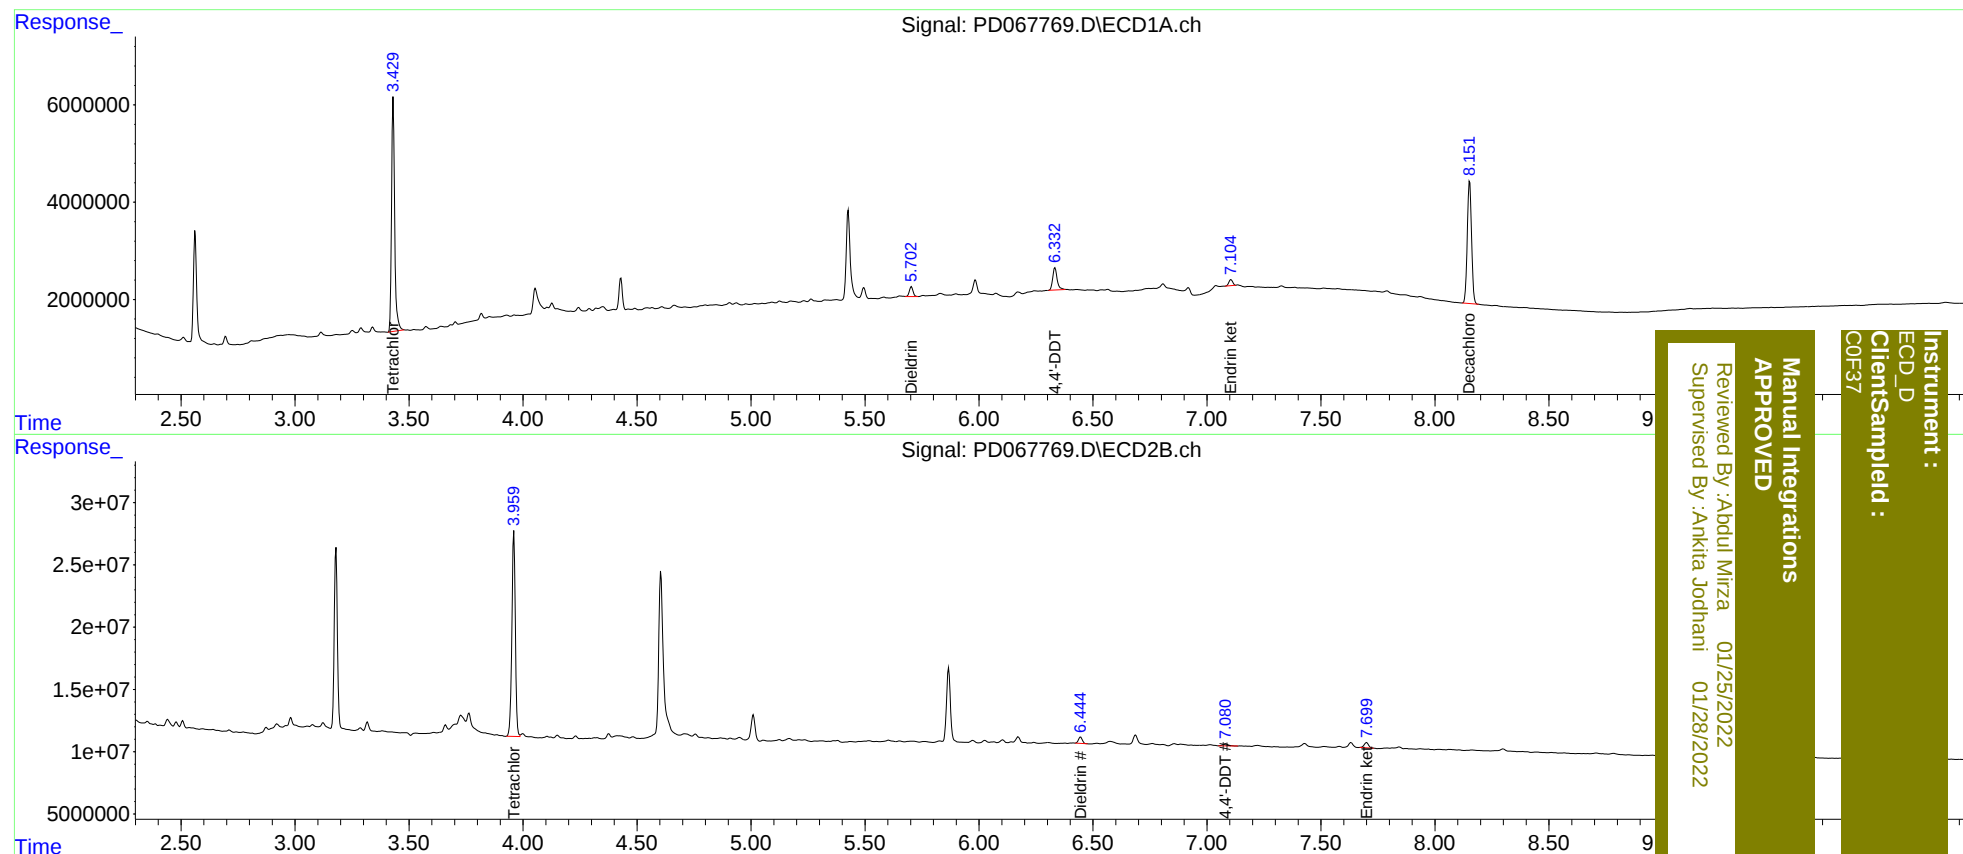

Instrument :
ECD_D
ClientSampled :
COF37

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/25/2022
Supervised By :Ankita Jodhani 01/28/2022