

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012422\
 Data File : PD067760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 10:43
 Operator : AR\AJ
 Sample : PB142200BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS200

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/25/2022
 Supervised By :Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 05:31:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	3.960	40482096	155.9E6	17.868	19.235
27)	SA Decachlor...	8.152	9.012	35950844	175.1E6	37.537	34.657m
Target Compounds							
2)	A alpha-BHC	3.866	4.354	13101776	48430725	3.953	4.621
3)	MA gamma-BHC...	4.148	4.639	13474149	47682523	4.259	4.833
4)	MA Heptachlor	4.440	5.137	13686526	43390156	4.416	4.852m
5)	MB Aldrin	4.684	5.441	14226038	42173521	4.550m	5.029
6)	B beta-BHC	4.397	4.818	6963739	24722451	5.182	5.346
7)	B delta-BHC	4.598	5.031	10125378	36670363	3.423	3.911
8)	B Heptachlo...	5.126	5.831	13494812	49350336	4.855	5.883
9)	A Endosulfan I	5.462	6.187	12961880	34968710	4.897	4.867
10)	B trans-Chl...	5.350	6.064	13756022	36347956	4.873	4.860
11)	B cis-Chlor...	5.408	6.135	13584851	37007872	4.956	5.022
12)	B 4,4'-DDE	5.572	6.296	25638190	68394311	10.207	10.130
13)	MA Dieldrin	5.704	6.445	26149033	71366690	9.277	9.491
14)	MA Endrin	5.961	6.663	23109376	58127347	10.373	10.420
15)	B Endosulfa...	6.234	6.879	22560770	62719620	10.429	9.929
16)	A 4,4'-DDD	6.085	6.791	19453190	58439775	9.765m	9.943
17)	MA 4,4'-DDT	6.325	7.088	17685449	53098044	8.588	9.140
18)	B Endrin al...	6.404	7.002	18405784	53192083	11.817	11.255m
19)	B Endosulfa...	6.615	7.227	17044340	49759156	9.381	8.529
20)	A Methoxychlor	6.872	7.549	46083994	137.7E6	52.251	49.956m
21)	B Endrin ke...	7.105	7.700	19245161	67197275	10.114m	10.148

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012422\
Data File : PD067760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 10:43
Operator : AR\AJ
Sample : PB142200BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 05:31:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

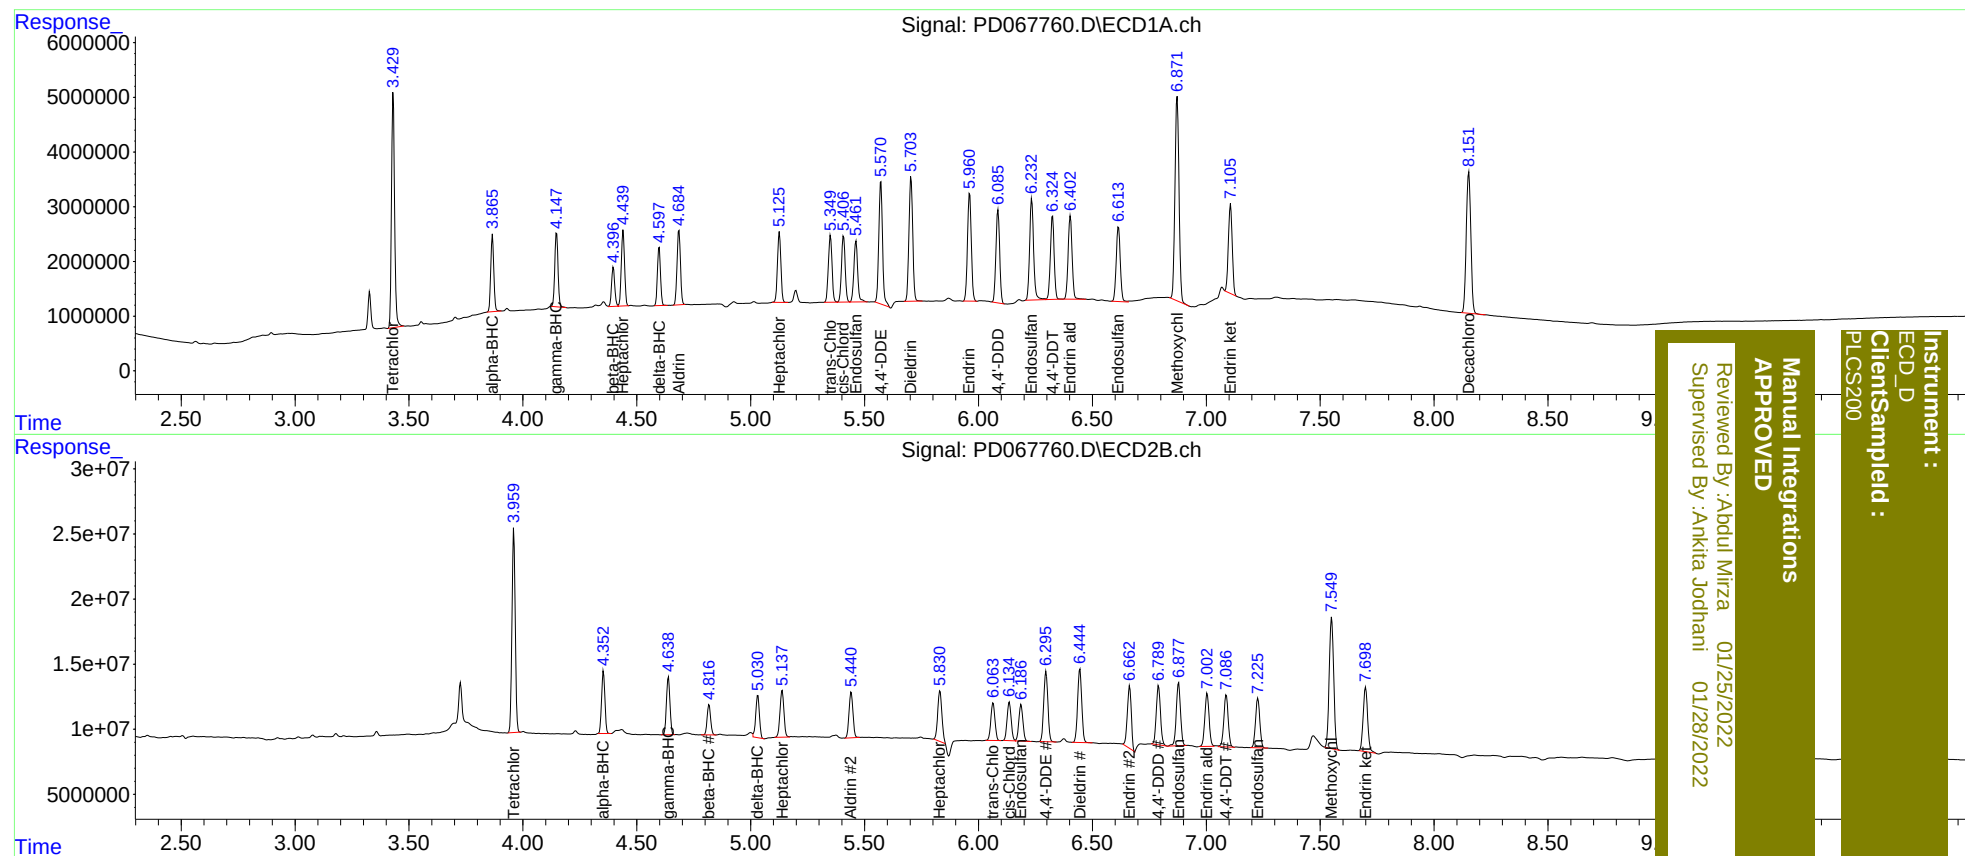

Reviewed By: Abdul Mirza 01/25/2022
Supervised By: Ankita Jodhani 01/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS200