

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012422\
 Data File : PD067772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2022 13:37
 Operator : AR\AJ
 Sample : N1199-12MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0Q07MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/25/2022
 Supervised By : Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 05:35:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 28 14:32:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	3.945	3657.8E6	14414.3E6	1614.438m	1778.495m
27)	SA Decachlor...	8.151	9.014	33088614	184.8E6	34.548m	36.574
Target Compounds							
2)	A alpha-BHC	3.867	4.354	132.5E6	360.2E6	39.968	34.368
3)	MA gamma-BHC...	4.147	4.633	124.4E6	726.3E6	39.319m	73.612m#
4)	MA Heptachlor	4.432	5.137	281.5E6	288.3E6	90.808m	32.237m#
5)	MB Aldrin	4.686	5.442	129.5E6	282.3E6	41.412	33.666
6)	B beta-BHC	4.398	4.816	59272087	152.9E6	44.104	33.064m#
7)	B delta-BHC	4.599	5.030	71370295	157.5E6	24.130	16.795 #
8)	B Heptachlo...	5.126	5.831	120.5E6	255.7E6	43.331	30.480 #
9)	A Endosulfan I	5.462	6.188	106.3E6	248.5E6	40.163	34.581
10)	B trans-Chl...	5.350	6.064	121.8E6	279.4E6	43.140	37.357
11)	B cis-Chlor...	5.408	6.136	113.2E6	244.2E6	41.281	33.137
12)	B 4,4'-DDE	5.572	6.297	221.9E6	532.1E6	88.345	78.800
13)	MA Dieldrin	5.704	6.446	246.1E6	584.9E6	87.320	77.787
14)	MA Endrin	5.961	6.664	214.6E6	502.8E6	96.324	90.144
15)	B Endosulfa...	6.234	6.879	193.8E6	484.0E6	89.569	76.622
16)	A 4,4'-DDD	6.085	6.791	179.4E6	453.0E6	90.037m	77.079
17)	MA 4,4'-DDT	6.324	7.088	183.4E6	462.8E6	89.049	79.667
18)	B Endrin al...	6.403	7.004	159.0E6	467.4E6	102.094	98.911
19)	B Endosulfa...	6.615	7.227	150.5E6	429.8E6	82.820	73.664
20)	A Methoxychlor	6.872	7.551	416.5E6	1143.1E6	472.286	414.590
21)	B Endrin ke...	7.106	7.698	183.1E6	568.4E6	96.226	85.841m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012422\
Data File : PD067772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2022 13:37
Operator : AR\AJ
Sample : N1199-12MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 05:35:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD122921CLP.M
Quant Title : GC Extractables
QLast Update : Tue Dec 28 14:32:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

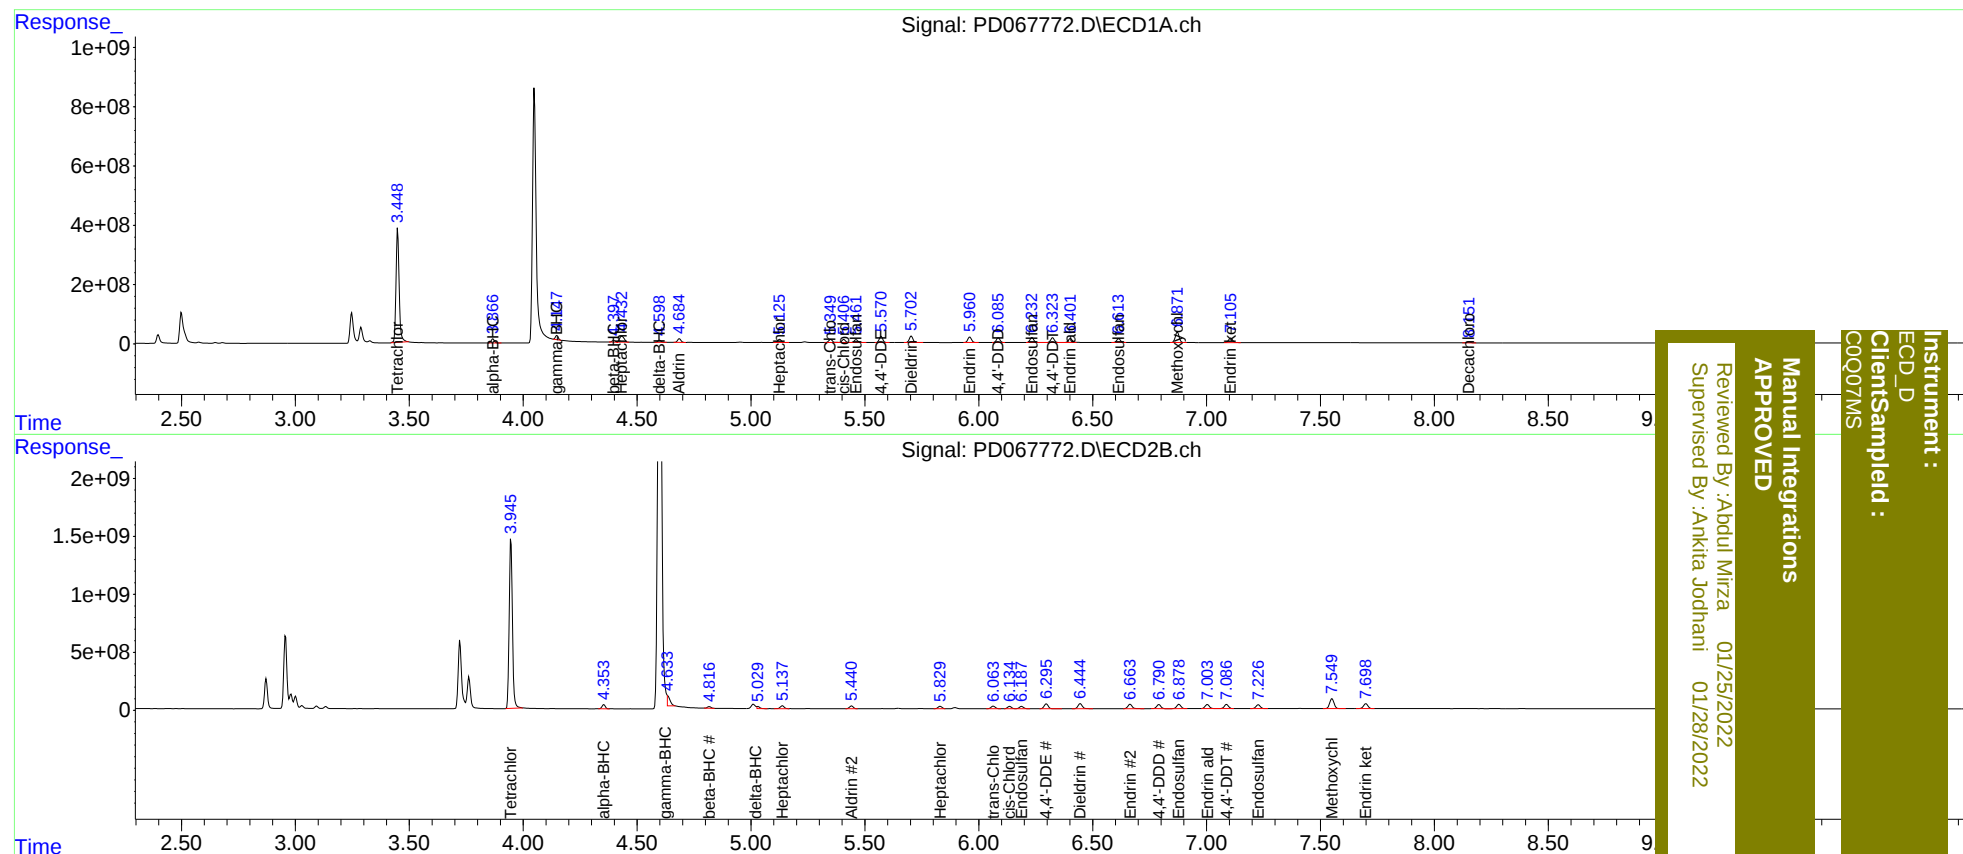

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 01/25/2022
Supervised By: Ankita Jodhani 01/28/2022

Instrument :
ECD_D
Client Sampled :
C0007MS