

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012423\
 Data File : PD073722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2023 09:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 10:21:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 19 02:45:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.777	53041373	29292215	22.692	23.009
28)	SA Decachlor...	9.100	7.933	59072627	24701913	20.962	21.231
Target Compounds							
4)	MA Heptachlor	4.923f	0.000	229540	0	0.062	N.D. #
6)	B beta-BHC	4.511f	3.916	149130	81213	0.096	0.123 #
7)	B delta-BHC	4.781	0.000	3289487	0	0.978	N.D. #
8)	B Heptachlo...	5.702	0.000	1497704	0	0.469	N.D. #
10)	B gamma-Chl...	5.974	0.000	242960	0	0.074	N.D. #
15)	B Endosulfa...	6.844f	0.000	470925	0	0.178	N.D. #
21)	B Endrin ke...	7.700f	0.000	597210	0	0.197	N.D. #
24)	Chlordane-2	0.000	4.351	0	328377	N.D.	6.576 #
25)	Chlordane-3	5.974	0.000	242960	0	0.519	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012423\
Data File : PD073722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2023 09:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 10:21:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD011823.M
Quant Title : GC Extractables
QLast Update : Thu Jan 19 02:45:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

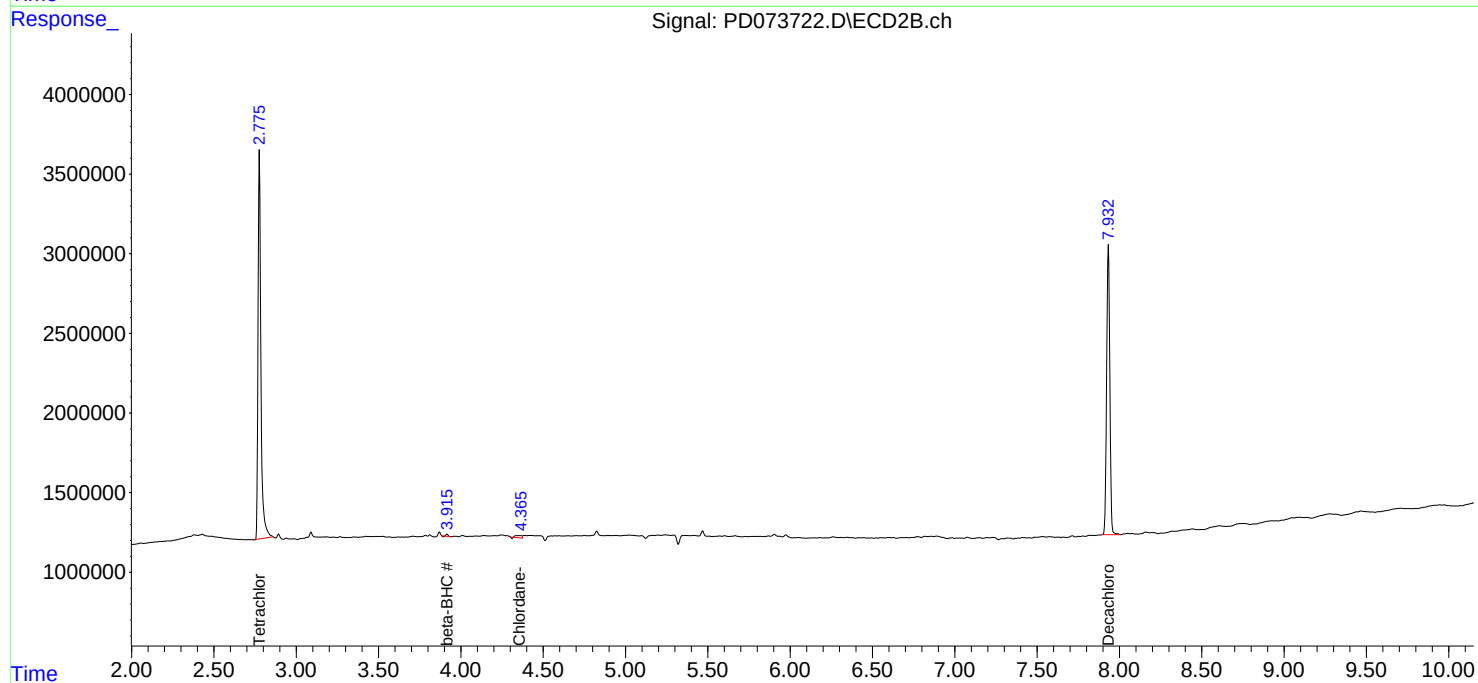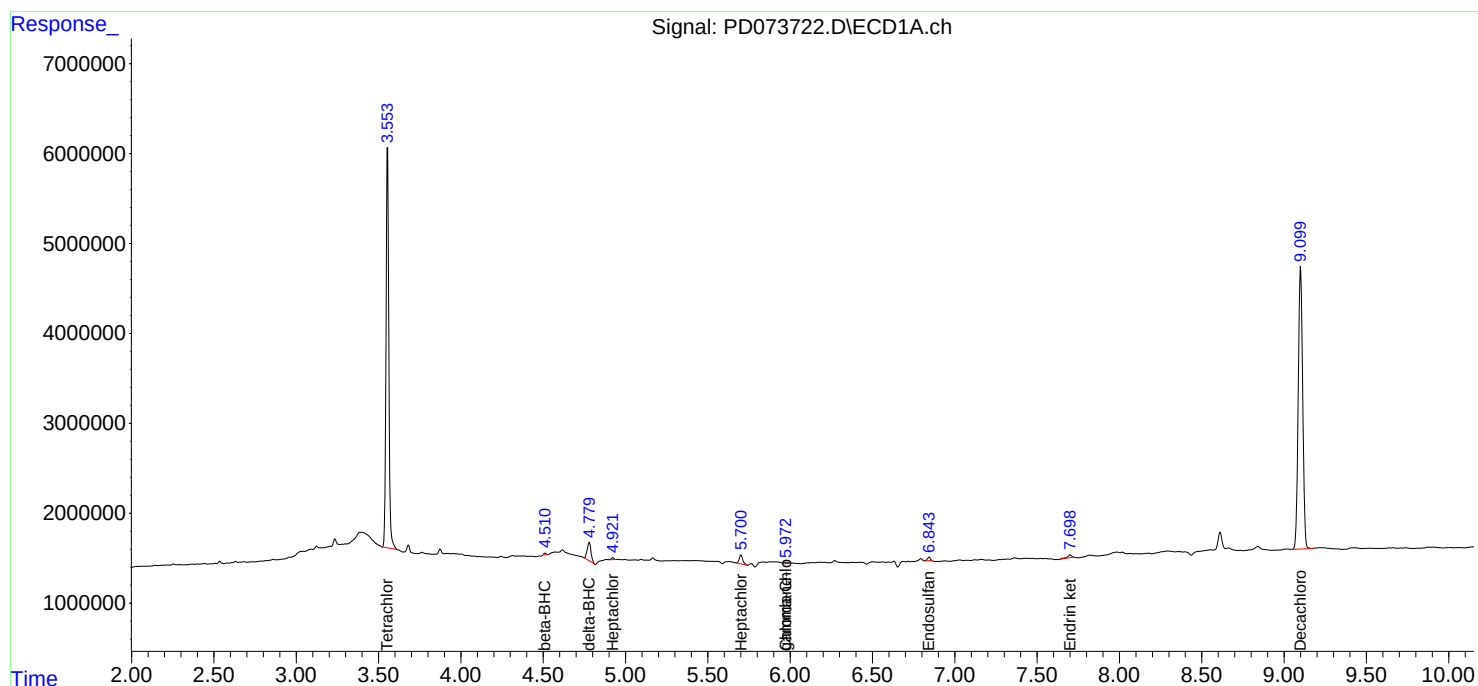


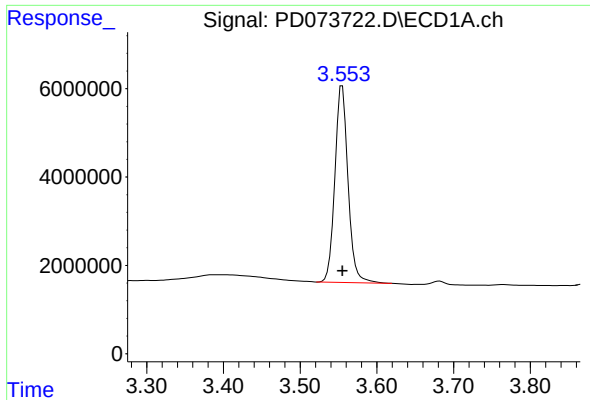

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 53041373
Conc: 22.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

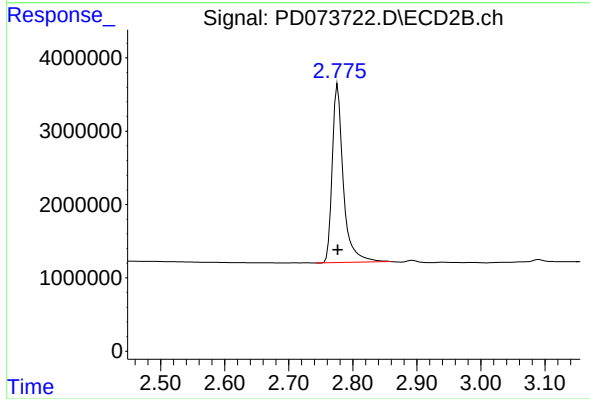


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 29292215
Conc: 23.01 ng/ml

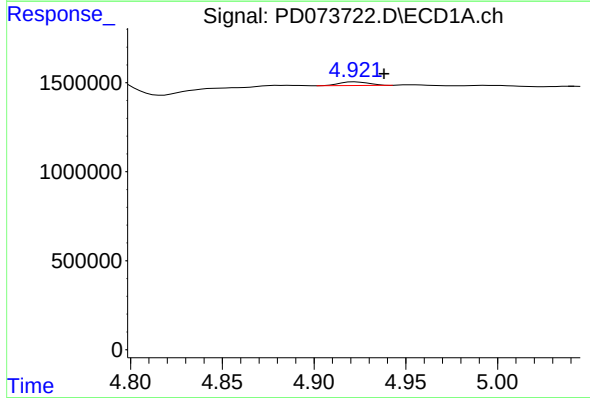


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: -0.015 min
Response: 229540
Conc: 0.06 ng/ml

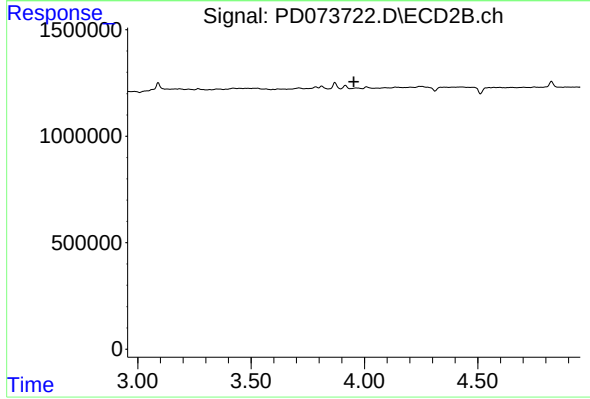

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.953 min
Response: 0
Conc: N.D.

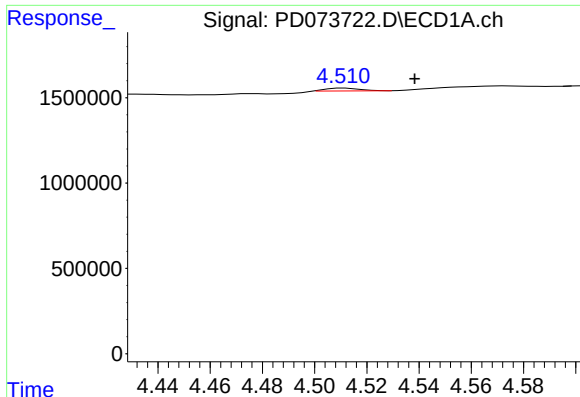

#6 beta-BHC


R.T.: 4.511 min
Delta R.T.: -0.027 min
Response: 149130
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

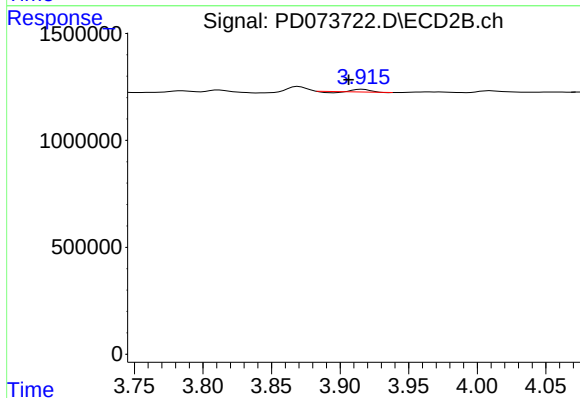


#6 beta-BHC

R.T.: 3.916 min
Delta R.T.: 0.010 min
Response: 81213
Conc: 0.12 ng/ml

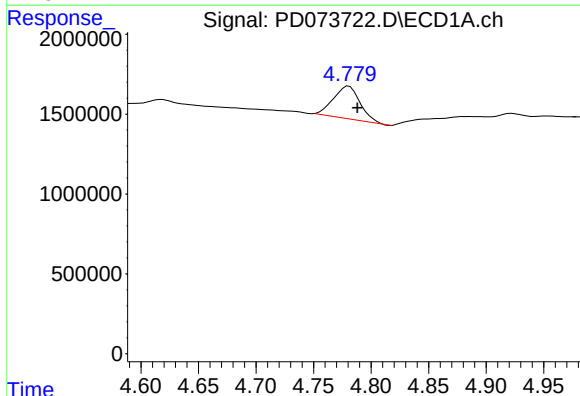


#7 delta-BHC

R.T.: 4.781 min
Delta R.T.: -0.007 min
Response: 3289487
Conc: 0.98 ng/ml

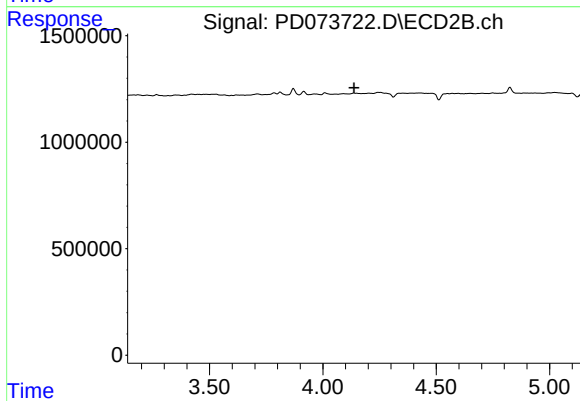

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.137 min
Response: 0
Conc: N.D.

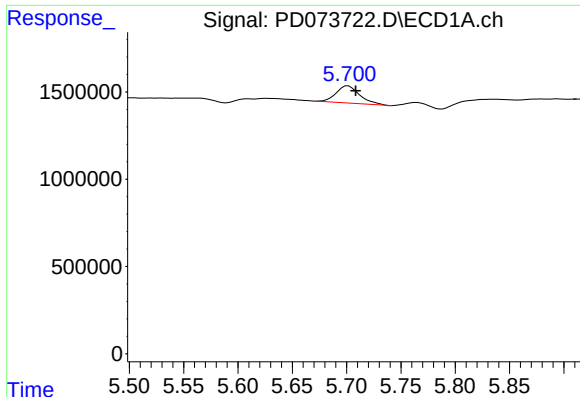

#8 Heptachlor epoxide


R.T.: 5.702 min
Delta R.T.: -0.007 min
Response: 1497704
Conc: 0.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

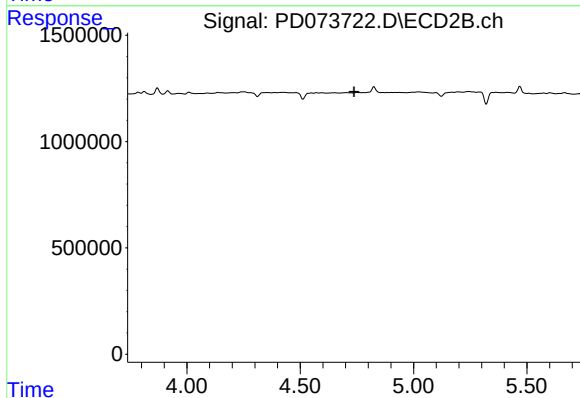


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.738 min
Response: 0
Conc: N.D.

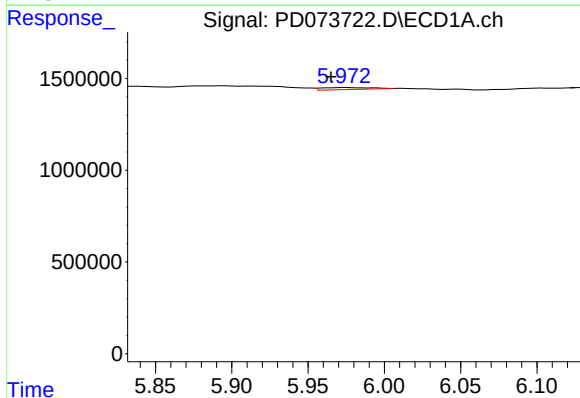


#10 gamma-Chlordane

R.T.: 5.974 min
Delta R.T.: 0.009 min
Response: 242960
Conc: 0.07 ng/ml

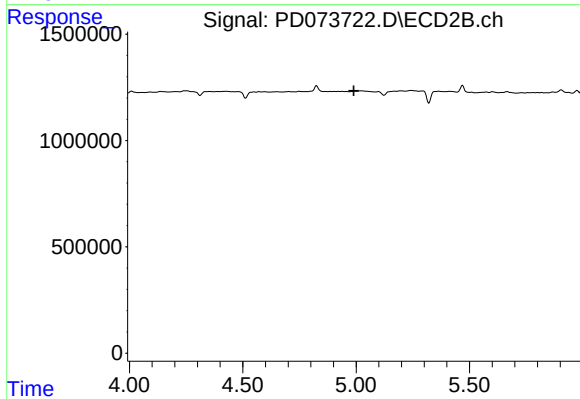

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

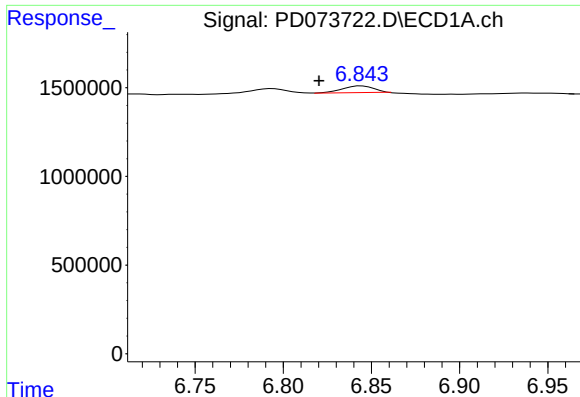

#15 Endosulfan II


R.T.: 6.844 min
Delta R.T.: 0.024 min
Response: 470925
Conc: 0.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

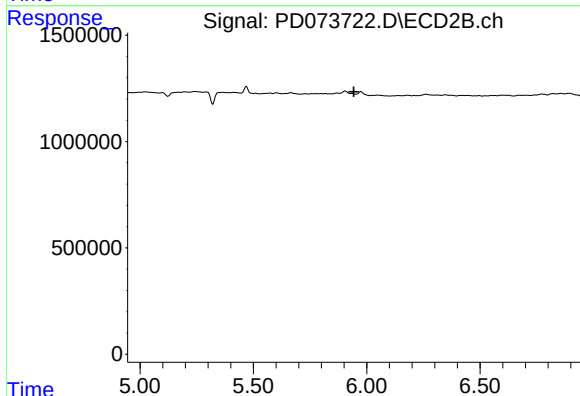


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.943 min
Response: 0
Conc: N.D.

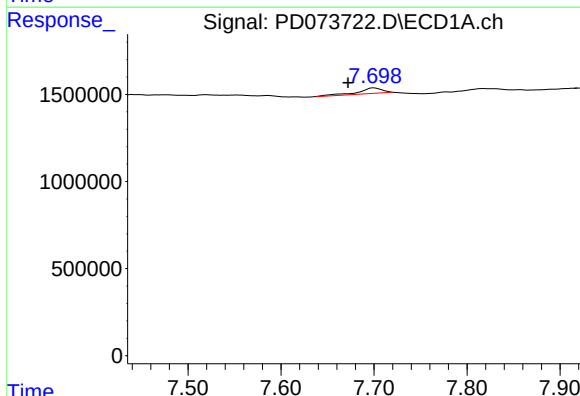


#21 Endrin ketone

R.T.: 7.700 min
Delta R.T.: 0.028 min
Response: 597210
Conc: 0.20 ng/ml

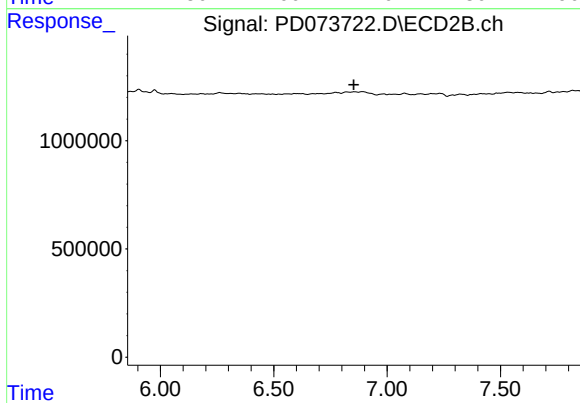

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

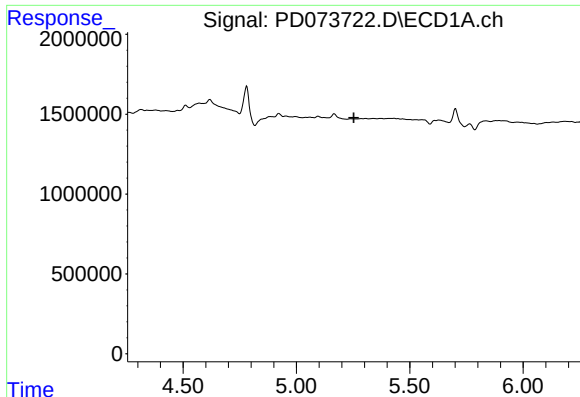

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.253 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

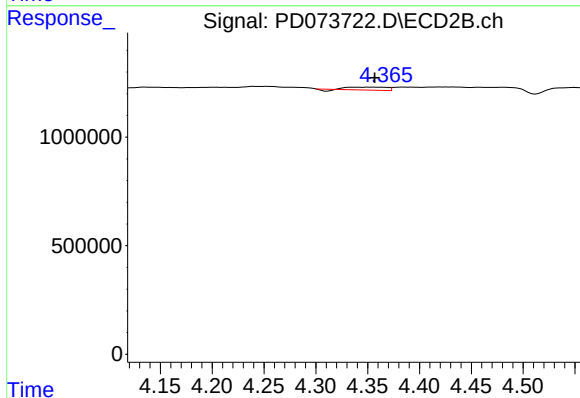


#24 Chlordane-2

R.T.: 4.351 min
Delta R.T.: -0.006 min
Response: 328377
Conc: 6.58 ng/ml

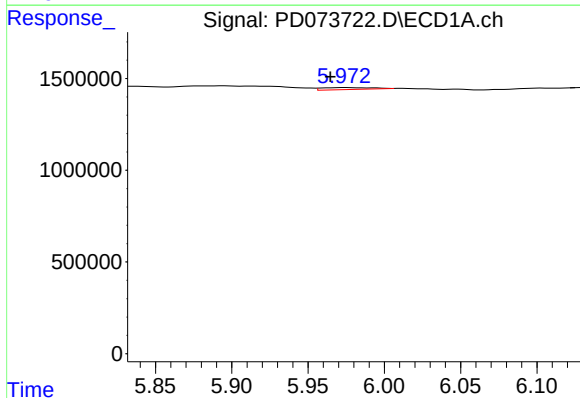


#25 Chlordane-3

R.T.: 5.974 min
Delta R.T.: 0.010 min
Response: 242960
Conc: 0.52 ng/ml

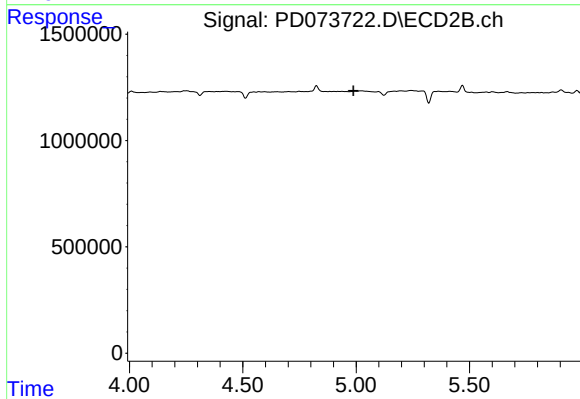

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 4.989 min
Response: 0
Conc: N.D.

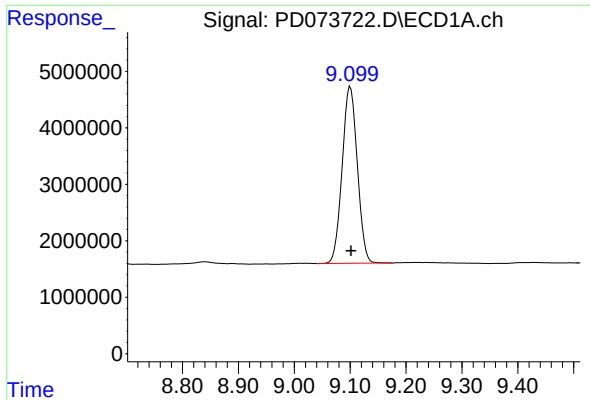

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: -0.001 min
Response: 59072627
Conc: 20.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

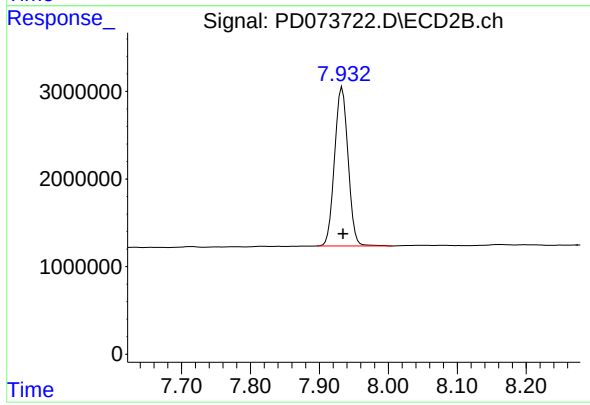

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: -0.001 min
Response: 24701913
Conc: 21.23 ng/ml