

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
 Data File : PD080831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 15:19
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 00:55:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 24 20:16:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	28053517	47609348	19.762	19.902
28)	SA Decachlor...	9.108	7.933	40880757	52901680	20.314	19.861
Target Compounds							
2)	A alpha-BHC	0.000	3.288	0	225936	N.D.	0.059 #
4)	MA Heptachlor	4.933f	0.000	363550	0	0.147	N.D. #
7)	B delta-BHC	4.792	0.000	719623	0	0.287	N.D. #
14)	MA Endrin	0.000	5.674f	0	310189	N.D.	0.105 #
15)	B Endosulfa...	6.802f	0.000	809009	0	0.418	N.D. #
17)	MA 4,4'-DDT	7.036f	0.000	127096	0	0.071	N.D. #
18)	B Endrin al...	0.000	6.140	0	283284	N.D.	0.126 #
21)	B Endrin ke...	7.708f	0.000	281609	0	0.135	N.D. #
24)	Chlordane-2	0.000	4.342f	0	152913	N.D.	1.248 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
Data File : PD080831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 15:19
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 00:55:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Wed Jan 24 20:16:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

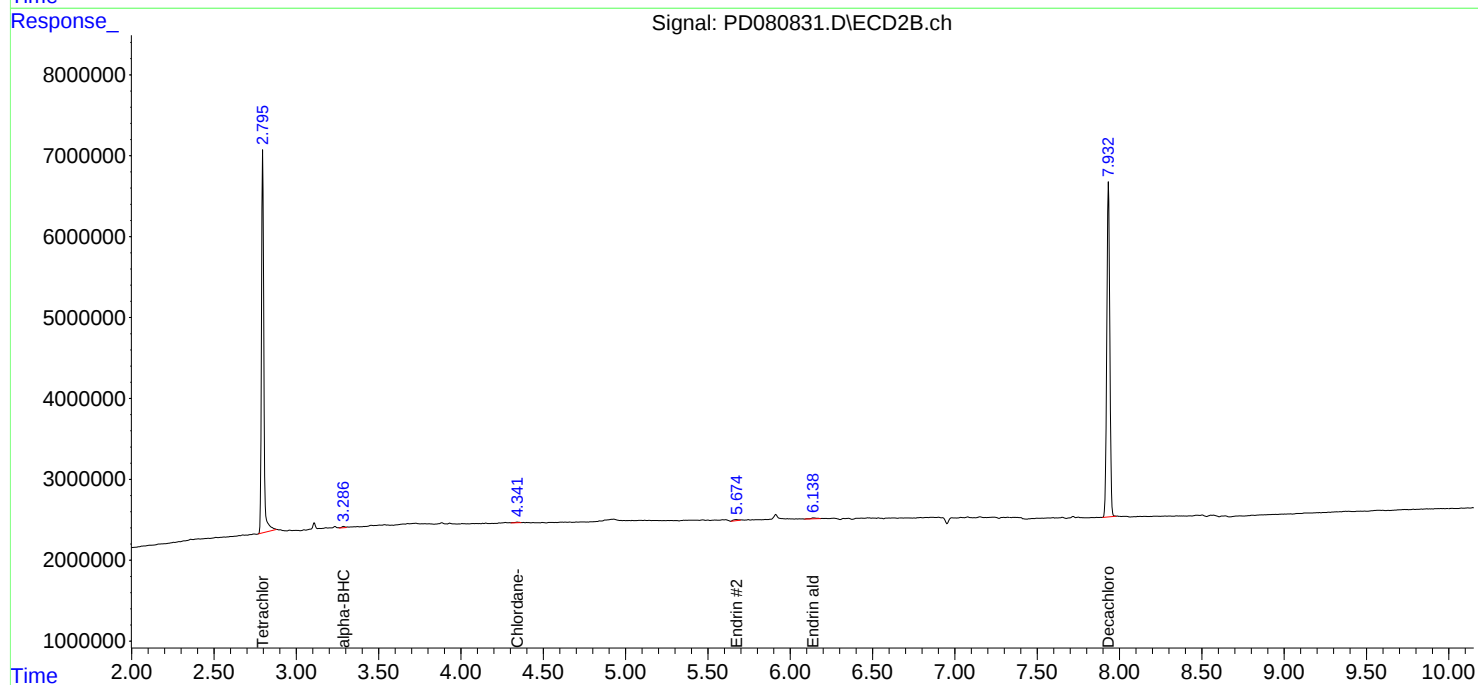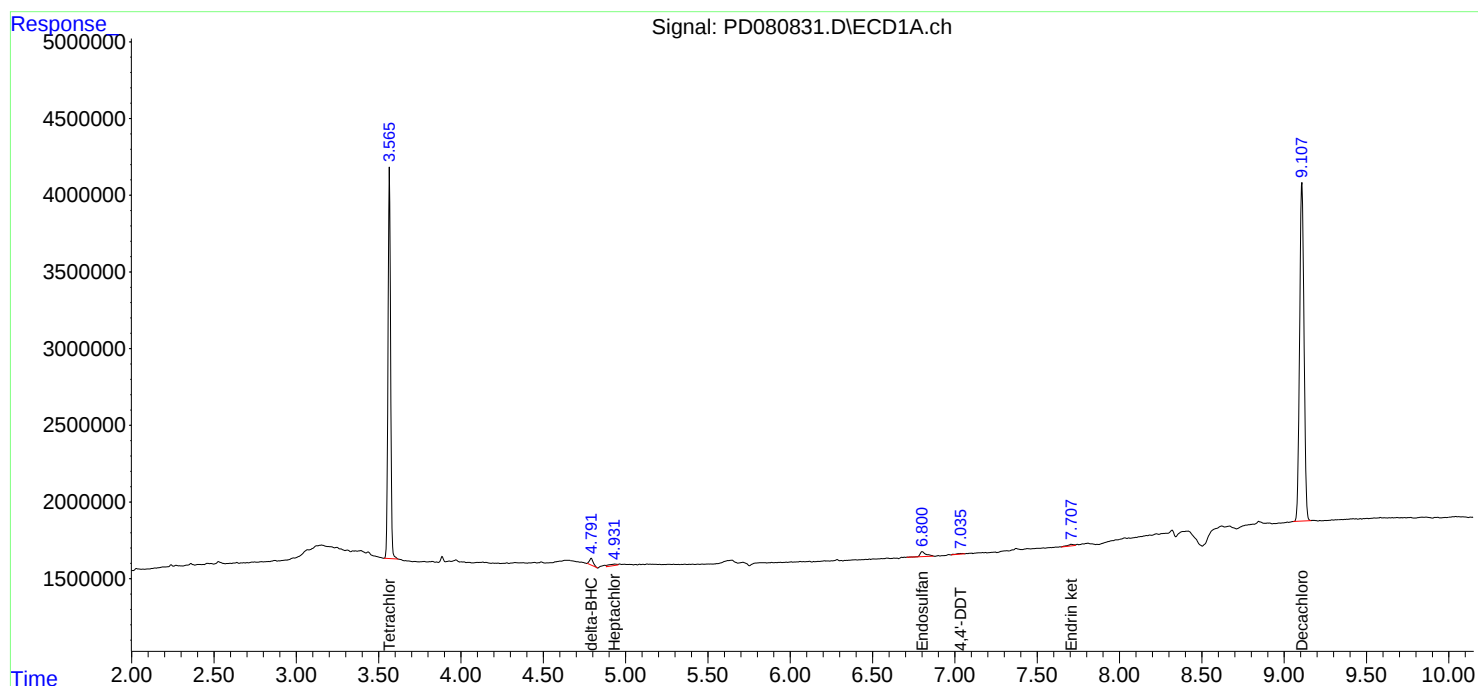


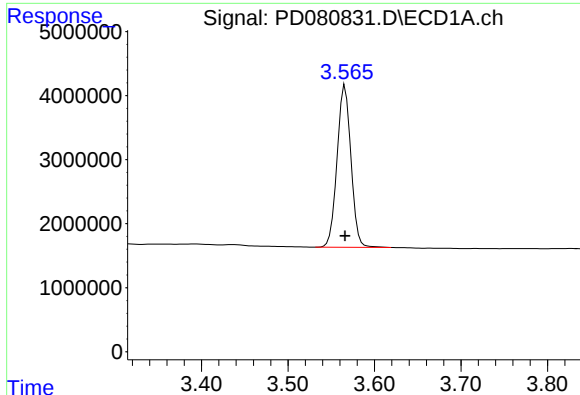

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 28053517
Conc: 19.76 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

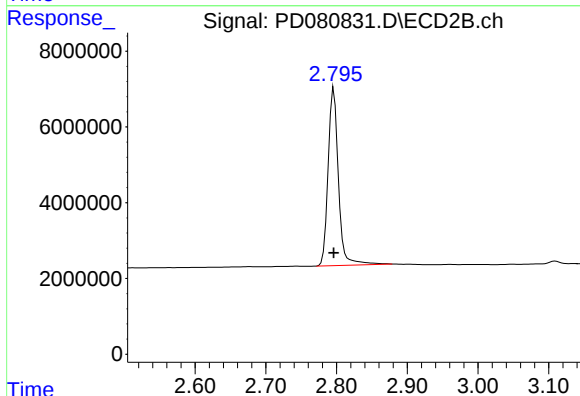


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 47609348
Conc: 19.90 ng/ml

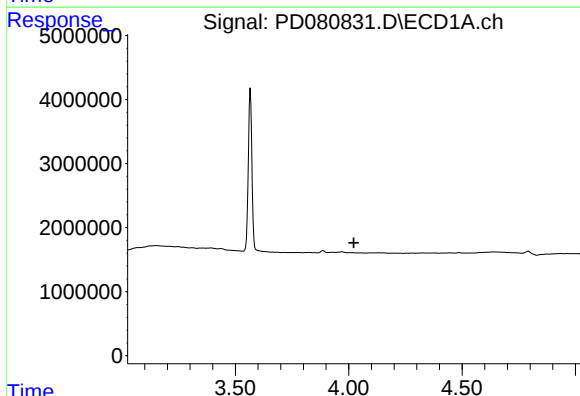


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.022 min
Response: 0
Conc: N.D.

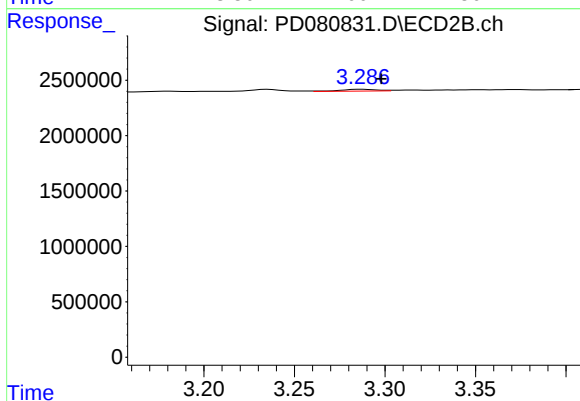

#2 alpha-BHC


R.T.: 3.288 min
Delta R.T.: -0.010 min
Response: 225936
Conc: 0.06 ng/ml

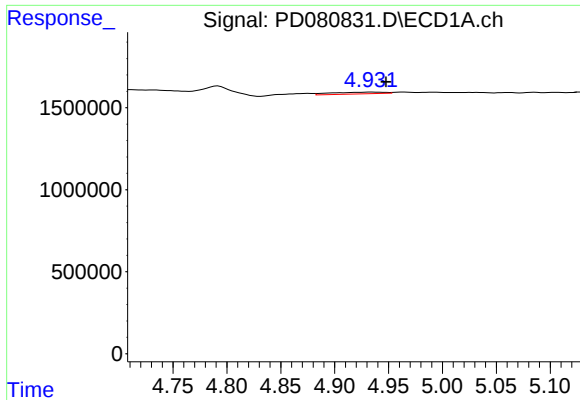

#4 Heptachlor


R.T.: 4.933 min
Delta R.T.: -0.015 min
Response: 363550
Conc: 0.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

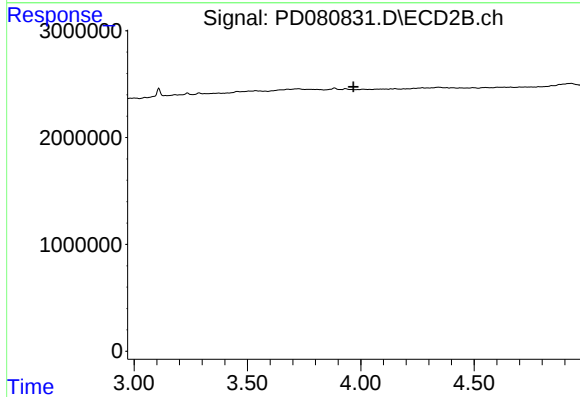


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.968 min
Response: 0
Conc: N.D.

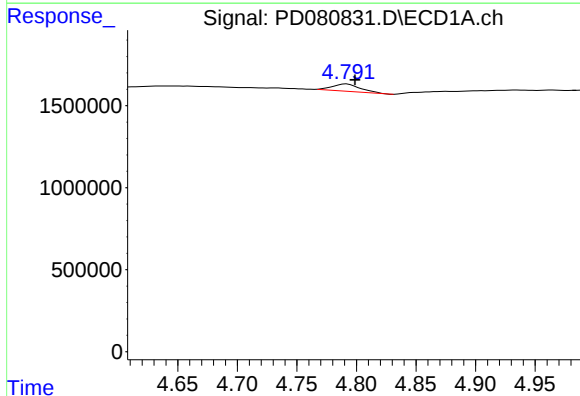


#7 delta-BHC

R.T.: 4.792 min
Delta R.T.: -0.007 min
Response: 719623
Conc: 0.29 ng/ml

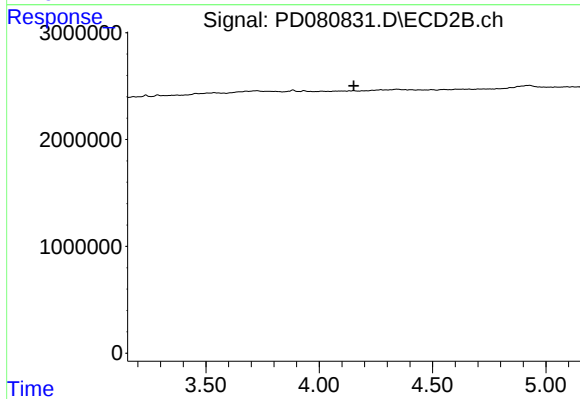

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

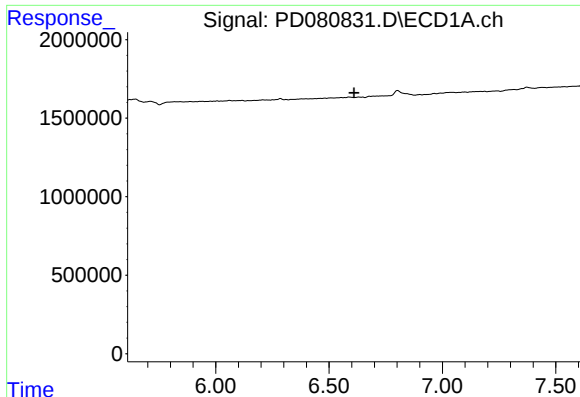

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

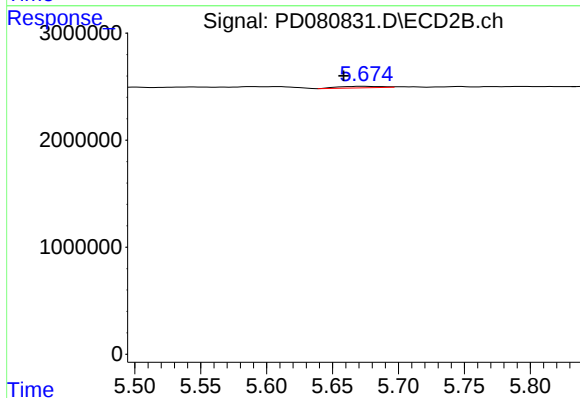


#14 Endrin

R.T.: 5.674 min
Delta R.T.: 0.016 min
Response: 310189
Conc: 0.10 ng/ml

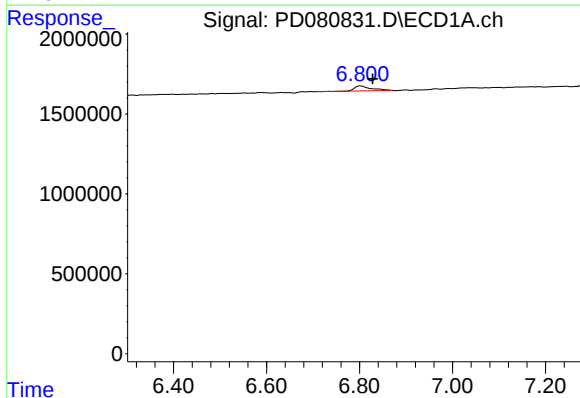


#15 Endosulfan II

R.T.: 6.802 min
Delta R.T.: -0.026 min
Response: 809009
Conc: 0.42 ng/ml

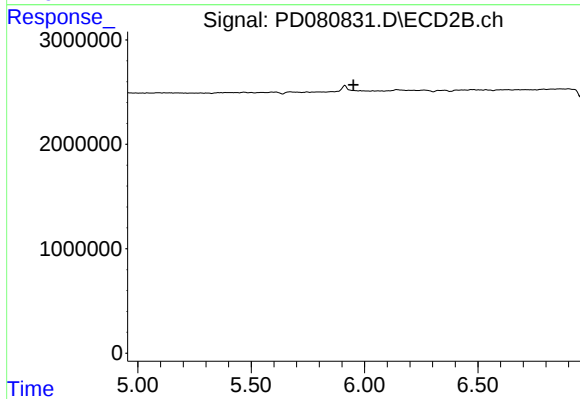

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

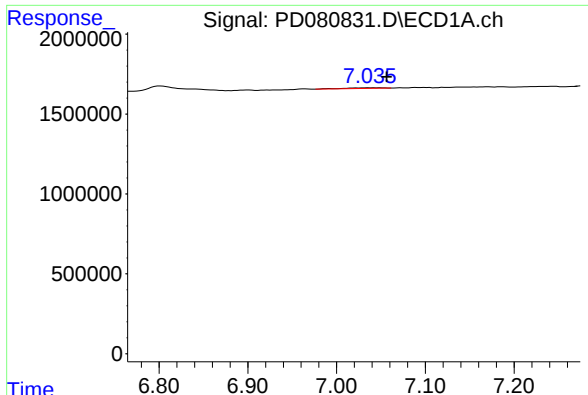

#17 4,4'-DDT


R.T.: 7.036 min
Delta R.T.: -0.021 min
Response: 127096
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

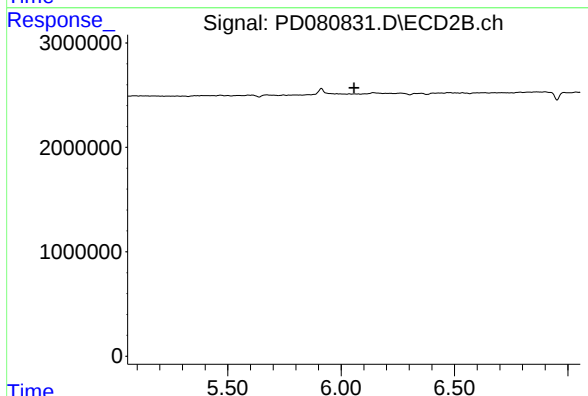


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.057 min
Response: 0
Conc: N.D.

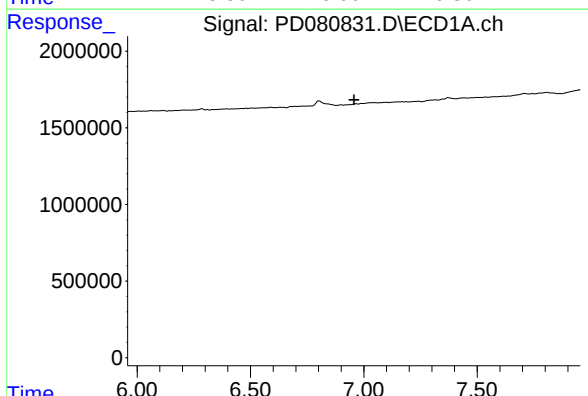


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.958 min
Response: 0
Conc: N.D.

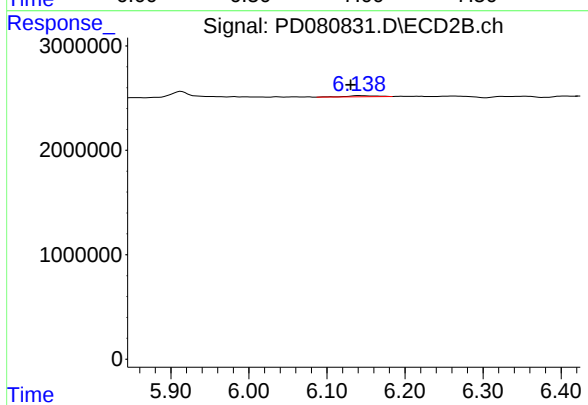

#18 Endrin aldehyde


R.T.: 6.140 min
Delta R.T.: 0.010 min
Response: 283284
Conc: 0.13 ng/ml

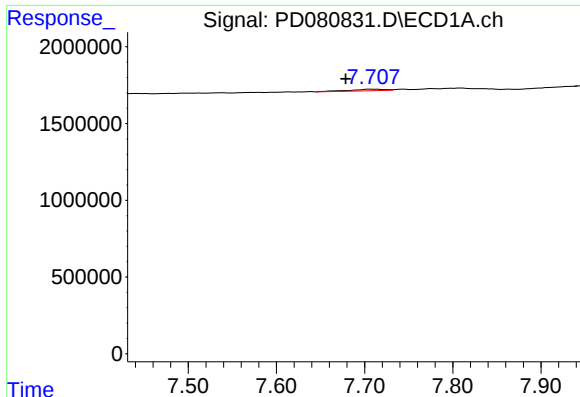

#21 Endrin ketone


R.T.: 7.708 min
Delta R.T.: 0.030 min
Response: 281609
Conc: 0.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

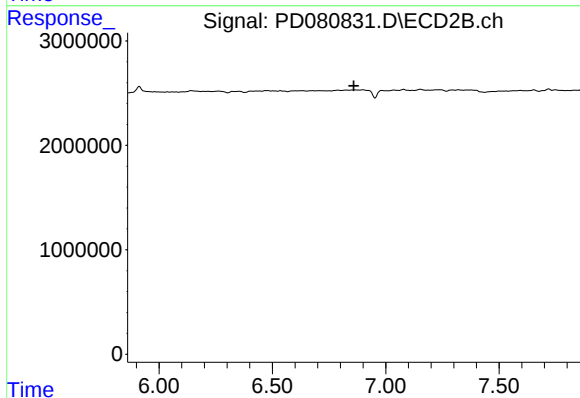


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

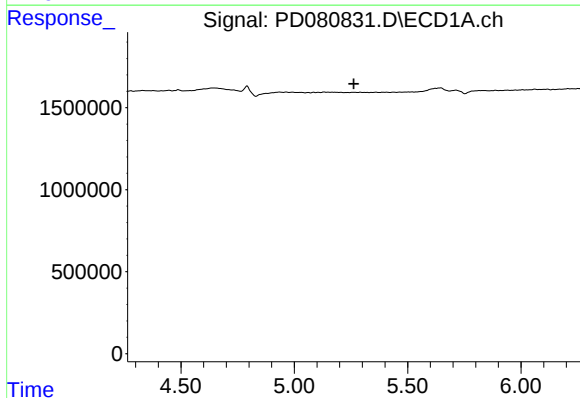


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.263 min
Response: 0
Conc: N.D.

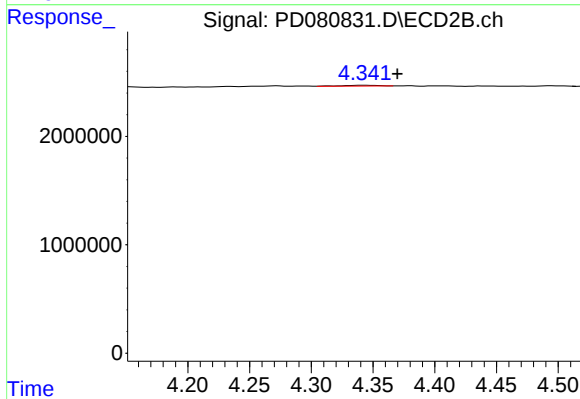

#24 Chlordane-2


R.T.: 4.342 min
Delta R.T.: -0.027 min
Response: 152913
Conc: 1.25 ng/ml

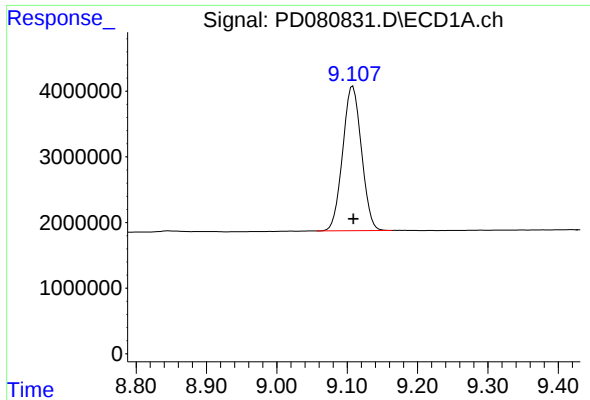

#28 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: 0.000 min
Response: 40880757
Conc: 20.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

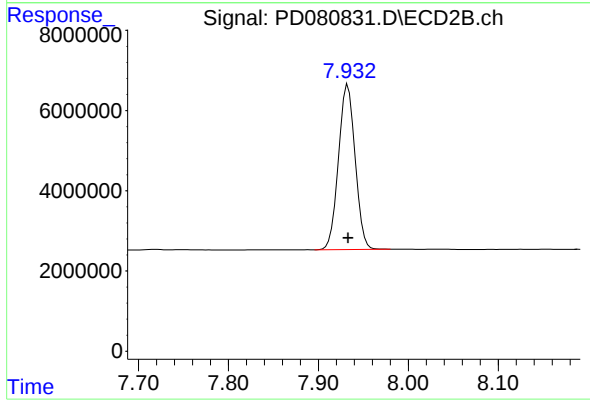

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 52901680
Conc: 19.86 ng/ml