

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
 Data File : PD080842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 17:46
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 17:57:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 24 17:57:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	36362169	73128842	25.776	25.137
28)	SA Decachlor...	9.109	7.933	52921832	71213005	26.677	26.197
Target Compounds							
23)	Chlordane-1	4.733	3.794	20847591	25408216	274.620	255.300
24)	Chlordane-2	5.262	4.370	22627577	31068321	284.743	267.358
25)	Chlordane-3	5.974	4.999	82445802	82953561	263.952	250.118
26)	Chlordane-4	6.057	5.063	99473473	77872681	266.437	248.919
27)	Chlordane-5	6.908	5.958	17612898	30386303	258.395	253.481



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
Data File : PD080842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 17:46
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 17:57:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Wed Jan 24 17:57:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

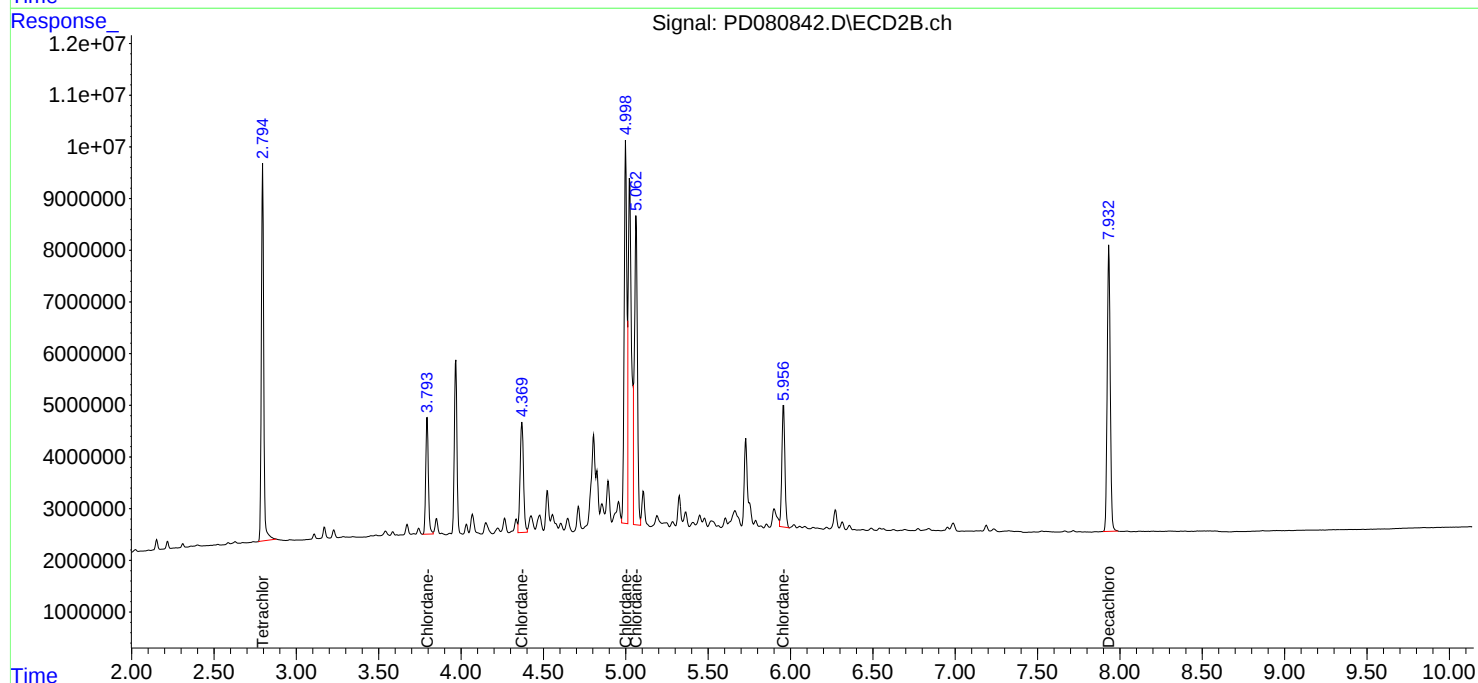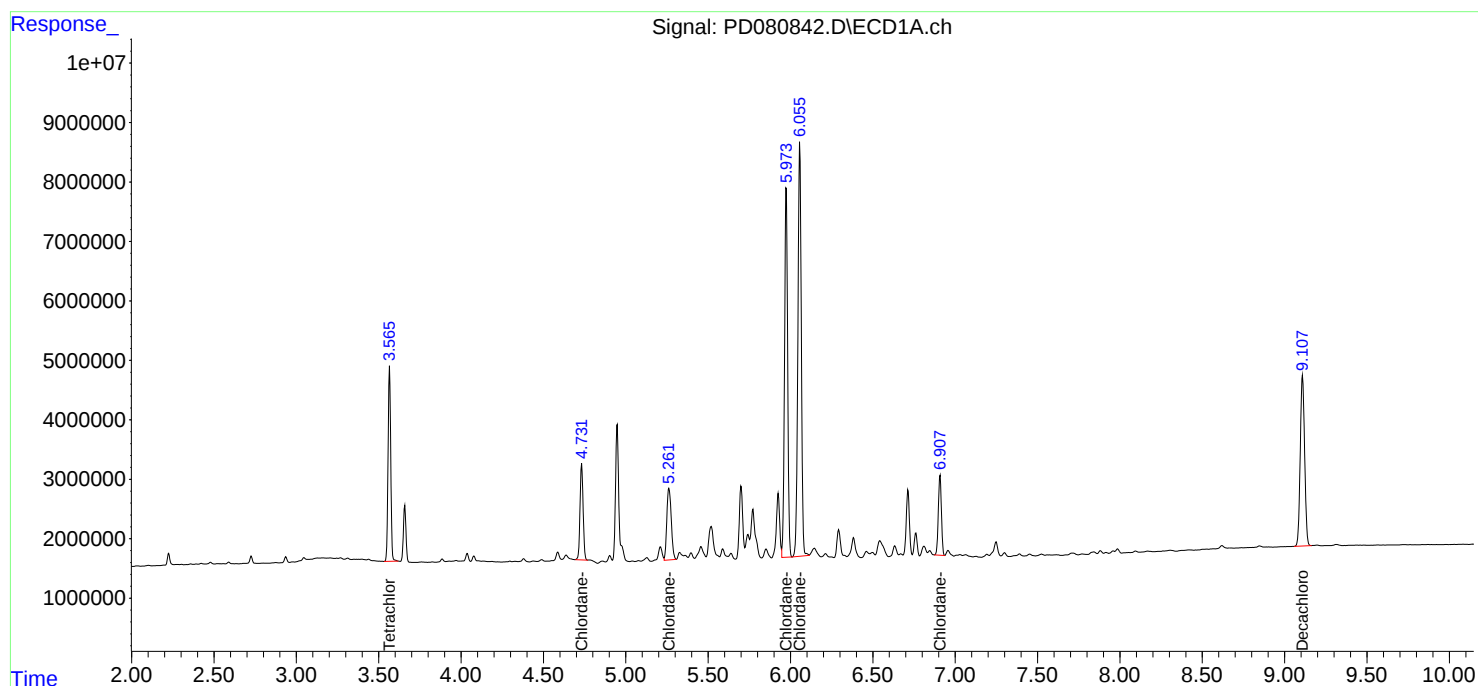


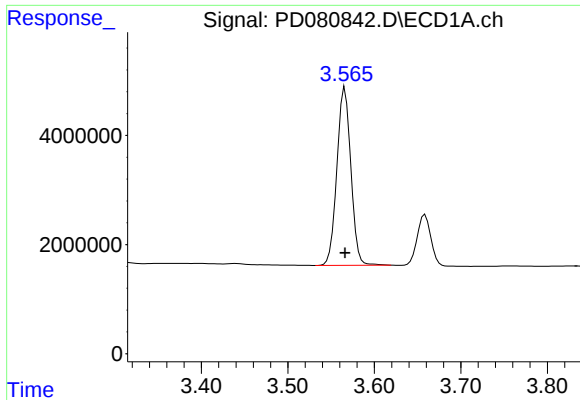

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 36362169
Conc: 25.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

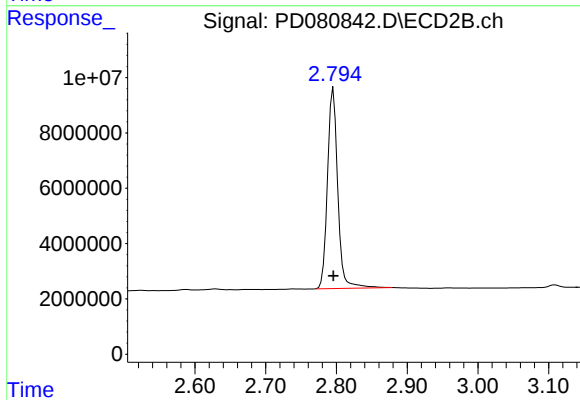


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 73128842
Conc: 25.14 ng/ml

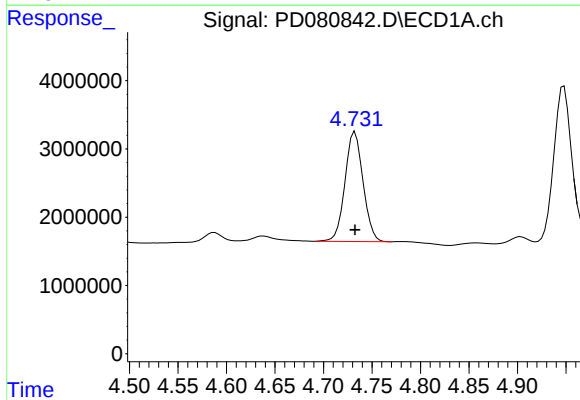


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 20847591
Conc: 274.62 ng/ml

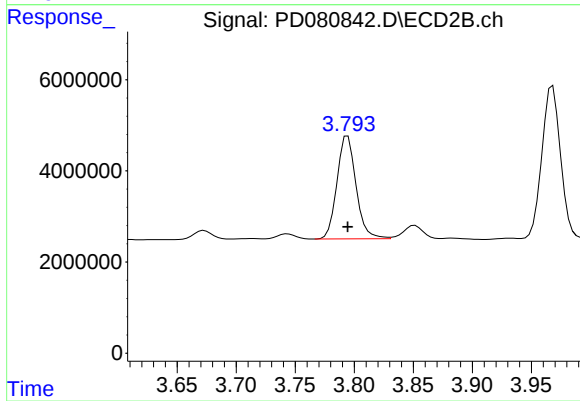

#23 Chlordane-1


R.T.: 3.794 min
Delta R.T.: 0.000 min
Response: 25408216
Conc: 255.30 ng/ml

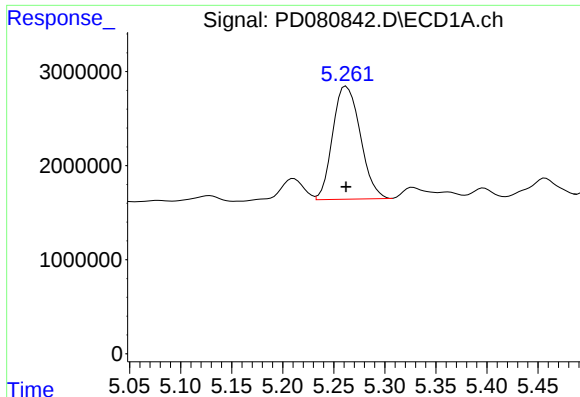

#24 Chlordane-2


R.T.: 5.262 min
Delta R.T.: 0.000 min
Response: 22627577
Conc: 284.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

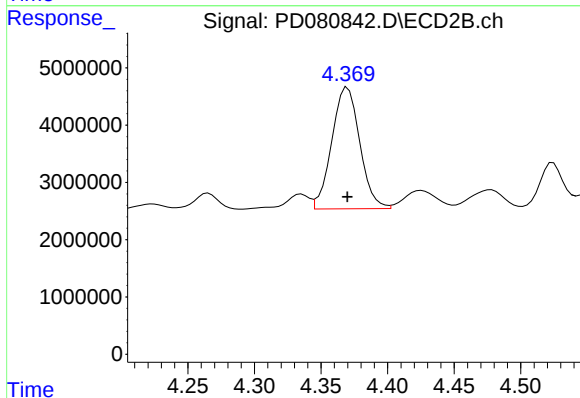


#24 Chlordane-2

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 31068321
Conc: 267.36 ng/ml

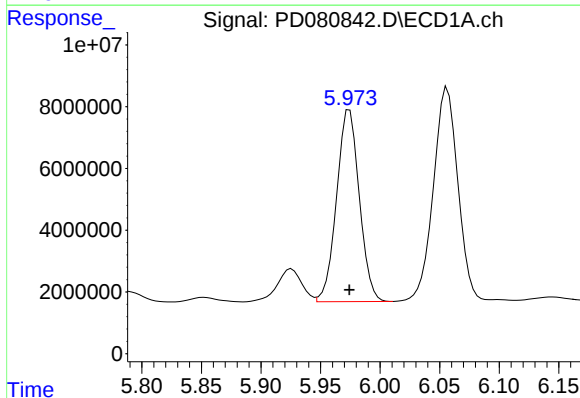


#25 Chlordane-3

R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 82445802
Conc: 263.95 ng/ml

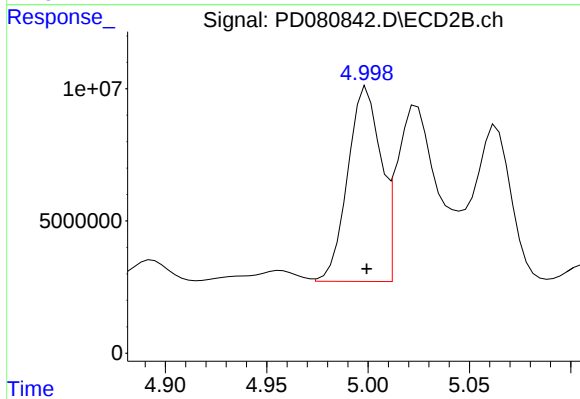

#25 Chlordane-3


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 82953561
Conc: 250.12 ng/ml

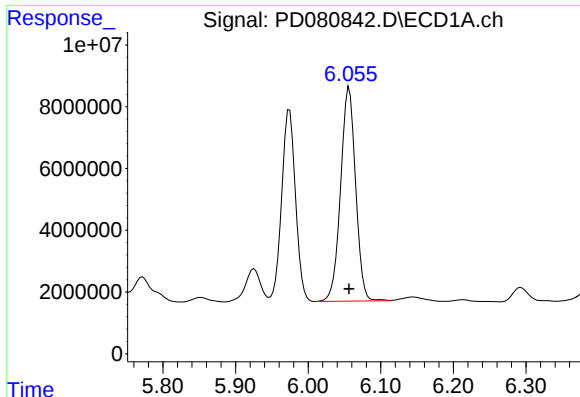

#26 Chlordane-4


R.T.: 6.057 min
Delta R.T.: 0.000 min
Response: 99473473
Conc: 266.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

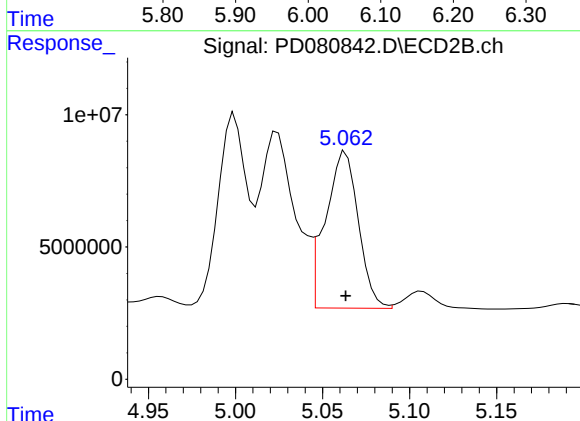


#26 Chlordane-4

R.T.: 5.063 min
Delta R.T.: 0.000 min
Response: 77872681
Conc: 248.92 ng/ml

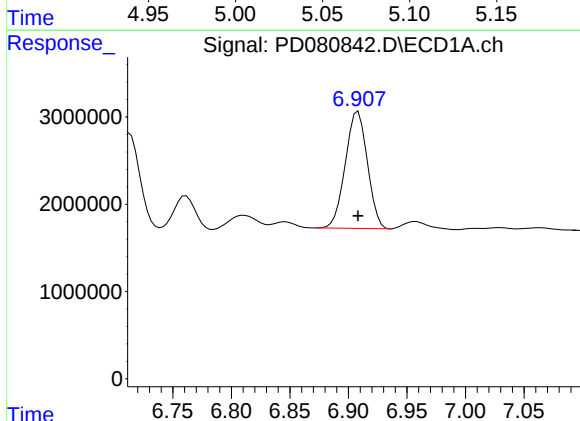


#27 Chlordane-5

R.T.: 6.908 min
Delta R.T.: 0.000 min
Response: 17612898
Conc: 258.39 ng/ml

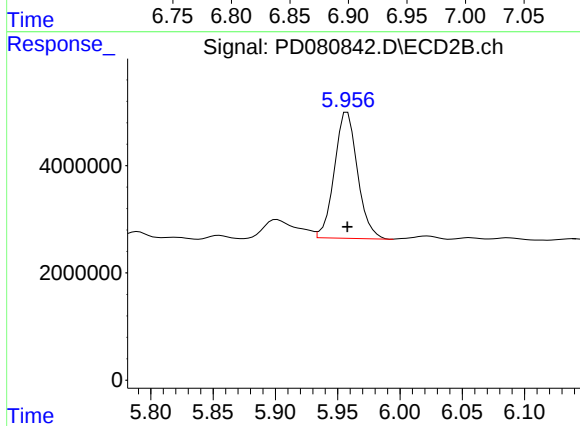

#27 Chlordane-5


R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 30386303
Conc: 253.48 ng/ml

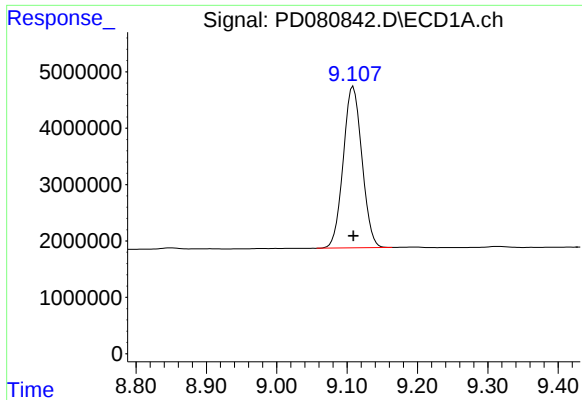

#28 Decachlorobiphenyl

R.T.: 9.109 min
Delta R.T.: 0.000 min
Response: 52921832
Conc: 26.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

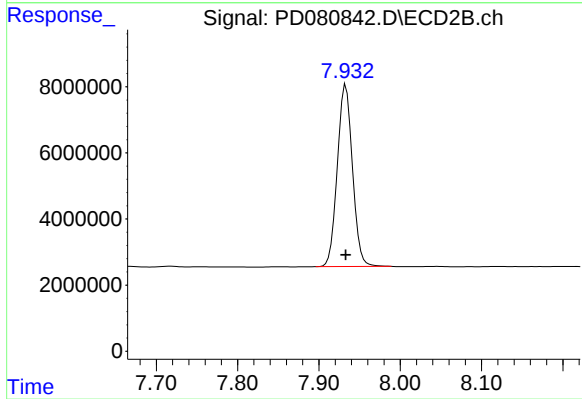

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 71213005
Conc: 26.20 ng/ml