

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
 Data File : PD080833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 15:46
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 00:56:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
 Quant Title : GC Extractables
 QLast Update : Wed Jan 24 20:16:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.796	28909945	47636703	20.365	19.914
28)	SA Decachlor...	9.110	7.933	41865014	54152447	20.803	20.330
Target Compounds							
9)	A Endosulfan I	6.105	5.120	20427853	29705845	9.849	9.699
10)	B gamma-Chl...	5.974	5.000	22241800	32818897	10.160	10.033
12)	B 4,4'-DDE	6.224	5.252	38679879	59002396	19.008	19.261
13)	MA Dieldrin	6.380	5.384	40996708	63742775	18.553	18.743
19)	B Endosulfa...	7.193	6.353	36511115	54189034	19.229	19.427
20)	A Methoxychlor	7.530	6.631	90132130	143.0E6	87.568	91.328
21)	B Endrin ke...	7.679	6.859	39977056	61789883	19.117	19.148



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD012424\
Data File : PD080833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 15:46
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 00:56:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD012424.M
Quant Title : GC Extractables
QLast Update : Wed Jan 24 20:16:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

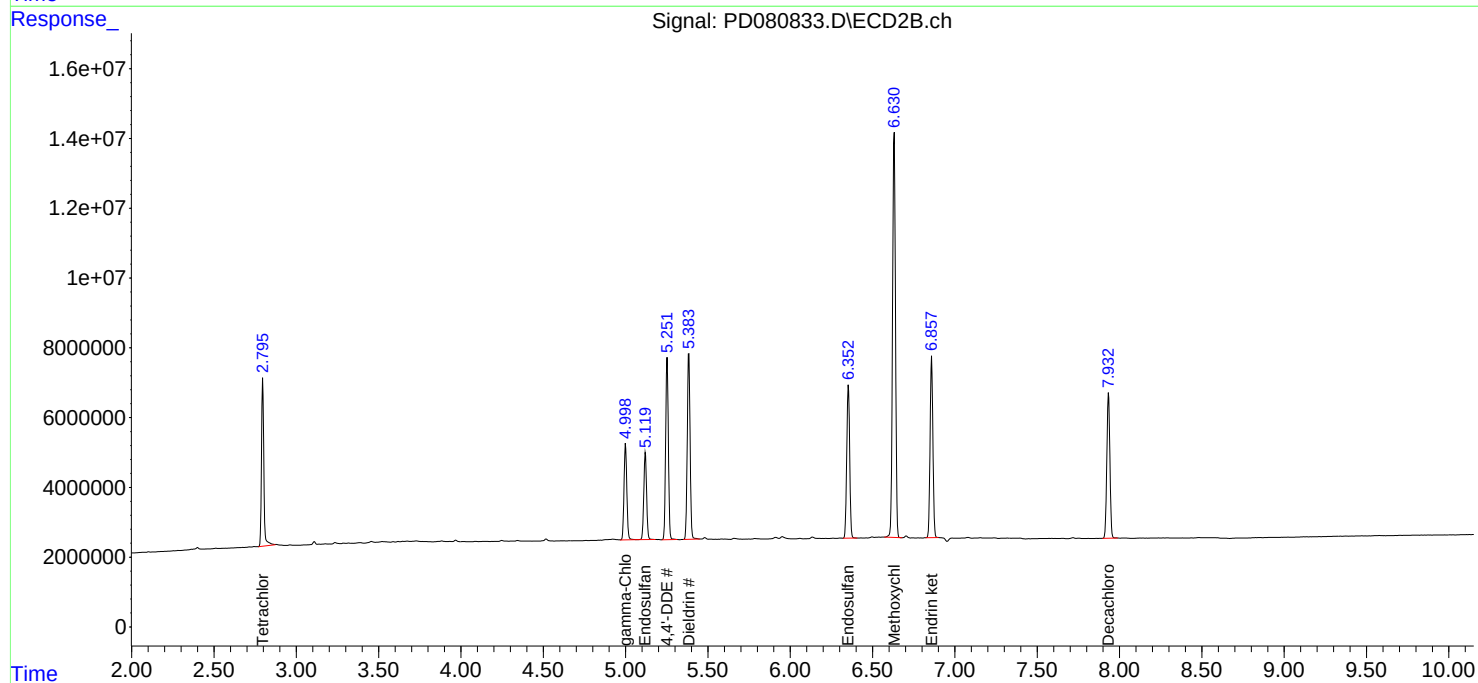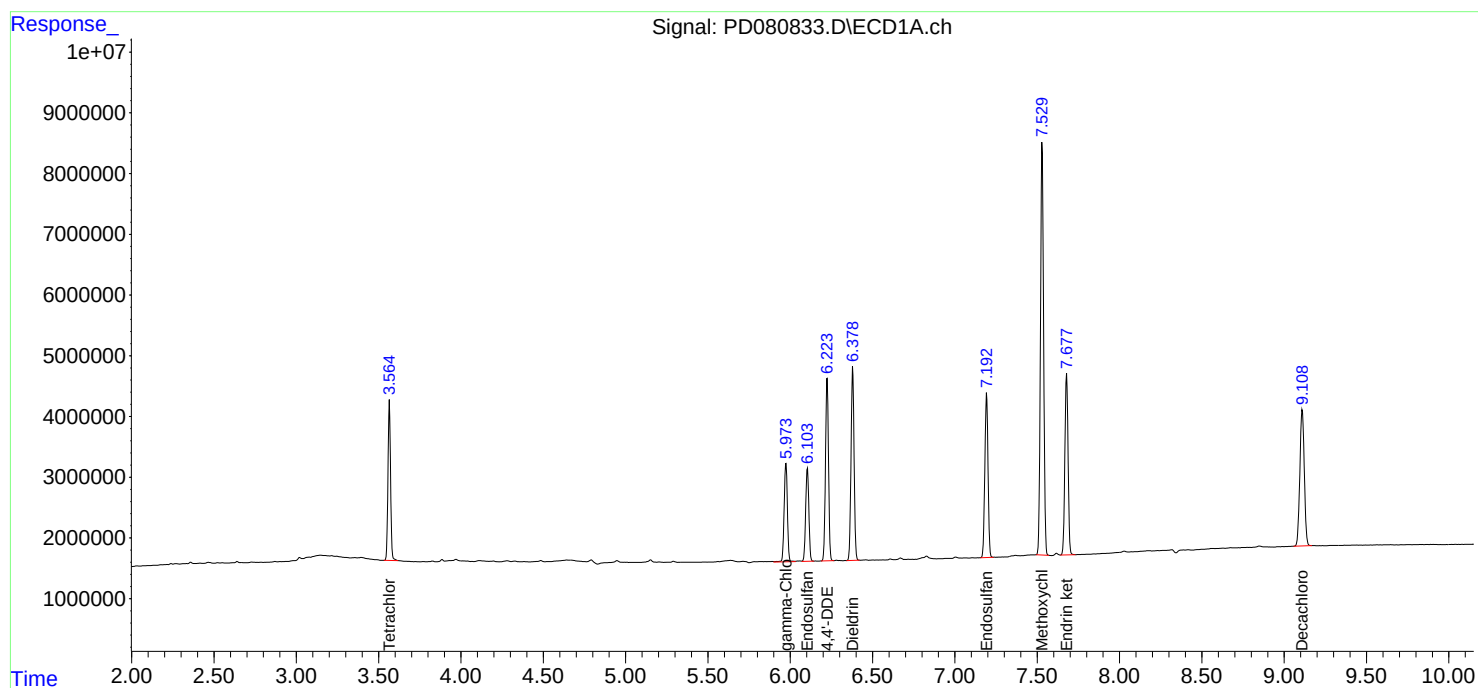


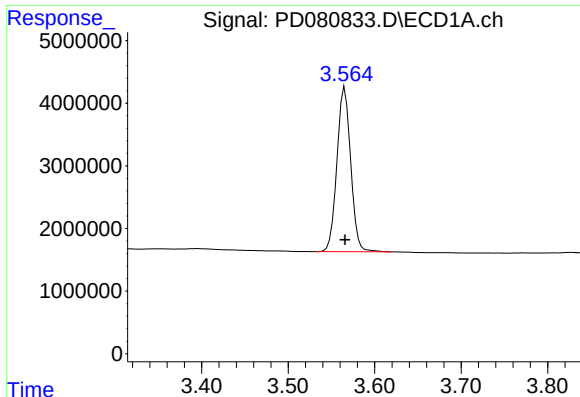

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: 0.000 min
Response: 28909945
Conc: 20.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

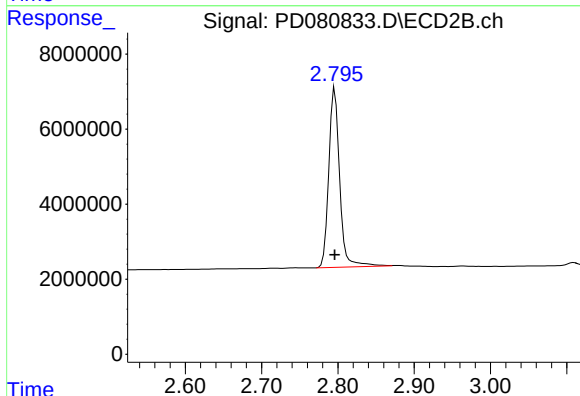


#1 Tetrachloro-m-xylene

R.T.: 2.796 min
Delta R.T.: 0.000 min
Response: 47636703
Conc: 19.91 ng/ml

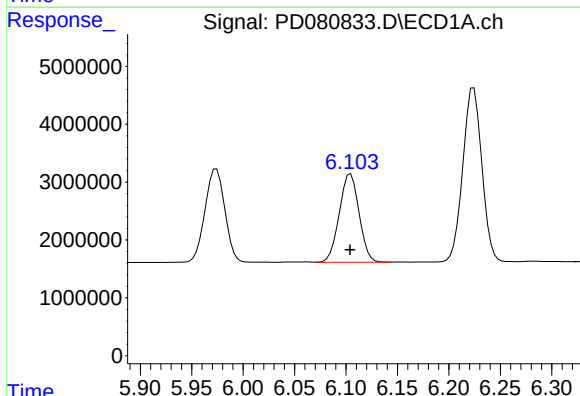


#9 Endosulfan I

R.T.: 6.105 min
Delta R.T.: 0.000 min
Response: 20427853
Conc: 9.85 ng/ml

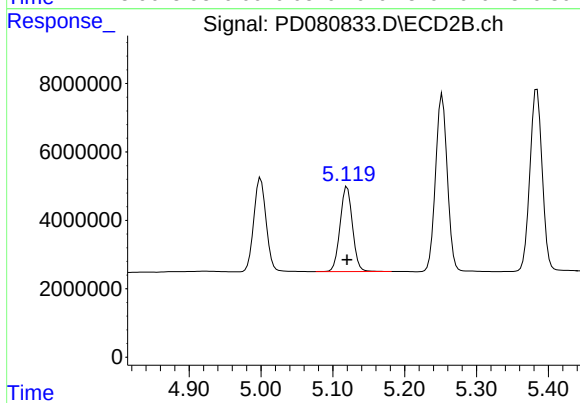

#9 Endosulfan I


R.T.: 5.120 min
Delta R.T.: 0.000 min
Response: 29705845
Conc: 9.70 ng/ml

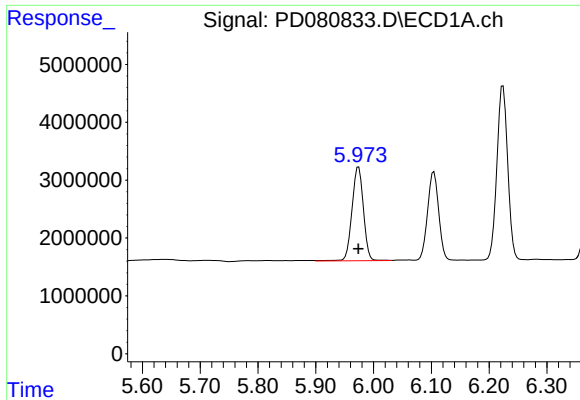

#10 gamma-Chlordane


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 22241800
Conc: 10.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

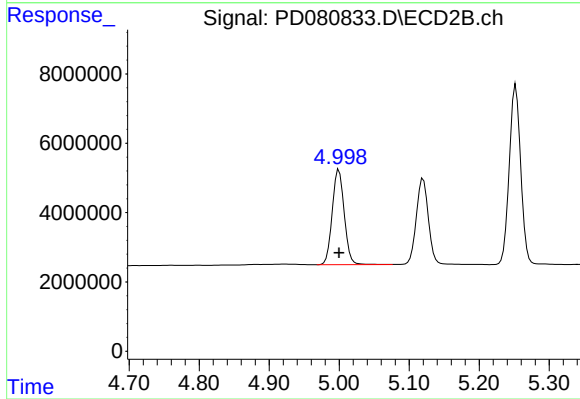


#10 gamma-Chlordane

R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 32818897
Conc: 10.03 ng/ml

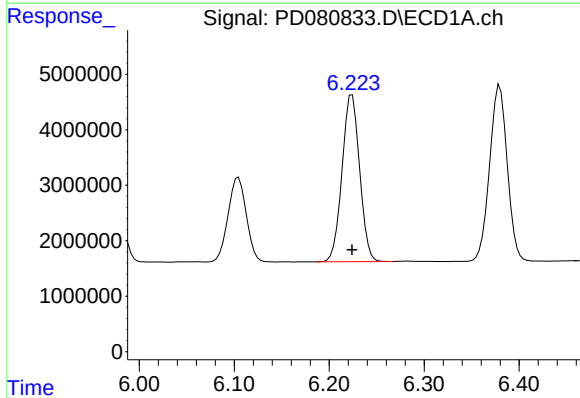


#12 4,4'-DDE

R.T.: 6.224 min
Delta R.T.: 0.000 min
Response: 38679879
Conc: 19.01 ng/ml

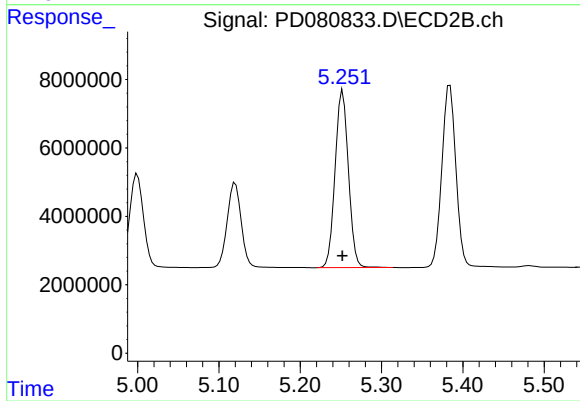

#12 4,4'-DDE


R.T.: 5.252 min
Delta R.T.: 0.000 min
Response: 59002396
Conc: 19.26 ng/ml

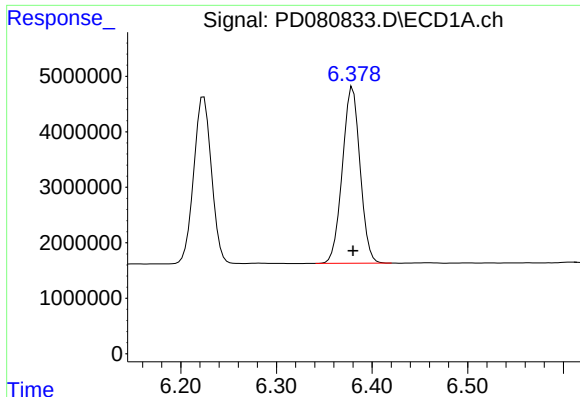

#13 Dieldrin


R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 40996708
Conc: 18.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

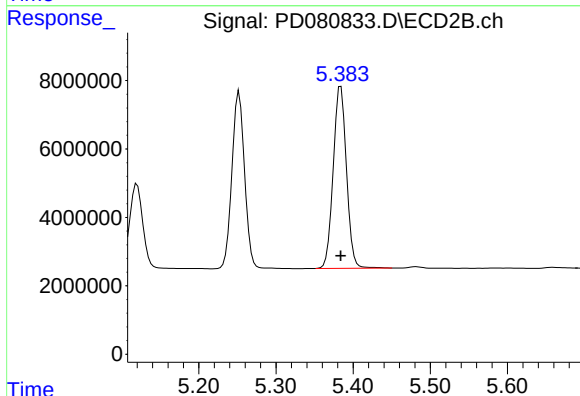


#13 Dieldrin

R.T.: 5.384 min
Delta R.T.: 0.000 min
Response: 63742775
Conc: 18.74 ng/ml

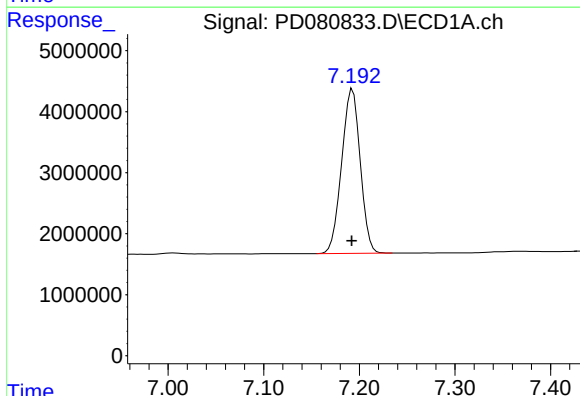


#19 Endosulfan Sulfate

R.T.: 7.193 min
Delta R.T.: 0.000 min
Response: 36511115
Conc: 19.23 ng/ml

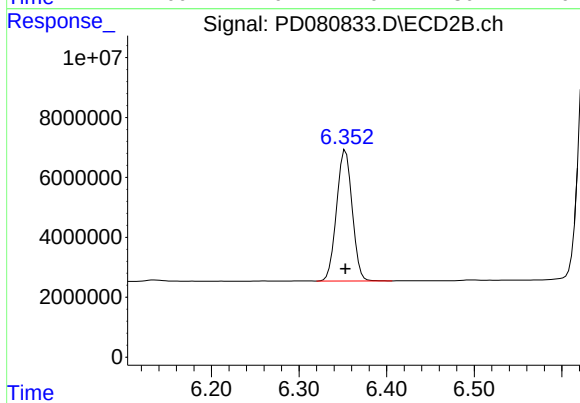

#19 Endosulfan Sulfate


R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 54189034
Conc: 19.43 ng/ml

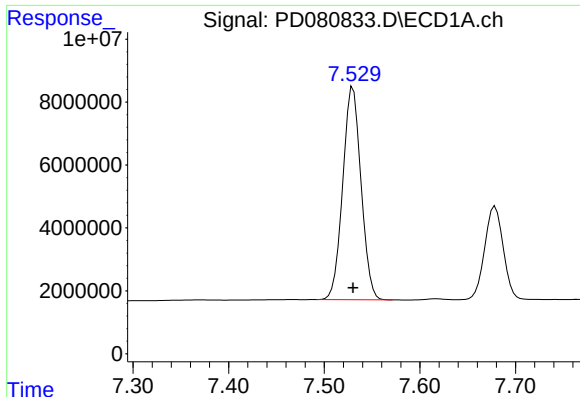

#20 Methoxychlor


R.T.: 7.530 min
Delta R.T.: 0.000 min
Response: 90132130
Conc: 87.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

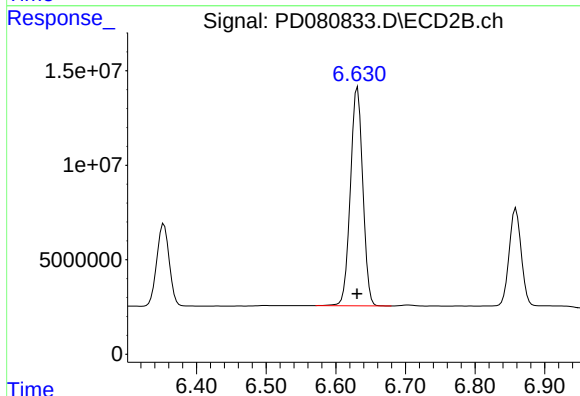


#20 Methoxychlor

R.T.: 6.631 min
Delta R.T.: 0.000 min
Response: 142951815
Conc: 91.33 ng/ml

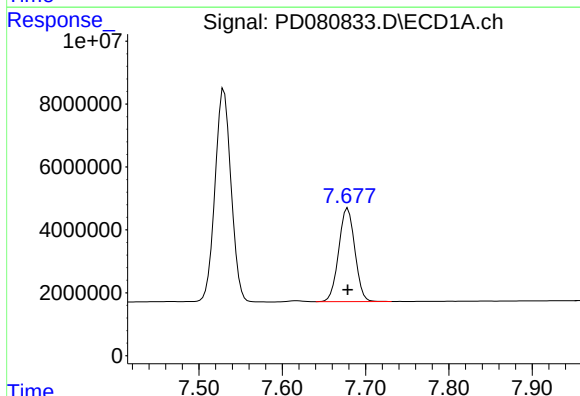


#21 Endrin ketone

R.T.: 7.679 min
Delta R.T.: 0.000 min
Response: 39977056
Conc: 19.12 ng/ml

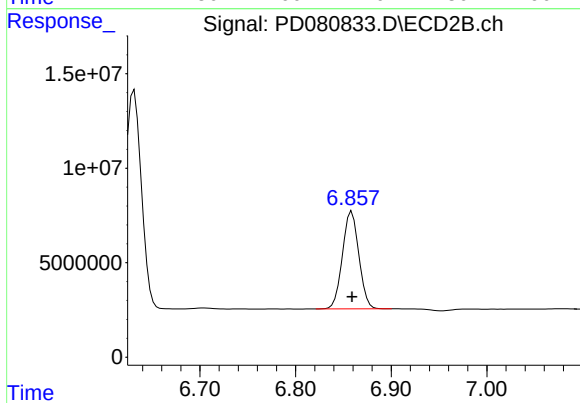

#21 Endrin ketone


R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 61789883
Conc: 19.15 ng/ml

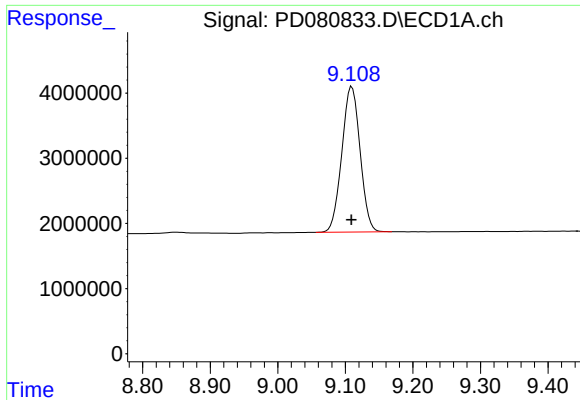

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.000 min
Response: 41865014
Conc: 20.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

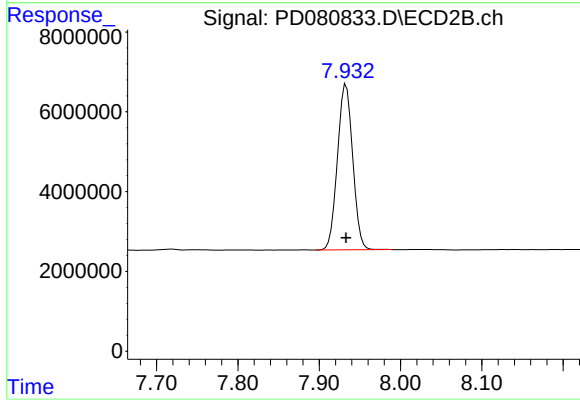

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 54152447
Conc: 20.33 ng/ml